

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
 Data File : PL077534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 11:34
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 12:27:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 12:26:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.628	126.8E6	228.4E6	72.517	72.384
28)	SA Decachlor...	8.908	7.730	101.8E6	139.6E6	68.175	71.264
Target Compounds							
23)	Chlordane-1	4.577	3.607	48345646	64438449	719.166	722.697
24)	Chlordane-2	5.110	4.177	52482441	70411858	699.393	710.250
25)	Chlordane-3	5.822	4.800	203.4E6	206.2E6	723.471	720.158
26)	Chlordane-4	5.900	4.861	248.8E6	217.0E6	716.126	721.874
27)	Chlordane-5	6.759	5.526	42602709	51470851	698.410	732.456



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
Data File : PL077534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 11:34
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 12:27:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 12:26:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

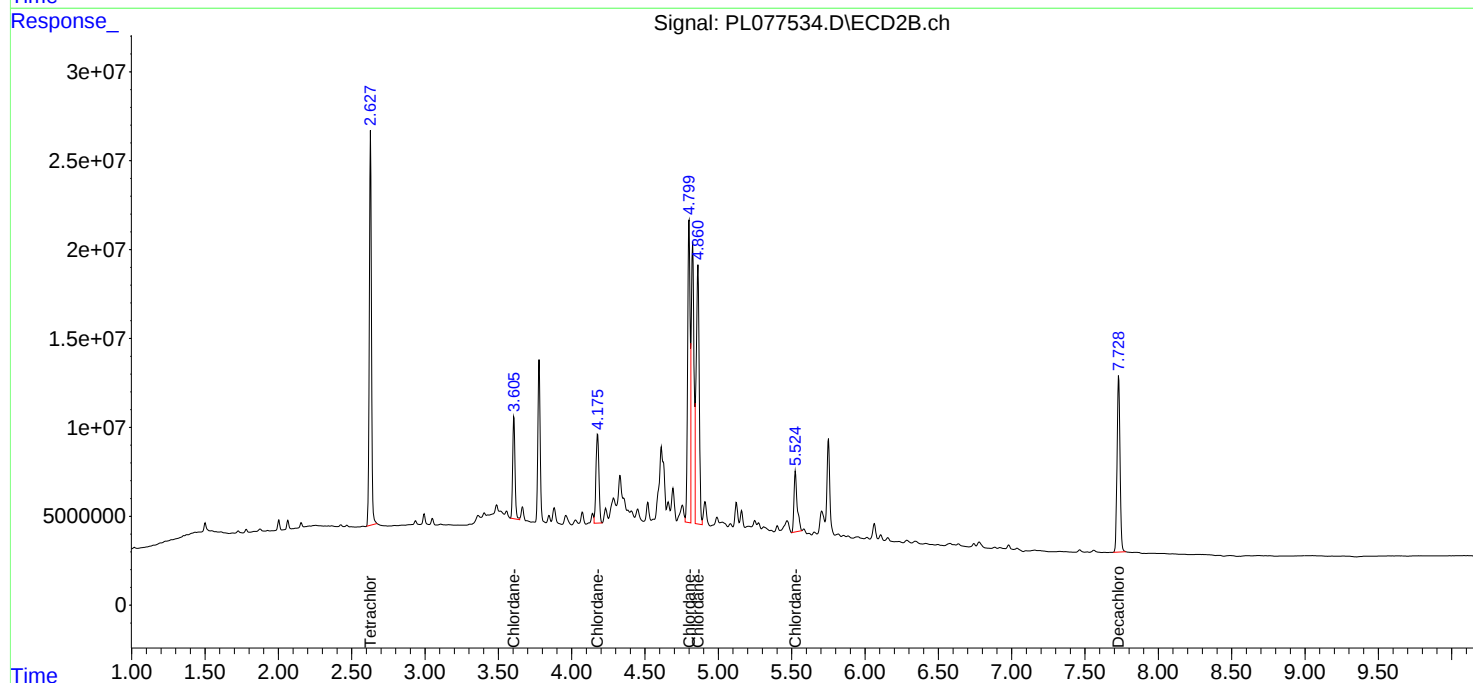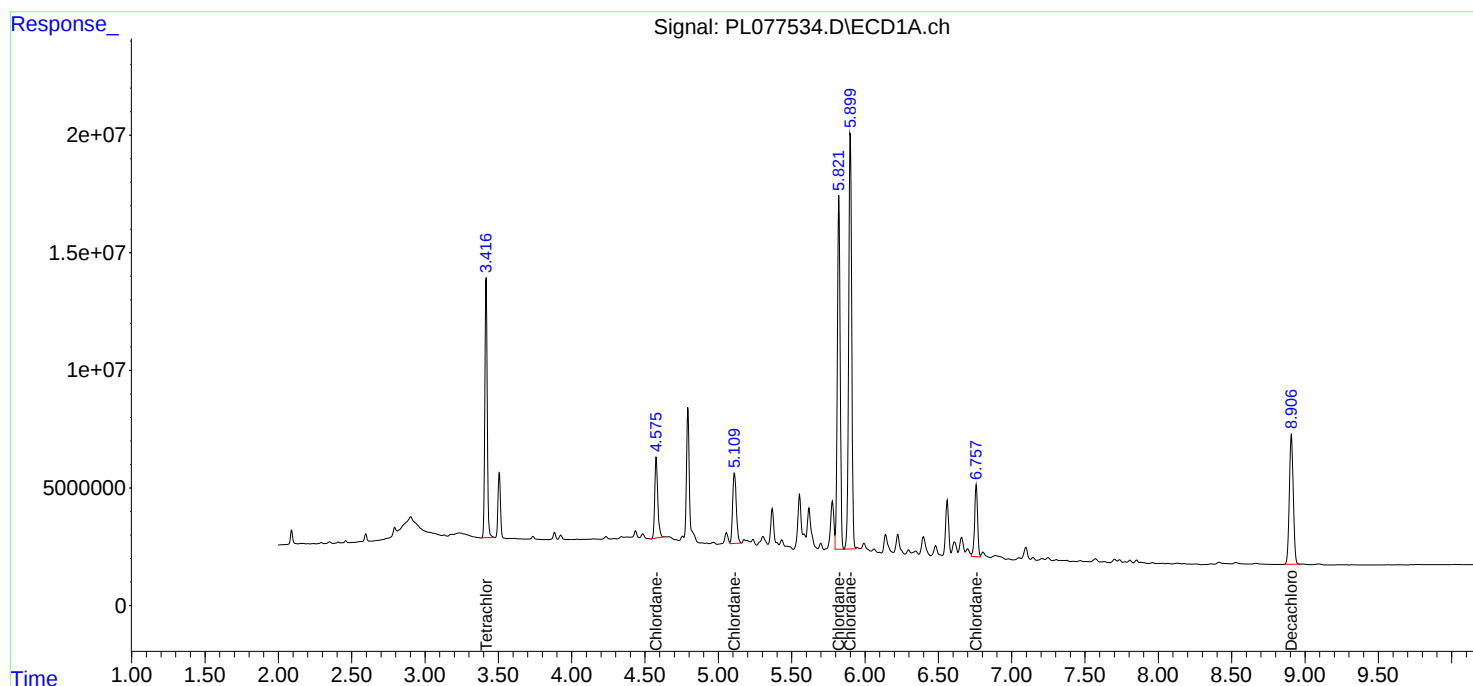


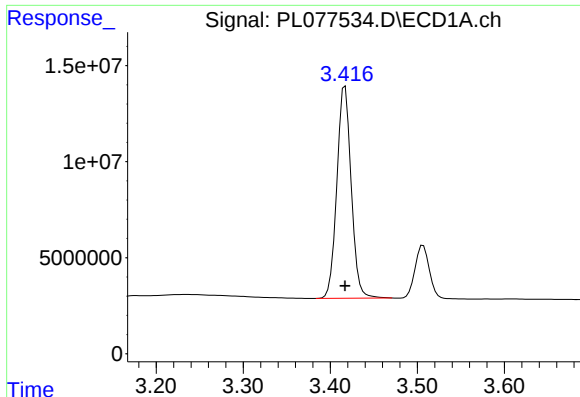

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 126773463
Conc: 72.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

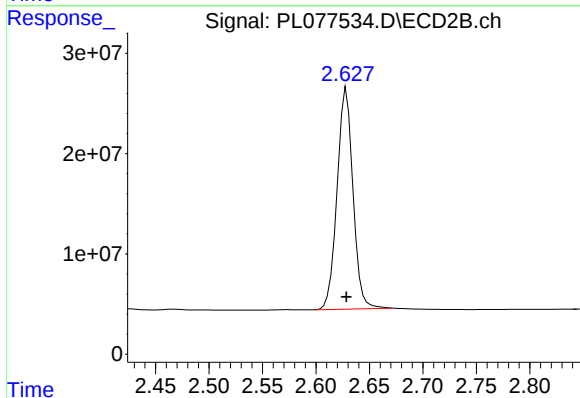


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 228350369
Conc: 72.38 ng/ml

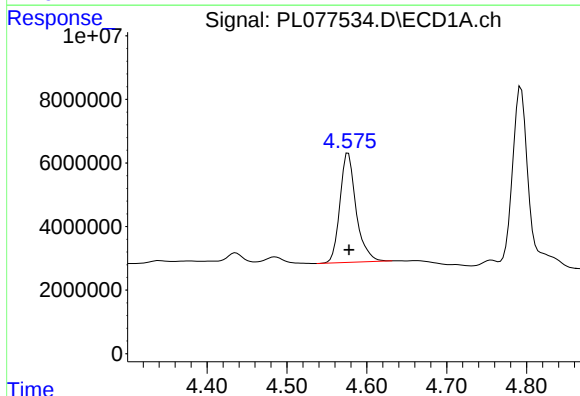


#23 Chlordane-1

R.T.: 4.577 min
Delta R.T.: 0.000 min
Response: 48345646
Conc: 719.17 ng/ml

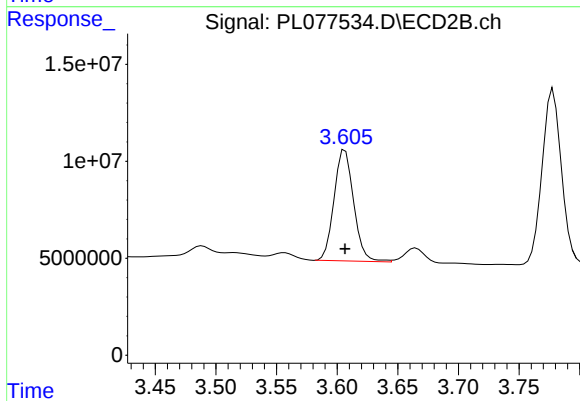

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 64438449
Conc: 722.70 ng/ml

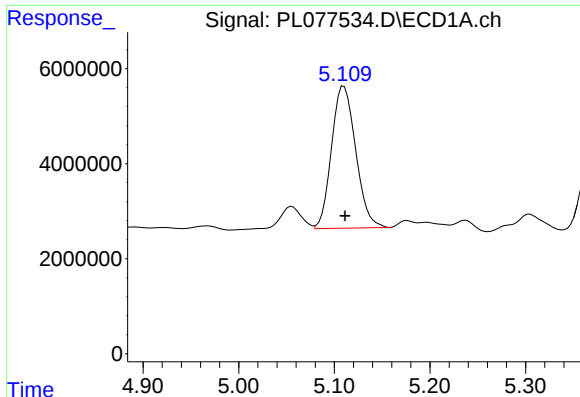

#24 Chlordane-2


R.T.: 5.110 min
Delta R.T.: -0.001 min
Response: 52482441
Conc: 699.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

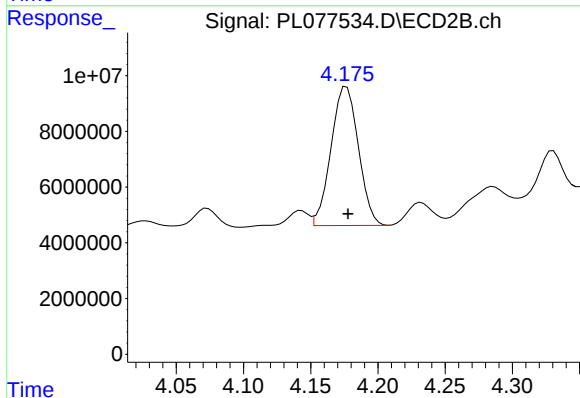


#24 Chlordane-2

R.T.: 4.177 min
Delta R.T.: -0.001 min
Response: 70411858
Conc: 710.25 ng/ml

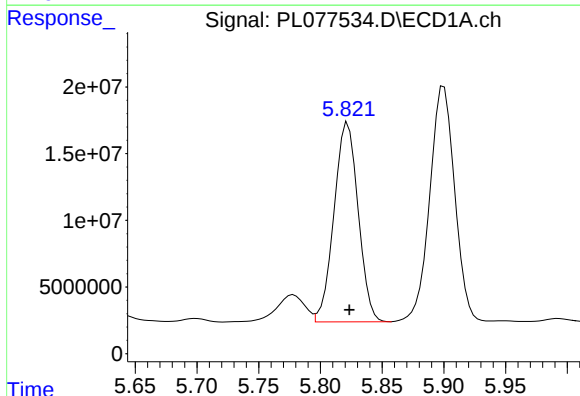


#25 Chlordane-3

R.T.: 5.822 min
Delta R.T.: -0.001 min
Response: 203413219
Conc: 723.47 ng/ml

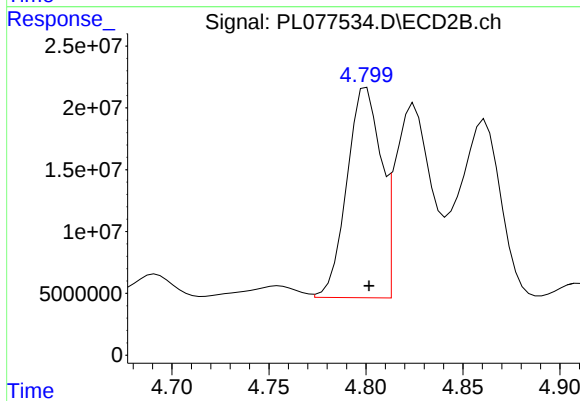

#25 Chlordane-3


R.T.: 4.800 min
Delta R.T.: -0.001 min
Response: 206233158
Conc: 720.16 ng/ml

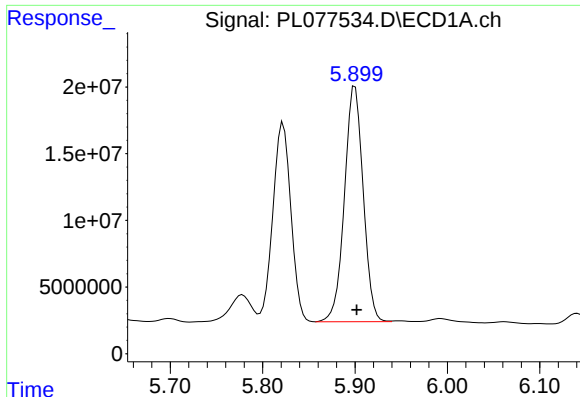

#26 Chlordane-4


R.T.: 5.900 min
Delta R.T.: -0.002 min
Response: 248829982
Conc: 716.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

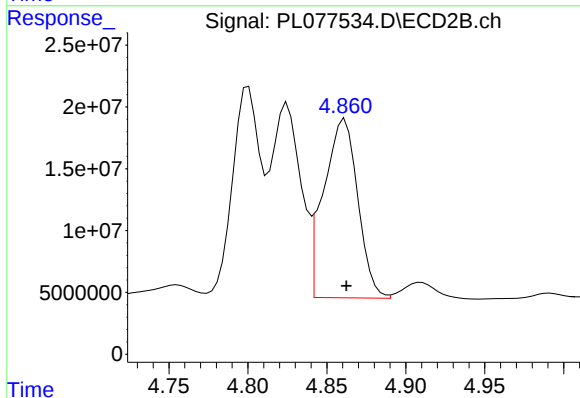


#26 Chlordane-4

R.T.: 4.861 min
Delta R.T.: -0.001 min
Response: 216991636
Conc: 721.87 ng/ml

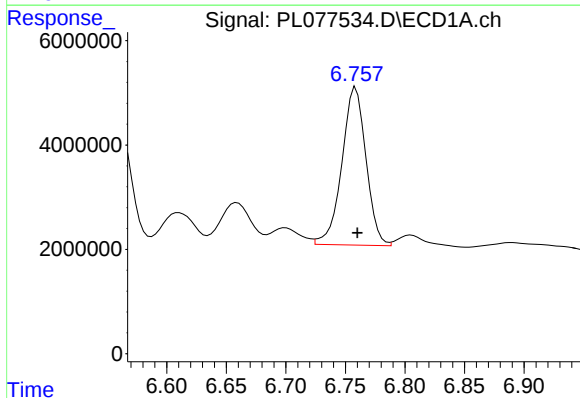


#27 Chlordane-5

R.T.: 6.759 min
Delta R.T.: -0.001 min
Response: 42602709
Conc: 698.41 ng/ml

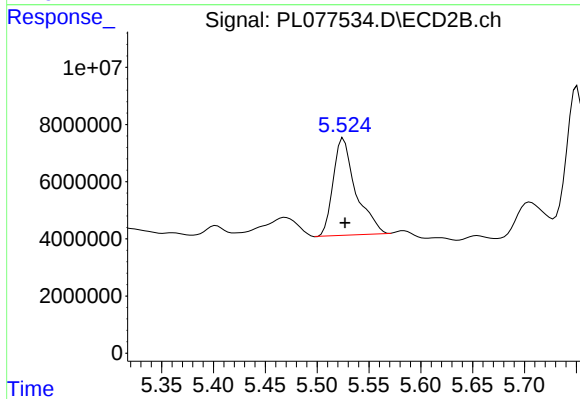

#27 Chlordane-5


R.T.: 5.526 min
Delta R.T.: -0.001 min
Response: 51470851
Conc: 732.46 ng/ml

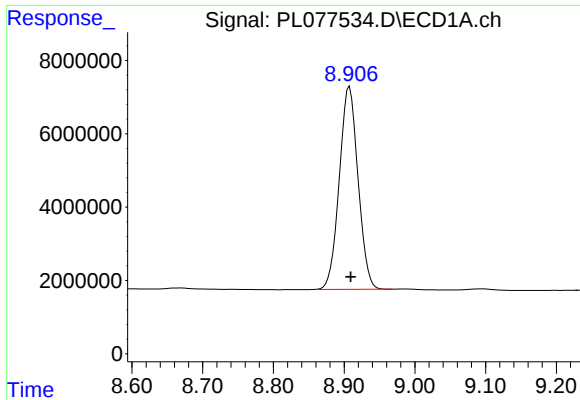

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: -0.002 min
Response: 101758868
Conc: 68.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

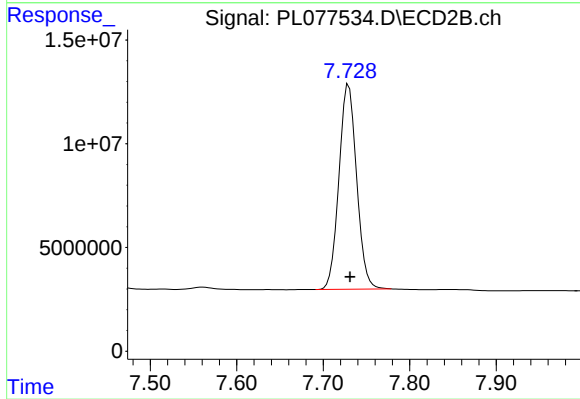

#28 Decachlorobiphenyl

R.T.: 7.730 min
Delta R.T.: -0.002 min
Response: 139562014
Conc: 71.26 ng/ml