

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
 Data File : PL077544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 13:52
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL090722CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 14:31:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 14:28:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.628	88756443	162.2E6	51.975	51.741
28)	SA Decachlor...	8.909	7.730	77724372	103.0E6	51.947	52.454
Target Compounds							
23)	Chlordane-1	4.577	3.606	35070619	47371414	542.331	566.350
24)	Chlordane-2	5.111	4.177	38348444	51283066	506.046	520.709
25)	Chlordane-3	5.823	4.801	146.5E6	151.5E6	540.780	530.276
26)	Chlordane-4	5.902	4.862	176.4E6	158.2E6	527.345	533.736
27)	Chlordane-5	6.760	5.526	29623643	38317819	491.818	552.283



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
Data File : PL077544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 13:52
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL090722CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 14:31:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 14:28:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

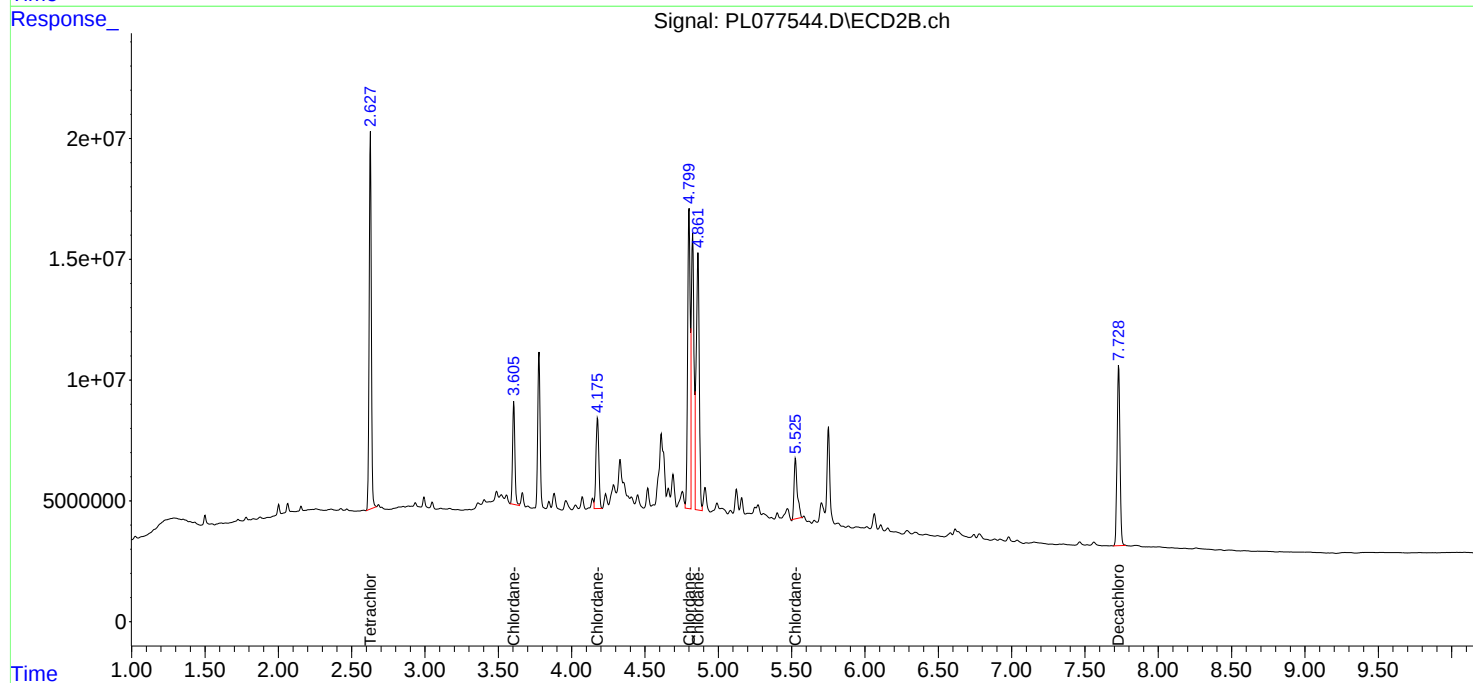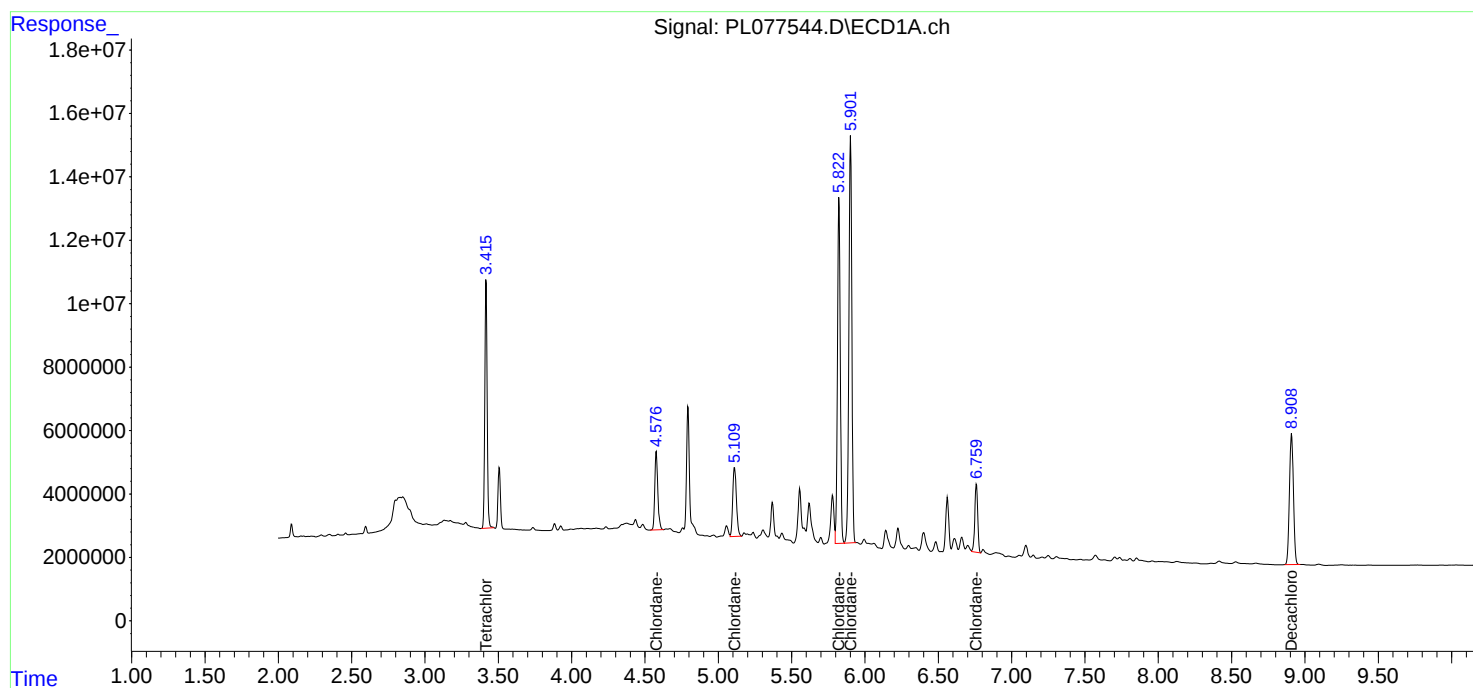


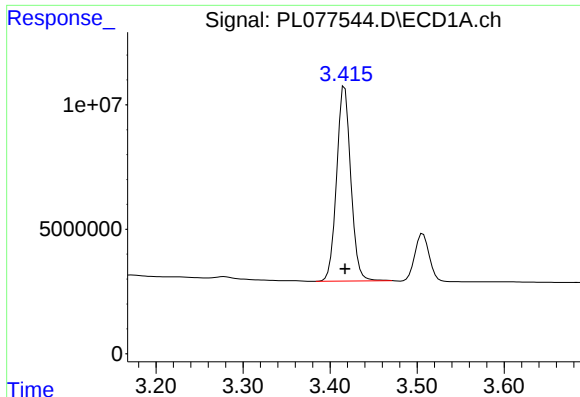

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 88756443
Conc: 51.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090722CHLOR

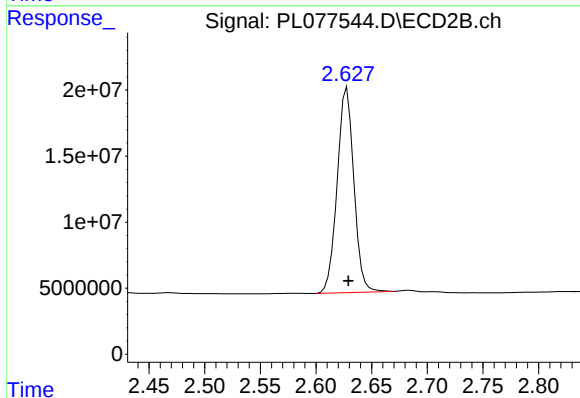


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: -0.001 min
Response: 162164478
Conc: 51.74 ng/ml

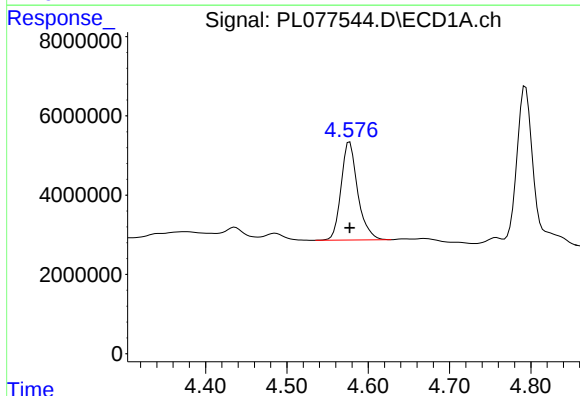


#23 Chlordane-1

R.T.: 4.577 min
Delta R.T.: 0.000 min
Response: 35070619
Conc: 542.33 ng/ml

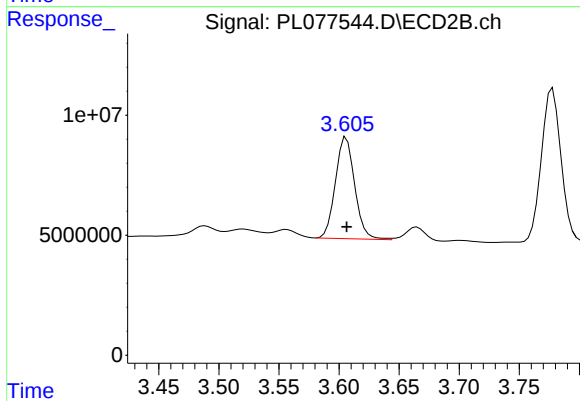

#23 Chlordane-1


R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 47371414
Conc: 566.35 ng/ml

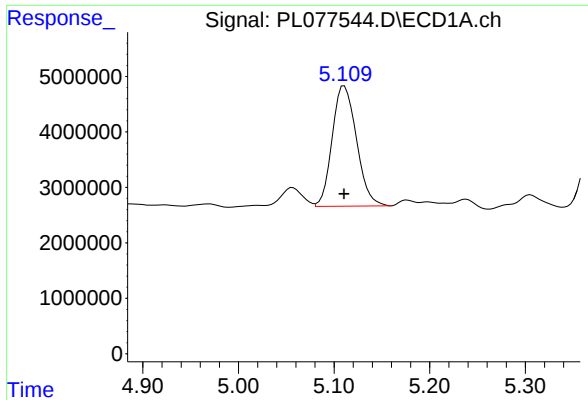

#24 Chlordane-2


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 38348444
Conc: 506.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090722CHLOR

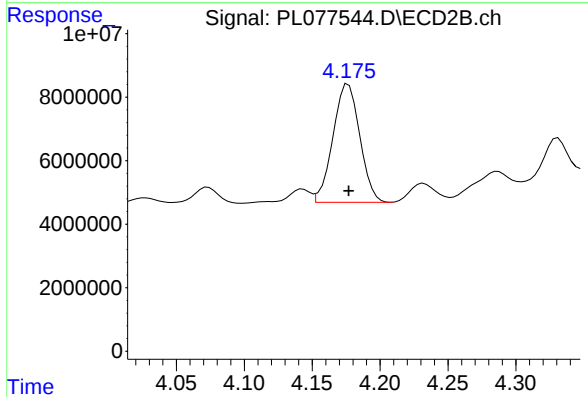


#24 Chlordane-2

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 51283066
Conc: 520.71 ng/ml

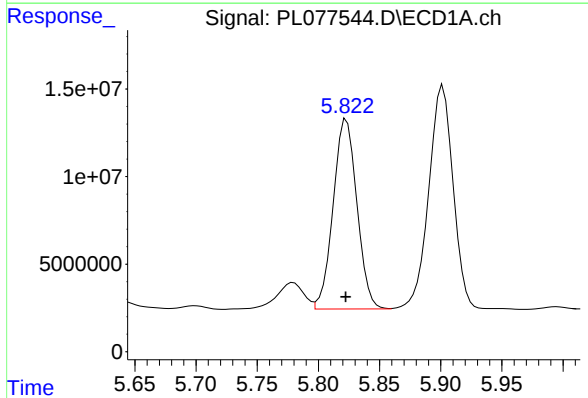


#25 Chlordane-3

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 146531291
Conc: 540.78 ng/ml

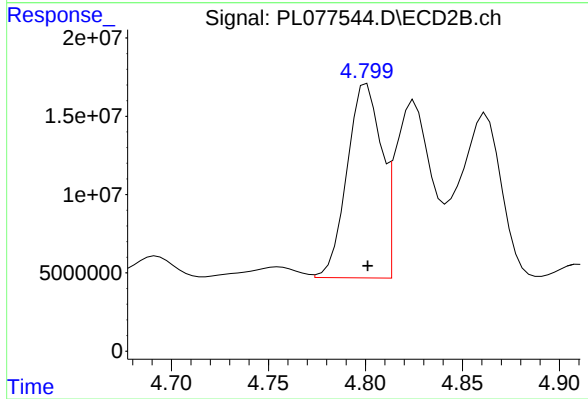

#25 Chlordane-3


R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 151465326
Conc: 530.28 ng/ml

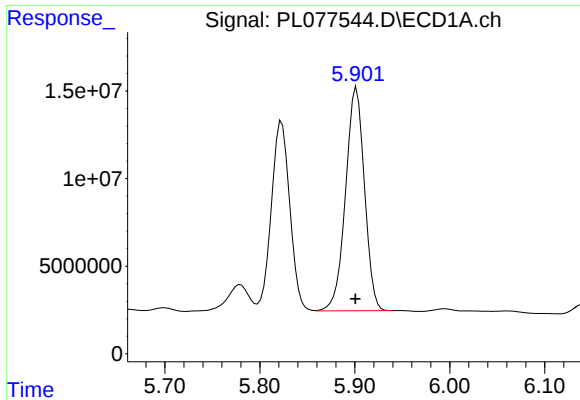

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.001 min
Response: 176390833
Conc: 527.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090722CHLOR

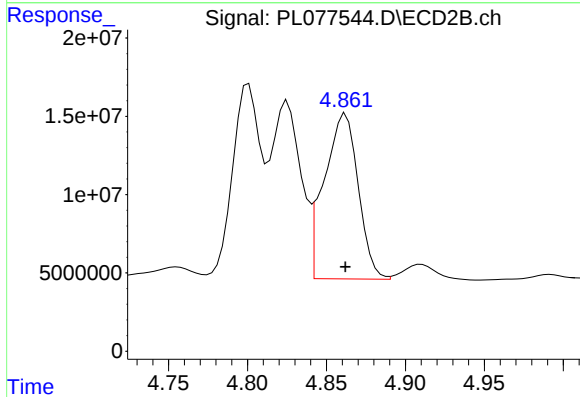


#26 Chlordane-4

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 158214901
Conc: 533.74 ng/ml

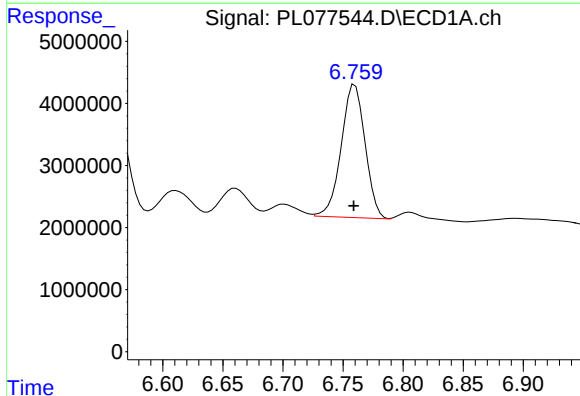


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 29623643
Conc: 491.82 ng/ml

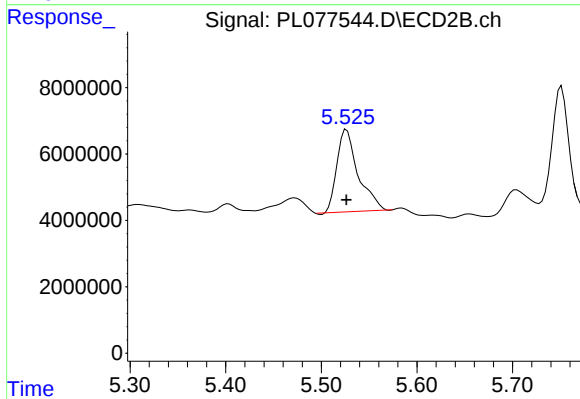

#27 Chlordane-5


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 38317819
Conc: 552.28 ng/ml

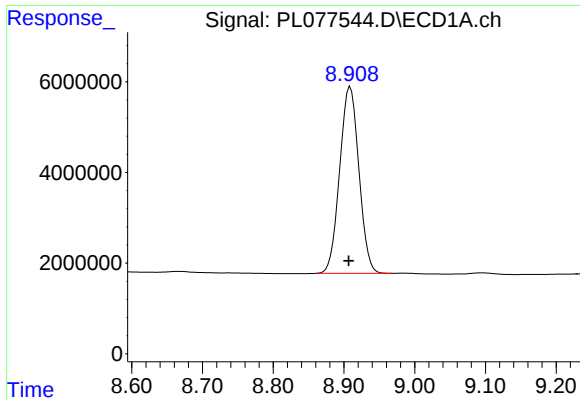

#28 Decachlorobiphenyl

R.T.: 8.909 min
Delta R.T.: 0.002 min
Response: 77724372
Conc: 51.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090722CHLOR

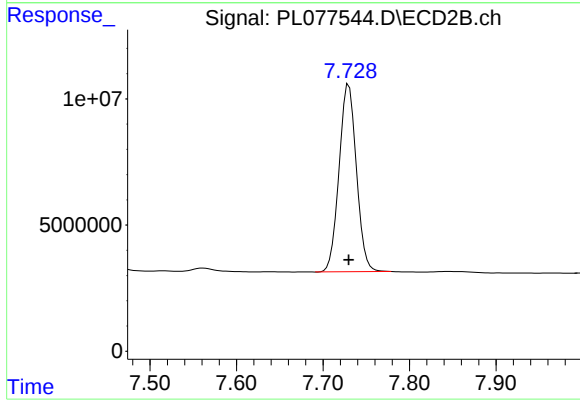

#28 Decachlorobiphenyl

R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 103047466
Conc: 52.45 ng/ml