

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090723\
 Data File : PL085151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 16:52
 Operator : AR\AJ
 Sample : 04267-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 22:06:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.684	55267399	24452765	22.046	20.714
27)	SA Decachlor...	9.028	7.863	37778410	28686705	22.044	21.180
Target Compounds							
4)	MA Heptachlor	4.859	0.000	15668148	0	4.046	N.D. #
5)	MB Aldrin	0.000	4.177f	0	4293	N.D.	<MDL
6)	B beta-BHC	4.458	3.789f	10499096	1917199	5.945	2.334 #
7)	B delta-BHC	4.716	0.000	45955630	0	12.594	N.D. #
9)	A Endosulfan I	0.000	4.993	0	1178956	N.D.	0.874
10)	B trans-Chl...	5.887	0.000	5847047	0	1.854	N.D. #
11)	B cis-Chlor...	0.000	4.993	0	1178956	N.D.	0.762


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080723\
Data File : PL085151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 16:52
Operator : AR\AJ
Sample : 04267-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 22:06:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

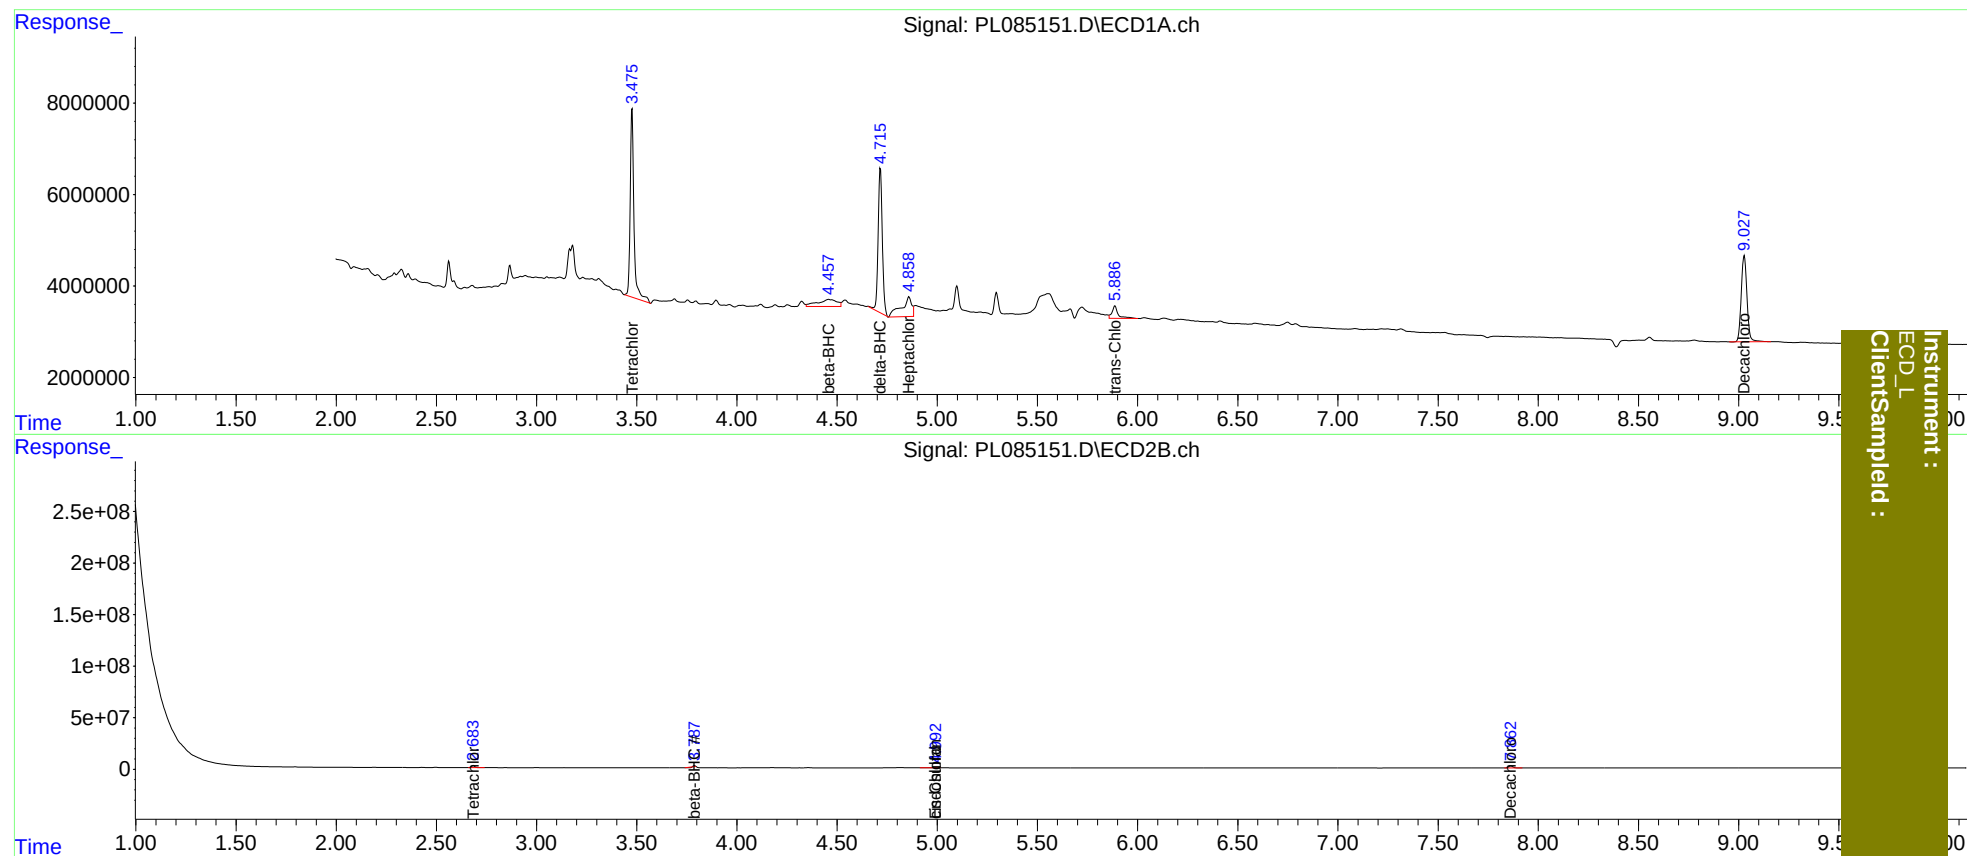


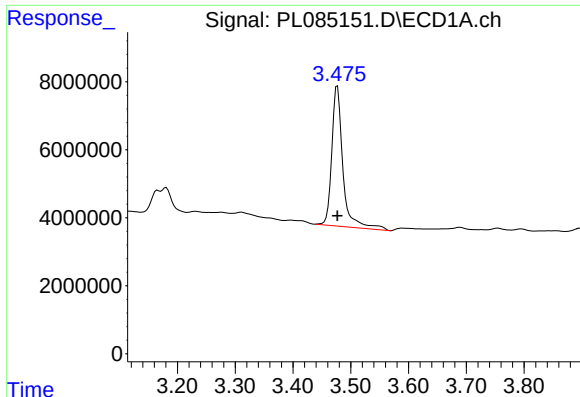

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 55267399
Conc: 22.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

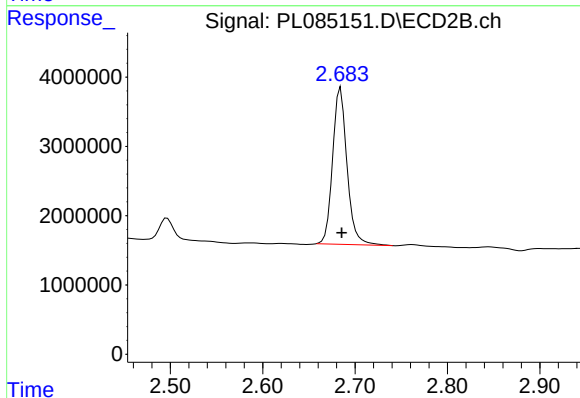


#1 Tetrachloro-m-xylene

R.T.: 2.684 min
Delta R.T.: -0.001 min
Response: 24452765
Conc: 20.71 ng/ml

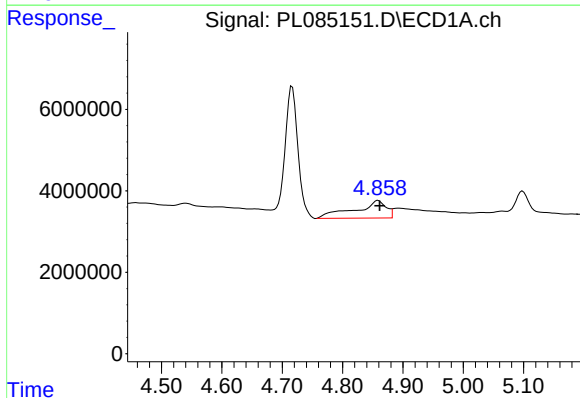


#4 Heptachlor

R.T.: 4.859 min
Delta R.T.: -0.003 min
Response: 15668148
Conc: 4.05 ng/ml

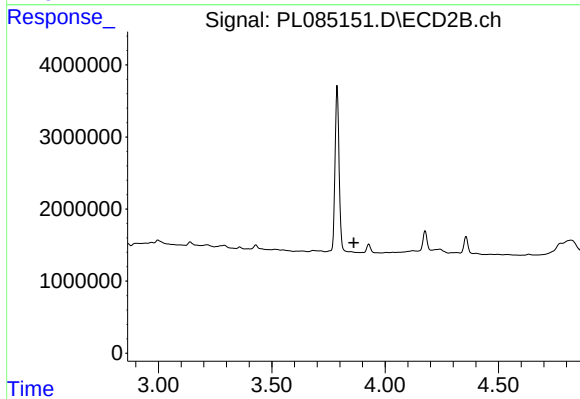

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

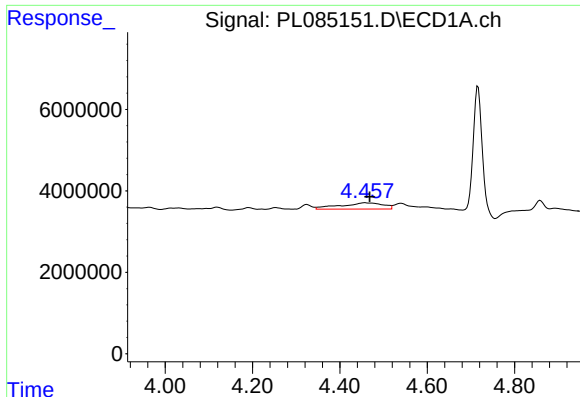

#6 beta-BHC


R.T.: 4.458 min
Delta R.T.: -0.011 min
Response: 10499096
Conc: 5.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

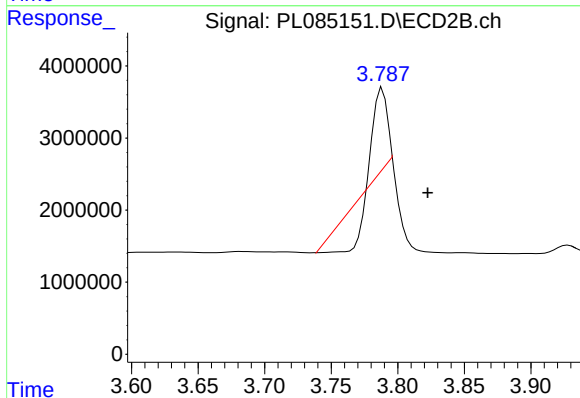


#6 beta-BHC

R.T.: 3.789 min
Delta R.T.: -0.034 min
Response: 1917199
Conc: 2.33 ng/ml

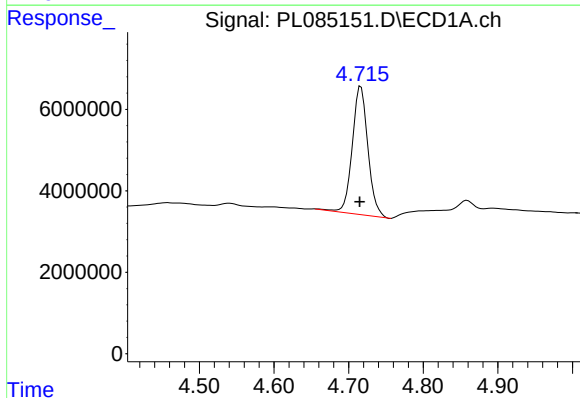


#7 delta-BHC

R.T.: 4.716 min
Delta R.T.: 0.002 min
Response: 45955630
Conc: 12.59 ng/ml

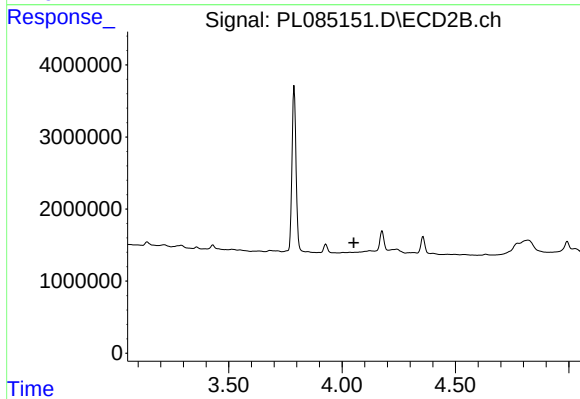

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

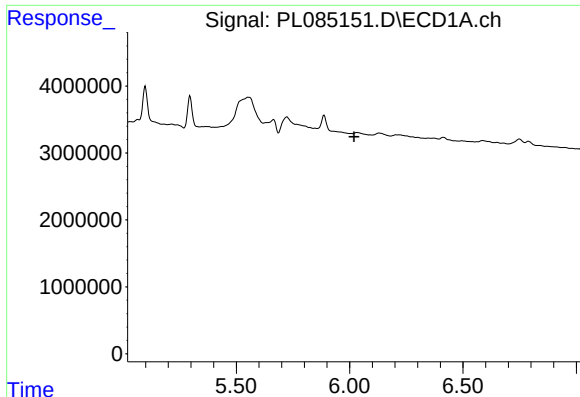

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

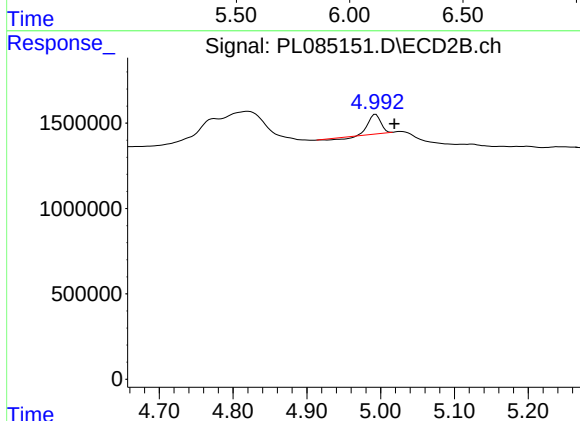


#9 Endosulfan I

R.T.: 4.993 min
Delta R.T.: -0.026 min
Response: 1178956
Conc: 0.87 ng/ml

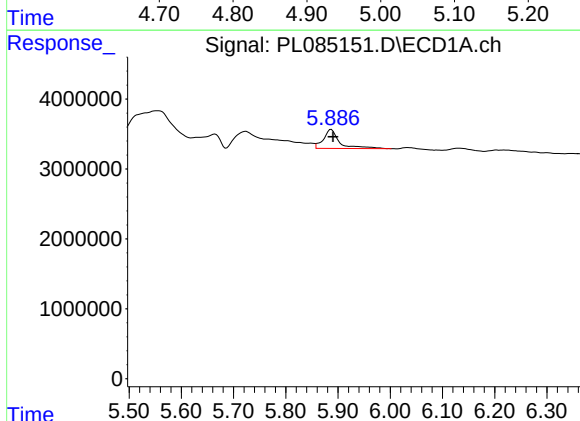


#10 trans-Chlordane

R.T.: 5.887 min
Delta R.T.: -0.004 min
Response: 5847047
Conc: 1.85 ng/ml

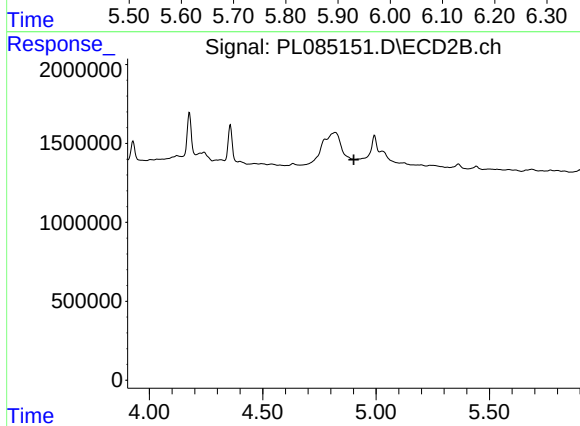

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.901 min
Response: 0
Conc: N.D.

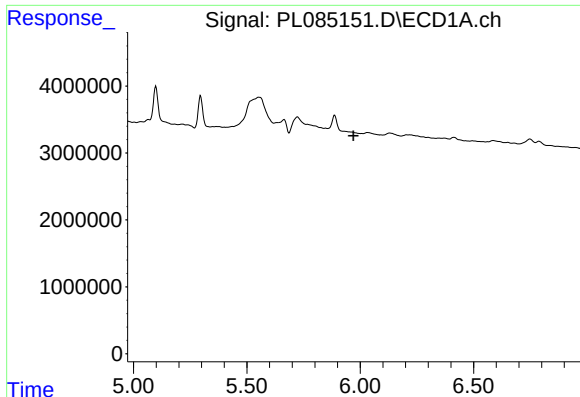

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

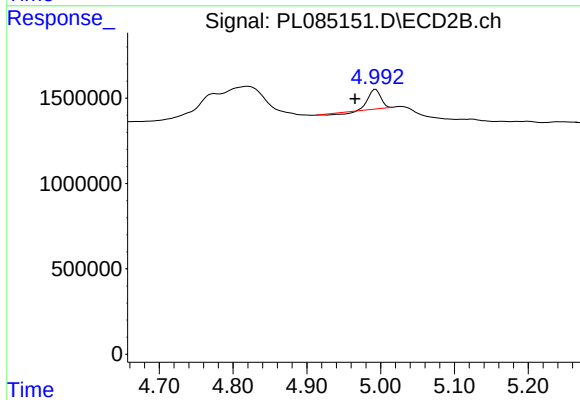


#11 cis-Chlordane

R.T.: 4.993 min
Delta R.T.: 0.028 min
Response: 1178956
Conc: 0.76 ng/ml

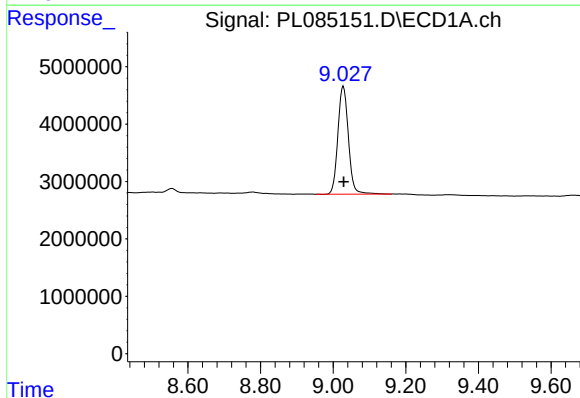

#27 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: 0.000 min
Response: 37778410
Conc: 22.04 ng/ml

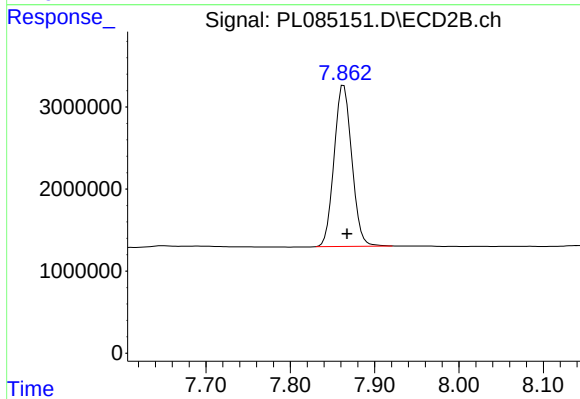

#27 Decachlorobiphenyl

R.T.: 7.863 min
Delta R.T.: -0.004 min
Response: 28686705
Conc: 21.18 ng/ml