

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090723\
 Data File : PL085154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 17:34
 Operator : AR\AJ
 Sample : PIBLK226
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 22:07:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.684	58577635	23357823	23.366	19.786
2)	SA Decachlor...	9.027	7.864	67552420	51665443	39.418	38.146
Target Compounds							
4)	MA Heptachlor	4.901f	0.000	12182285	0	3.146	N.D. #
6)	B beta-BHC	4.474	0.000	15574829	0	8.819	N.D. #
8)	B Heptachlo...	5.673f	0.000	3471432	0	1.040	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090723\
Data File : PL085154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 17:34
Operator : AR\AJ
Sample : PIBLK226
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 22:07:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

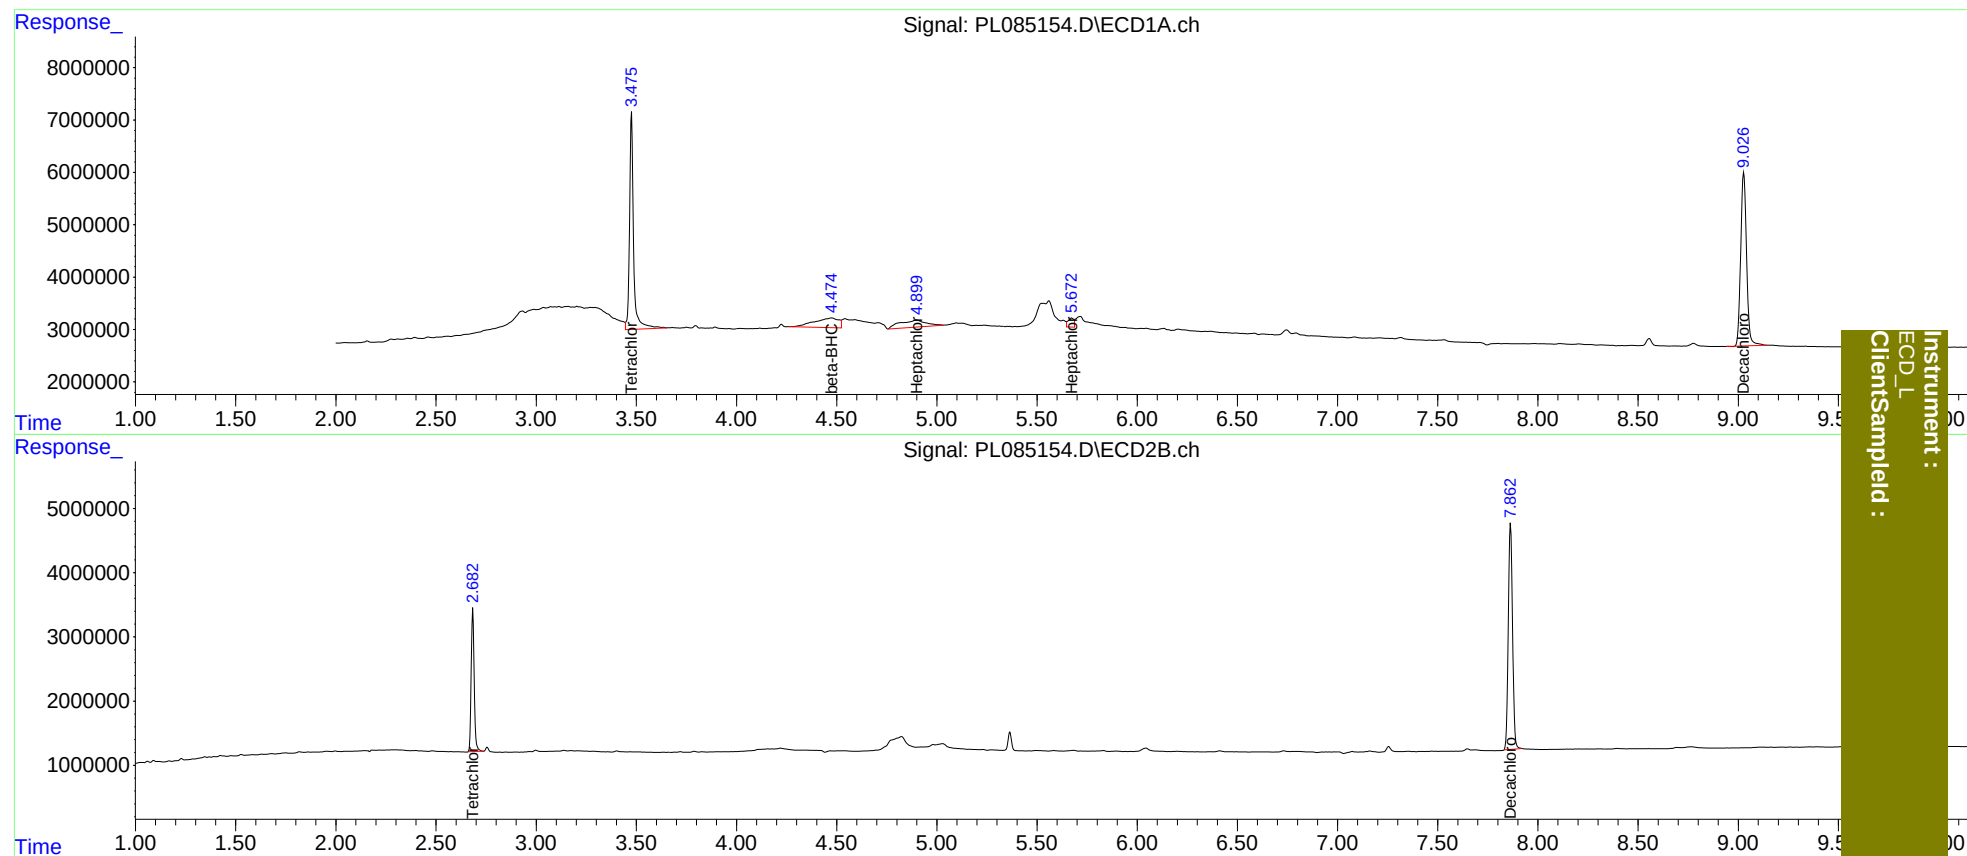


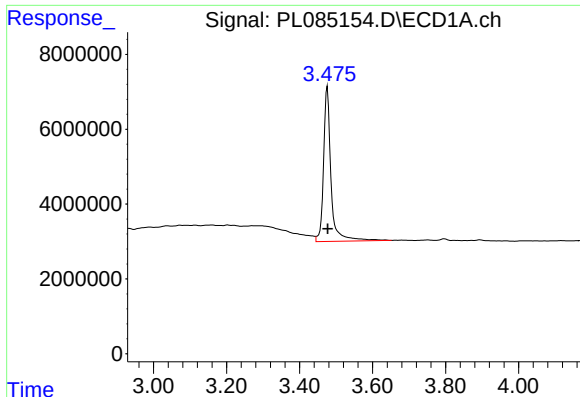

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 58577635
Conc: 23.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

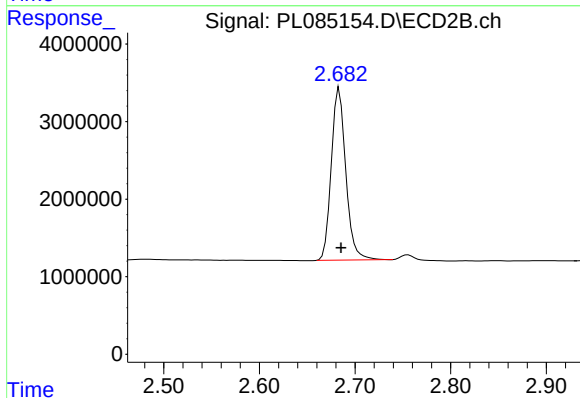


#1 Tetrachloro-m-xylene

R.T.: 2.684 min
Delta R.T.: -0.002 min
Response: 23357823
Conc: 19.79 ng/ml

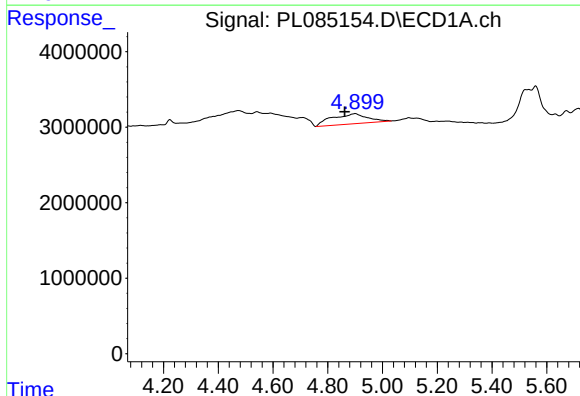


#4 Heptachlor

R.T.: 4.901 min
Delta R.T.: 0.040 min
Response: 12182285
Conc: 3.15 ng/ml

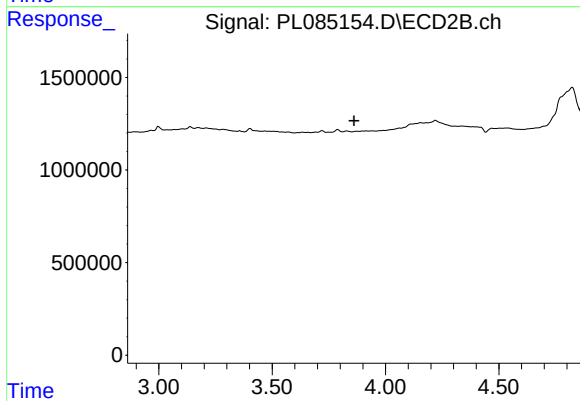

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.862 min
Response: 0
Conc: N.D.

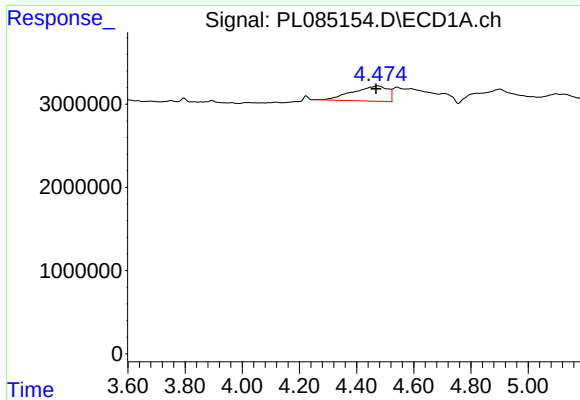

#6 beta-BHC


R.T.: 4.474 min
Delta R.T.: 0.006 min
Response: 15574829
Conc: 8.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

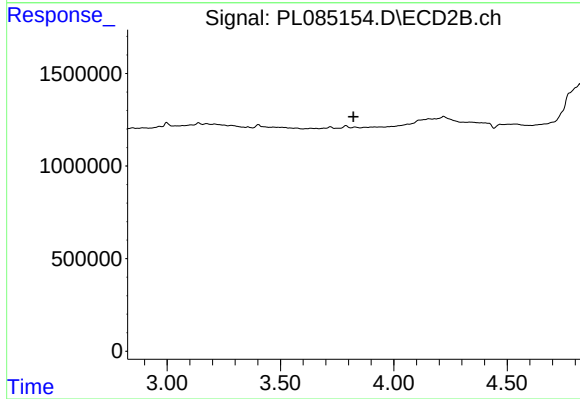


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.822 min
Response: 0
Conc: N.D.

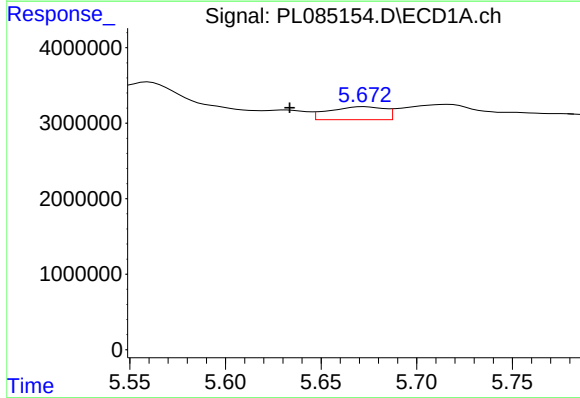


#8 Heptachlor epoxide

R.T.: 5.673 min
Delta R.T.: 0.039 min
Response: 3471432
Conc: 1.04 ng/ml

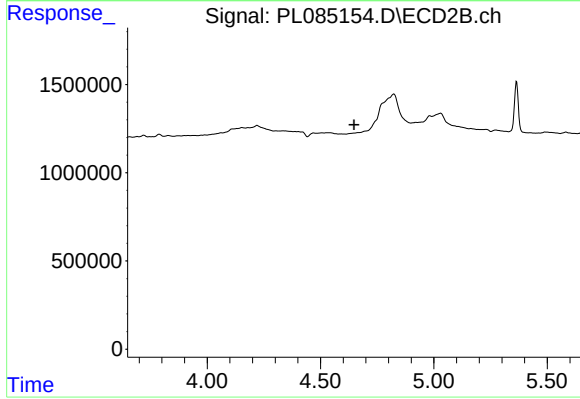

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

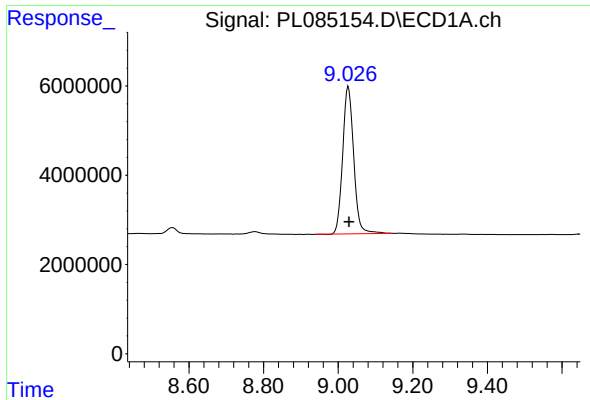

#27 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.002 min
Response: 67552420
Conc: 39.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

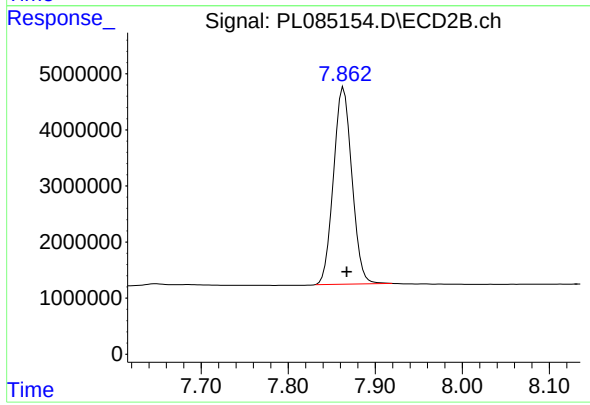

#27 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: -0.003 min
Response: 51665443
Conc: 38.15 ng/ml