

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090723\
 Data File : PL085163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 20:18
 Operator : AR\AJ
 Sample : 04195-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 22:09:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.684	14900067	6754042	5.944	5.721
2) SA Decachlor...	9.027	7.864	10571064	8992220	6.168	6.639
Target Compounds						
2) A alpha-BHC	3.895f	0.000	6301931	0	1.743	N.D. #
4) MA Heptachlor	4.901f	0.000	28147064	0	7.268	N.D. #
6) B beta-BHC	4.484	0.000	90977086	0	51.515	N.D. #
8) B Heptachlo...	5.665	0.000	3075104	0	0.921	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090723\
Data File : PL085163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 20:18
Operator : AR\AJ
Sample : 04195-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 22:09:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

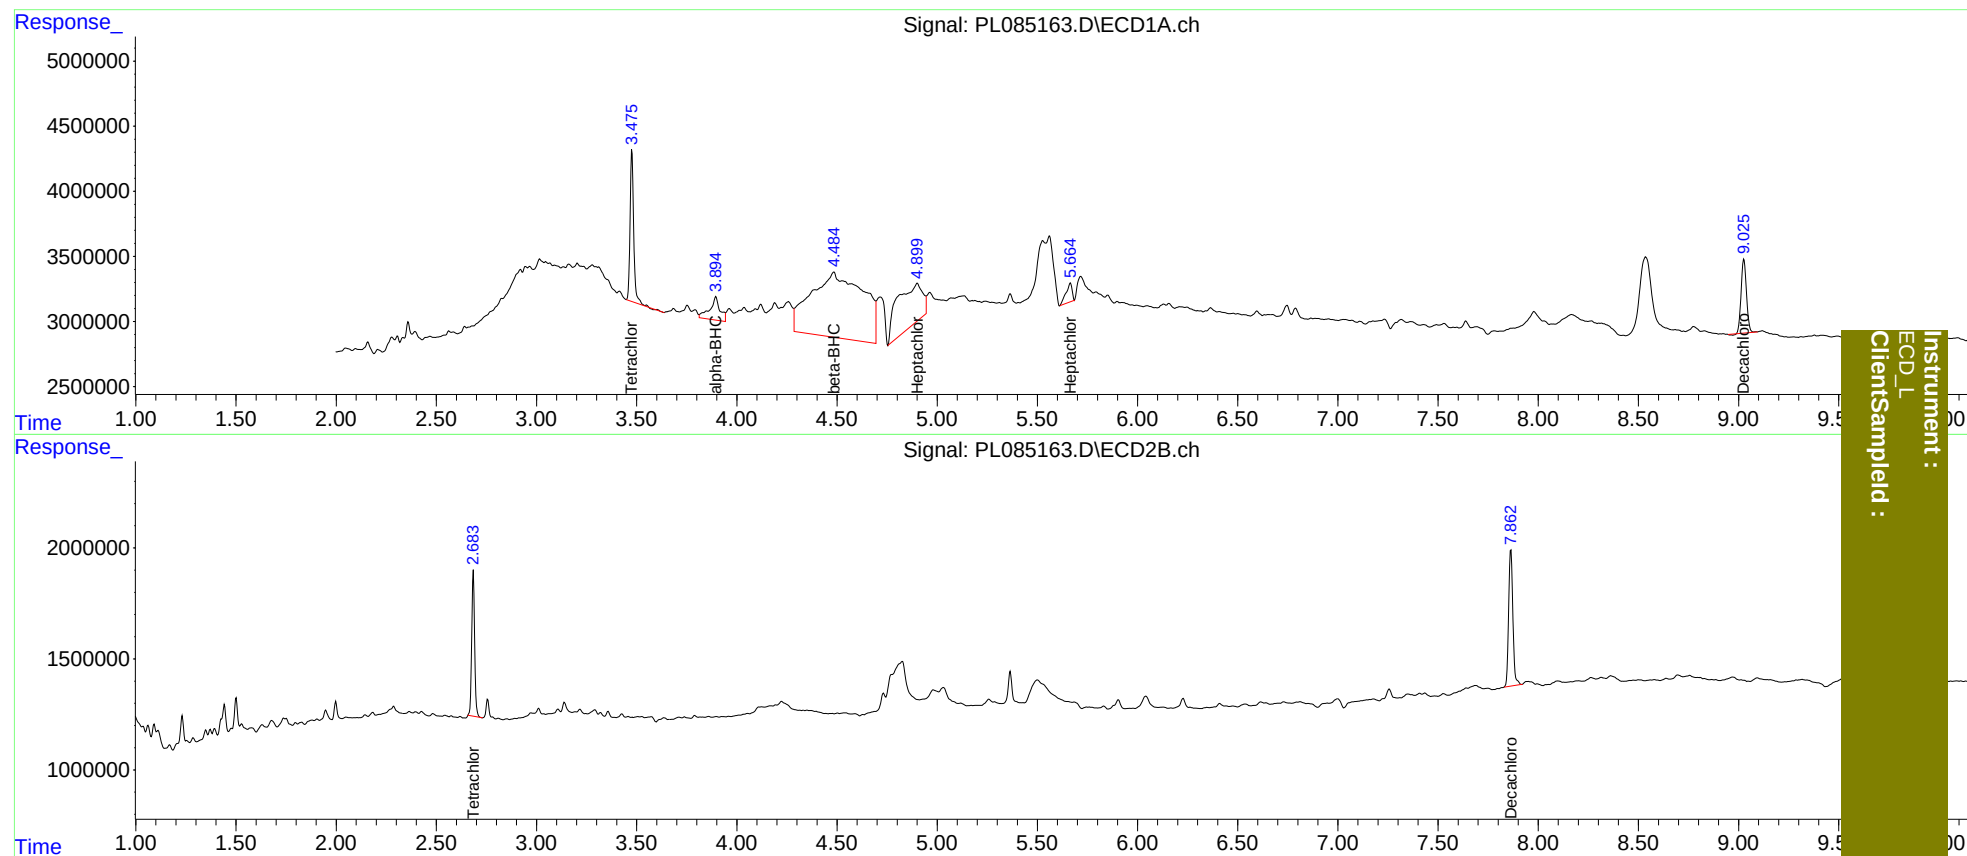


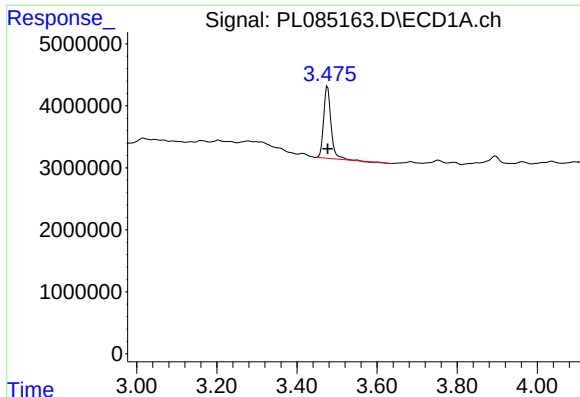

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 14900067
Conc: 5.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

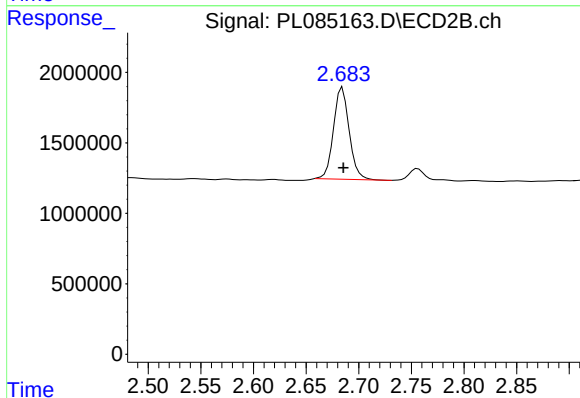


#1 Tetrachloro-m-xylene

R.T.: 2.684 min
Delta R.T.: -0.001 min
Response: 6754042
Conc: 5.72 ng/ml

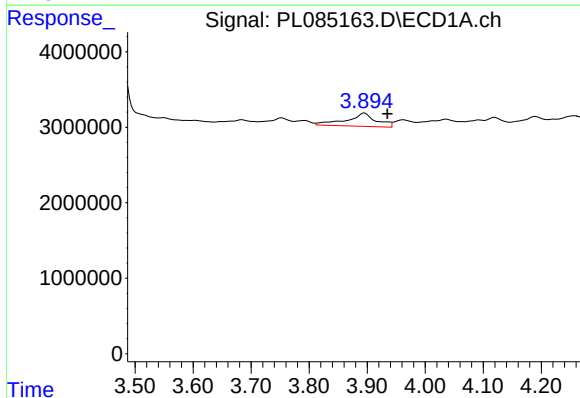


#2 alpha-BHC

R.T.: 3.895 min
Delta R.T.: -0.040 min
Response: 6301931
Conc: 1.74 ng/ml

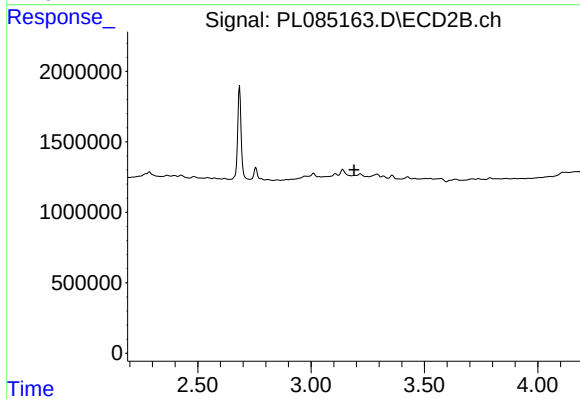

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.190 min
Response: 0
Conc: N.D.

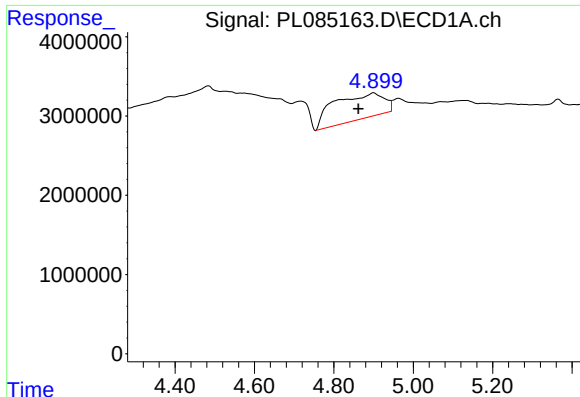

#4 Heptachlor


R.T.: 4.901 min
Delta R.T.: 0.039 min
Response: 28147064
Conc: 7.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

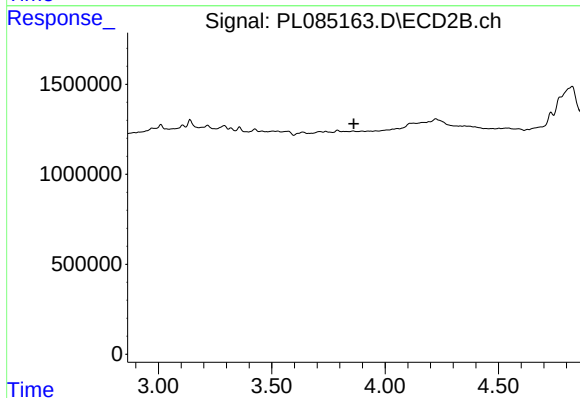


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

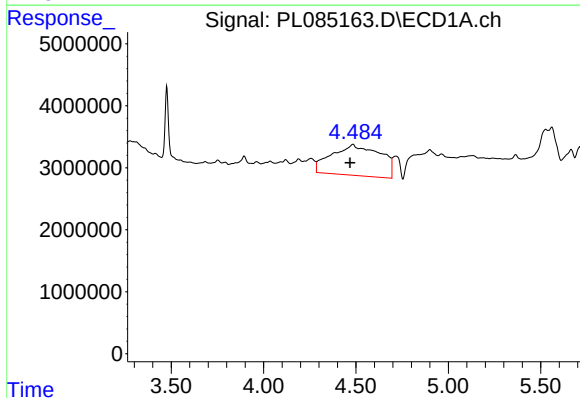


#6 beta-BHC

R.T.: 4.484 min
Delta R.T.: 0.016 min
Response: 90977086
Conc: 51.52 ng/ml

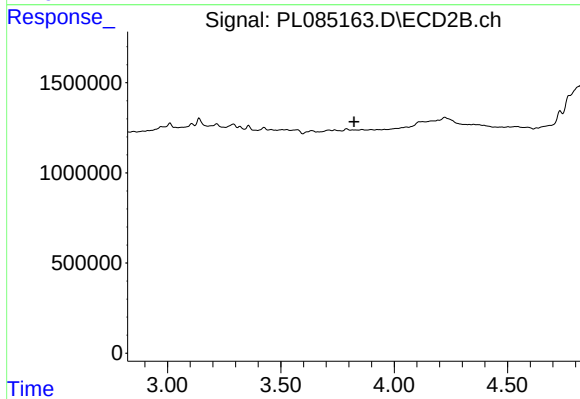

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.822 min
Response: 0
Conc: N.D.

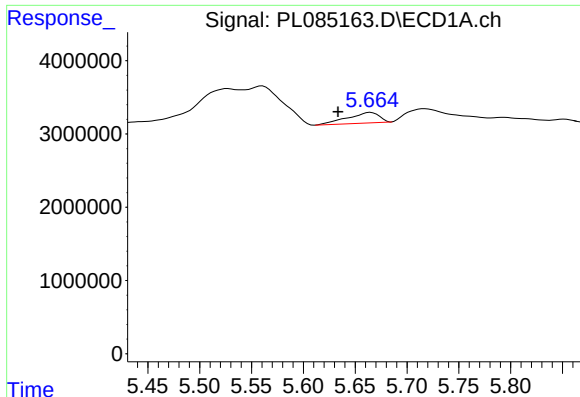

#8 Heptachlor epoxide


R.T.: 5.665 min
Delta R.T.: 0.031 min
Response: 3075104
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

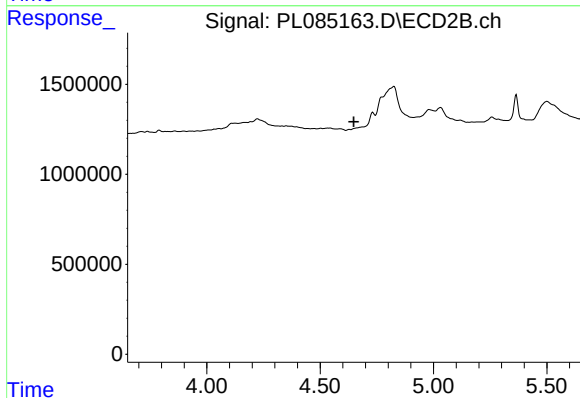


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

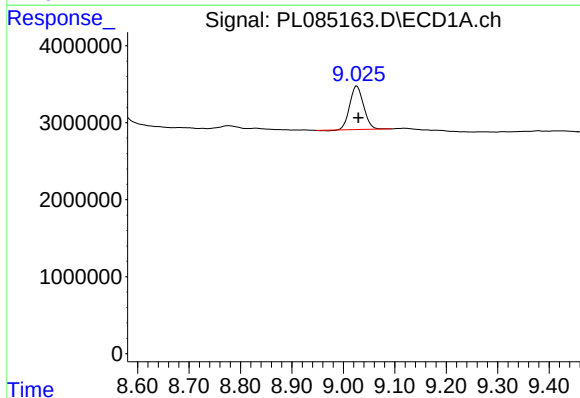

#27 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.003 min
Response: 10571064
Conc: 6.17 ng/ml

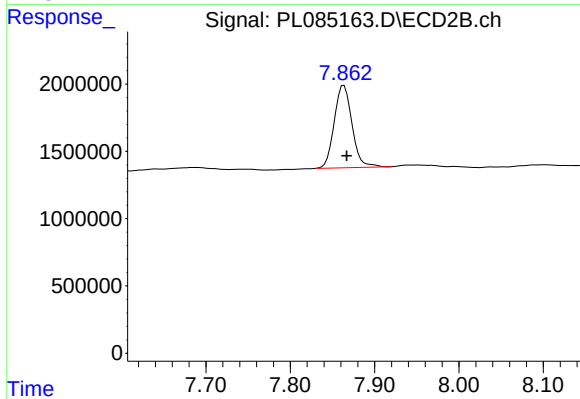

#27 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: -0.004 min
Response: 8992220
Conc: 6.64 ng/ml