

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090723\
 Data File : PL085162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 20:04
 Operator : AR\AJ
 Sample : 04195-07MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 YBY19MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/07/2023
 Supervised By :Ankita Jodhani 09/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 22:09:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.685	44779903	21631600	17.862m	18.324
27)	SA Decachlor...	9.027	7.864	34501760	27573932	20.132	20.359
Target Compounds							
2)	A alpha-BHC	3.935	3.189	189.9E6	92312413	52.533	54.422
3)	MA gamma-BHC...	4.268	3.520	167.8E6	85017290	48.448m	52.428
4)	MA Heptachlor	4.859	3.861	170.0E6	84646777	43.901m	52.242
5)	MB Aldrin	5.202	4.140	157.6E6	82528414	43.612m	52.614
6)	B beta-BHC	4.467	3.822	77517294	37757042	43.894m	45.961
7)	B delta-BHC	4.716	4.050	183.5E6	88240668	50.284	50.871
8)	B Heptachlo...	5.634	4.647	140.3E6	72745385	42.043	48.102
9)	A Endosulfan I	6.020	5.017	132.6E6	66292596	46.547	49.168
10)	B trans-Chl...	5.891	4.899	142.4E6	75548887	45.136	50.141
11)	B cis-Chlor...	5.971	4.964	140.7E6	75007612	44.154	48.487
12)	B 4,4'-DDE	6.150	5.161	246.1E6	151.7E6	93.036	103.534
13)	MA Dieldrin	6.297	5.283	262.9E6	162.4E6	91.919	104.787
14)	MA Endrin	6.527	5.559	227.0E6	148.4E6	99.623	107.791
15)	B Endosulfa...	6.748	5.856	223.7E6	136.9E6	95.104	98.550
16)	A 4,4'-DDD	6.669	5.719	187.0E6	120.2E6	98.831	100.535
17)	MA 4,4'-DDT	6.985	5.971	218.0E6	138.1E6	113.098	106.576
18)	B Endrin al...	6.879	6.038	158.5E6	102.4E6	85.210	90.024
19)	B Endosulfa...	7.114	6.263	199.5E6	134.0E6	90.170	98.050
20)	A Methoxychlor	7.466	6.556	456.6E6	351.3E6	470.565m	496.423
21)	B Endrin ke...	7.598	6.768	212.2E6	158.9E6	96.664	98.499

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080723\
Data File : PL085162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 20:04
Operator : AR\AJ
Sample : 04195-07MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 22:09:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

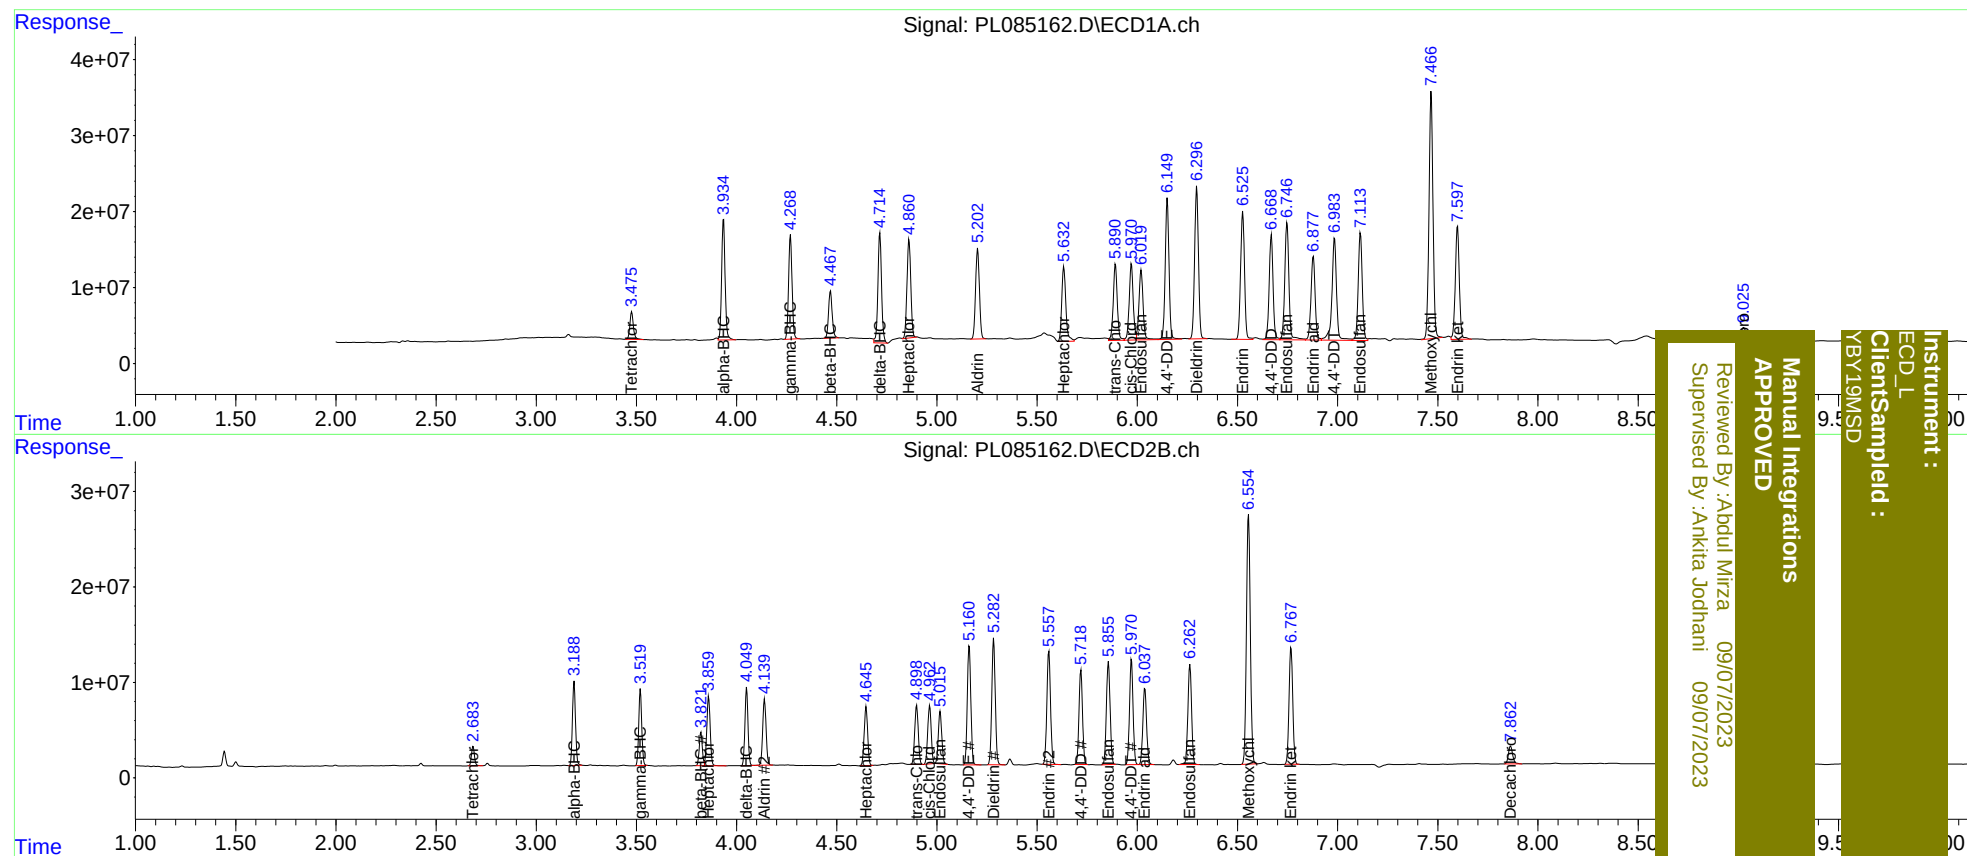

Reviewed By: Abdul Mirza 09/07/2023
Supervised By: Ankita Jodhani 09/07/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
YBY19MSD