

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
 Data File : PL061272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 12:17
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:33:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.009	35897053	64243087	20.814	20.885
28)	SA Decachlor...	8.215	9.097	36074975	51846040	21.623	21.926
Target Compounds							
16)	A 4,4'-DDD	0.000	6.820f	0	3312683	N.D.	1.290 #
24)	Chlordane-2	0.000	5.457	0	6664969	N.D.	54.570 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 12:17
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:33:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

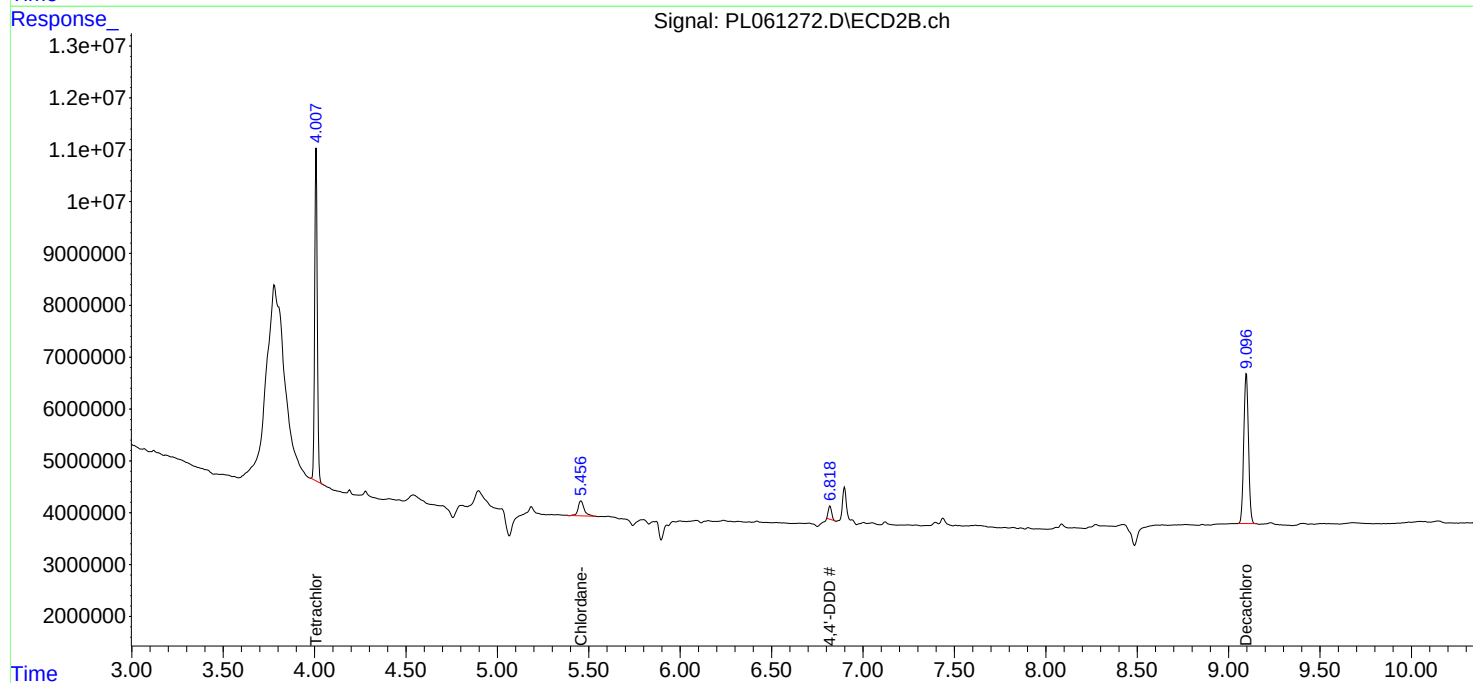


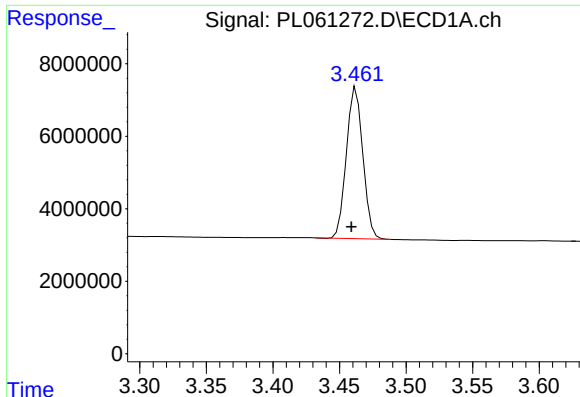

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.004 min
Response: 35897053
Conc: 20.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

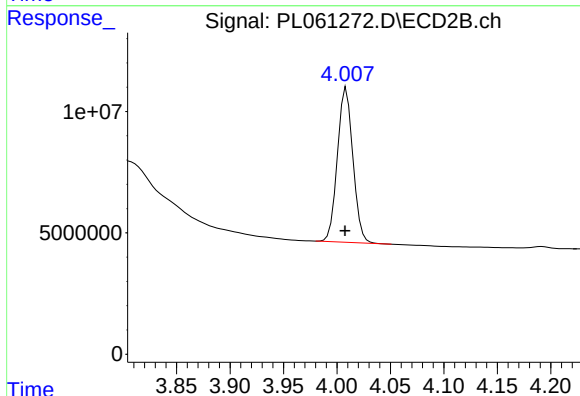


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.001 min
Response: 64243087
Conc: 20.89 ng/ml

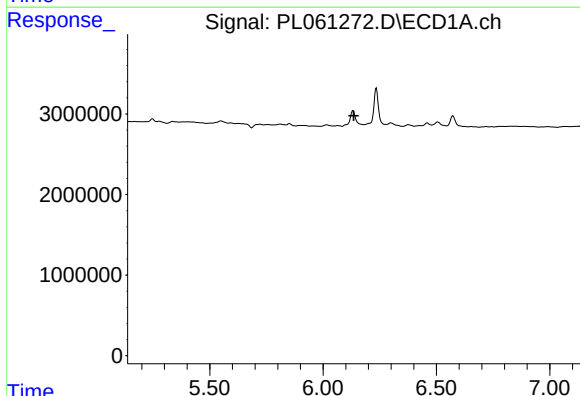


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

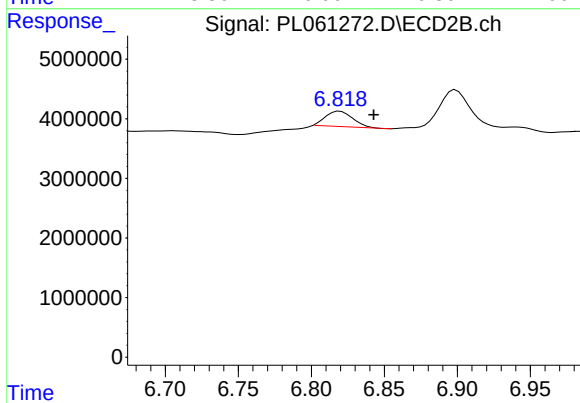

#16 4,4'-DDD


R.T.: 6.820 min
Delta R.T.: -0.023 min
Response: 3312683
Conc: 1.29 ng/ml

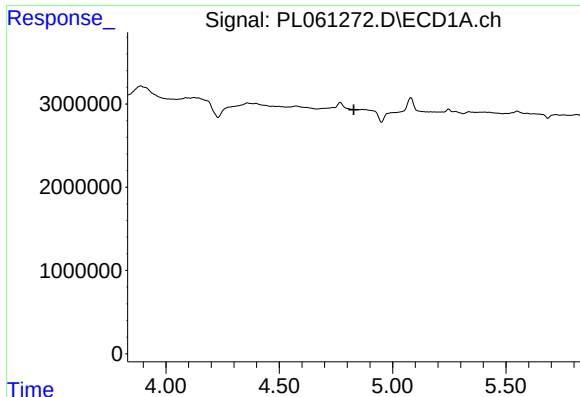

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.829 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

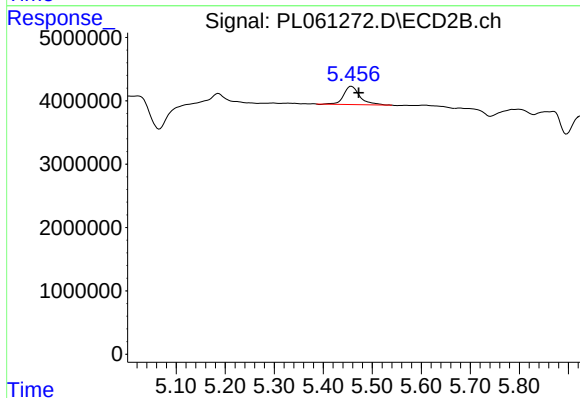


#24 Chlordane-2

R.T.: 5.457 min
Delta R.T.: -0.015 min
Response: 6664969
Conc: 54.57 ng/ml

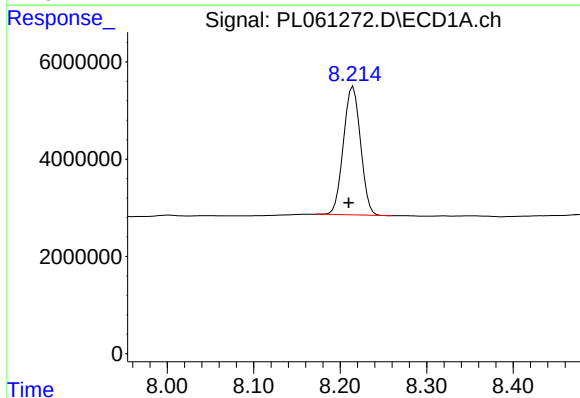

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.005 min
Response: 36074975
Conc: 21.62 ng/ml

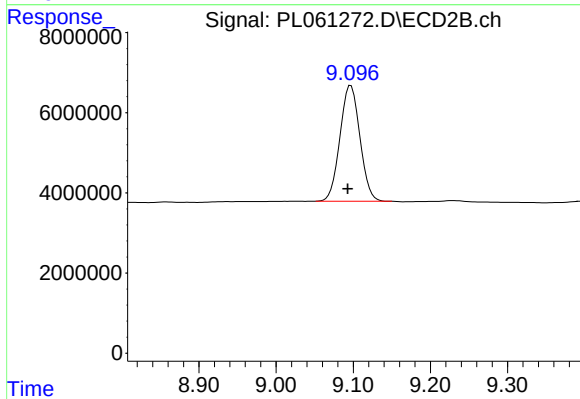

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.004 min
Response: 51846040
Conc: 21.93 ng/ml