

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
 Data File : PL061280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 14:10
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:15:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:15:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	99405598	156.6E6	50.000	50.000
28)	SA Decachlor...	8.210	9.093	83423111	116.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.328	5.004	26228596	54347093	500.000	500.000
24)	Chlordane-2	4.829	5.472	30252764	61068569	500.000	500.000
25)	Chlordane-3	5.398	6.121	82923383	216.0E6	500.000	500.000
26)	Chlordane-4	5.456	6.196	68822944	261.7E6	500.000	500.000
27)	Chlordane-5	6.290	7.002	28103410	41844107	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 14:10
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:15:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:15:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

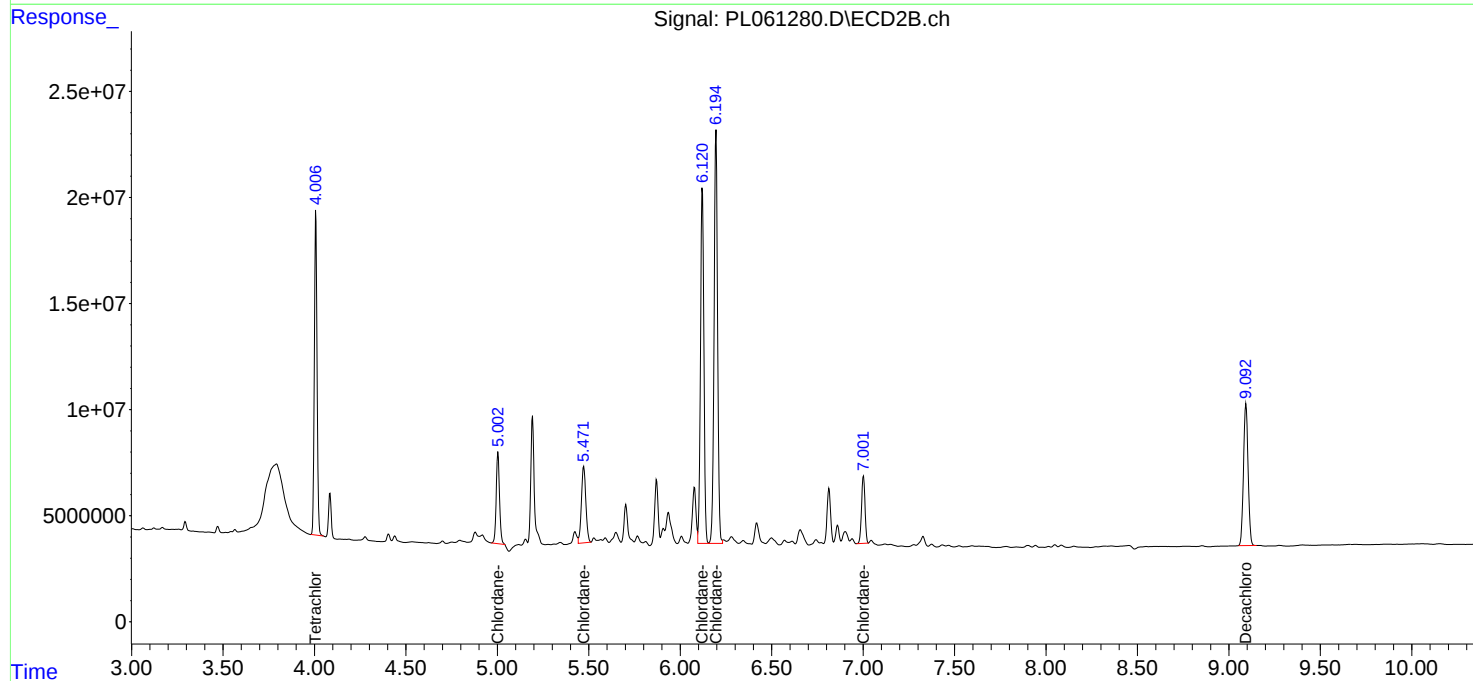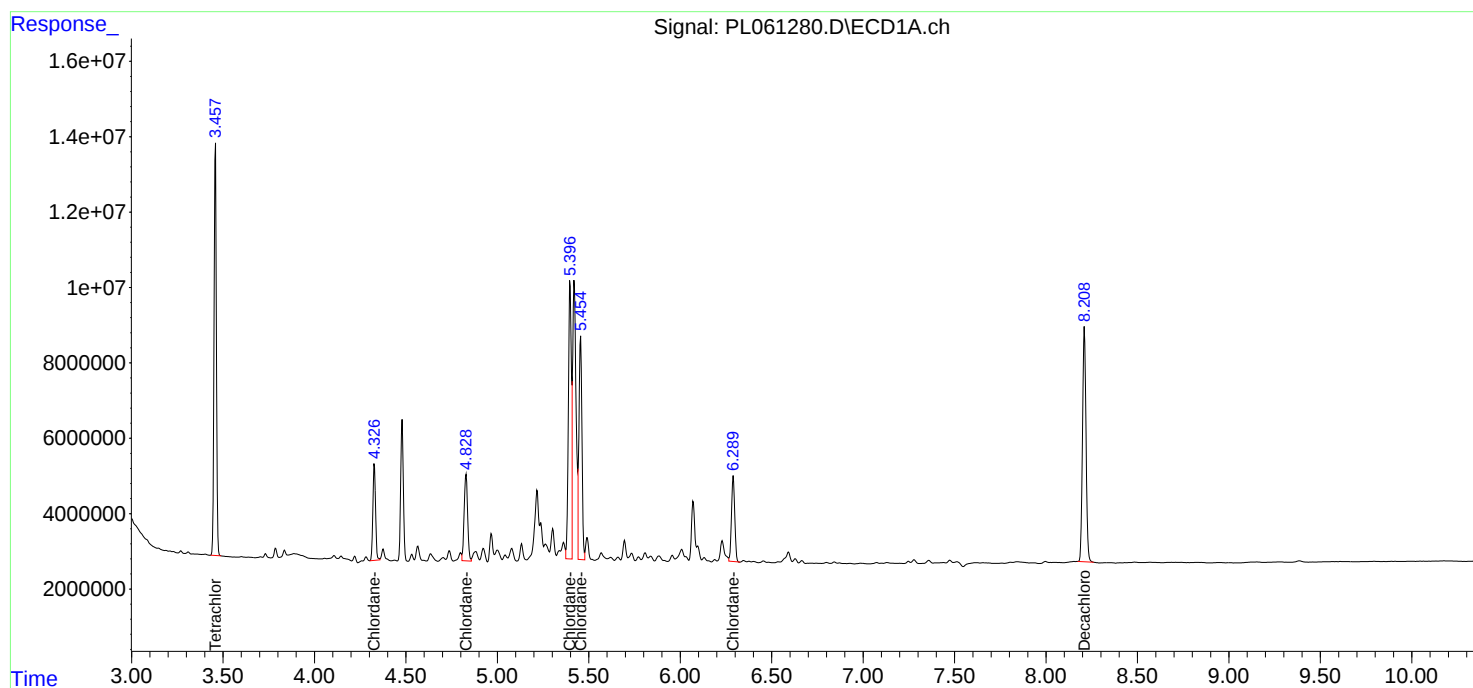


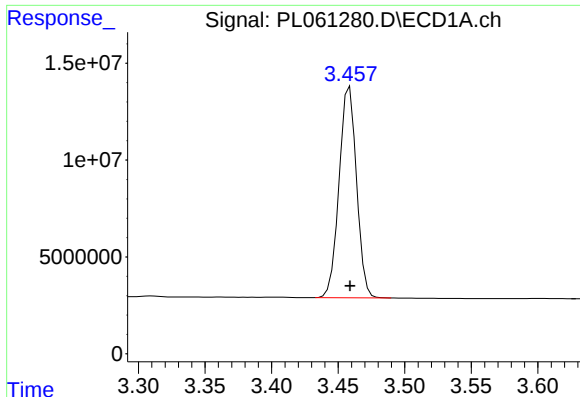

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 99405598
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

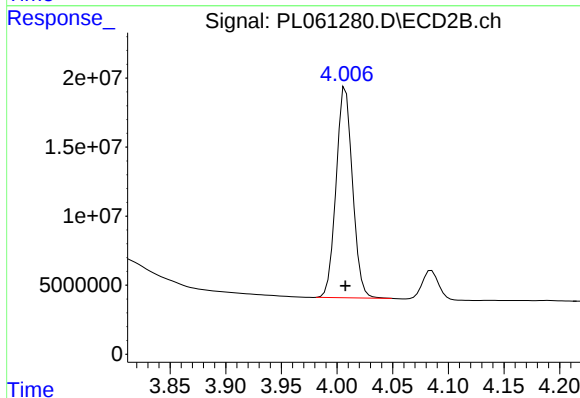


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 156625880
Conc: 50.00 ng/ml

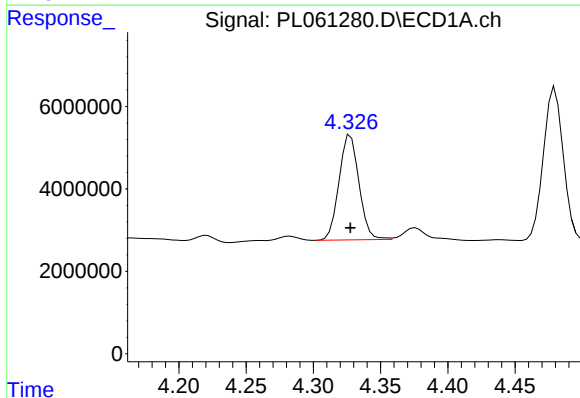


#23 Chlordane-1

R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 26228596
Conc: 500.00 ng/ml

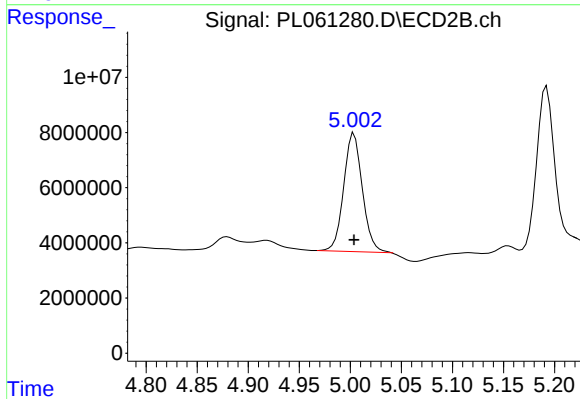

#23 Chlordane-1


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 54347093
Conc: 500.00 ng/ml

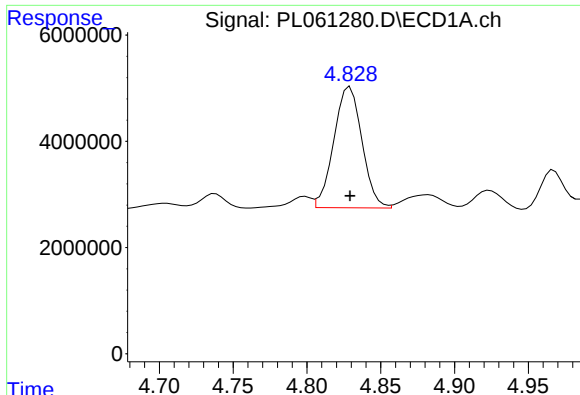

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.000 min
Response: 30252764
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

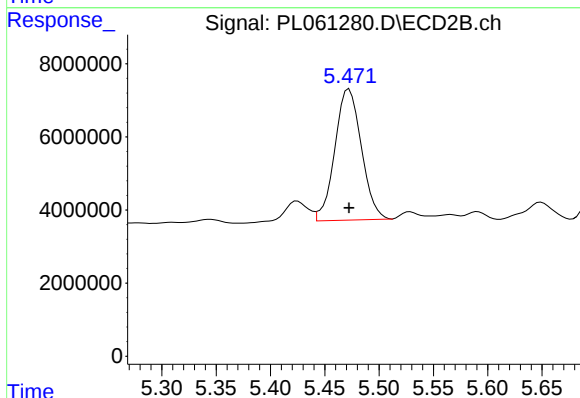


#24 Chlordane-2

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 61068569
Conc: 500.00 ng/ml

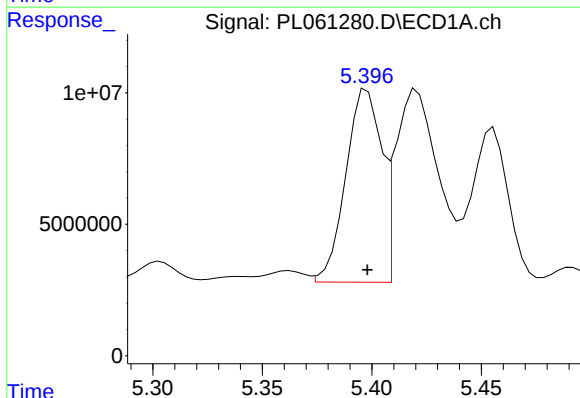


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 82923383
Conc: 500.00 ng/ml

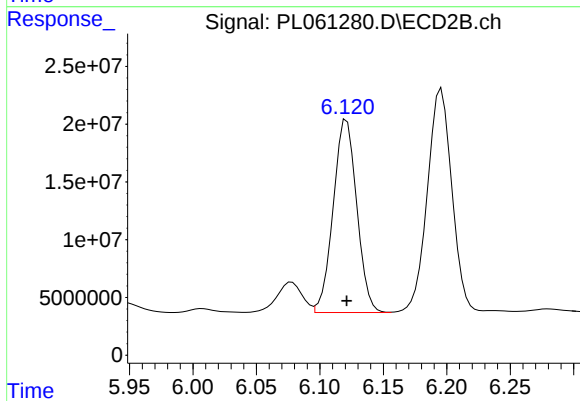

#25 Chlordane-3


R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 215988983
Conc: 500.00 ng/ml

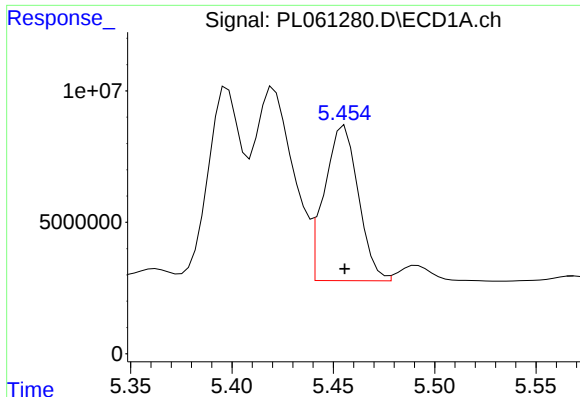

#26 Chlordane-4


R.T.: 5.456 min
Delta R.T.: 0.000 min
Response: 68822944
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

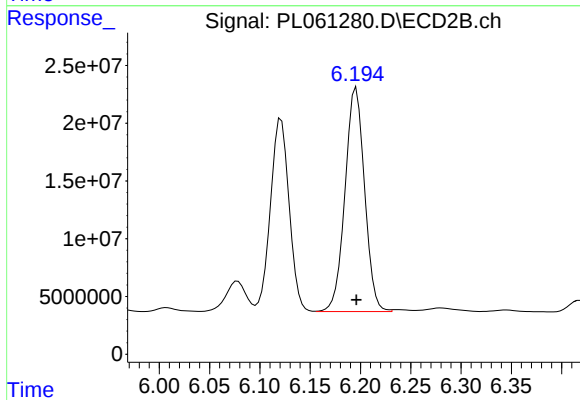


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 261736783
Conc: 500.00 ng/ml

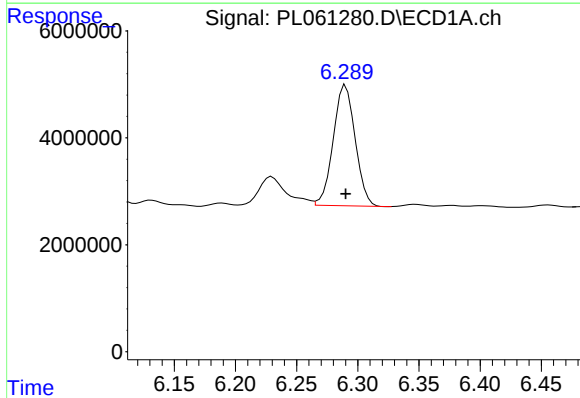


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 28103410
Conc: 500.00 ng/ml

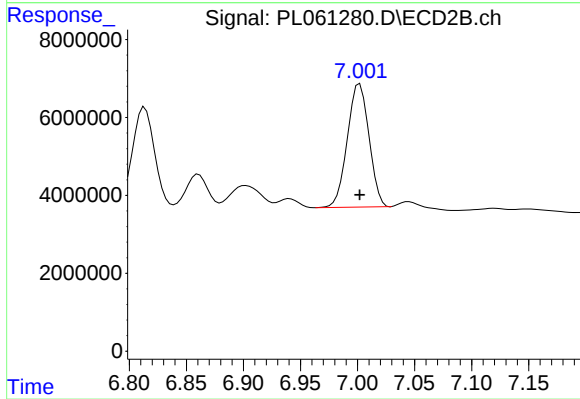

#27 Chlordane-5


R.T.: 7.002 min
Delta R.T.: 0.000 min
Response: 41844107
Conc: 500.00 ng/ml

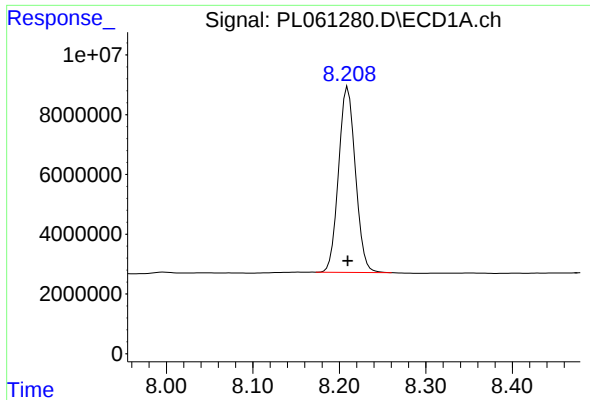

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 83423111
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

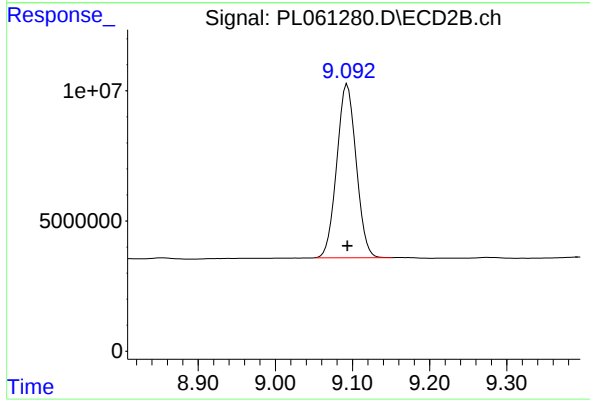

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 116303151
Conc: 50.00 ng/ml