

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
 Data File : PL061294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 17:44
 Operator : DD\AJ
 Sample : L3864-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:35:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	34802365	63062954	20.179	20.502
28)	SA Decachlor...	8.211	9.094	30406185	43151194	18.226	18.249
Target Compounds							
22)	Mirex	7.360f	0.000	4287579	0	2.867	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 17:44
Operator : DD\AJ
Sample : L3864-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:35:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

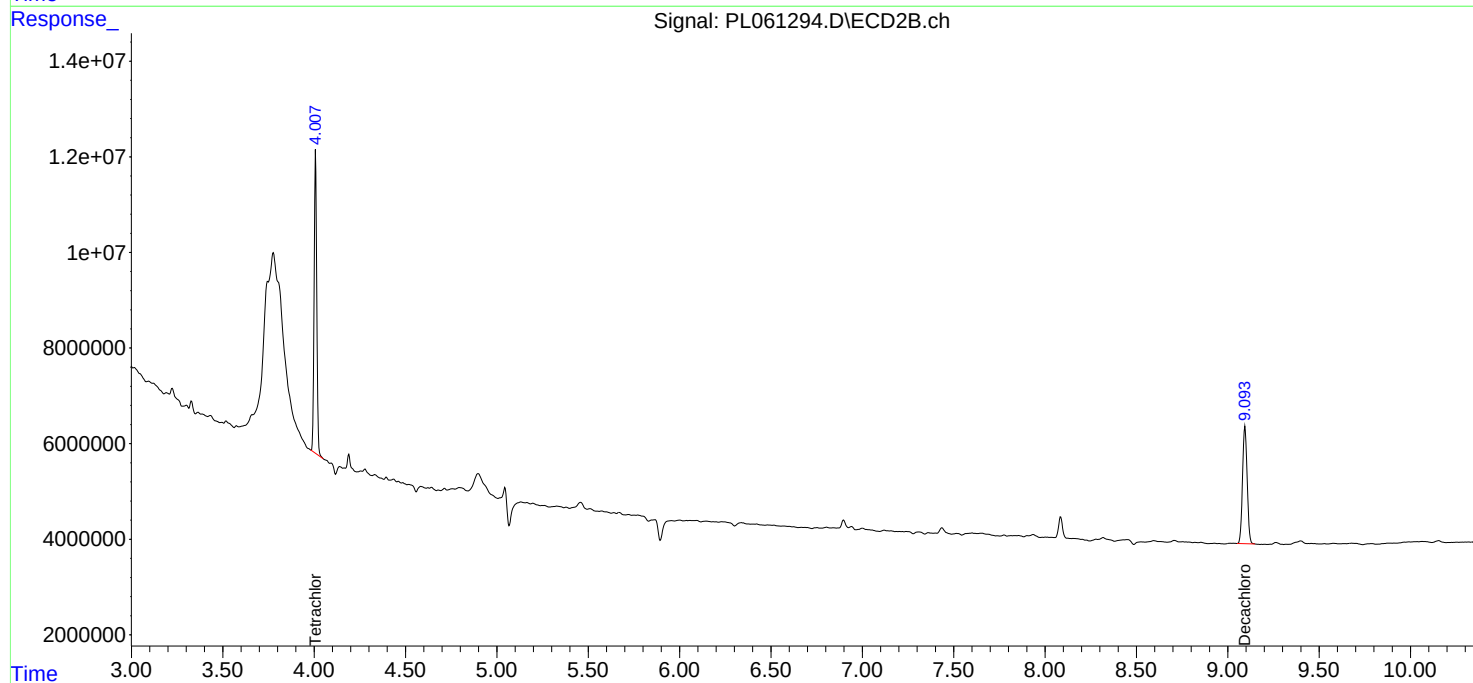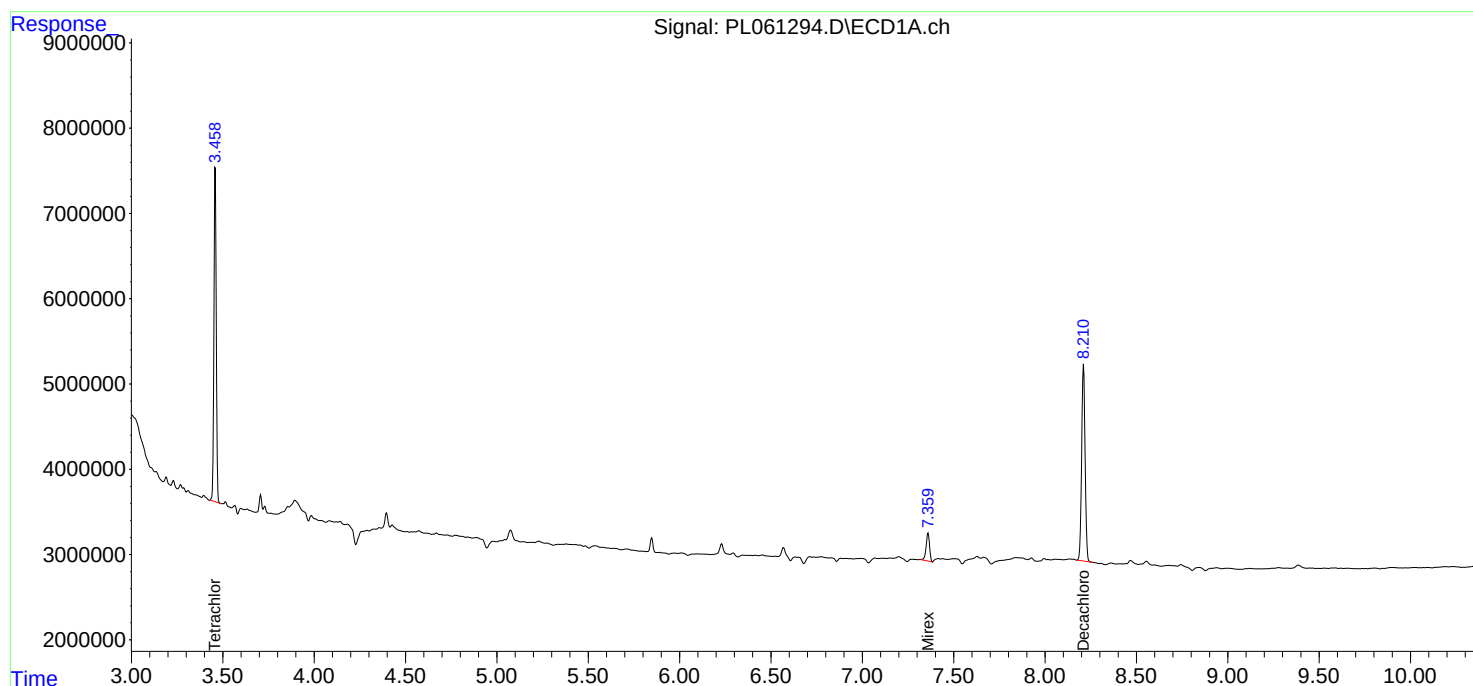


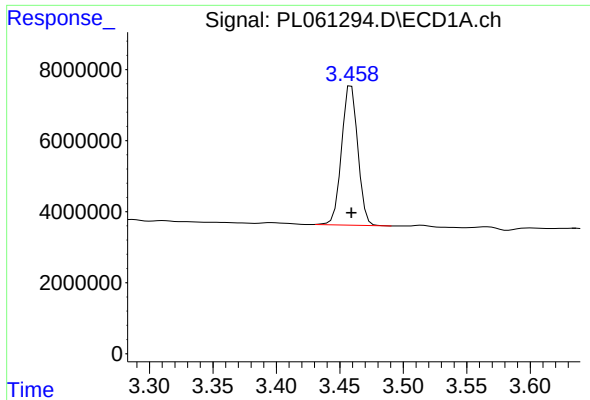

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 34802365
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

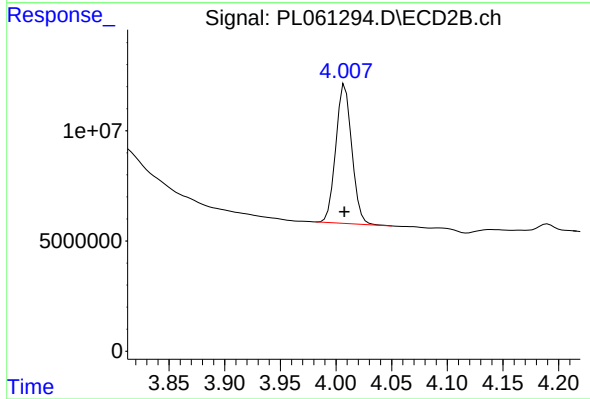


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 63062954
Conc: 20.50 ng/ml

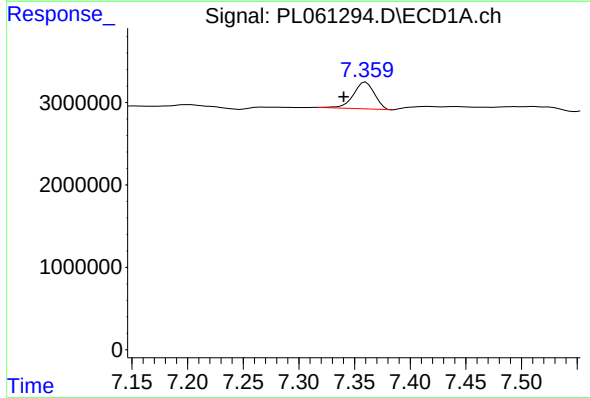


#22 Mirex

R.T.: 7.360 min
Delta R.T.: 0.020 min
Response: 4287579
Conc: 2.87 ng/ml

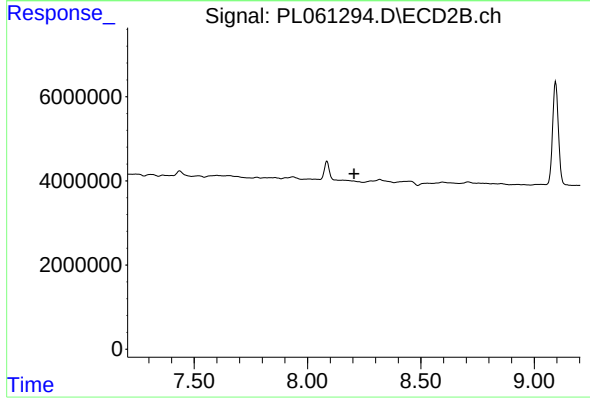

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.205 min
Response: 0
Conc: N.D.

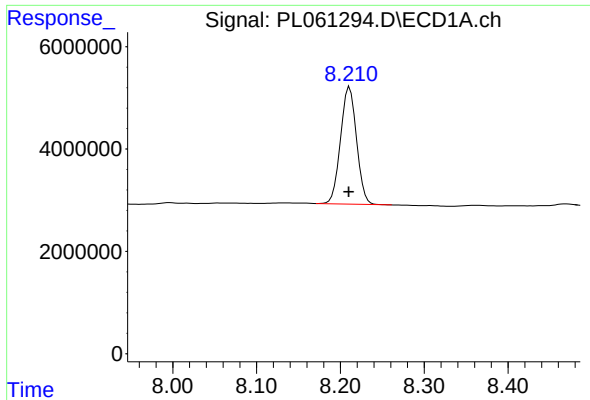

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.001 min
Response: 30406185
Conc: 18.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

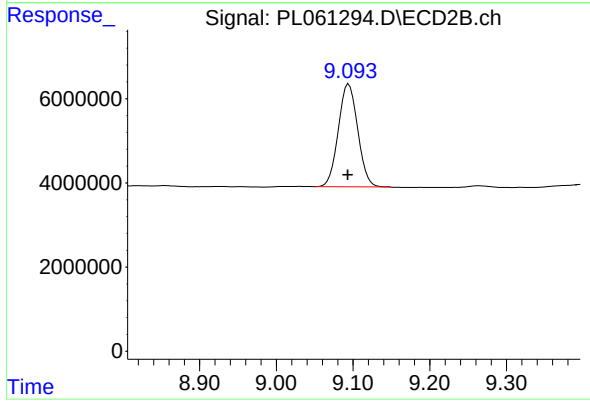

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.002 min
Response: 43151194
Conc: 18.25 ng/ml