

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
 Data File : PL061307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 20:47
 Operator : DD\AJ
 Sample : L3808-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:37:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	37167905	68367964	21.551	22.226
28)	SA Decachlor...	8.210	9.094	34884350	49194744	20.910	20.805
Target Compounds							
9)	A Endosulfan I	5.530f	0.000	12692405	0	7.377	N.D. #
15)	B Endosulfa...	0.000	6.941	0	9239899	N.D.	3.128 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 20:47
Operator : DD\AJ
Sample : L3808-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:37:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

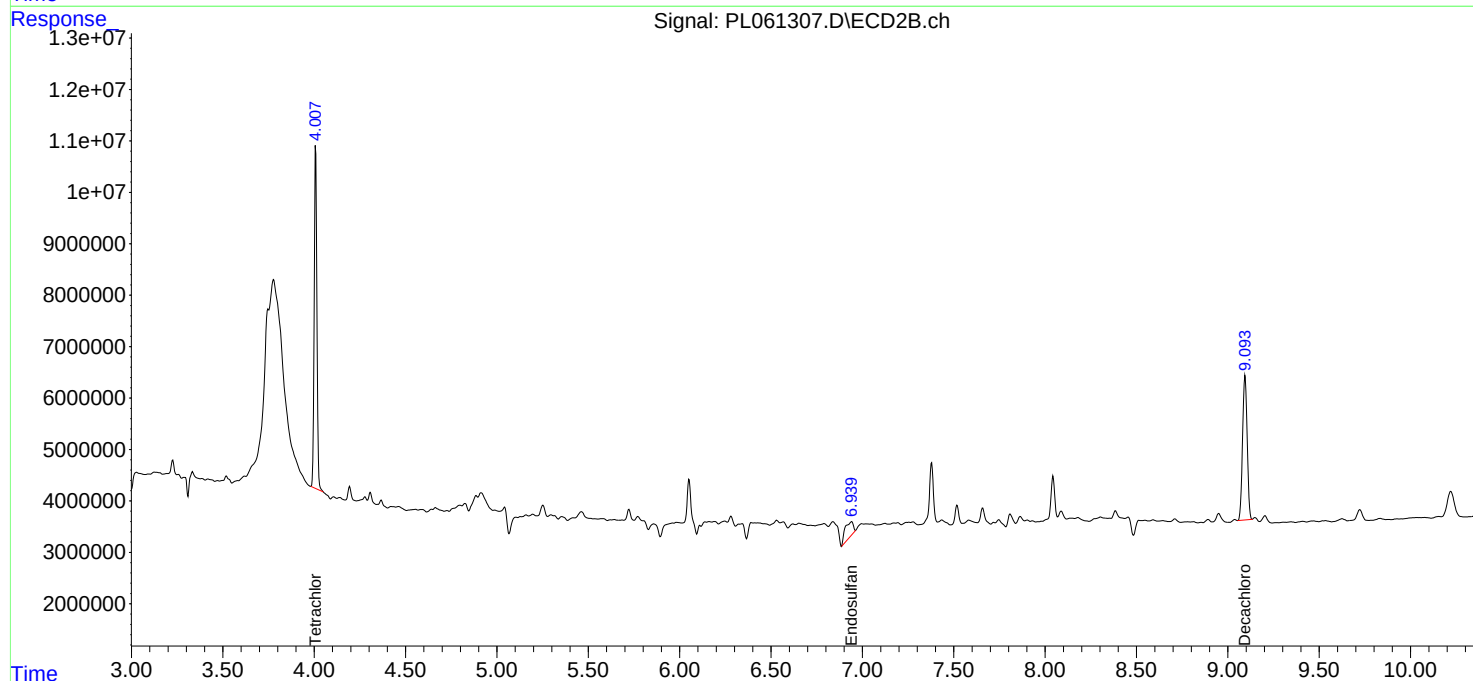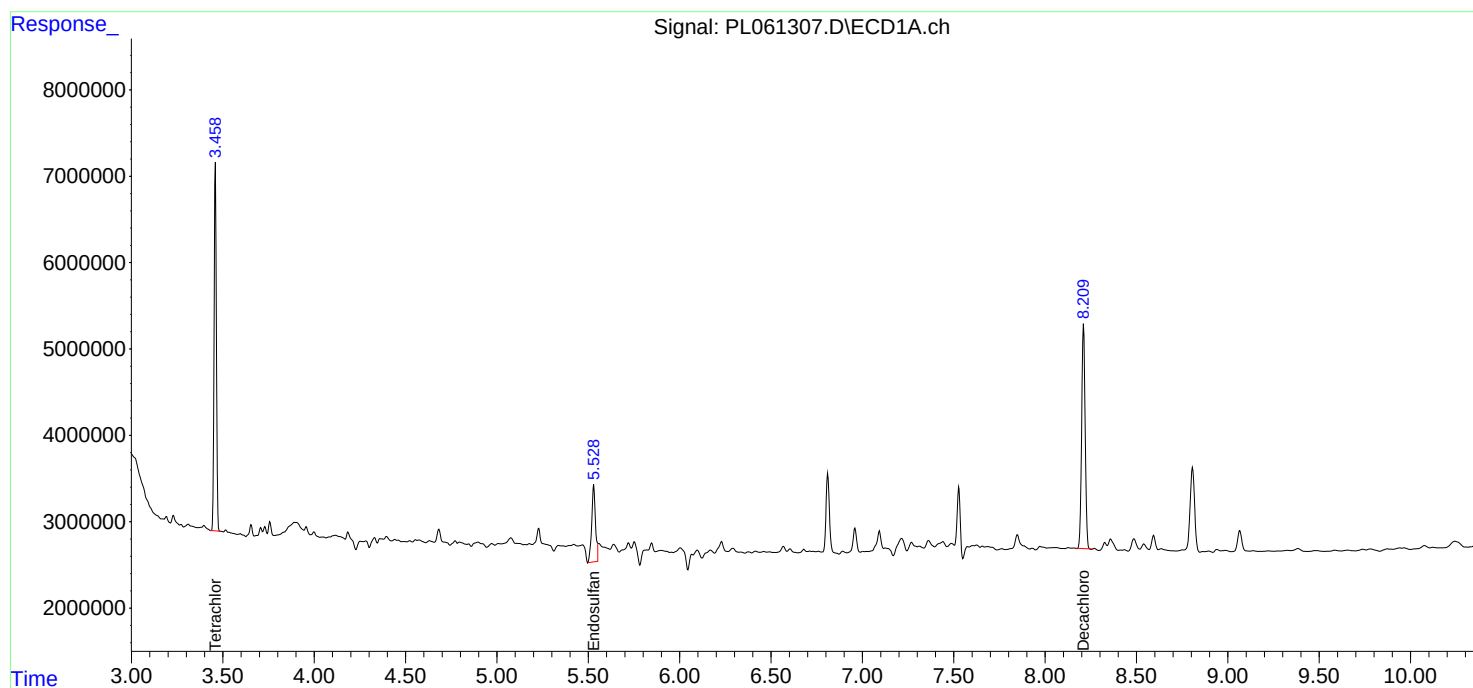


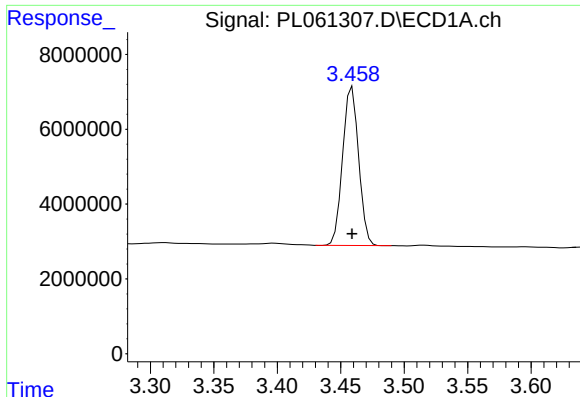

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 37167905
Conc: 21.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

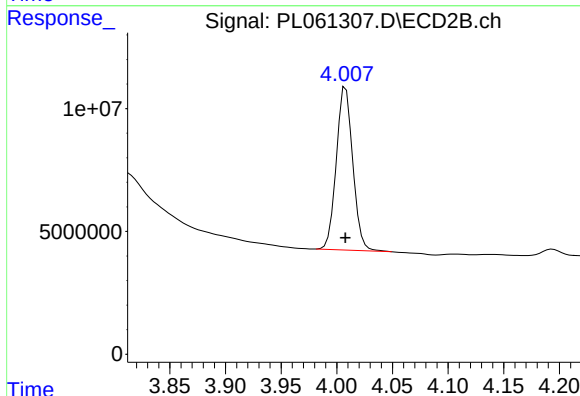


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 68367964
Conc: 22.23 ng/ml

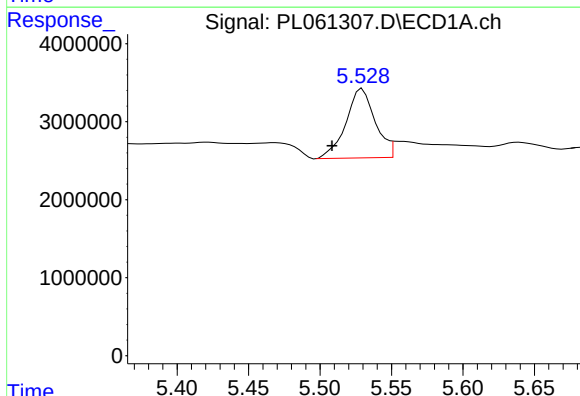


#9 Endosulfan I

R.T.: 5.530 min
Delta R.T.: 0.021 min
Response: 12692405
Conc: 7.38 ng/ml

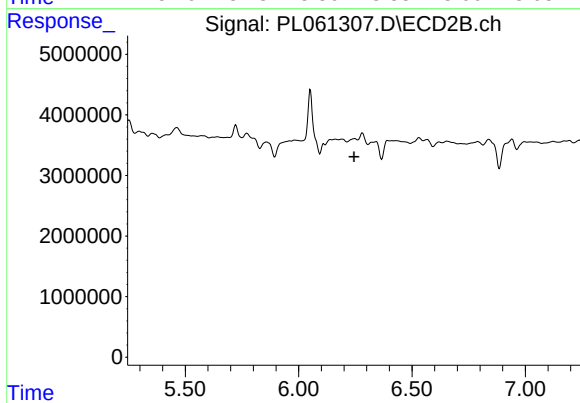

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.244 min
Response: 0
Conc: N.D.

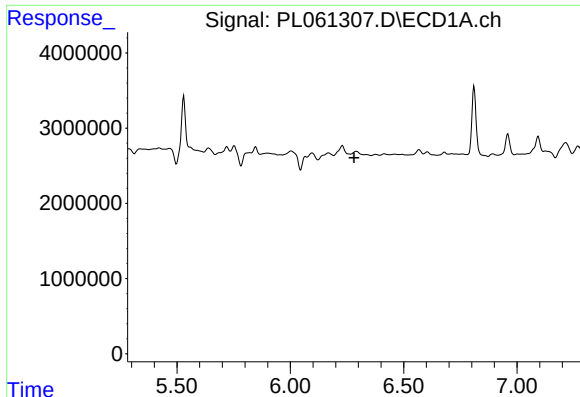

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

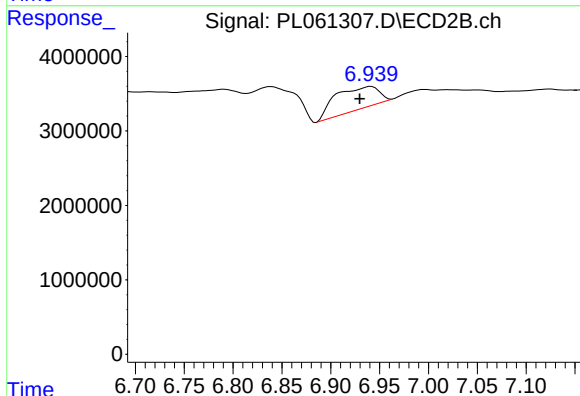


#15 Endosulfan II

R.T.: 6.941 min
Delta R.T.: 0.012 min
Response: 9239899
Conc: 3.13 ng/ml

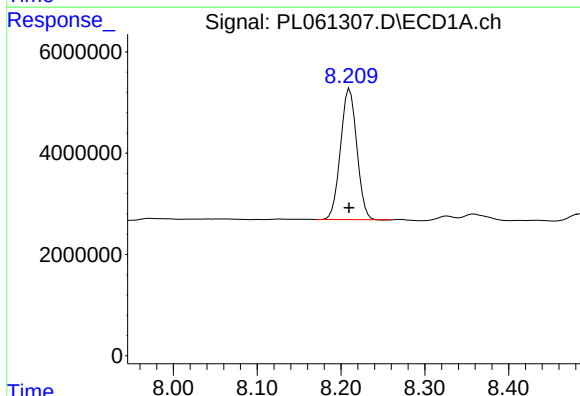

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 34884350
Conc: 20.91 ng/ml

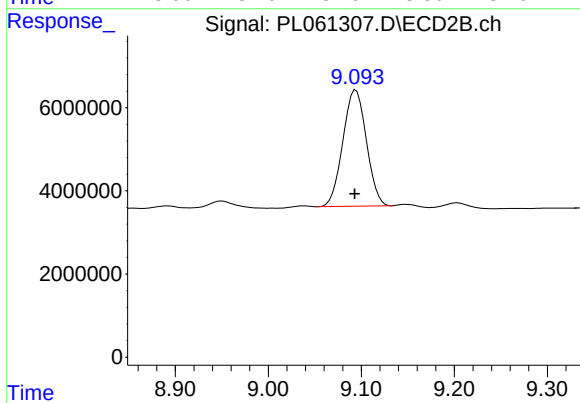

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.001 min
Response: 49194744
Conc: 20.80 ng/ml