

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
 Data File : PL061315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 22:40
 Operator : DD\AJ
 Sample : L3919-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:39:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	38690474	68664222	22.433	22.323
28)	SA Decachlor...	8.210	9.094	34205801	50132457	20.503	21.202
Target Compounds							
12)	B 4,4'-DDE	5.621	6.352	9649264	16893387	5.675	5.270
17)	MA 4,4'-DDT	6.377	7.143	4857058	9352989	3.537	3.737
22)	Mirex	7.360f	0.000	11141900	0	7.451	N.D. #
23)	Chlordane-1	4.332	0.000	196439	0	3.745	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 22:40
Operator : DD\AJ
Sample : L3919-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:39:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

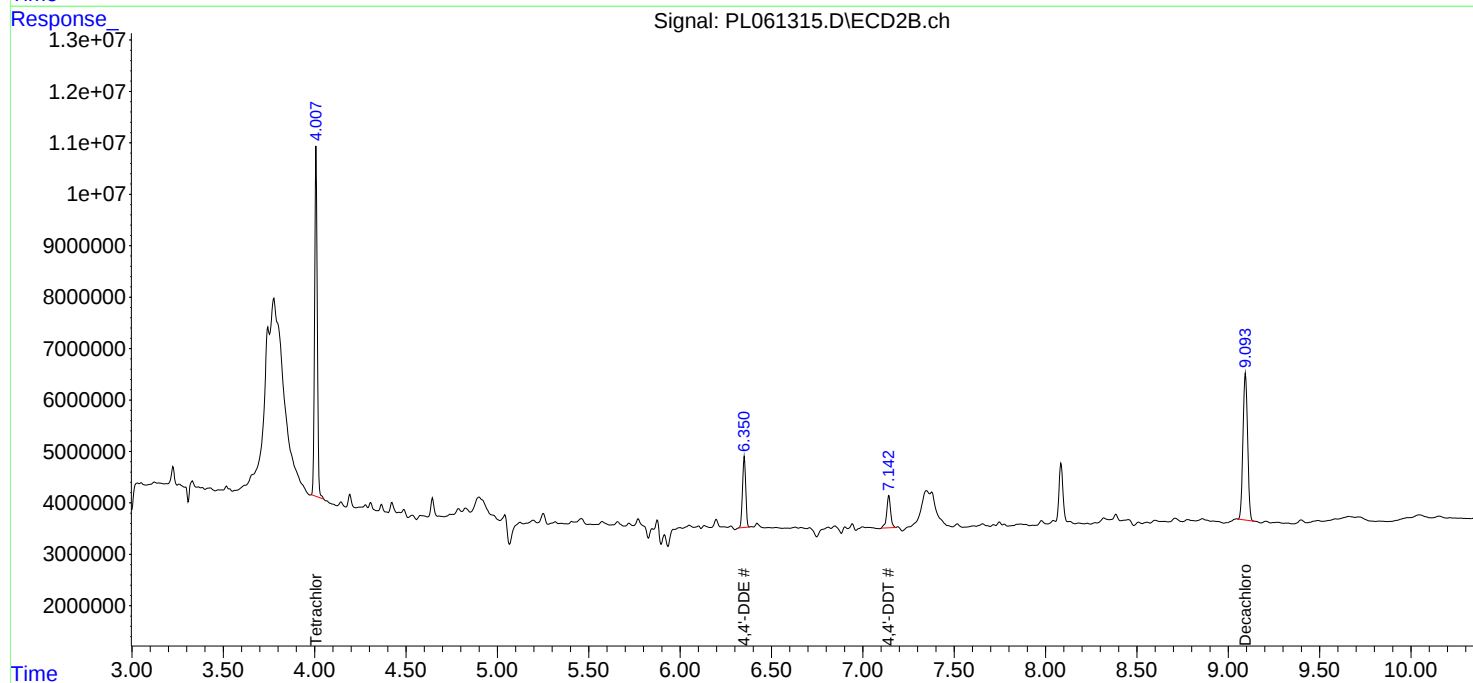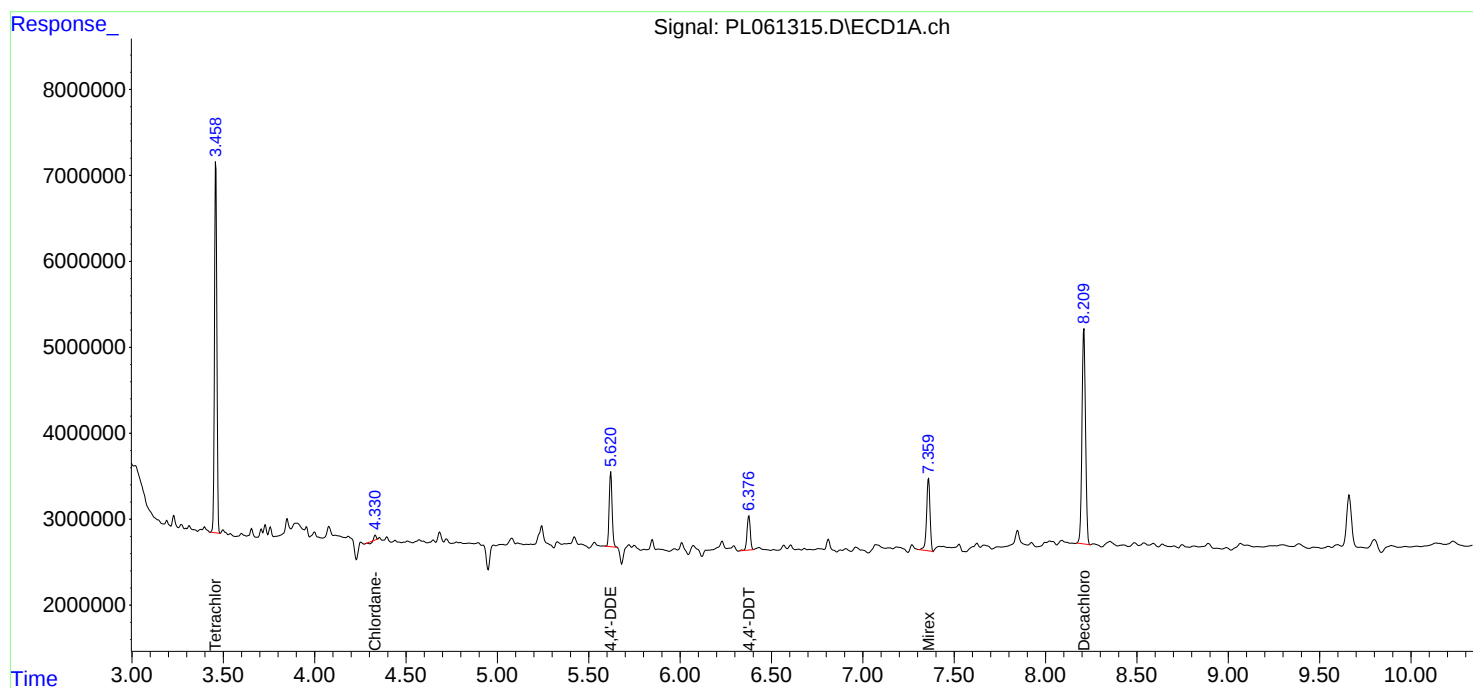


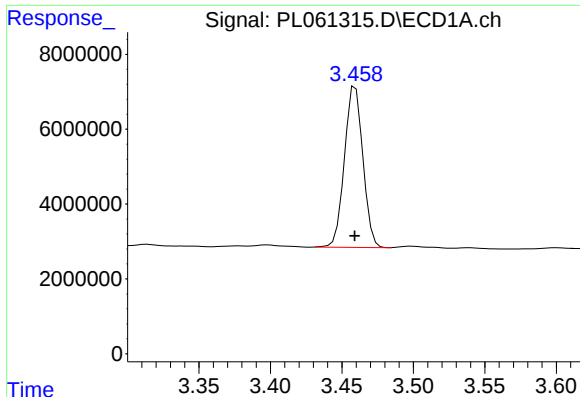

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 38690474
Conc: 22.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

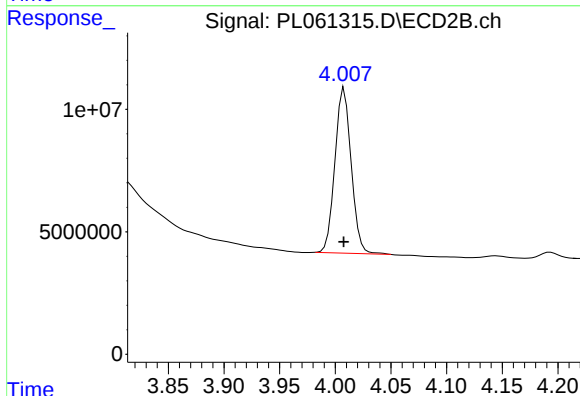


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 68664222
Conc: 22.32 ng/ml

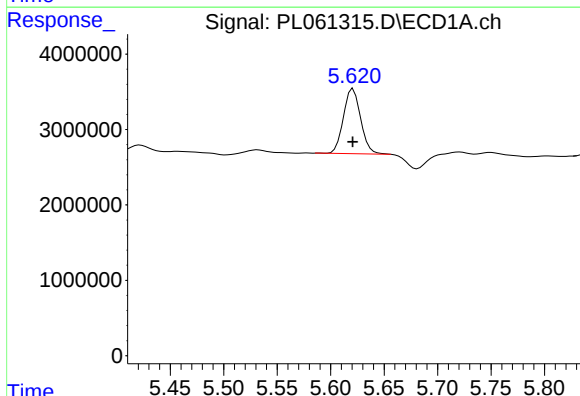


#12 4,4'-DDE

R.T.: 5.621 min
Delta R.T.: 0.000 min
Response: 9649264
Conc: 5.67 ng/ml

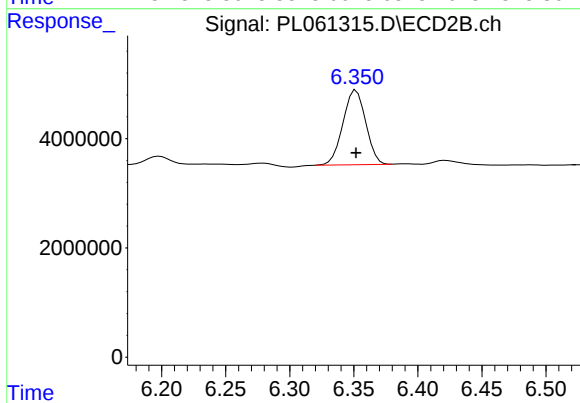

#12 4,4'-DDE


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 16893387
Conc: 5.27 ng/ml

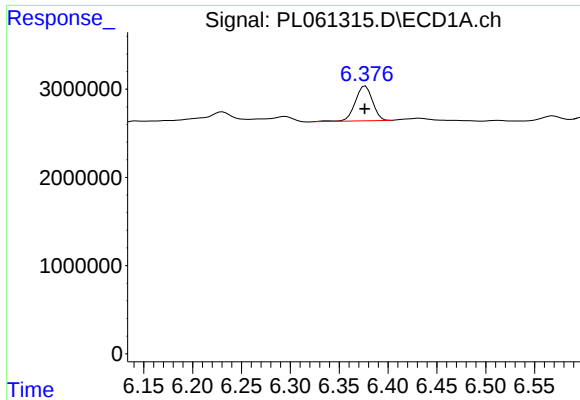

#17 4,4'-DDT


R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 4857058
Conc: 3.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

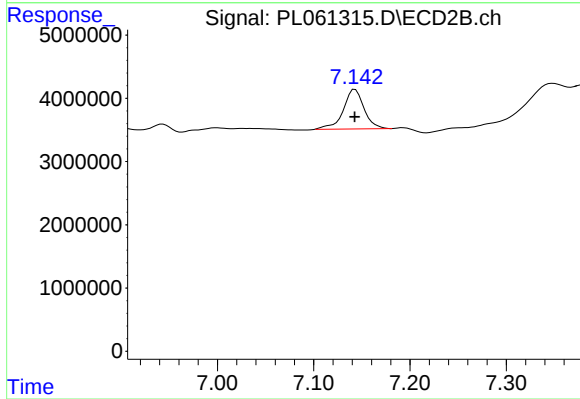


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 9352989
Conc: 3.74 ng/ml

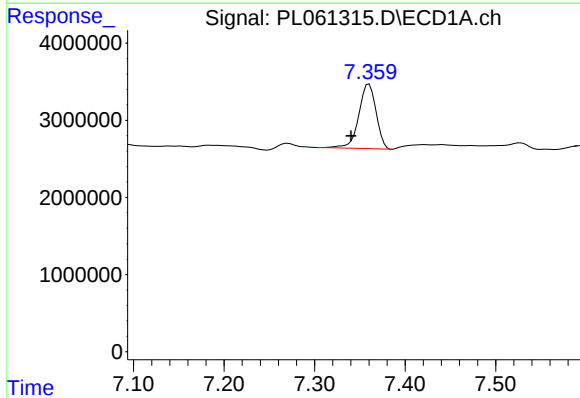


#22 Mirex

R.T.: 7.360 min
Delta R.T.: 0.020 min
Response: 11141900
Conc: 7.45 ng/ml

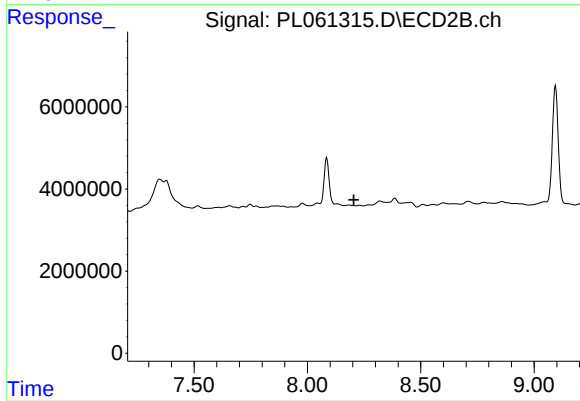

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.205 min
Response: 0
Conc: N.D.

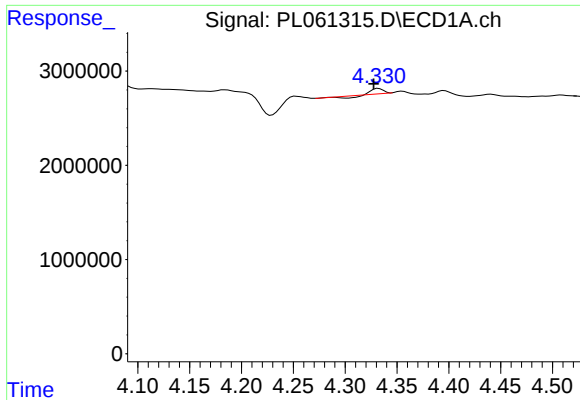

#23 Chlordane-1


R.T.: 4.332 min
Delta R.T.: 0.005 min
Response: 196439
Conc: 3.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

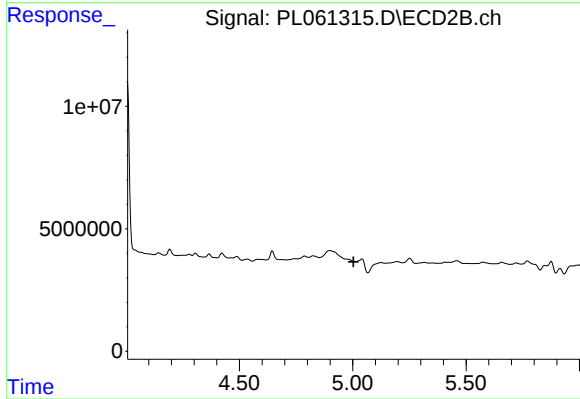


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

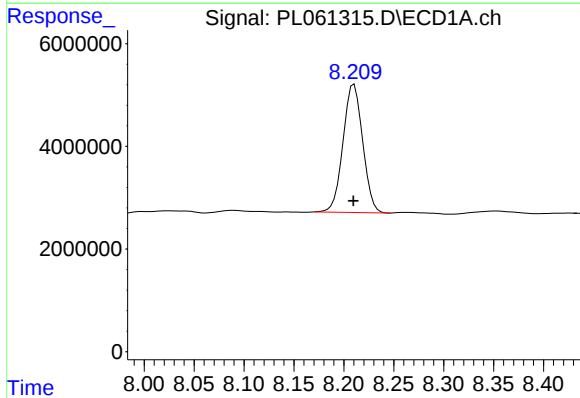

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 34205801
Conc: 20.50 ng/ml

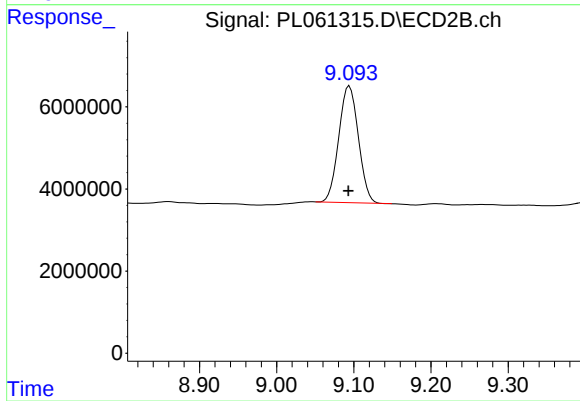

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.002 min
Response: 50132457
Conc: 21.20 ng/ml