

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
 Data File : PL061319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 23:37
 Operator : DD\AJ
 Sample : L3919-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:40:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.009	37697644	64897575	21.858	21.098
28)	SA Decachlor...	8.211	9.094	31482194	43984324	18.871	18.601
Target Compounds							
11)	B alpha-Chl...	0.000	6.197	0	3531651	N.D.	1.015 #
12)	B 4,4'-DDE	0.000	6.352	0	3763181	N.D.	1.174 #
14)	MA Endrin	0.000	6.739f	0	3605287	N.D.	1.289 #
16)	A 4,4'-DDD	6.139	0.000	813846	0	0.563	N.D. #
17)	MA 4,4'-DDT	6.374	0.000	2517582	0	1.834	N.D. #
19)	B Endosulfa...	6.645f	7.278	15506834	25854640	9.422	9.451
21)	B Endrin ke...	7.180f	0.000	17160166	0	9.384	N.D. #
22)	Mirex	0.000	8.209	0	358654	N.D.	0.186 #
24)	Chlordane-2	0.000	5.463	0	13818741	N.D.	113.141 #
26)	Chlordane-4	0.000	6.197	0	3531651	N.D.	6.747 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 23:37
Operator : DD\AJ
Sample : L3919-17
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:40:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

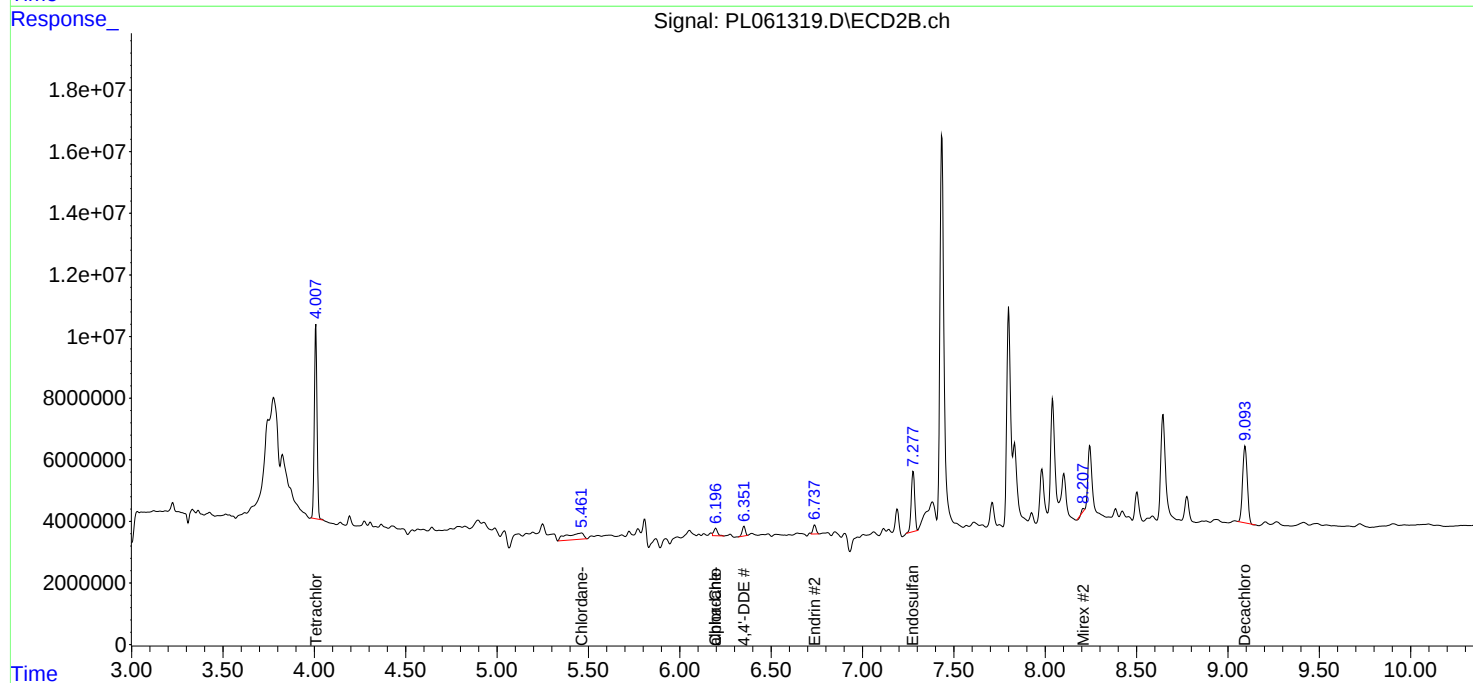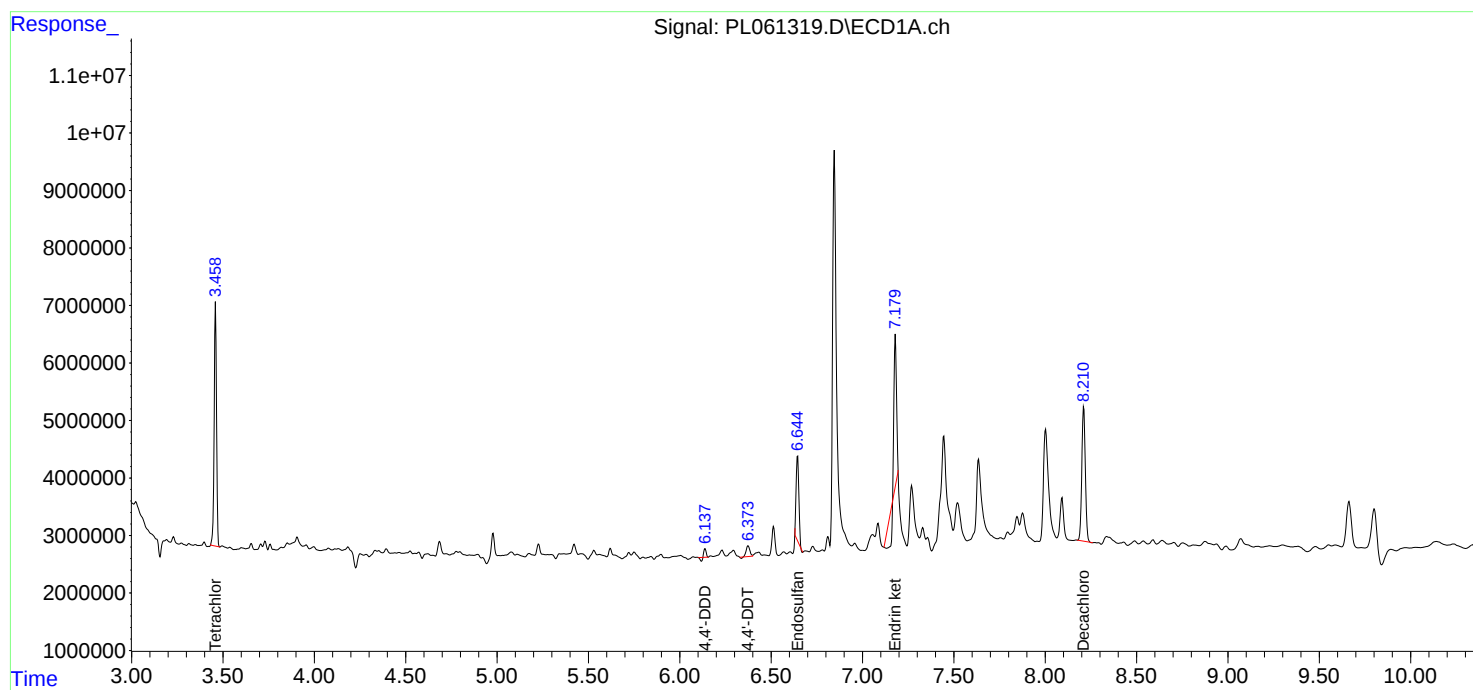


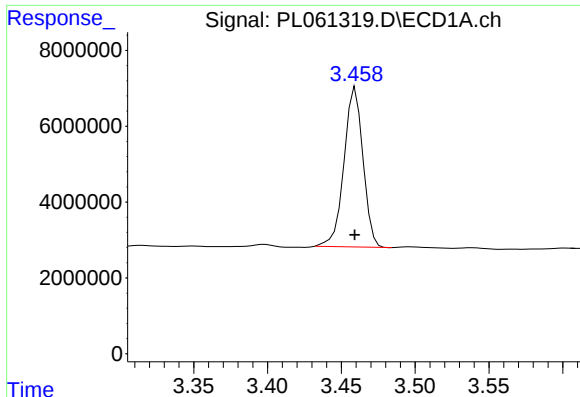

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 37697644
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

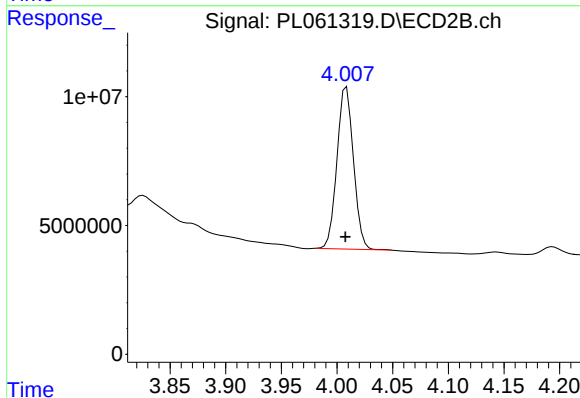


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 64897575
Conc: 21.10 ng/ml

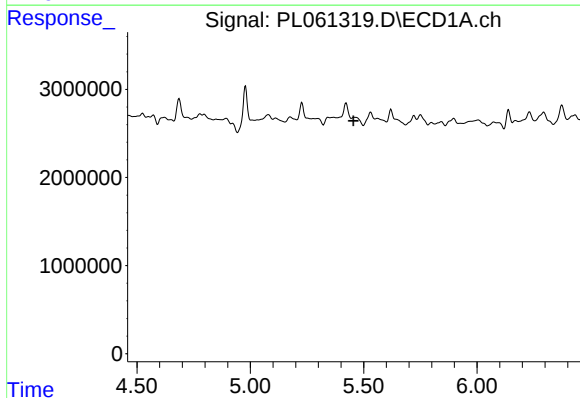


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.456 min
Response: 0
Conc: N.D.

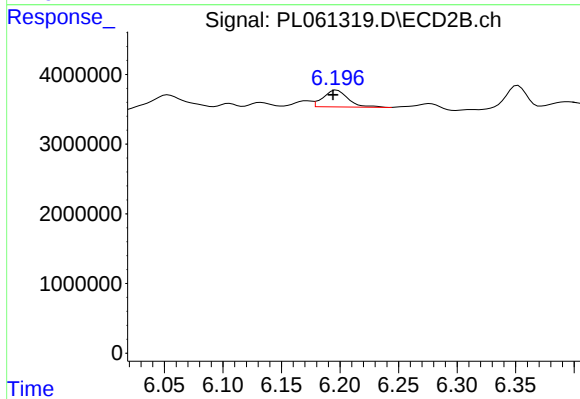

#11 alpha-Chlordane


R.T.: 6.197 min
Delta R.T.: 0.003 min
Response: 3531651
Conc: 1.01 ng/ml

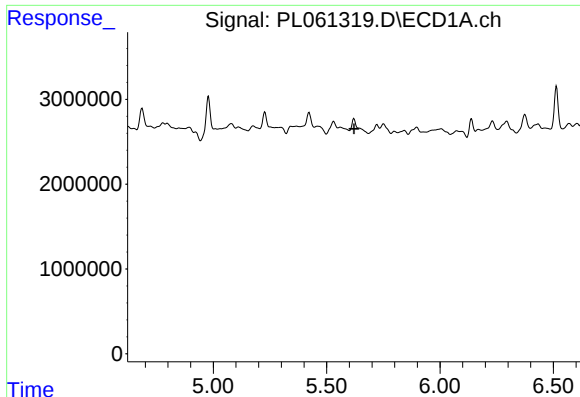

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.621 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15

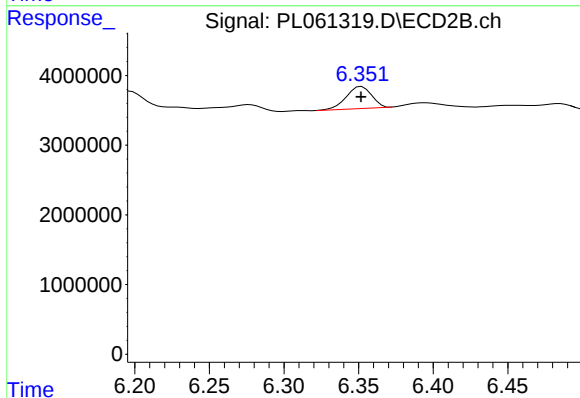


#12 4,4'-DDE

R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 3763181
Conc: 1.17 ng/ml

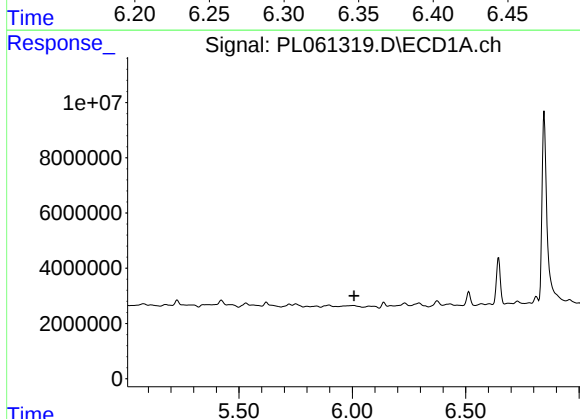


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.008 min
Response: 0
Conc: N.D.

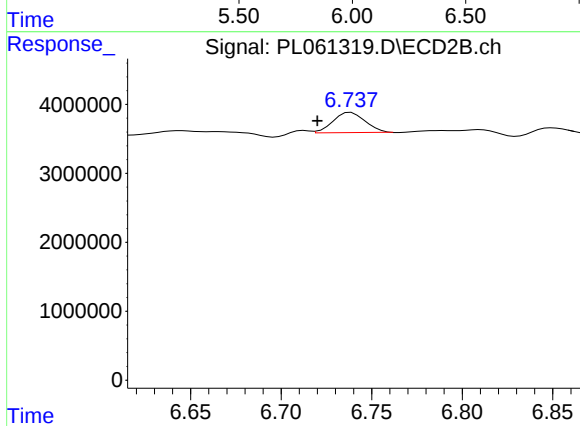

#14 Endrin


R.T.: 6.739 min
Delta R.T.: 0.019 min
Response: 3605287
Conc: 1.29 ng/ml

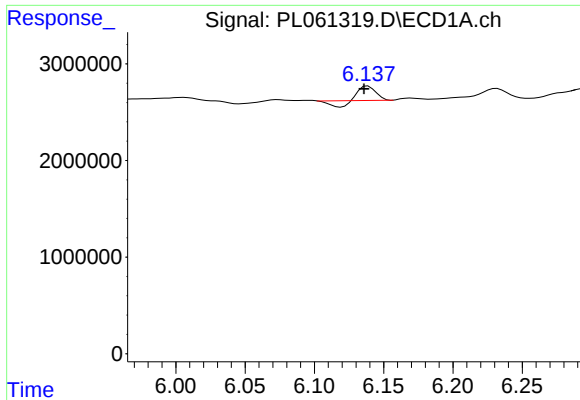

#16 4,4'-DDD


R.T.: 6.139 min
Delta R.T.: 0.003 min
Response: 813846
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

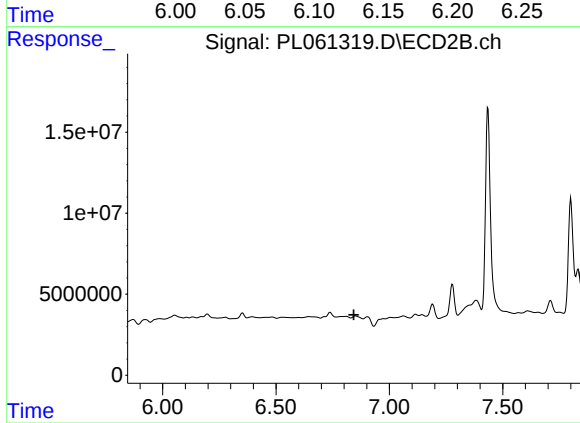


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

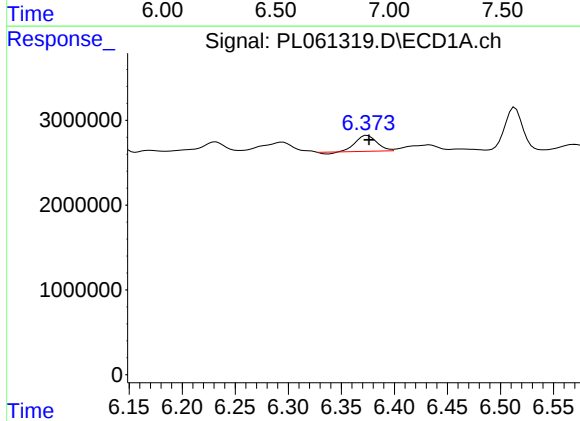


#17 4,4'-DDT

R.T.: 6.374 min
Delta R.T.: -0.002 min
Response: 2517582
Conc: 1.83 ng/ml

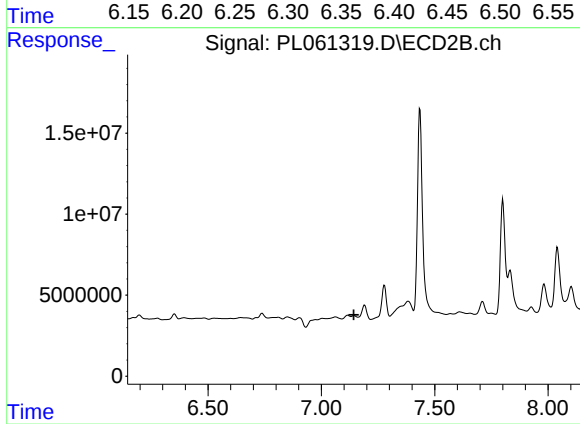

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.143 min
Response: 0
Conc: N.D.

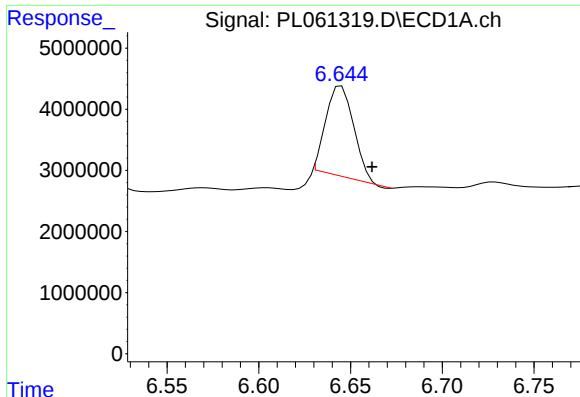

#19 Endosulfan Sulfate


R.T.: 6.645 min
Delta R.T.: -0.017 min
Response: 15506834
Conc: 9.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

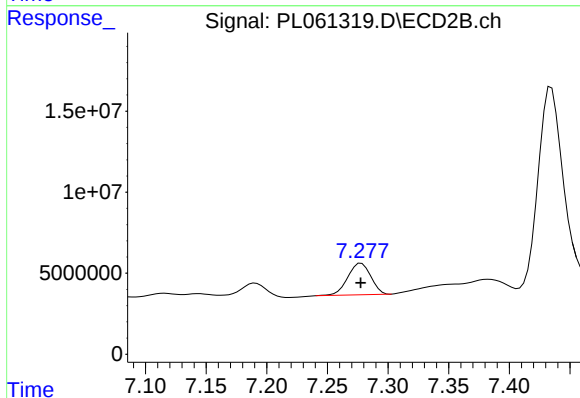


#19 Endosulfan Sulfate

R.T.: 7.278 min
Delta R.T.: 0.000 min
Response: 25854640
Conc: 9.45 ng/ml

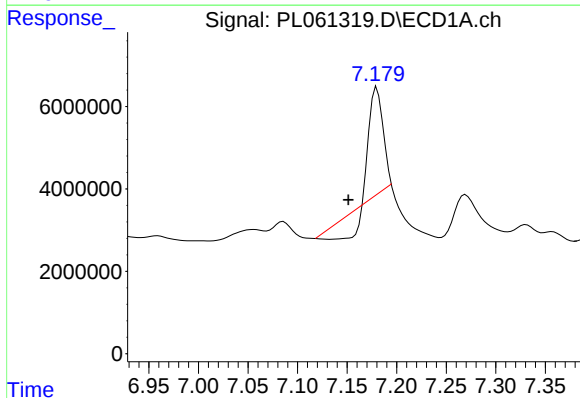


#21 Endrin ketone

R.T.: 7.180 min
Delta R.T.: 0.029 min
Response: 17160166
Conc: 9.38 ng/ml

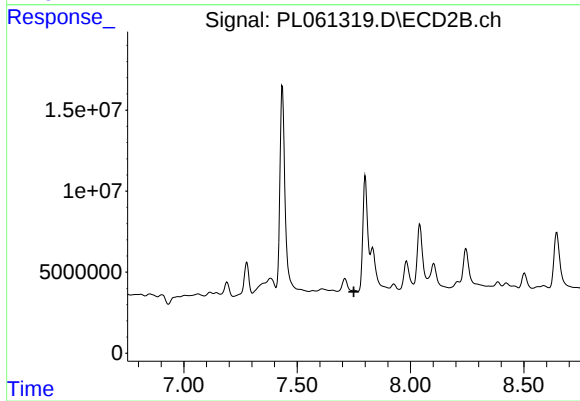

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.750 min
Response: 0
Conc: N.D.

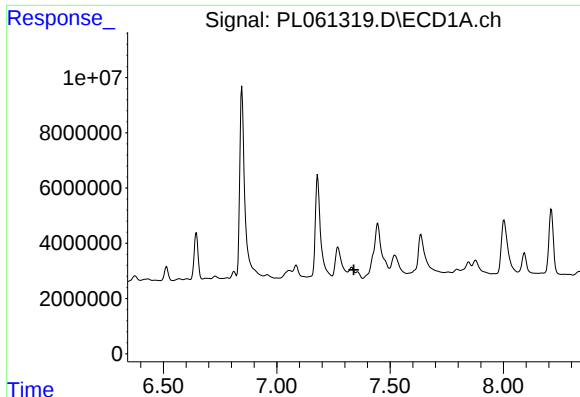

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15

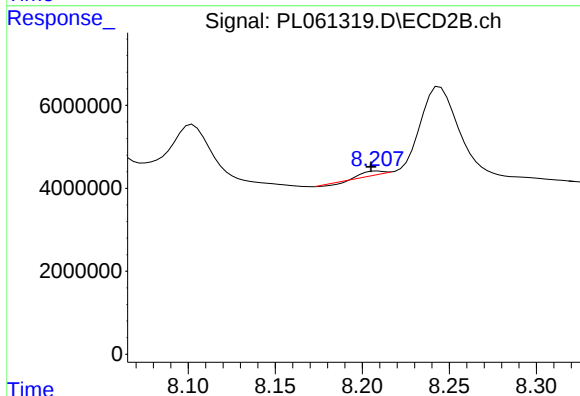


#22 Mirex

R.T.: 8.209 min
Delta R.T.: 0.004 min
Response: 358654
Conc: 0.19 ng/ml

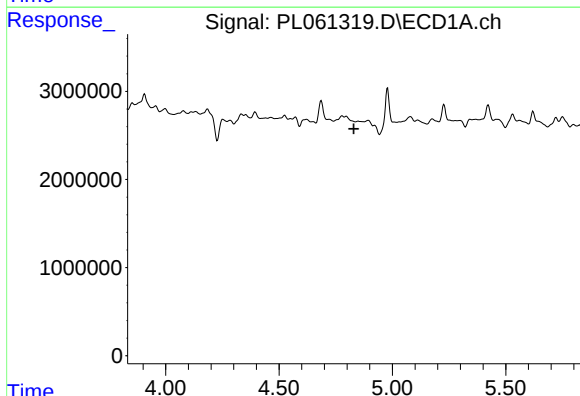


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.829 min
Response: 0
Conc: N.D.

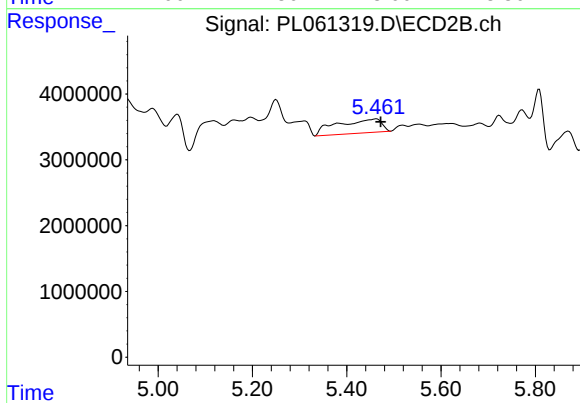

#24 Chlordane-2


R.T.: 5.463 min
Delta R.T.: -0.010 min
Response: 13818741
Conc: 113.14 ng/ml

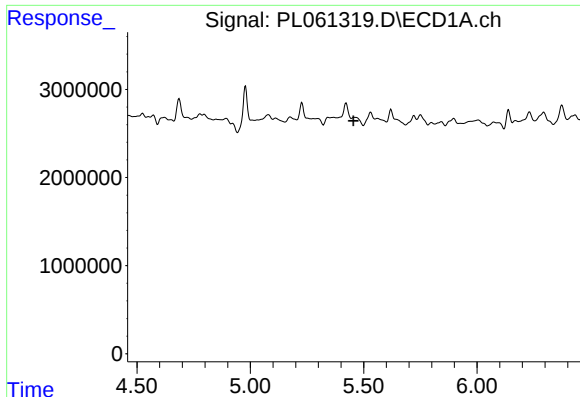

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15

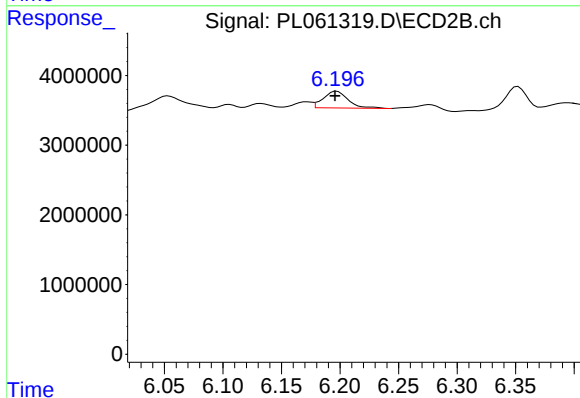


#26 Chlordane-4

R.T.: 6.197 min
Delta R.T.: 0.002 min
Response: 3531651
Conc: 6.75 ng/ml

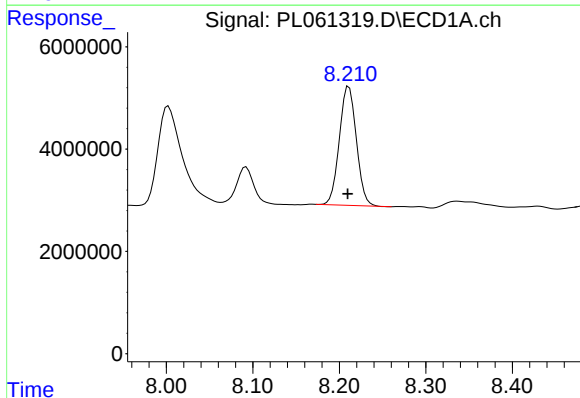

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.001 min
Response: 31482194
Conc: 18.87 ng/ml

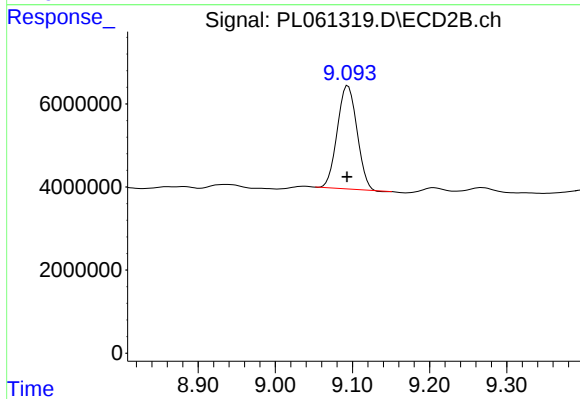

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.001 min
Response: 43984324
Conc: 18.60 ng/ml