

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
 Data File : PL061274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 12:46
 Operator : DD\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:33:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	37939620	68026683	21.998	22.116
28)	SA Decachlor...	8.211	9.094	35734172	51940864	21.419	21.966
Target Compounds							
9)	A Endosulfan I	5.509	6.245	16556694	31514609	9.624	9.824
10)	B gamma-Chl...	5.399	6.122	17801737	32637277	9.609	9.467
12)	B 4,4'-DDE	5.622	6.352	32430870	61468715	19.072	19.176
13)	MA Dieldrin	5.753	6.502	35008569	64015068	19.504	19.524
19)	B Endosulfa...	6.664	7.279	31102679	51720082	18.898	18.905
20)	A Methoxychlor	6.923	7.603	83954959	138.4E6	98.072	96.235
21)	B Endrin ke...	7.152	7.750	35139717	52667931	19.216	19.400



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 12:46
Operator : DD\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:33:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

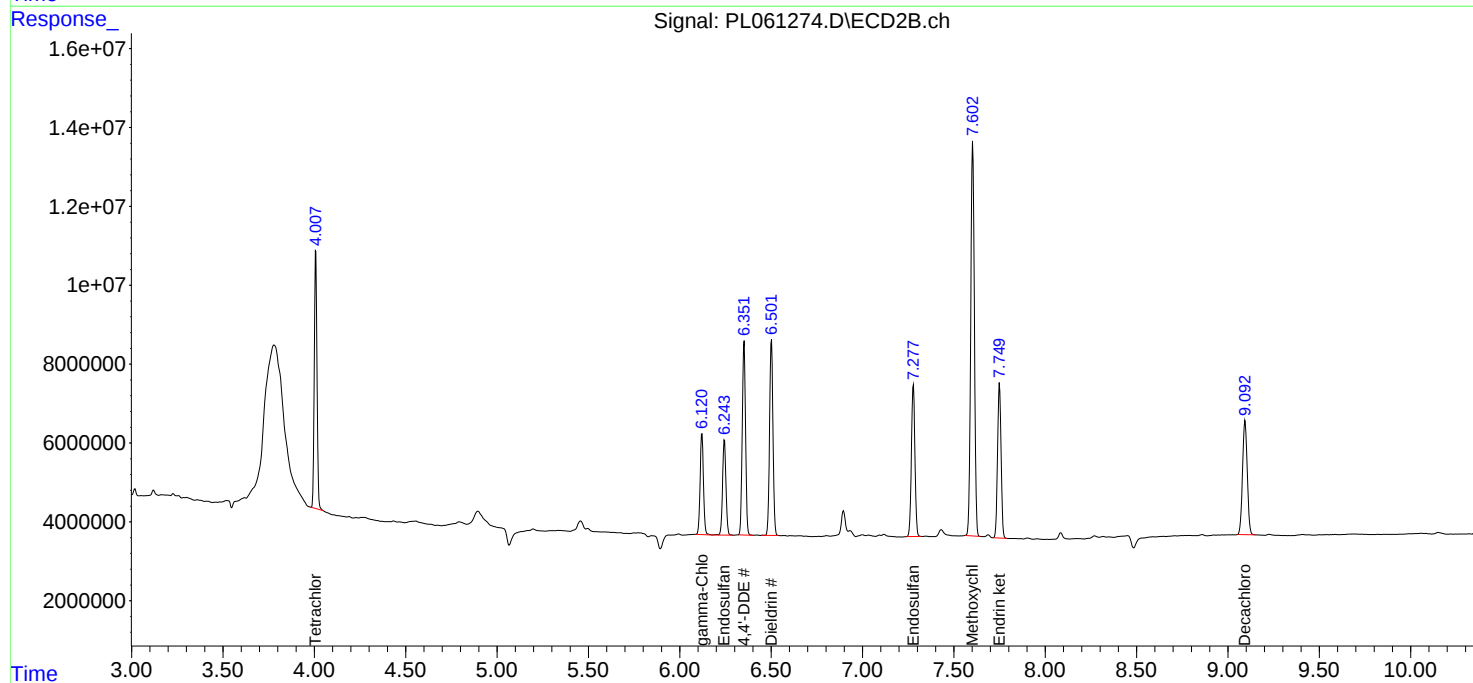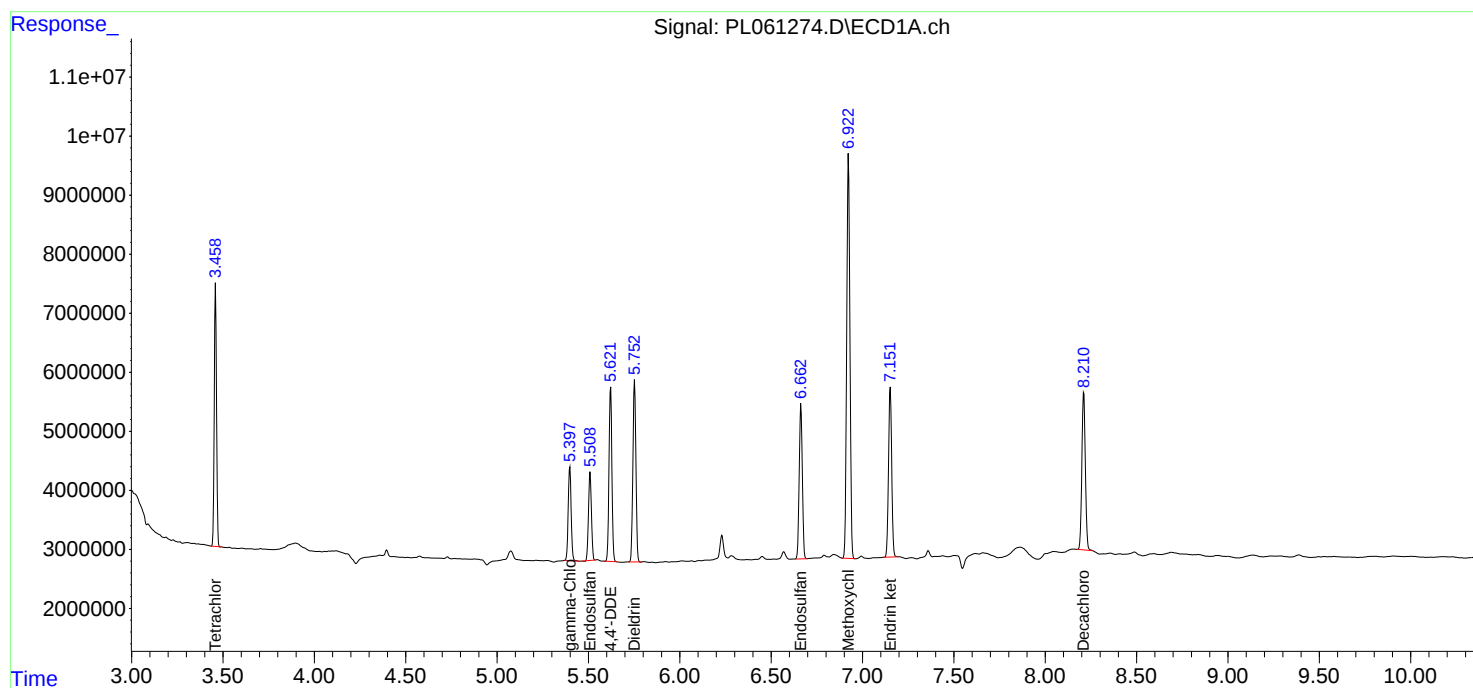


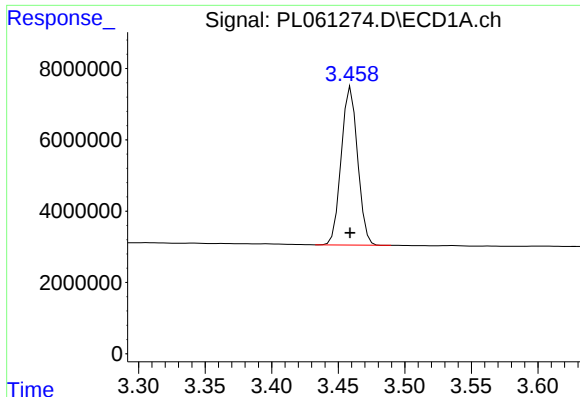

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 37939620
Conc: 22.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

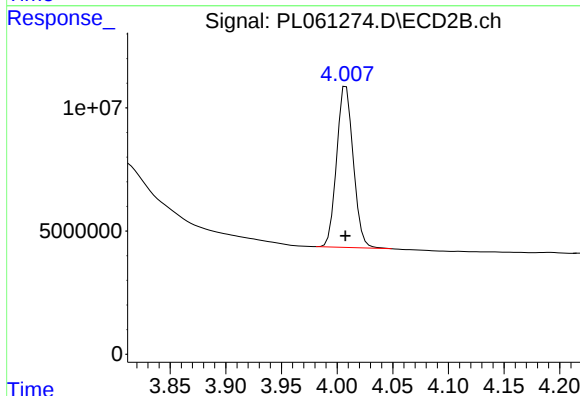


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 68026683
Conc: 22.12 ng/ml

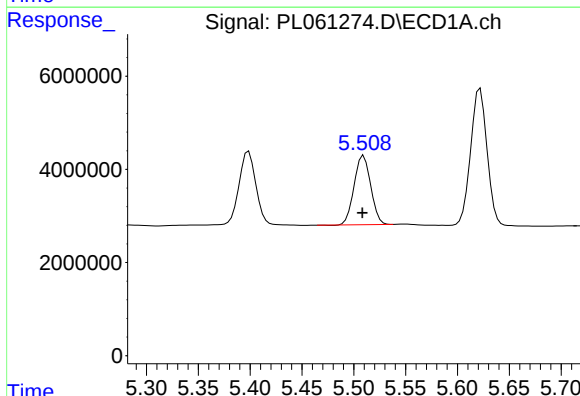


#9 Endosulfan I

R.T.: 5.509 min
Delta R.T.: 0.001 min
Response: 16556694
Conc: 9.62 ng/ml

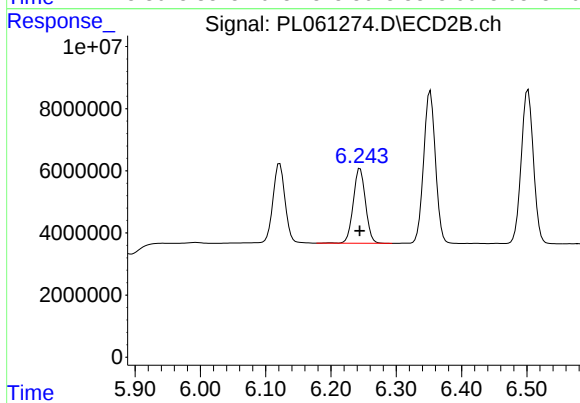

#9 Endosulfan I


R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 31514609
Conc: 9.82 ng/ml

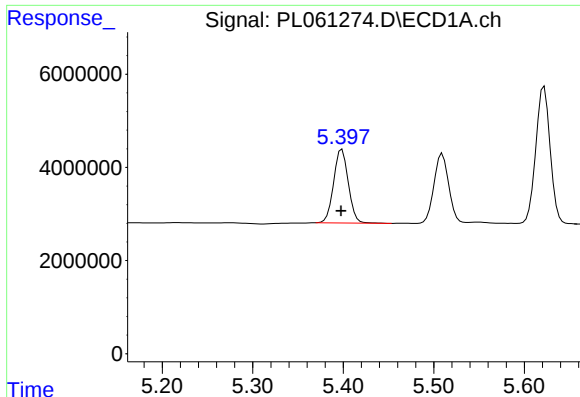

#10 gamma-Chlordane


R.T.: 5.399 min
Delta R.T.: 0.001 min
Response: 17801737
Conc: 9.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

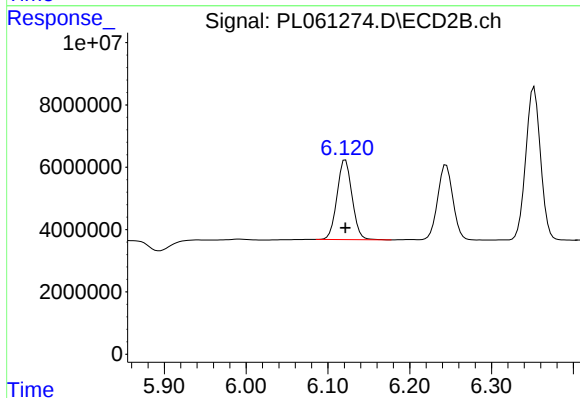


#10 gamma-Chlordane

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 32637277
Conc: 9.47 ng/ml

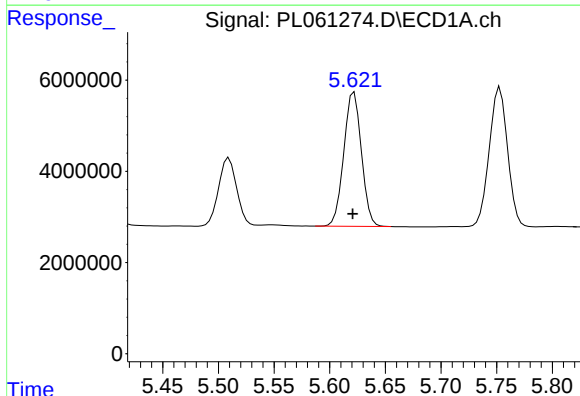


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: 0.001 min
Response: 32430870
Conc: 19.07 ng/ml

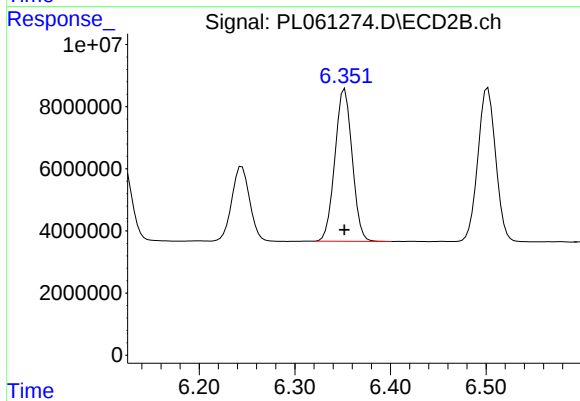

#12 4,4'-DDE


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 61468715
Conc: 19.18 ng/ml

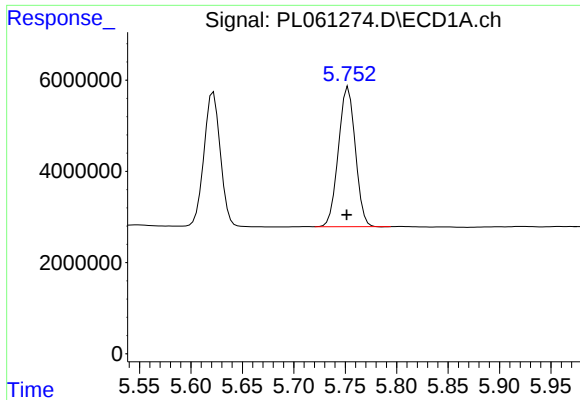

#13 Dieldrin


R.T.: 5.753 min
Delta R.T.: 0.001 min
Response: 35008569
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

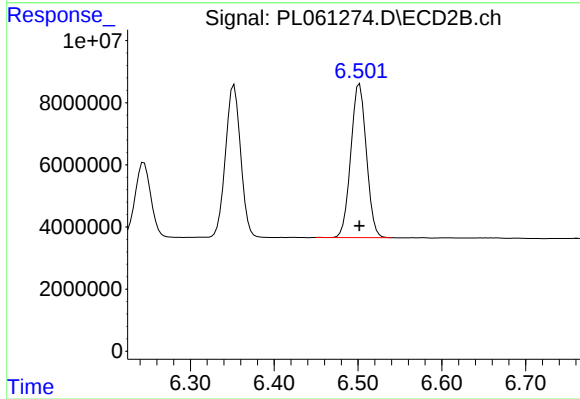


#13 Dieldrin

R.T.: 6.502 min
Delta R.T.: 0.000 min
Response: 64015068
Conc: 19.52 ng/ml

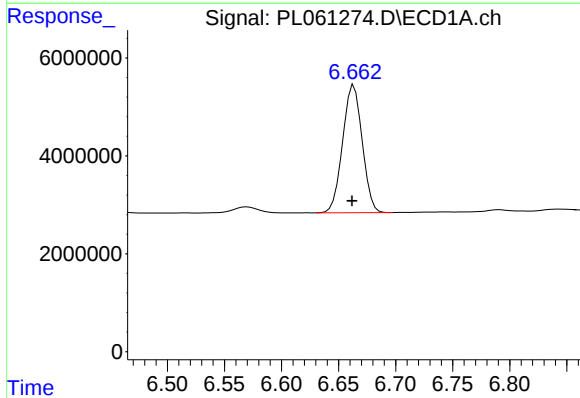


#19 Endosulfan Sulfate

R.T.: 6.664 min
Delta R.T.: 0.002 min
Response: 31102679
Conc: 18.90 ng/ml

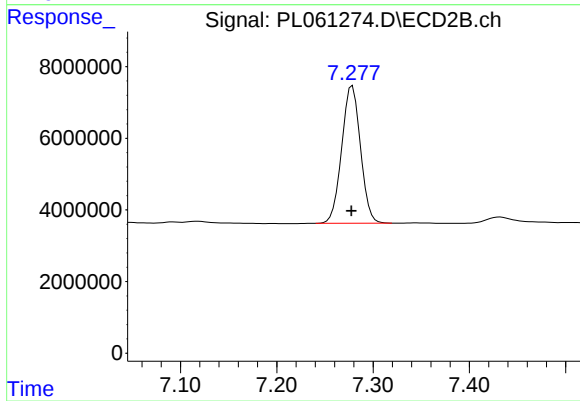

#19 Endosulfan Sulfate


R.T.: 7.279 min
Delta R.T.: 0.001 min
Response: 51720082
Conc: 18.91 ng/ml

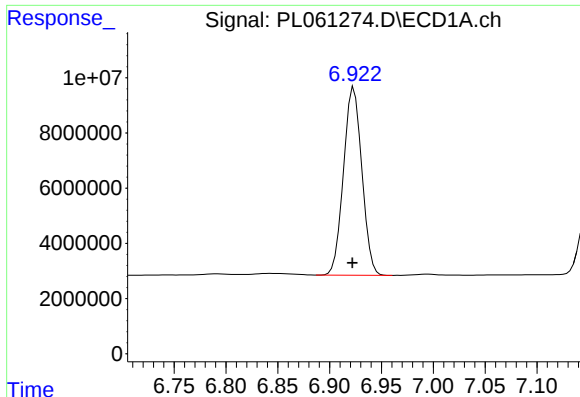

#20 Methoxychlor


R.T.: 6.923 min
Delta R.T.: 0.002 min
Response: 83954959
Conc: 98.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

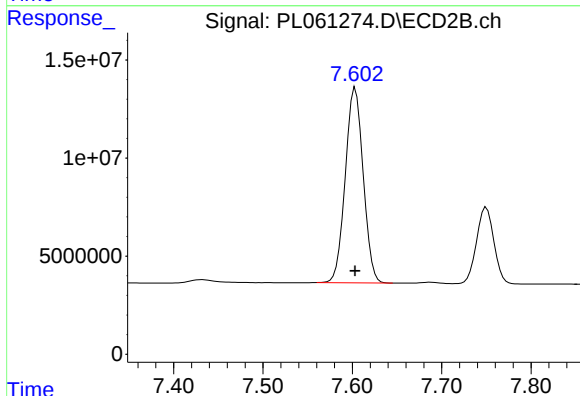


#20 Methoxychlor

R.T.: 7.603 min
Delta R.T.: 0.000 min
Response: 138428124
Conc: 96.23 ng/ml

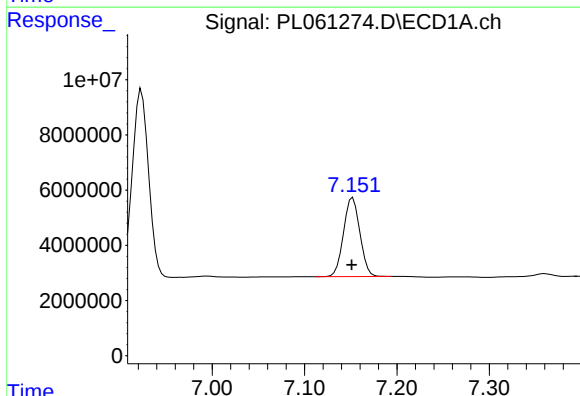


#21 Endrin ketone

R.T.: 7.152 min
Delta R.T.: 0.001 min
Response: 35139717
Conc: 19.22 ng/ml

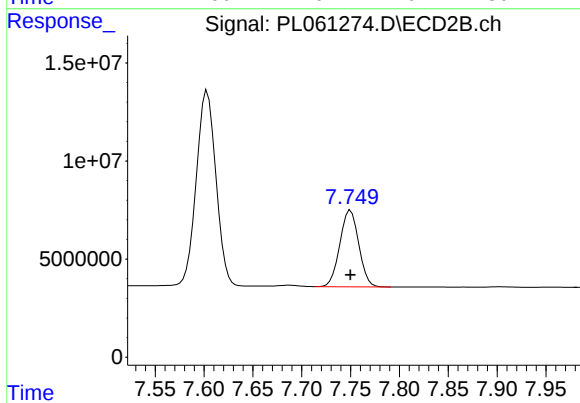

#21 Endrin ketone


R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 52667931
Conc: 19.40 ng/ml

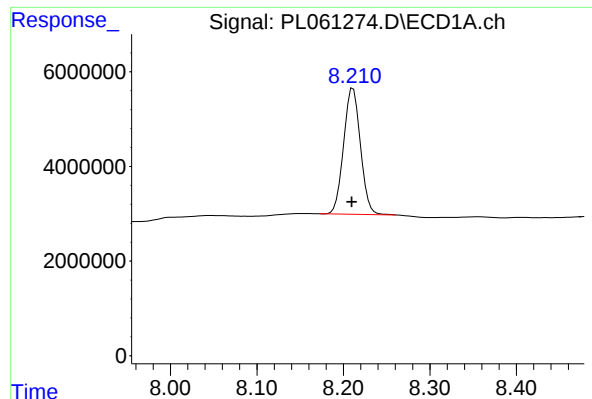

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.002 min
Response: 35734172
Conc: 21.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

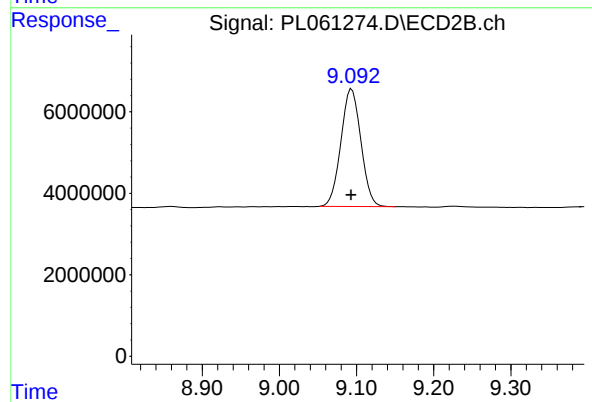

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.001 min
Response: 51940864
Conc: 21.97 ng/ml