

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090822\
 Data File : PL077596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2022 11:37
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 17:20:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 14:34:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.425	2.628	75856492	133.8E6	44.366	50.552
28)	SA Decachlor...	8.920	7.734	60131108	86563208	40.090	43.895
Target Compounds							
23)	Chlordane-1	4.586	3.607	31031228	41310837	479.866	493.893
24)	Chlordane-2	5.120	4.178	32774054	43614178	432.486	442.842
25)	Chlordane-3	5.833	4.803	123.5E6	128.5E6	455.715	449.775
26)	Chlordane-4	5.910	4.864	149.2E6	136.5E6	445.937	460.391
27)	Chlordane-5	6.769	5.529	24975813	33836992	414.653	487.700



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090822\
Data File : PL077596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2022 11:37
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 17:20:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 14:34:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

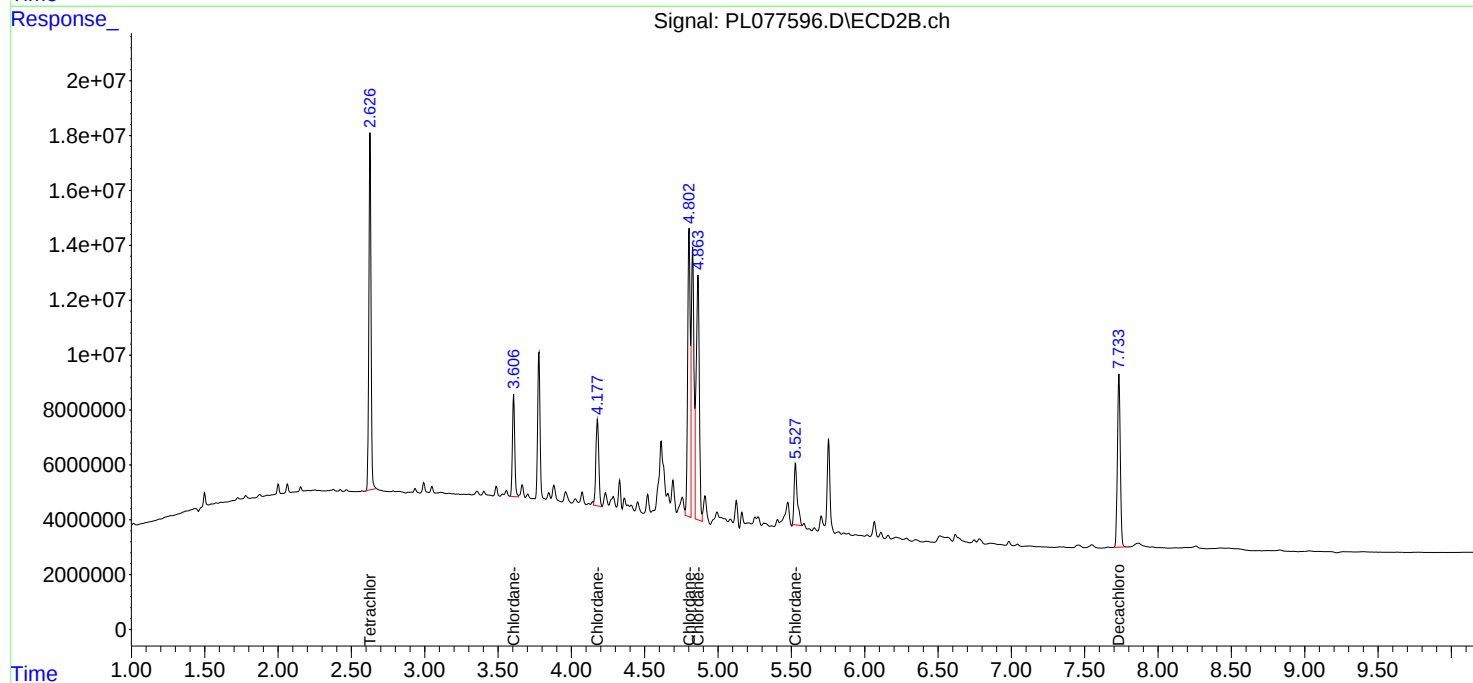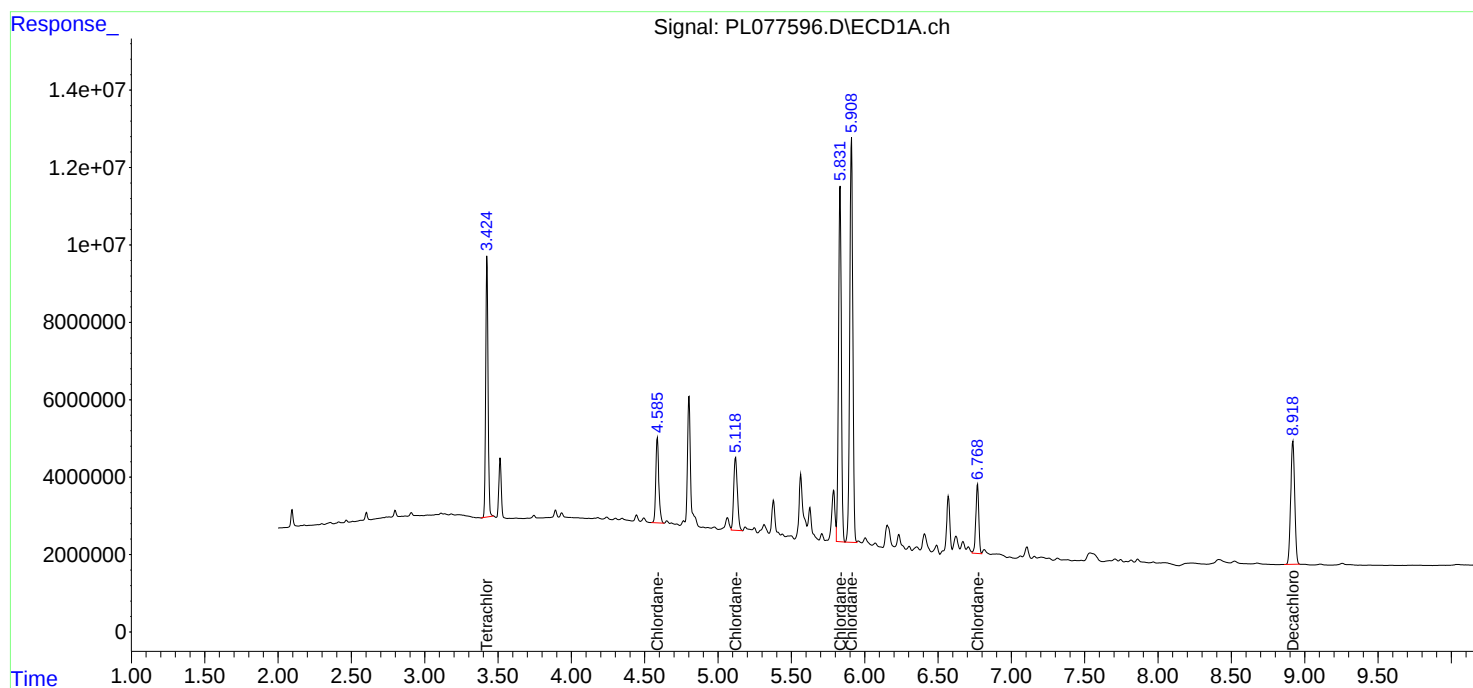


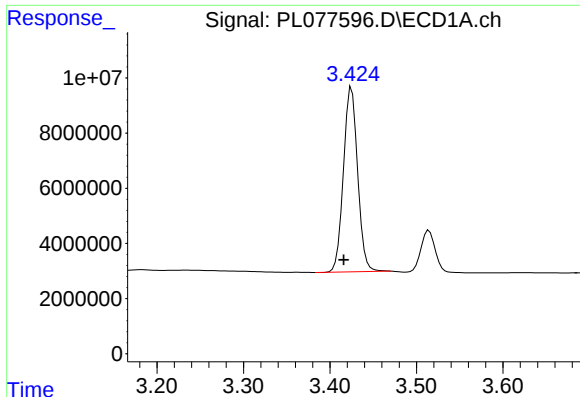

#1 Tetrachloro-m-xylene


R.T.: 3.425 min
Delta R.T.: 0.009 min
Response: 75856492
Conc: 44.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

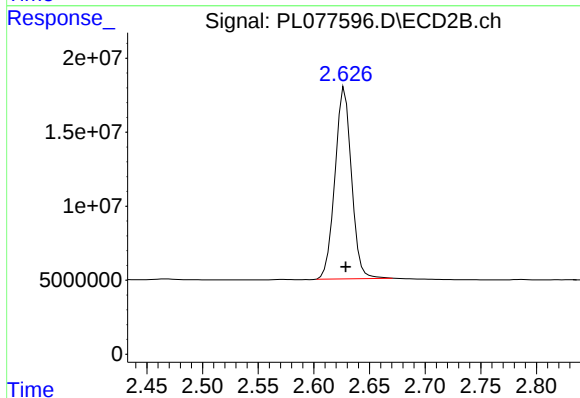


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 133767058
Conc: 50.55 ng/ml

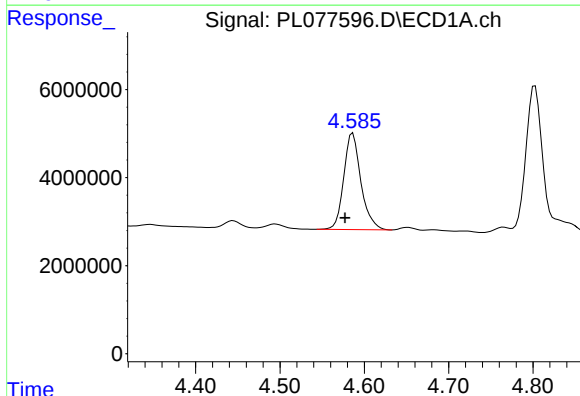


#23 Chlordane-1

R.T.: 4.586 min
Delta R.T.: 0.009 min
Response: 31031228
Conc: 479.87 ng/ml

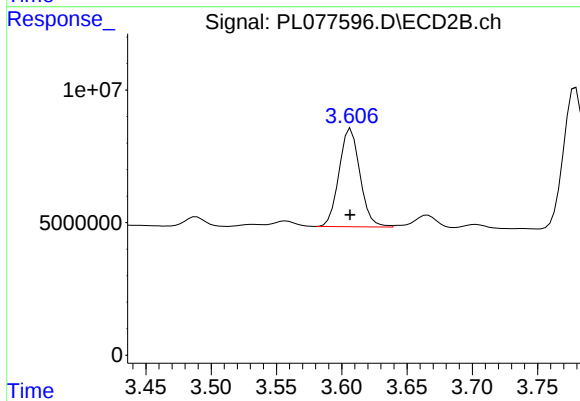

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 41310837
Conc: 493.89 ng/ml

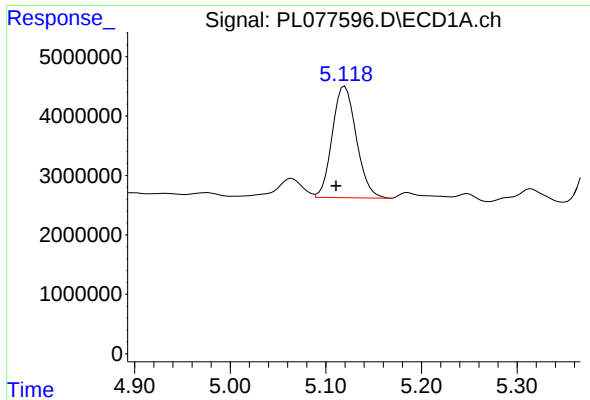

#24 Chlordane-2


R.T.: 5.120 min
Delta R.T.: 0.009 min
Response: 32774054
Conc: 432.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

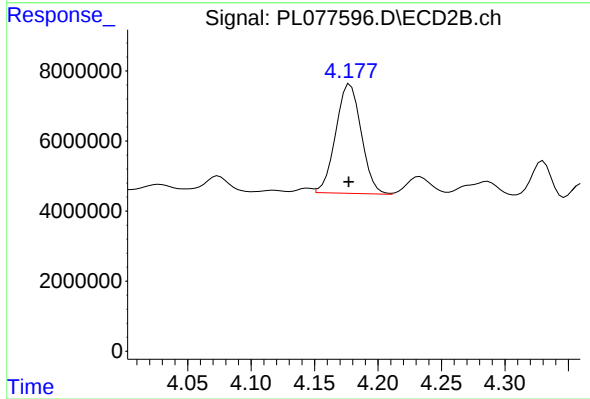


#24 Chlordane-2

R.T.: 4.178 min
Delta R.T.: 0.001 min
Response: 43614178
Conc: 442.84 ng/ml

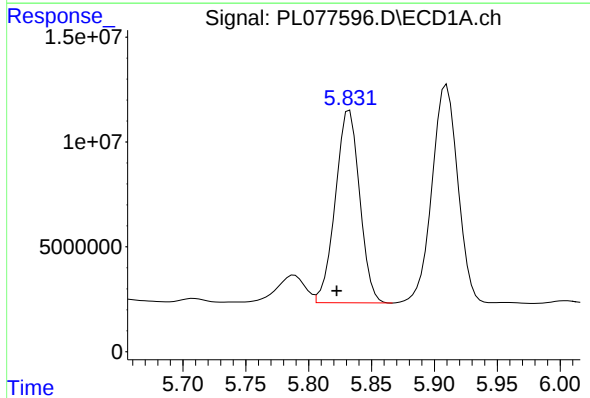


#25 Chlordane-3

R.T.: 5.833 min
Delta R.T.: 0.010 min
Response: 123481744
Conc: 455.71 ng/ml

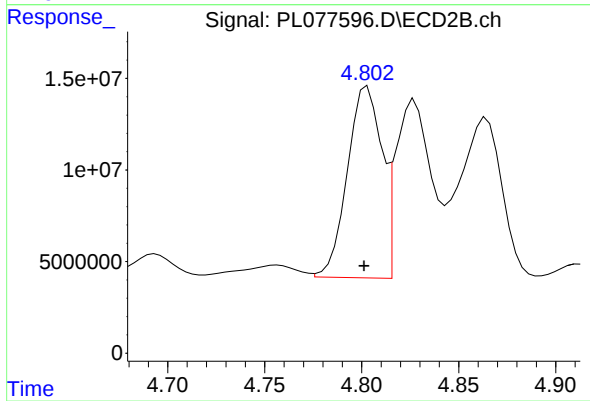

#25 Chlordane-3


R.T.: 4.803 min
Delta R.T.: 0.002 min
Response: 128471409
Conc: 449.77 ng/ml

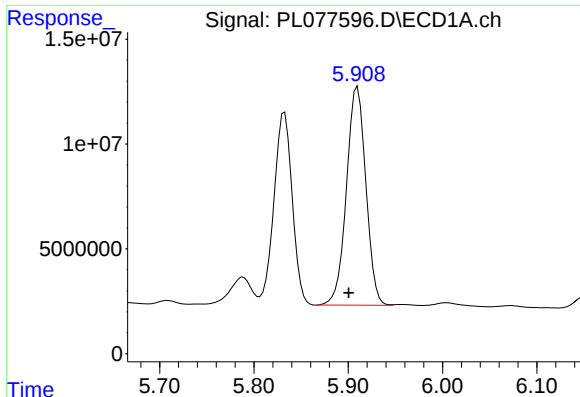

#26 Chlordane-4


R.T.: 5.910 min
Delta R.T.: 0.009 min
Response: 149160884
Conc: 445.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

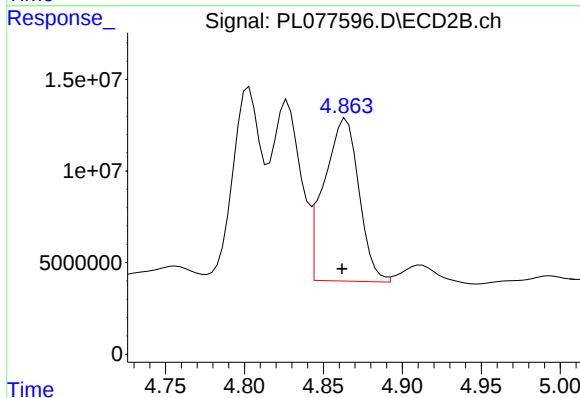


#26 Chlordane-4

R.T.: 4.864 min
Delta R.T.: 0.003 min
Response: 136473303
Conc: 460.39 ng/ml

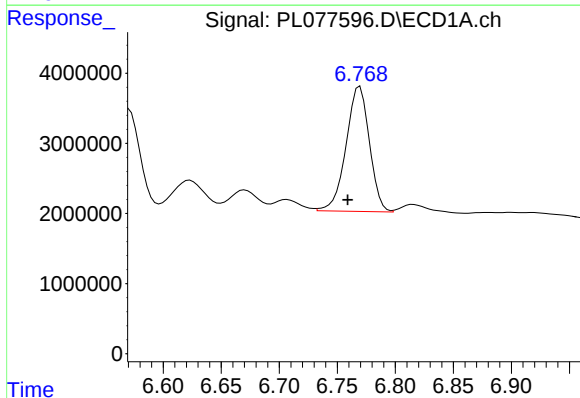


#27 Chlordane-5

R.T.: 6.769 min
Delta R.T.: 0.010 min
Response: 24975813
Conc: 414.65 ng/ml

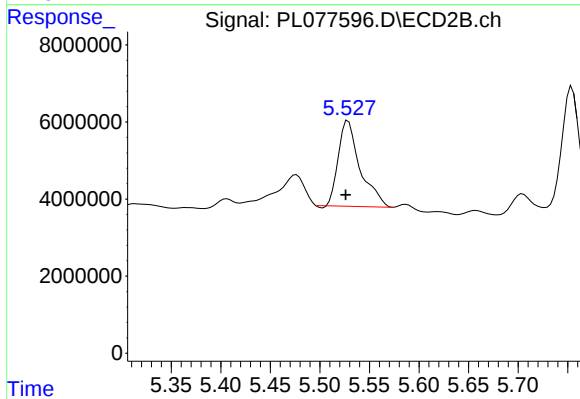

#27 Chlordane-5


R.T.: 5.529 min
Delta R.T.: 0.002 min
Response: 33836992
Conc: 487.70 ng/ml

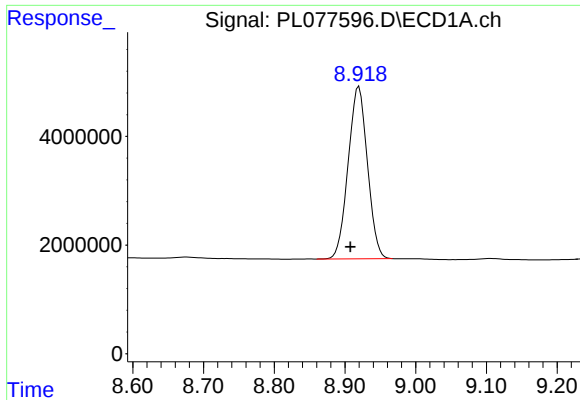

#28 Decachlorobiphenyl

R.T.: 8.920 min
Delta R.T.: 0.012 min
Response: 60131108
Conc: 40.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

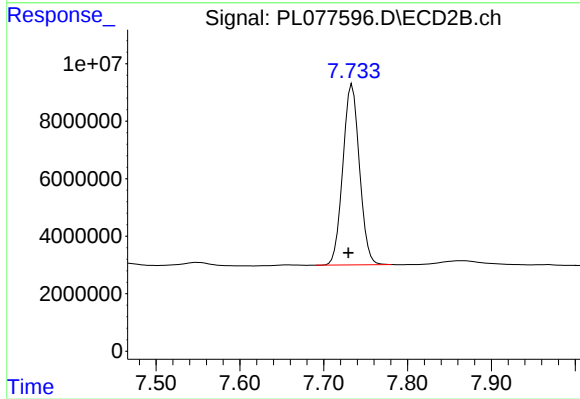

#28 Decachlorobiphenyl

R.T.: 7.734 min
Delta R.T.: 0.004 min
Response: 86563208
Conc: 43.89 ng/ml