

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090822\
 Data File : PL077607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2022 18:50
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 03:36:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 14:34:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.627	81981415	149.6E6	47.949	56.523
28)	SA Decachlor...	8.906	7.726	61797043	95590176	41.201	48.472
Target Compounds							
23)	Chlordane-1	4.576	3.605	33672814	47075492	520.716	562.812
24)	Chlordane-2	5.109	4.175	35405280	52218386	467.208	530.205
25)	Chlordane-3	5.822	4.799	132.8E6	147.9E6	490.011	517.836
26)	Chlordane-4	5.900	4.860	159.5E6	156.1E6	476.734	526.680
27)	Chlordane-5	6.759	5.524	25911018	39293155	430.180	566.341 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090822\
Data File : PL077607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2022 18:50
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 03:36:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 14:34:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

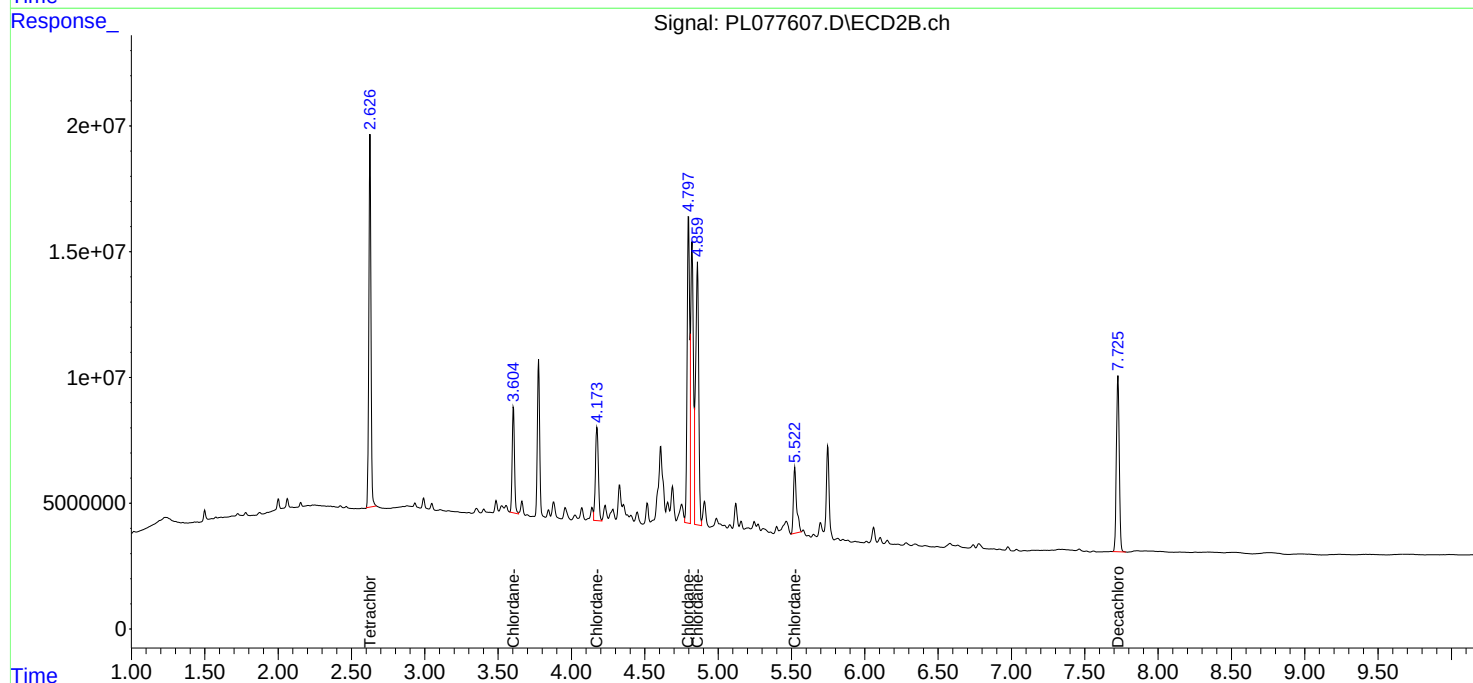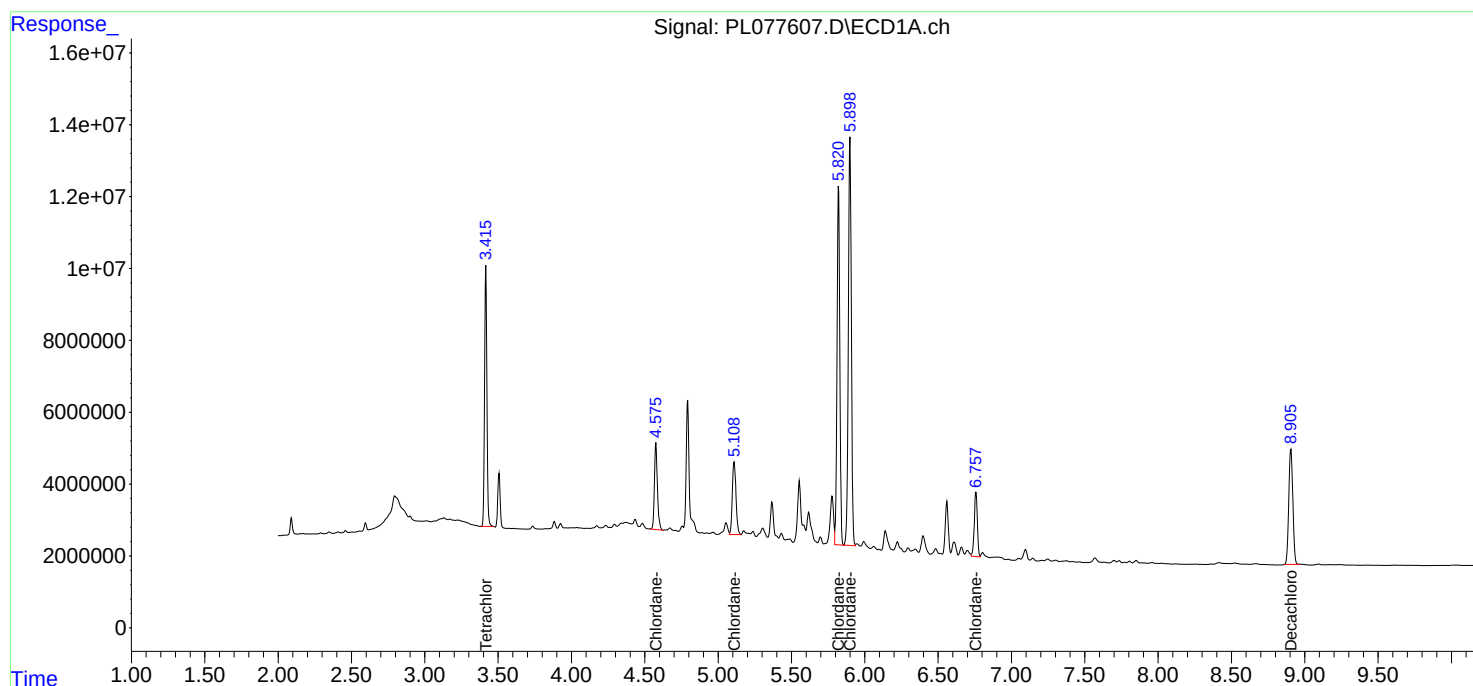


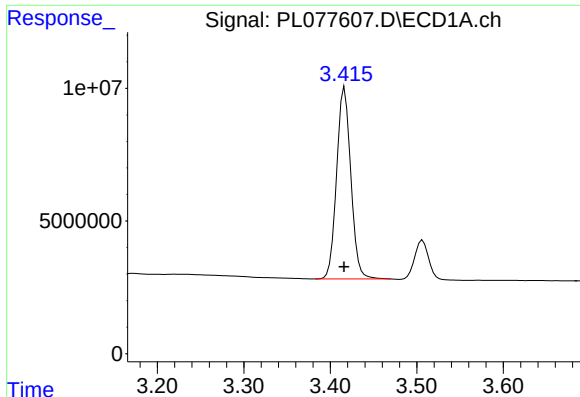

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 81981415
Conc: 47.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

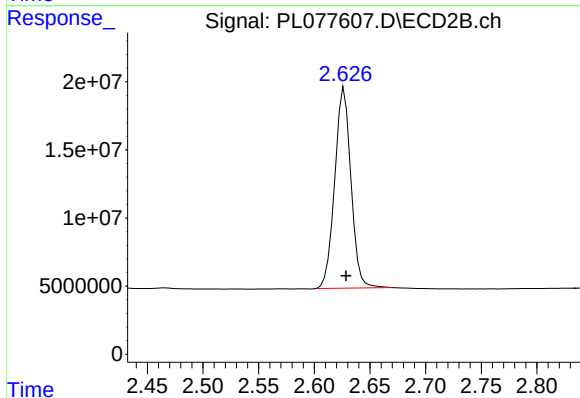


#1 Tetrachloro-m-xylene

R.T.: 2.627 min
Delta R.T.: -0.002 min
Response: 149567713
Conc: 56.52 ng/ml

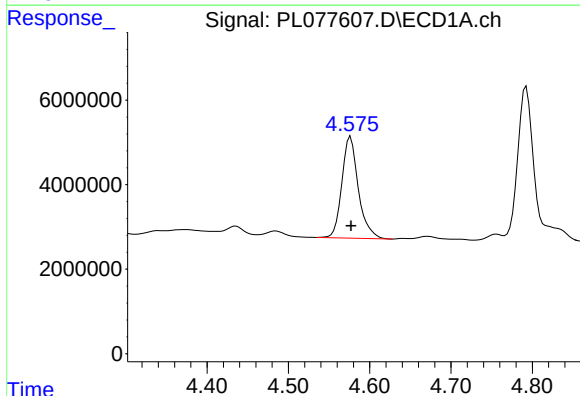


#23 Chlordane-1

R.T.: 4.576 min
Delta R.T.: 0.000 min
Response: 33672814
Conc: 520.72 ng/ml

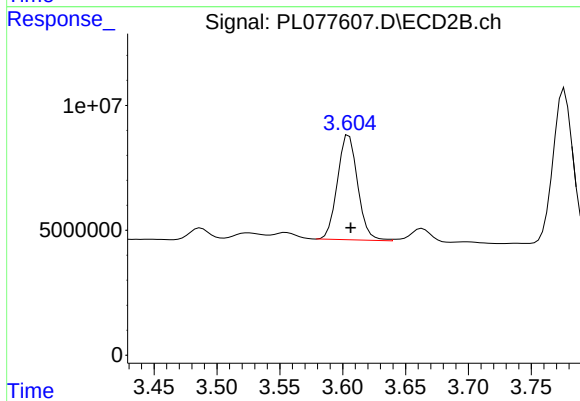

#23 Chlordane-1


R.T.: 3.605 min
Delta R.T.: -0.001 min
Response: 47075492
Conc: 562.81 ng/ml

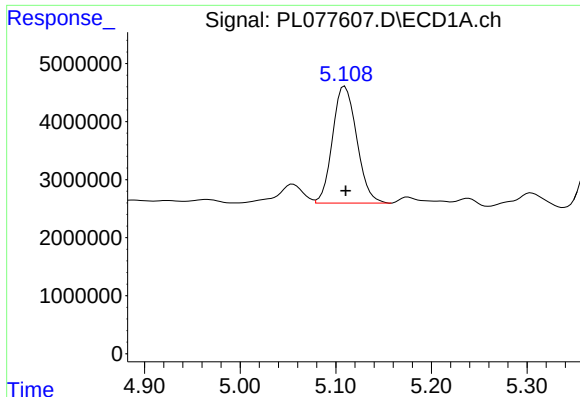

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: -0.001 min
Response: 35405280
Conc: 467.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

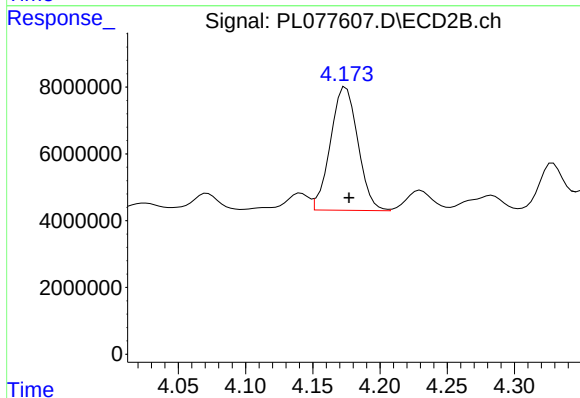


#24 Chlordane-2

R.T.: 4.175 min
Delta R.T.: -0.002 min
Response: 52218386
Conc: 530.21 ng/ml

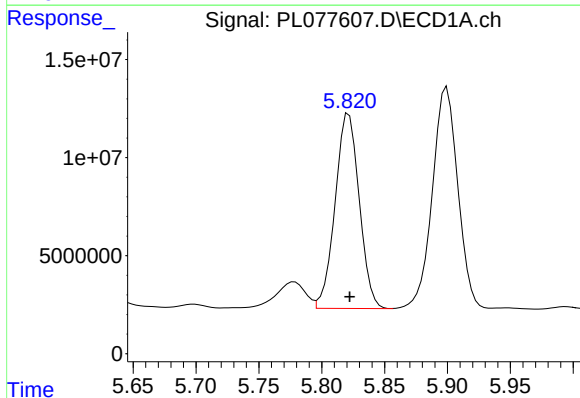


#25 Chlordane-3

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 132774869
Conc: 490.01 ng/ml

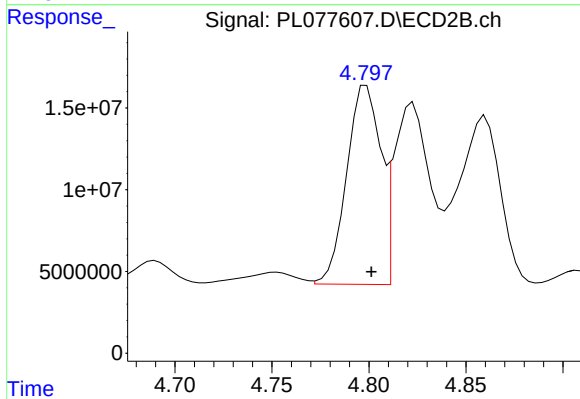

#25 Chlordane-3


R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 147912011
Conc: 517.84 ng/ml

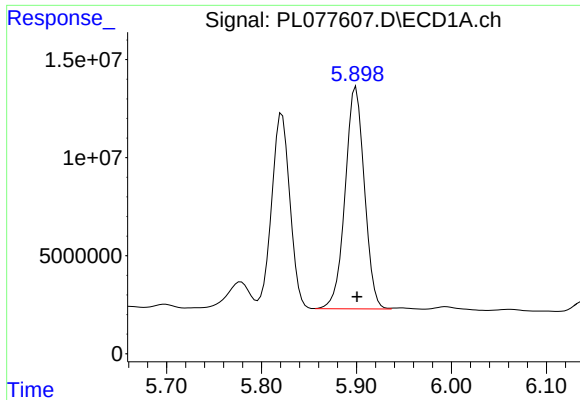

#26 Chlordane-4


R.T.: 5.900 min
Delta R.T.: 0.000 min
Response: 159461933
Conc: 476.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

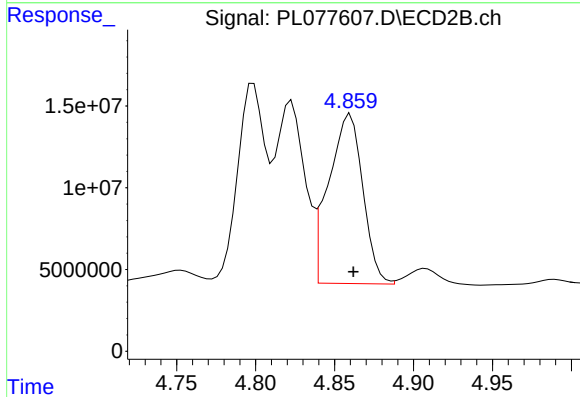


#26 Chlordane-4

R.T.: 4.860 min
Delta R.T.: -0.002 min
Response: 156123182
Conc: 526.68 ng/ml

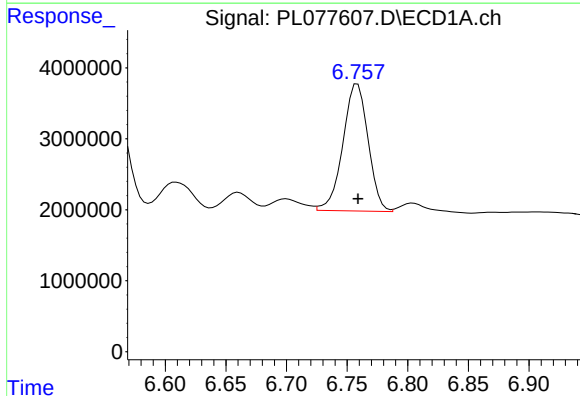


#27 Chlordane-5

R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 25911018
Conc: 430.18 ng/ml

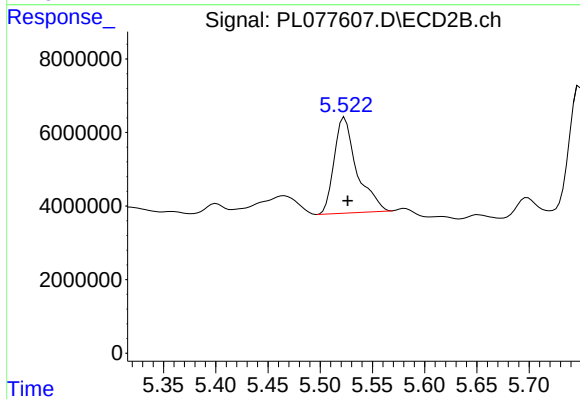

#27 Chlordane-5


R.T.: 5.524 min
Delta R.T.: -0.003 min
Response: 39293155
Conc: 566.34 ng/ml

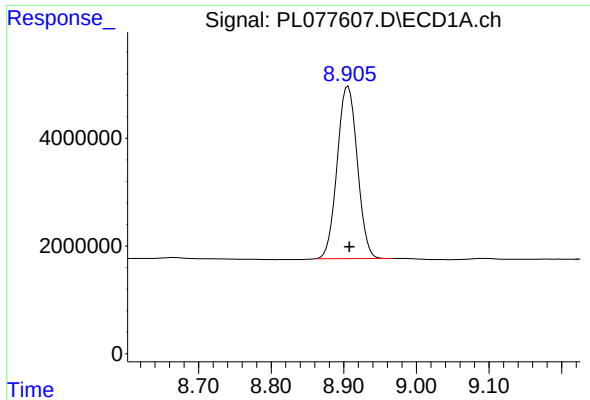

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: -0.002 min
Response: 61797043
Conc: 41.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

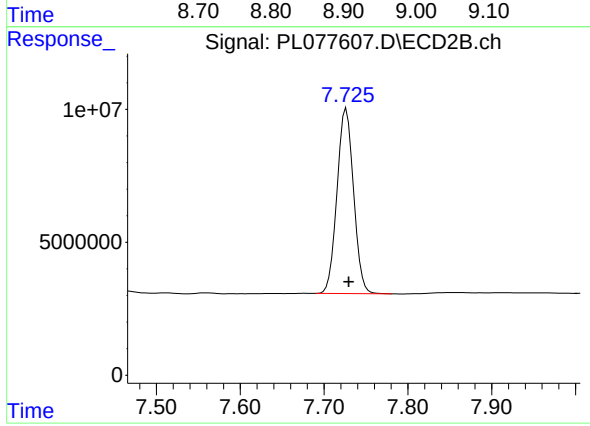

#28 Decachlorobiphenyl

R.T.: 7.726 min
Delta R.T.: -0.003 min
Response: 95590176
Conc: 48.47 ng/ml