

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090824\
 Data File : PL091562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2024 16:45
 Operator : AR\AJ
 Sample : P3857-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-D1-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/09/2024
 Supervised By :Ankita Jodhani 09/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 09:26:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.783	30910130	33095385	14.396m	16.955
2) SA Decachlor...	9.054	7.921	21502796	25946548	14.104	13.699

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090824\
Data File : PL091562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2024 16:45
Operator : AR\AJ
Sample : P3857-07
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-D1-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/09/2024
Supervised By : Ankita Jodhani 09/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 09:26:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

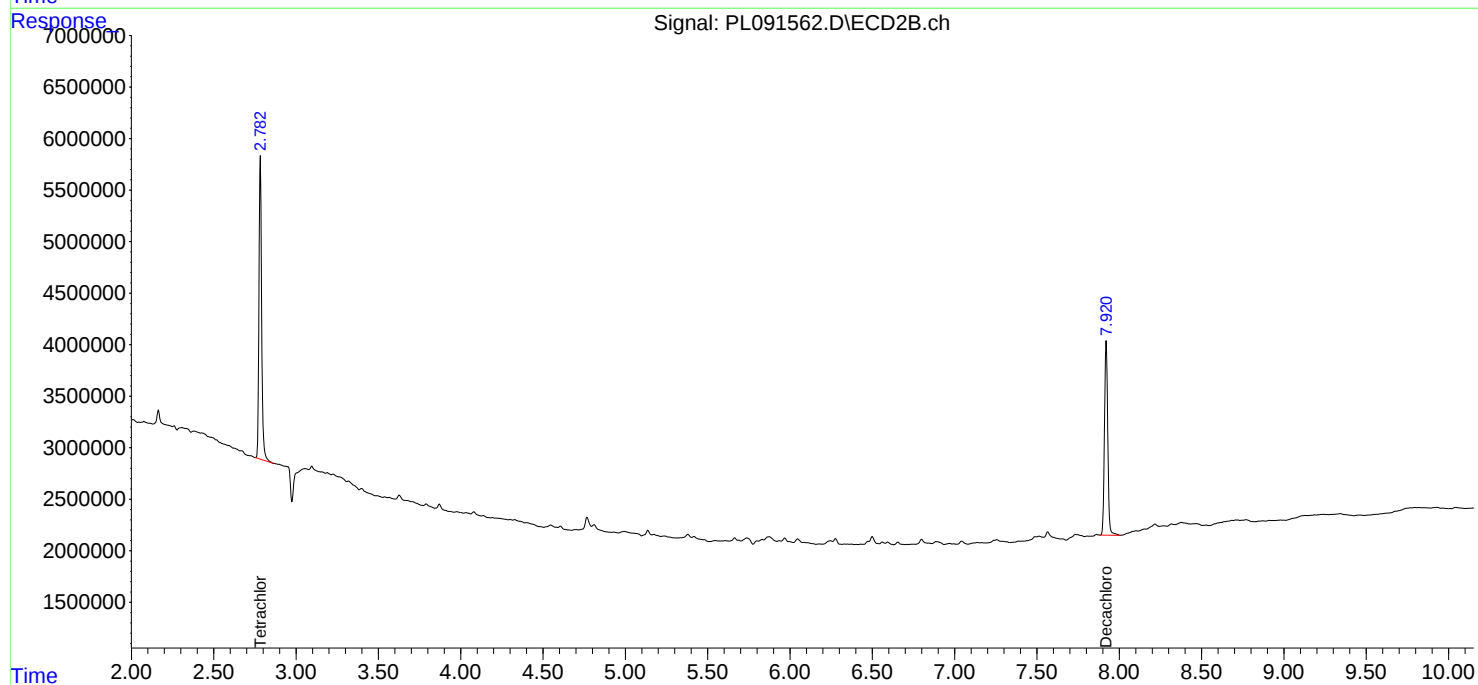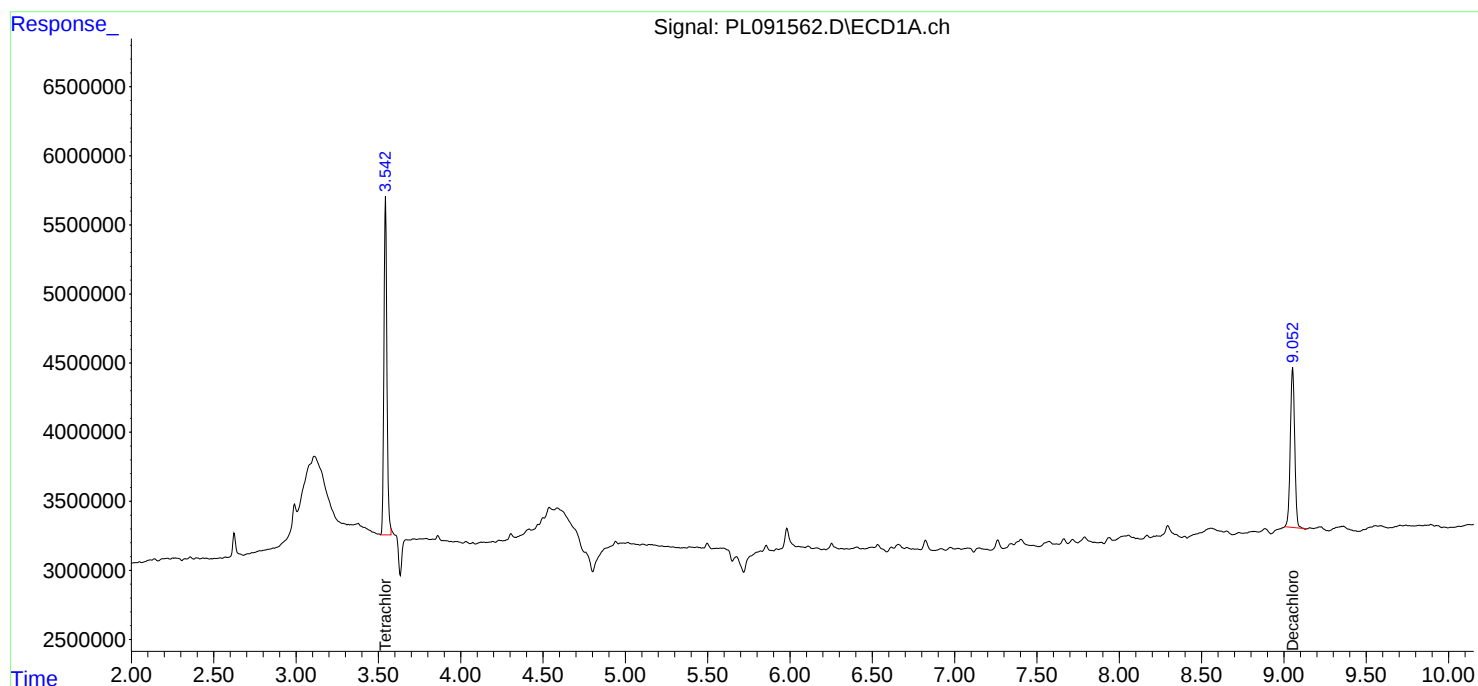

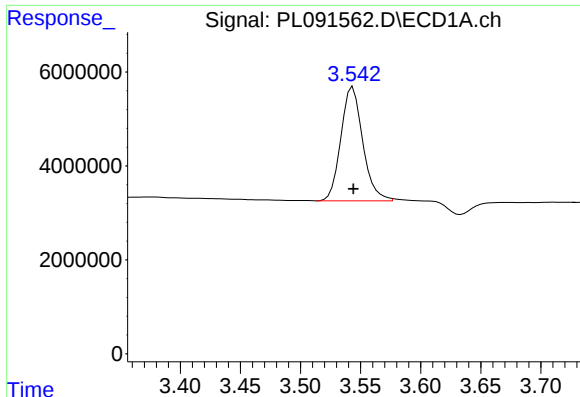


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 30910130
Conc: 14.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-D1-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/09/2024
Supervised By :Ankita Jodhani 09/09/2024

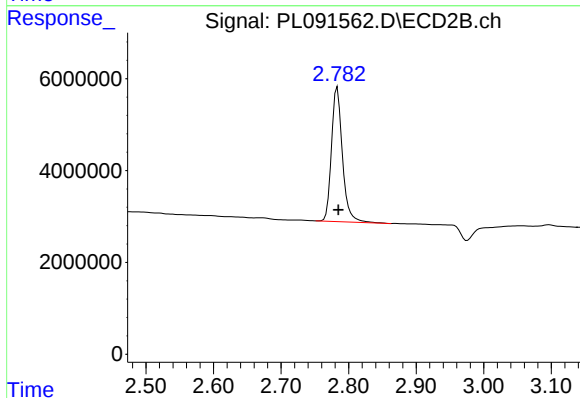


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: -0.002 min
Response: 33095385
Conc: 16.95 ng/ml

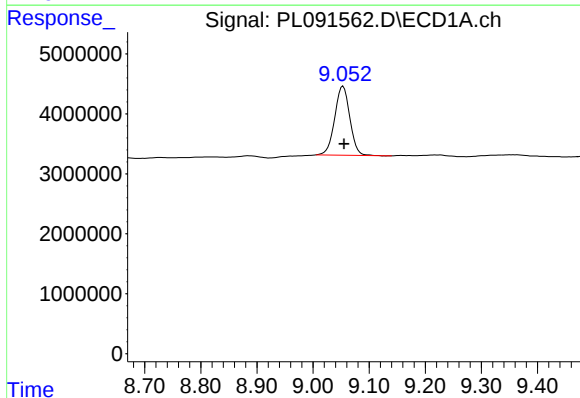

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.002 min
Response: 21502796
Conc: 14.10 ng/ml

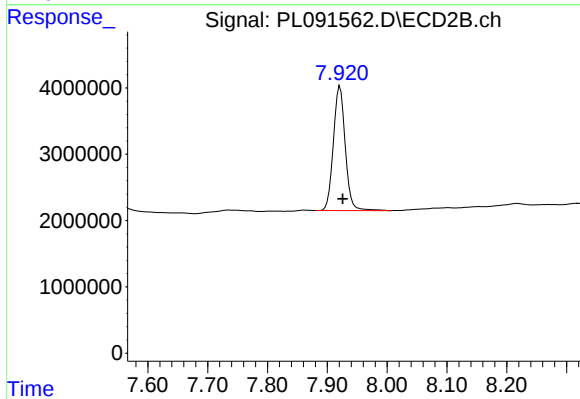

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.005 min
Response: 25946548
Conc: 13.70 ng/ml