

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090920\
 Data File : PL061330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 13:29
 Operator : DD\AJ
 Sample : L3930-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 16:50:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.007	38267125	66944593	22.188	21.764
28)	SA Decachlor...	8.209	9.091	28698031	41100489	17.202	17.382
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	8241489	N.D.	1.785 #
9)	A Endosulfan I	5.529f	0.000	3409407	0	1.982	N.D. #
12)	B 4,4'-DDE	5.620	6.351	128.0E6	230.8E6	75.298	71.995
14)	MA Endrin	6.010	6.748f	12274868	9578726	7.304	3.426 #
15)	B Endosulfa...	0.000	6.940	0	4147706	N.D.	1.404 #
17)	MA 4,4'-DDT	6.375	7.142	86075361	149.4E6	62.688	59.681
18)	B Endrin al...	6.432f	0.000	3167238	0	2.152	N.D. #
22)	Mirex	7.357f	0.000	5881654	0	3.934	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090920\
Data File : PL061330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 13:29
Operator : DD\AJ
Sample : L3930-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 16:50:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

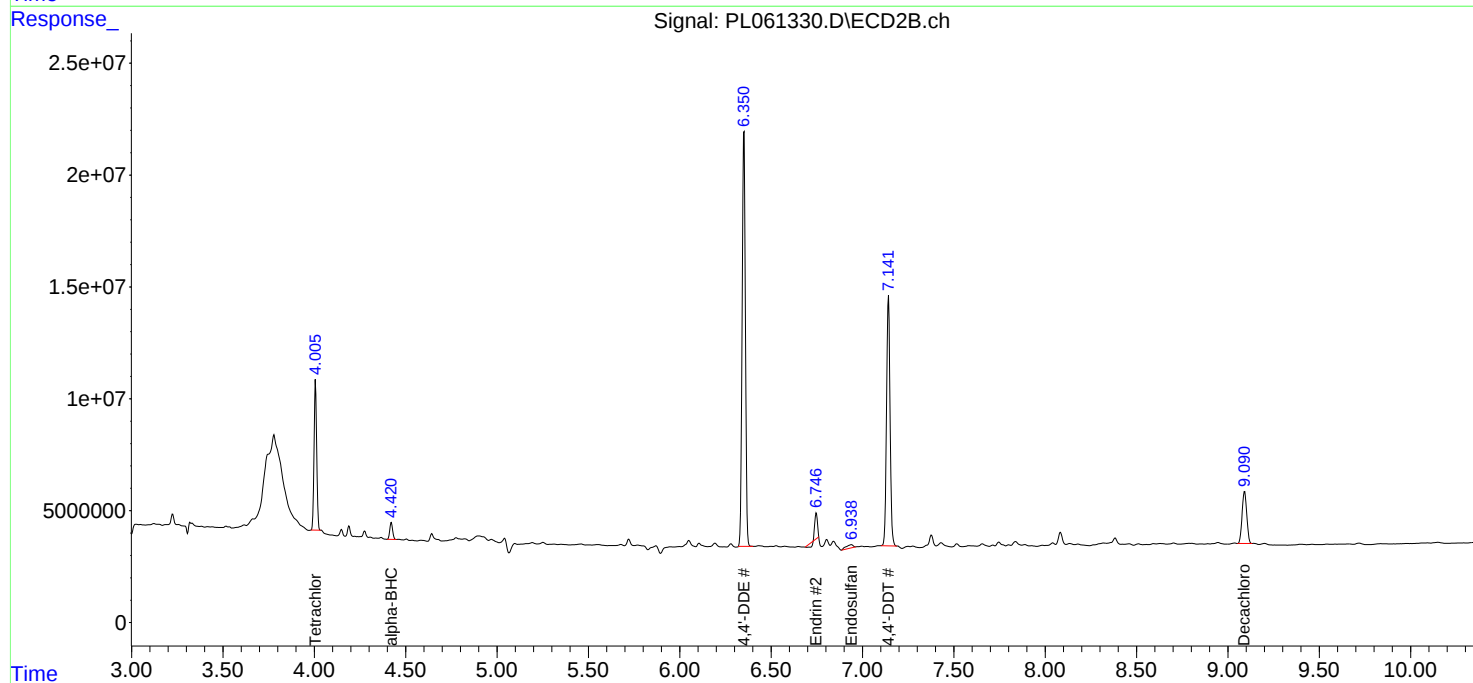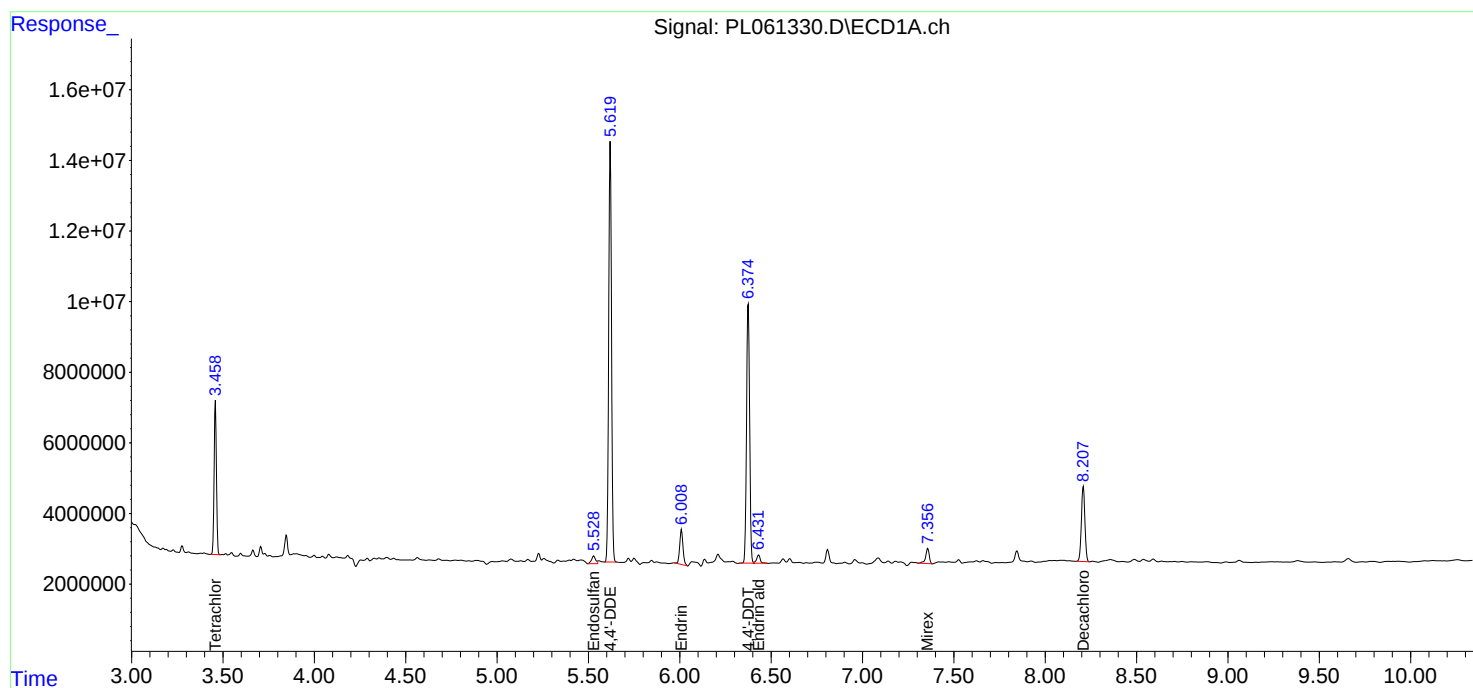


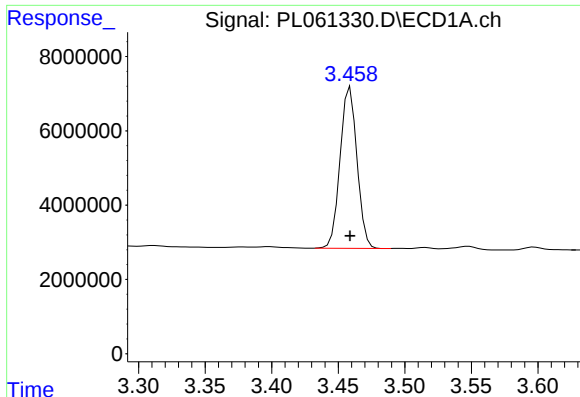

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 38267125
Conc: 22.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

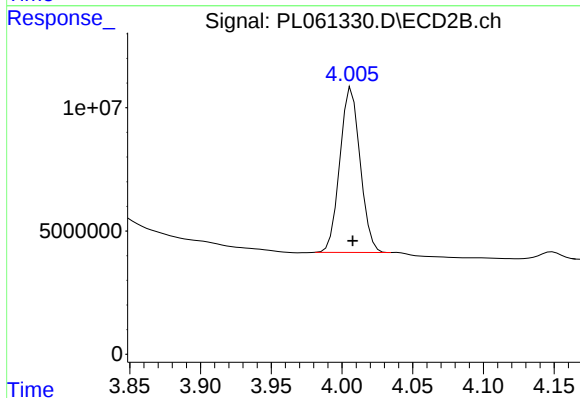


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 66944593
Conc: 21.76 ng/ml

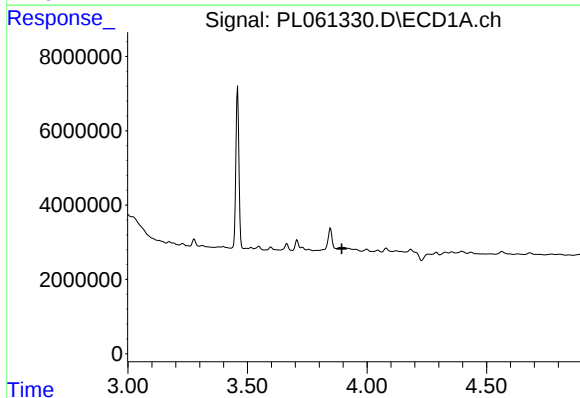


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.895 min
Response: 0
Conc: N.D.

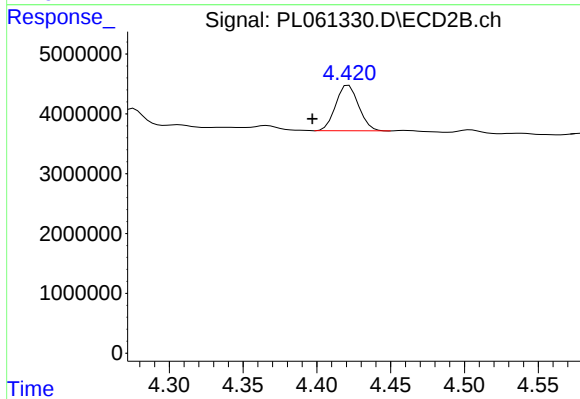

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.025 min
Response: 8241489
Conc: 1.78 ng/ml

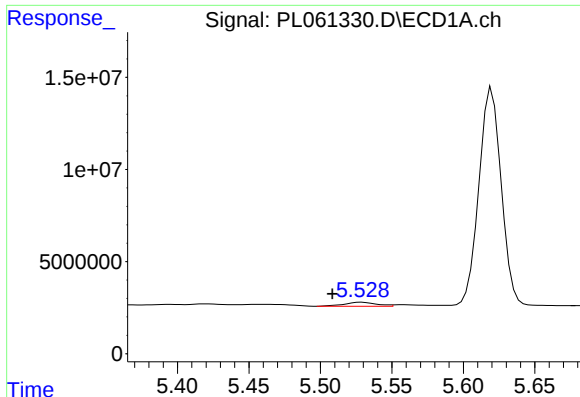

#9 Endosulfan I


R.T.: 5.529 min
Delta R.T.: 0.021 min
Response: 3409407
Conc: 1.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

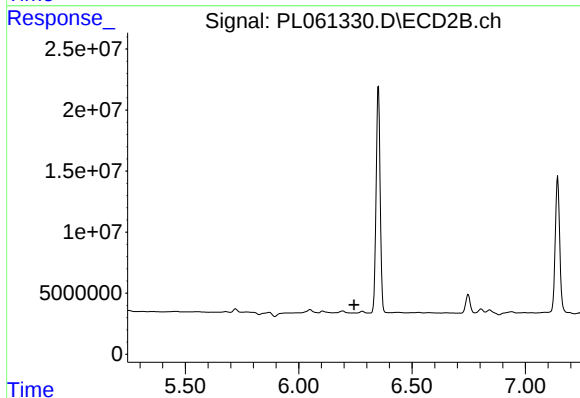


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

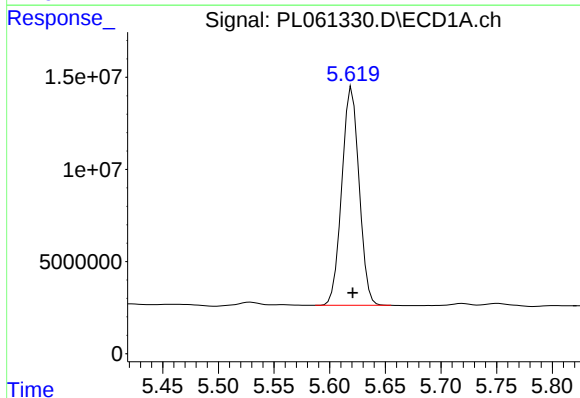


#12 4,4'-DDE

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 128038184
Conc: 75.30 ng/ml

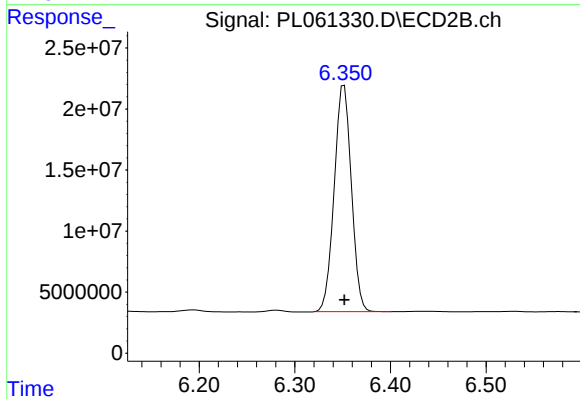

#12 4,4'-DDE


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 230773772
Conc: 71.99 ng/ml

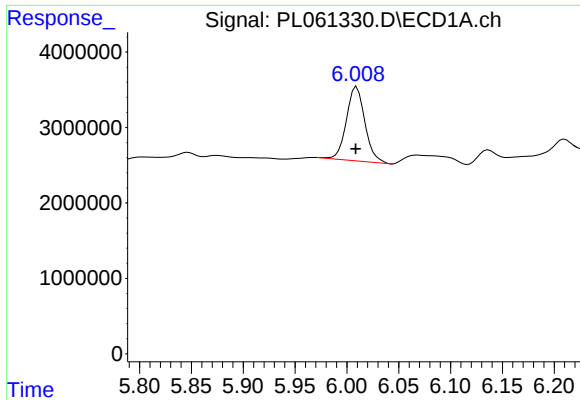

#14 Endrin


R.T.: 6.010 min
Delta R.T.: 0.001 min
Response: 12274868
Conc: 7.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

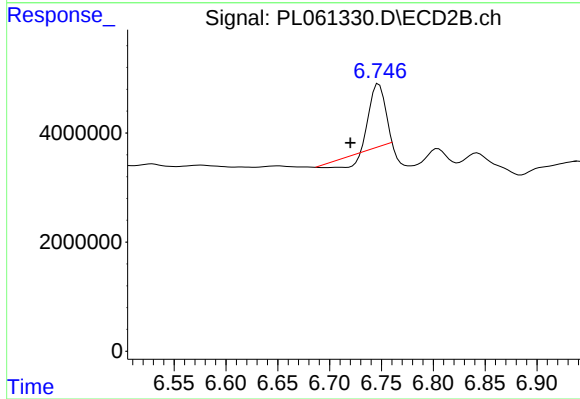


#14 Endrin

R.T.: 6.748 min
Delta R.T.: 0.028 min
Response: 9578726
Conc: 3.43 ng/ml

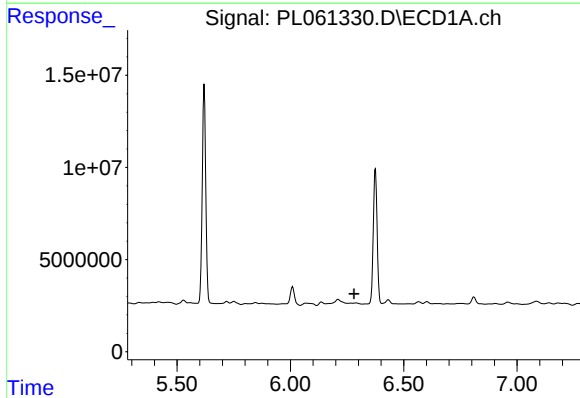


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

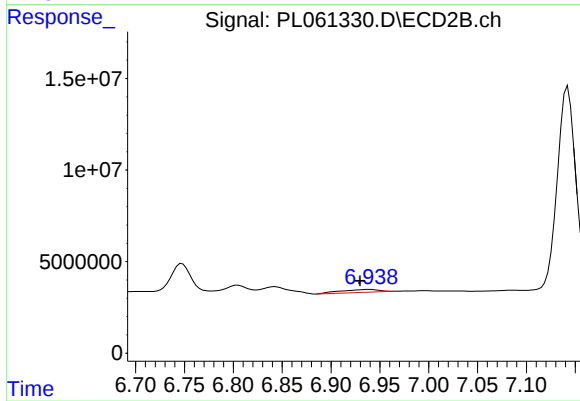

#15 Endosulfan II


R.T.: 6.940 min
Delta R.T.: 0.010 min
Response: 4147706
Conc: 1.40 ng/ml

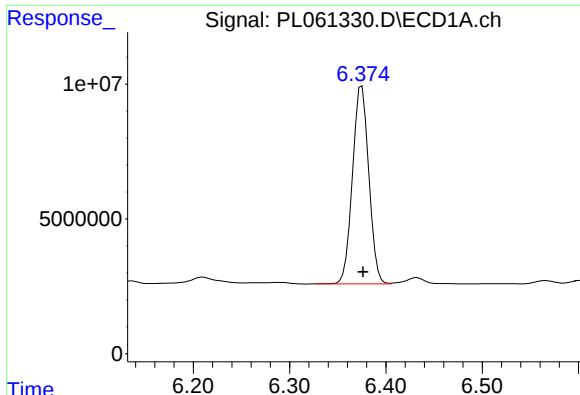

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: -0.001 min
Response: 86075361
Conc: 62.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

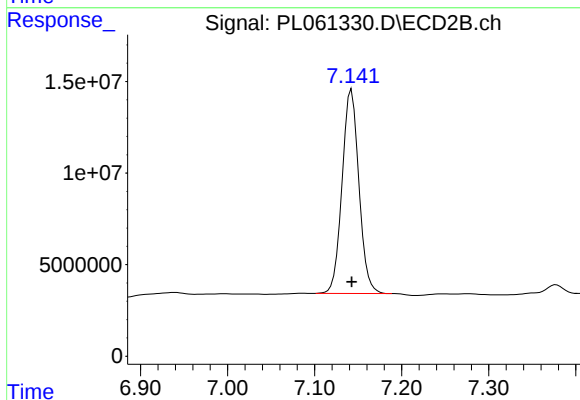


#17 4,4'-DDT

R.T.: 7.142 min
Delta R.T.: 0.000 min
Response: 149388002
Conc: 59.68 ng/ml

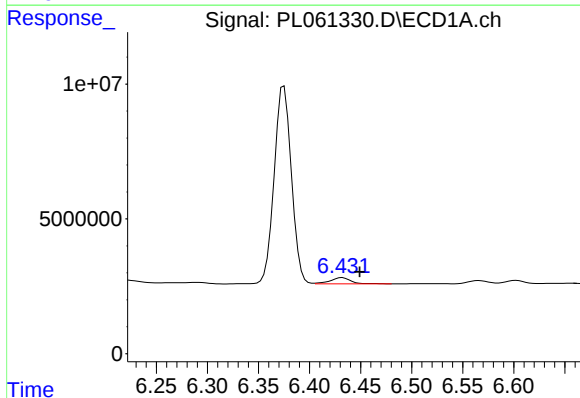


#18 Endrin aldehyde

R.T.: 6.432 min
Delta R.T.: -0.017 min
Response: 3167238
Conc: 2.15 ng/ml

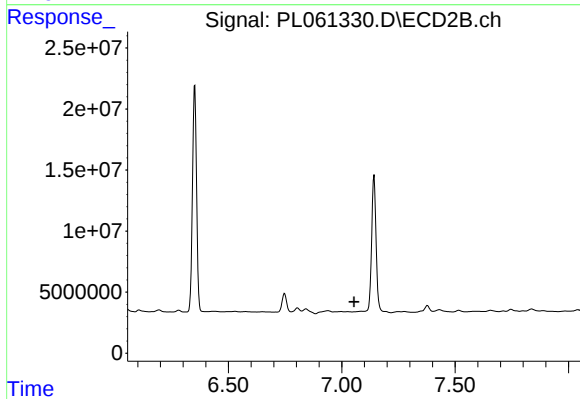

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.055 min
Response: 0
Conc: N.D.

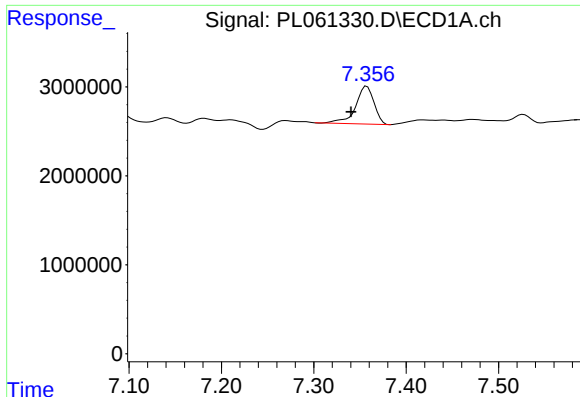

#22 Mirex


R.T.: 7.357 min
Delta R.T.: 0.017 min
Response: 5881654
Conc: 3.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

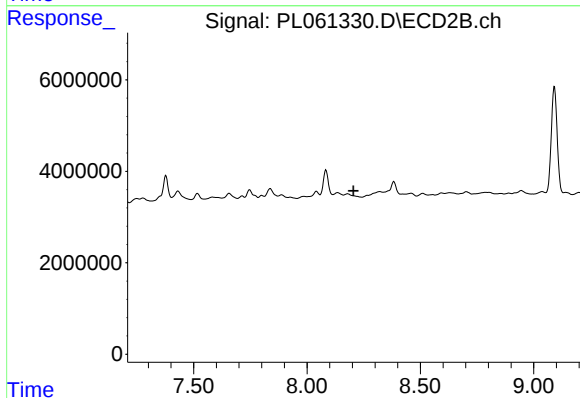


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.205 min
Response: 0
Conc: N.D.

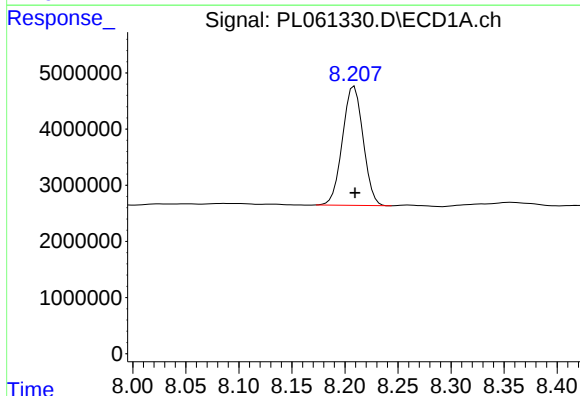

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 28698031
Conc: 17.20 ng/ml

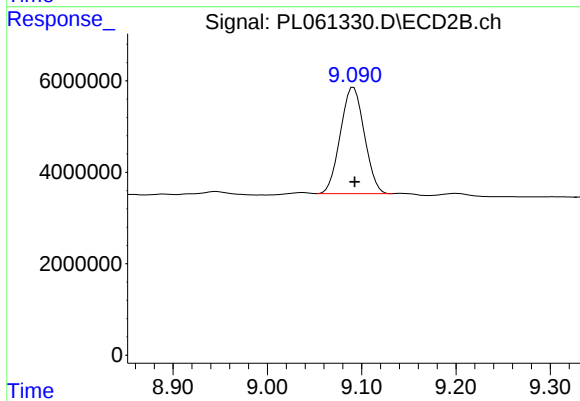

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: -0.001 min
Response: 41100489
Conc: 17.38 ng/ml