

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090920\
 Data File : PL061332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 13:57
 Operator : DD\AJ
 Sample : L3931-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-1-1

Manual Integrations
 APPROVED

Ankita
 9/10/2020 1:10:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 16:50:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	4.007	24548760	41738561	14.234	13.569
28) SA Decachlor...	8.209	9.092	20337359	31926207	12.190	13.502
Target Compounds						
10) B gamma-Chl...	5.396	6.119	784940	1834647	0.424m	0.532m#
11) B alpha-Chl...	5.453	6.194	1313844	3997577	0.709m	1.149 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090820\
Data File : PL061332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 13:57
Operator : DD\AJ
Sample : L3931-01
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
SP-1-1


Manual Integrations
APPROVED

Ankita
9/10/2020 1:10:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 16:50:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

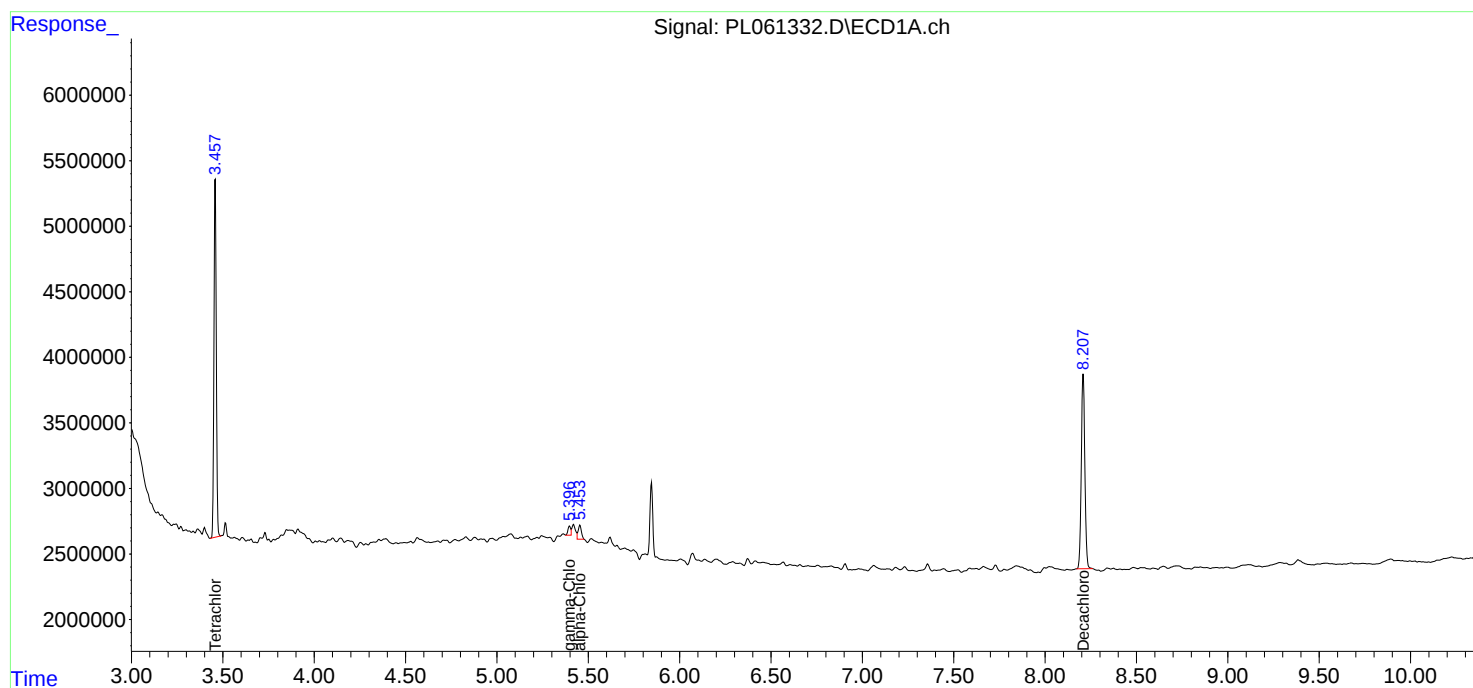

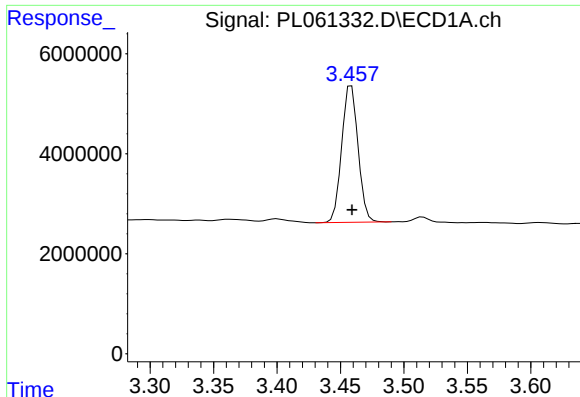


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 24548760
Conc: 14.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1-1


Manual Integrations
APPROVED

Ankita
9/10/2020 1:10:23 PM

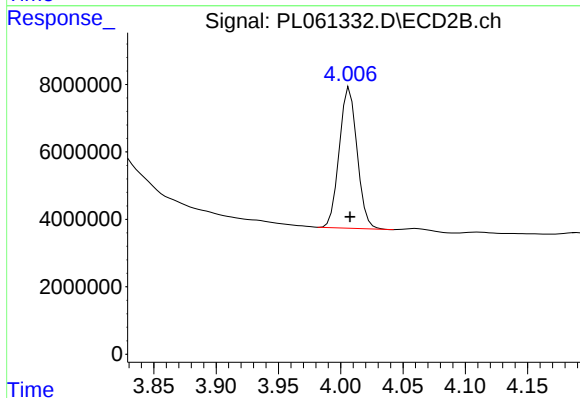


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 41738561
Conc: 13.57 ng/ml

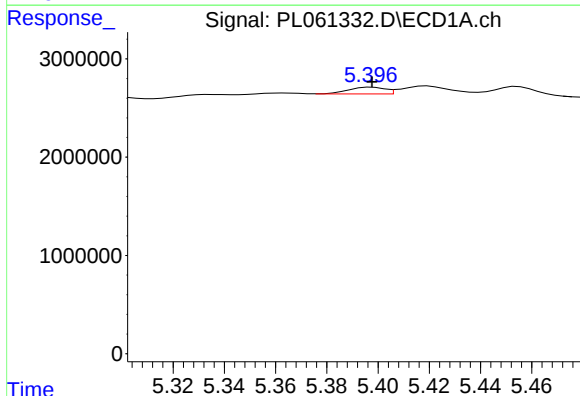


#10 gamma-Chlordane

R.T.: 5.396 min
Delta R.T.: -0.002 min
Response: 784940
Conc: 0.42 ng/ml m

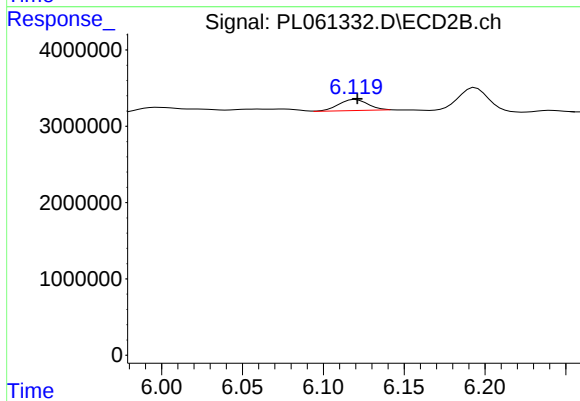

#10 gamma-Chlordane

R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 1834647
Conc: 0.53 ng/ml m

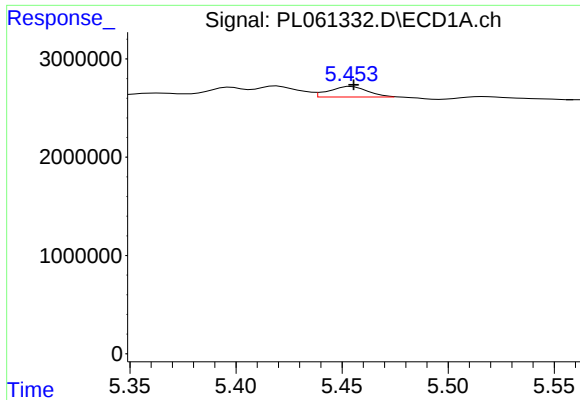


#11 alpha-Chlordane

R.T.: 5.453 min
Delta R.T.: -0.002 min
Response: 1313844
Conc: 0.71 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SP-1-1


Manual Integrations
APPROVED

Ankita
9/10/2020 1:10:23 PM

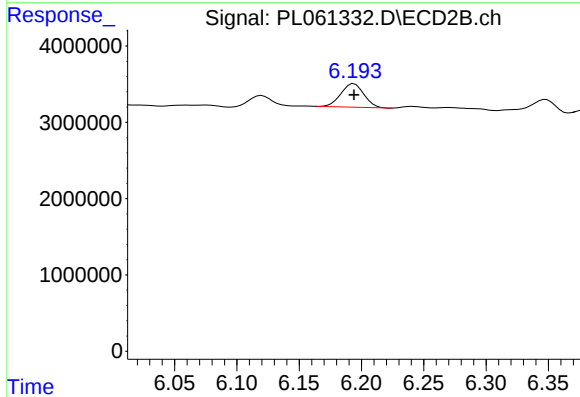


#11 alpha-Chlordane

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 3997577
Conc: 1.15 ng/ml

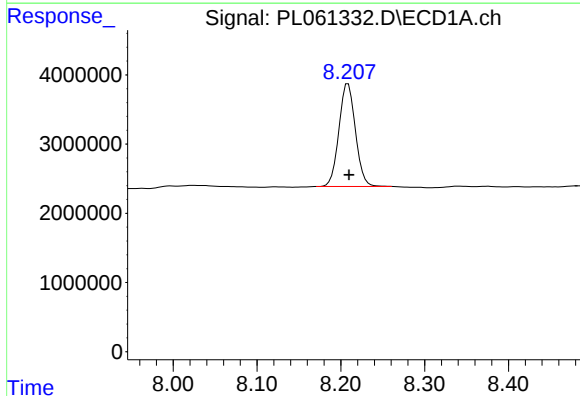

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.001 min
Response: 20337359
Conc: 12.19 ng/ml

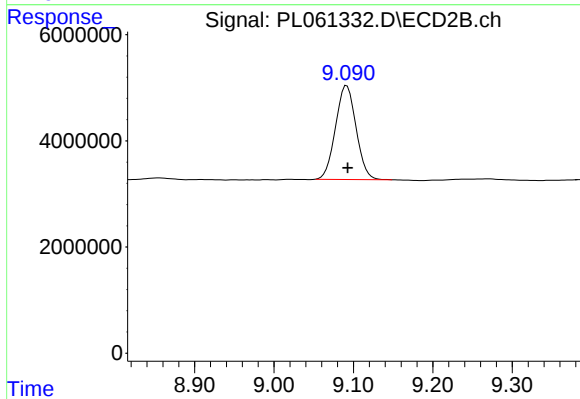

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.001 min
Response: 31926207
Conc: 13.50 ng/ml