

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090920\
 Data File : PL061345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 17:02
 Operator : DD\AJ
 Sample : L3939-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B44-090820-GW

Manual Integrations
 APPROVED

Ankita
 9/10/2020 1:10:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 18:36:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.006	35416236	60464640	20.535	19.657m
28)	SA Decachlor...	8.209	9.094	22069005	31268629	13.228m	13.224

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090920\
Data File : PL061345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 17:02
Operator : DD\AJ
Sample : L3939-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PAV-B44-090820-GW


Manual Integrations
APPROVED

Ankita
9/10/2020 1:10:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 18:36:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

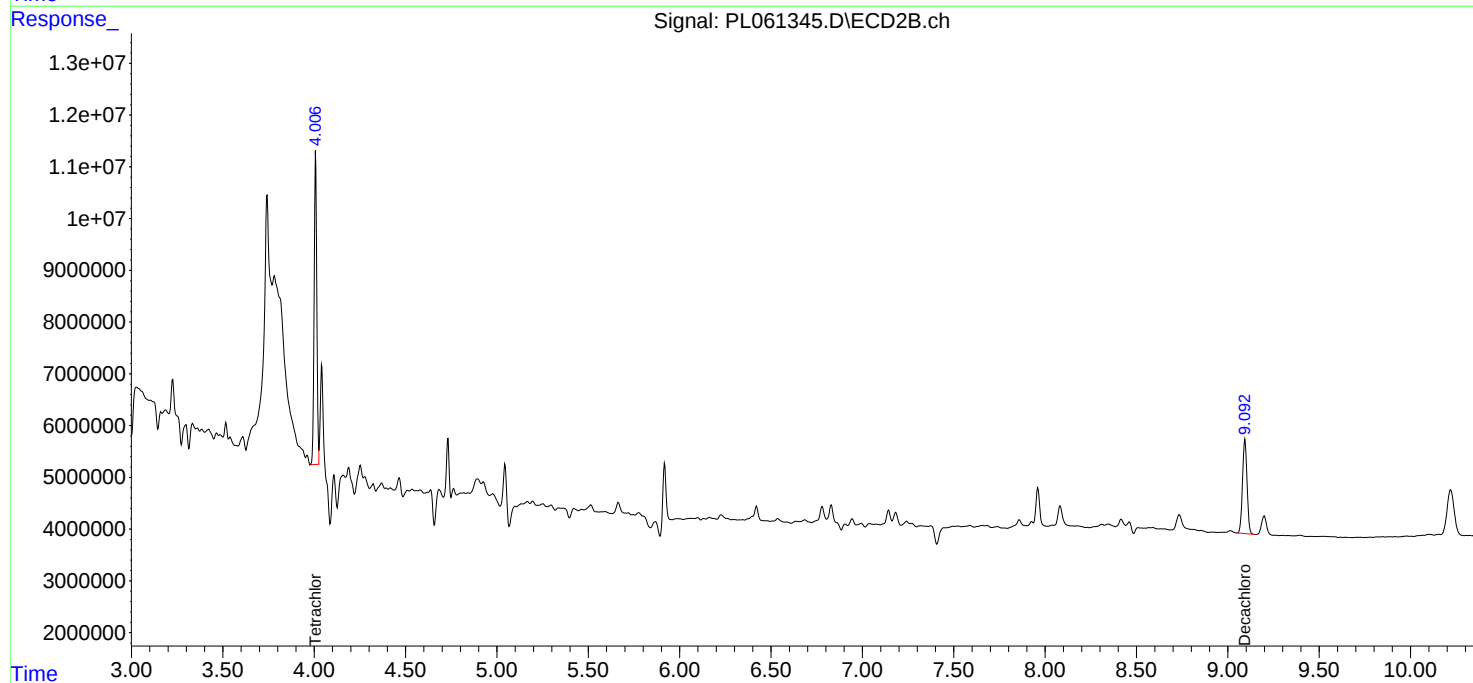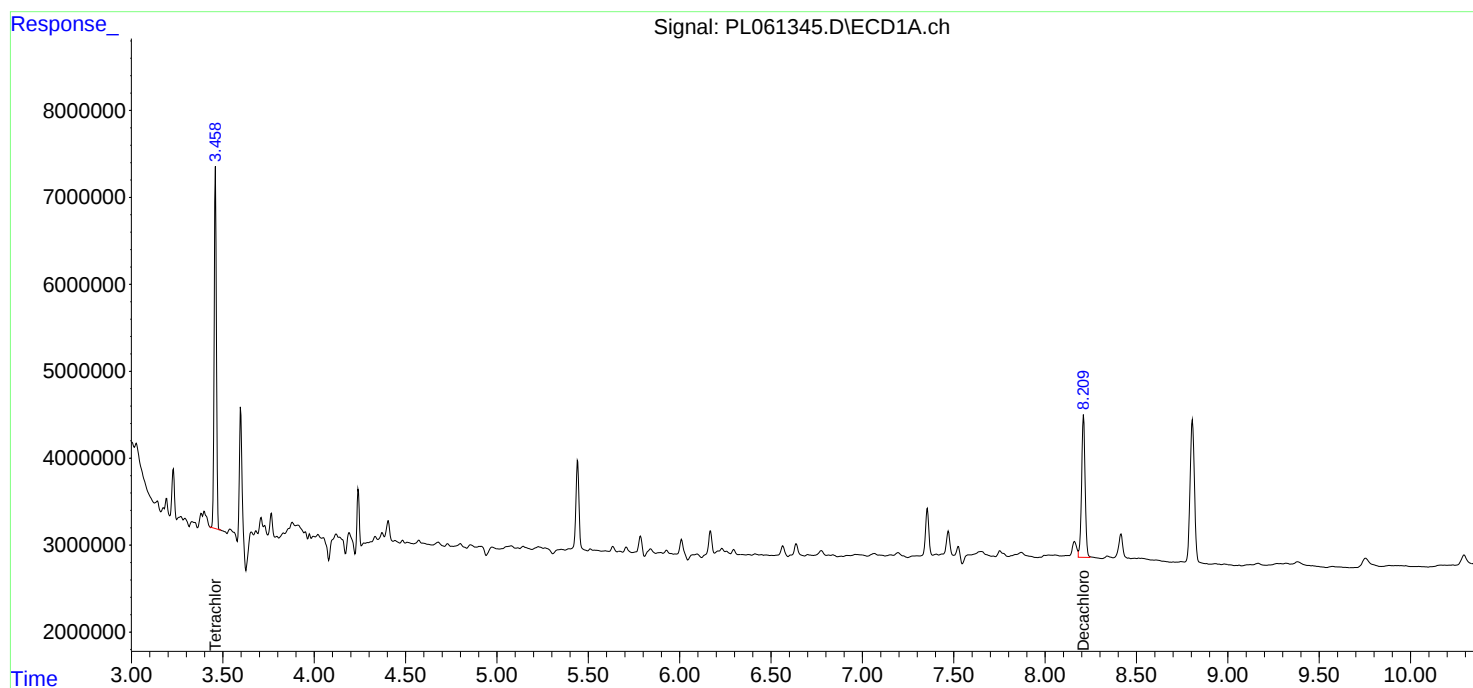

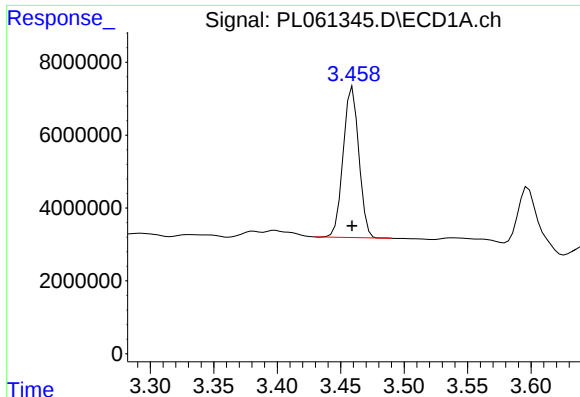


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 35416236
Conc: 20.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B44-090820-GW


Manual Integrations
APPROVED

Ankita
9/10/2020 1:10:30 PM

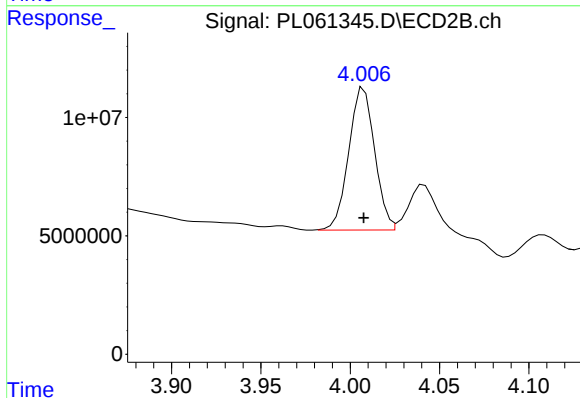


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: -0.001 min
Response: 60464640
Conc: 19.66 ng/ml m

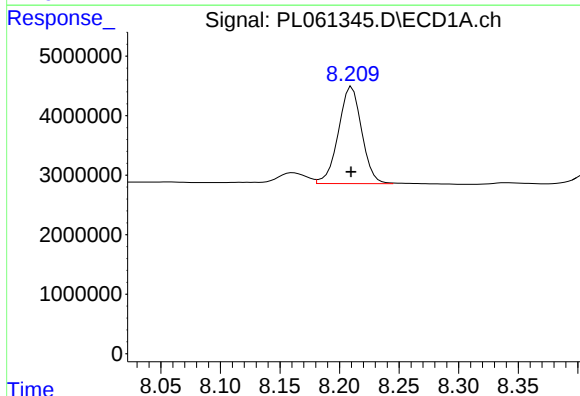

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 22069005
Conc: 13.23 ng/ml m

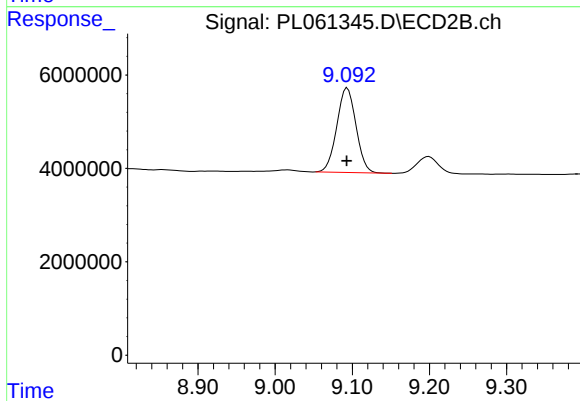

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 31268629
Conc: 13.22 ng/ml