

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090921\
 Data File : PL069772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2021 10:16
 Operator : AR\AJ
 Sample : M3263-02
 Misc : PEST MDL 1 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT4-2021-08

Manual Integrations
 APPROVED

mohammad
 9/10/2021 10:58:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 07:44:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 08 10:30:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.569	8003599	23951443	18.828	17.602
27)	SA Decachlor...	10.402	11.496	27058615	41222450	35.575	35.182
Target Compounds							
2)	A alpha-BHC	5.338	6.149	1092593	2021546	1.872	1.104 #
3)	MA gamma-BHC...	5.763	6.546	704599	1795273	1.212	1.026
4)	MA Heptachlor	6.173	7.196	739928	1832271	1.099	1.053
5)	MB Aldrin	6.498	7.567	719572	1668536	1.181	1.036
6)	B beta-BHC	6.141	6.801	358896	1185286	1.157m	1.188
7)	B delta-BHC	6.404	7.068	665467	2297775	1.168	1.289
8)	B Heptachlo...	7.075	8.034	826389	1514477	1.335	1.089
9)	A Endosulfan I	7.478	8.441	793434	1452346	1.284	1.061
10)	B trans-Chl...	7.352	8.304	856232	1819184	1.295	1.245
11)	B cis-Chlor...	7.422	8.385	881168	1630070	1.311	1.138
12)	B 4,4'-DDE	7.636	8.572	671189	1536611	1.145	1.097
13)	MA Dieldrin	7.765	8.730	809385	1624010	1.216	1.107
14)	MA Endrin	8.056	8.968	790219	1302186	1.269	1.064m
15)	B Endosulfa...	8.366	9.203	818950	1565098	1.329	1.277
16)	A 4,4'-DDD	8.220	9.112	593903	1594402	1.109m	1.363
17)	MA 4,4'-DDT	8.482	9.430	720824	1249792	1.162	1.032
18)	B Endrin al...	8.555	9.339	734211	1331695	1.488	1.401
19)	B Endosulfa...	8.785	9.576	971923	1451570	1.553	1.287
20)	A Methoxychlor	9.075	9.916	485980	883708	1.305m	1.407
21)	B Endrin ke...	9.305	10.075	942011	1923200	1.284	1.501

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090921\
Data File : PL069772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2021 10:16
Operator : AR\AJ
Sample : M3263-02
Misc : PEST MDL 1 PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 07:44:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 08 10:30:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

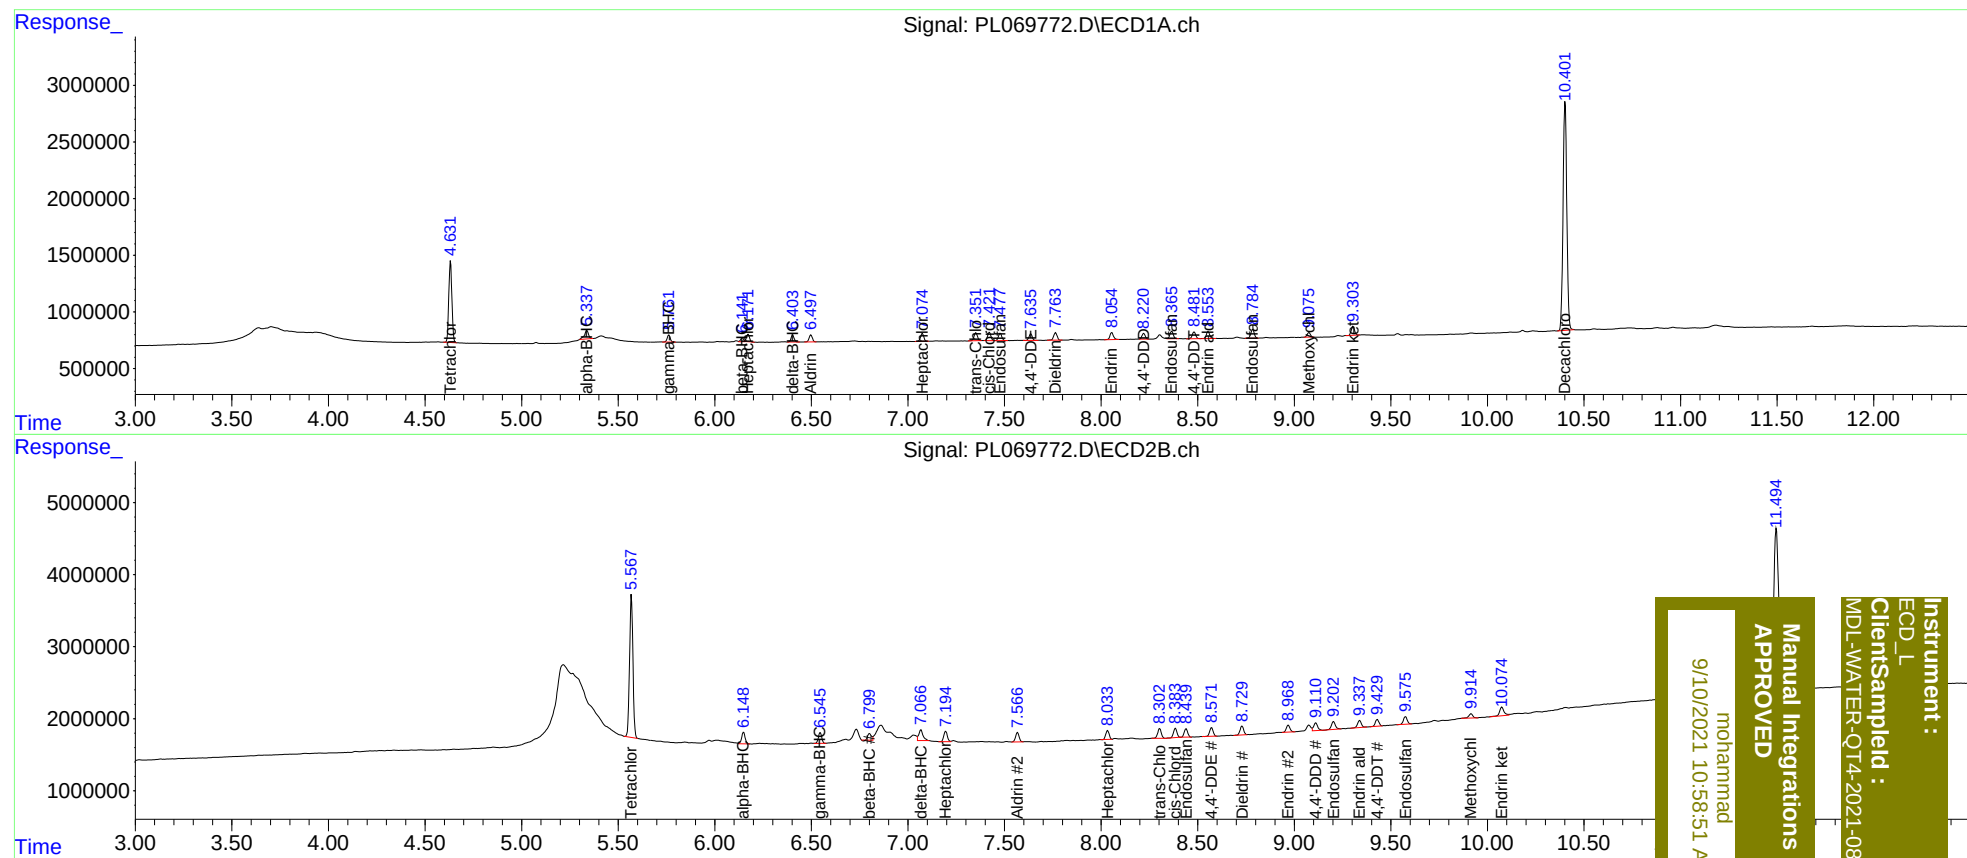

9/10/2021 10:58:51 AM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT4-2021-08