

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090922\
 Data File : PL077633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2022 23:26
 Operator : AR\AJ
 Sample : N4520-03 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 600540642

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/13/2022
 Supervised By : Ankita Jodhani 09/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 03:14:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 14:34:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.416	2.628	3358464	8377762	1.964m	3.166 #
28) SA Decachlor...	8.907	7.725	3591944	5595741	2.395	2.837

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090922\
Data File : PL077633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2022 23:26
Operator : AR\AJ
Sample : N4520-03 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
600540642


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/13/2022
Supervised By : Ankita Jodhani 09/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:14:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 14:34:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

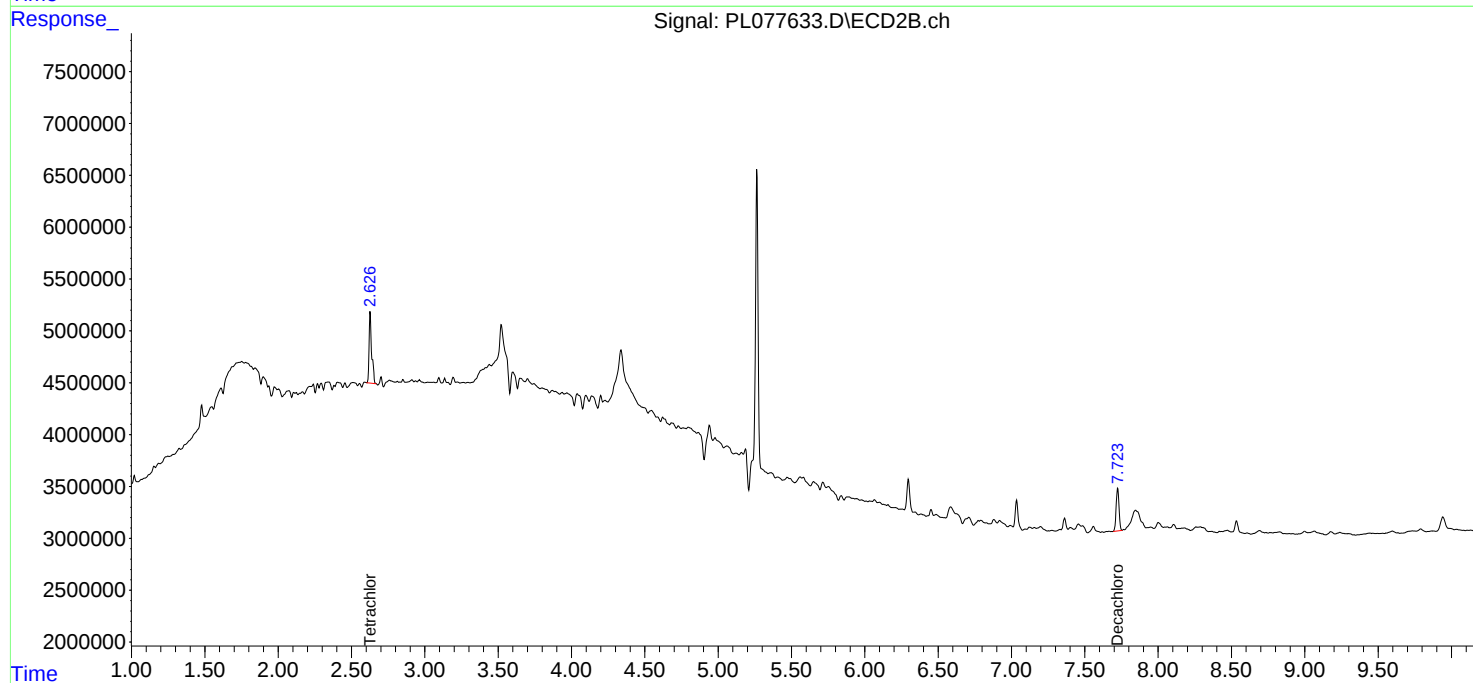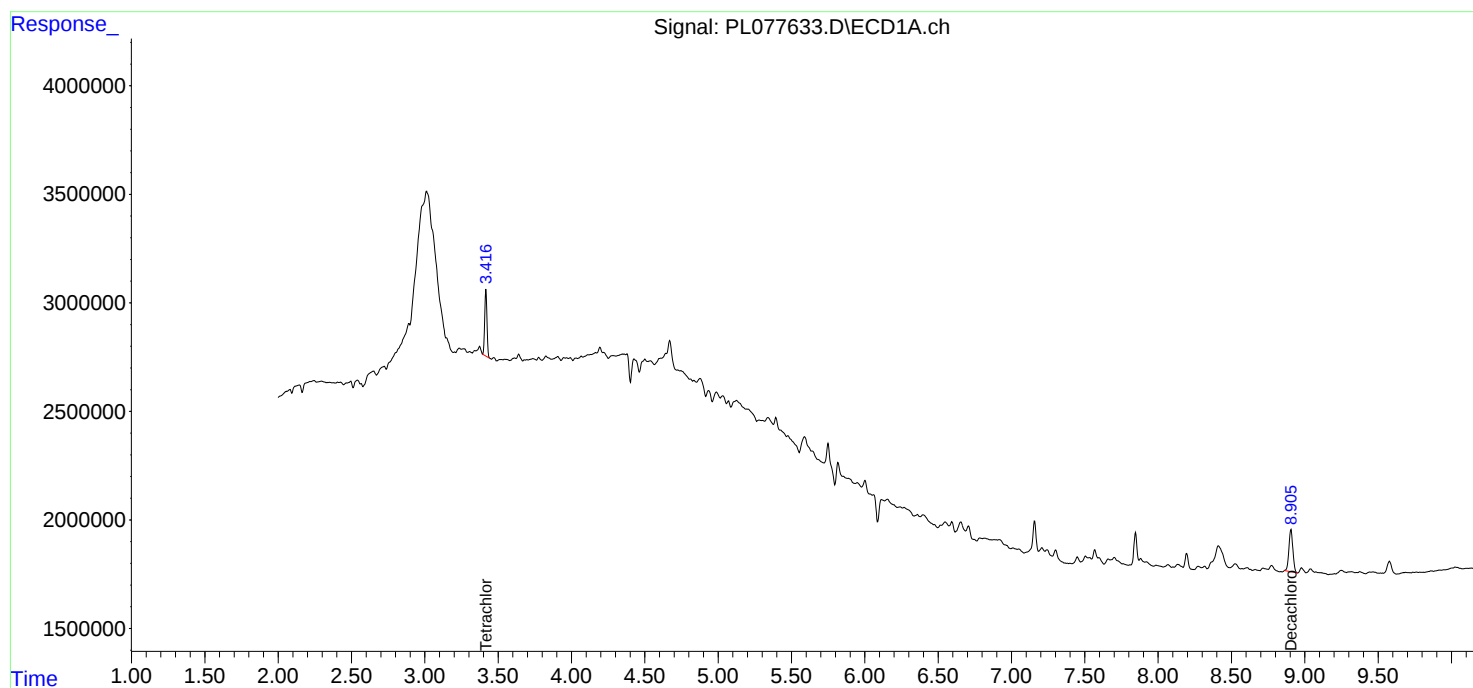

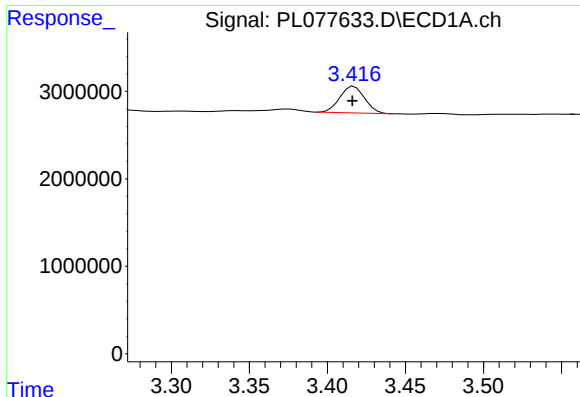


#1 Tetrachloro-m-xylene

R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 3358464
Conc: 1.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
600540642


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/13/2022
Supervised By :Ankita Jodhani 09/13/2022

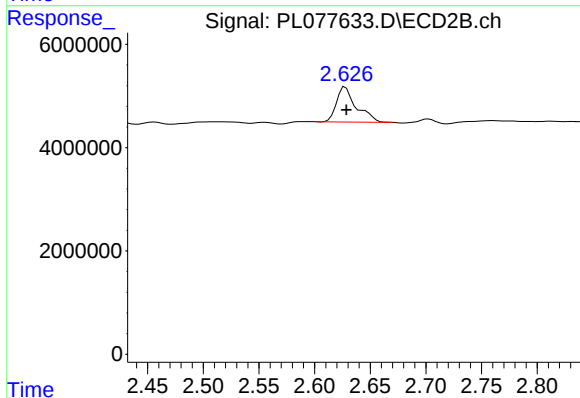


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 8377762
Conc: 3.17 ng/ml

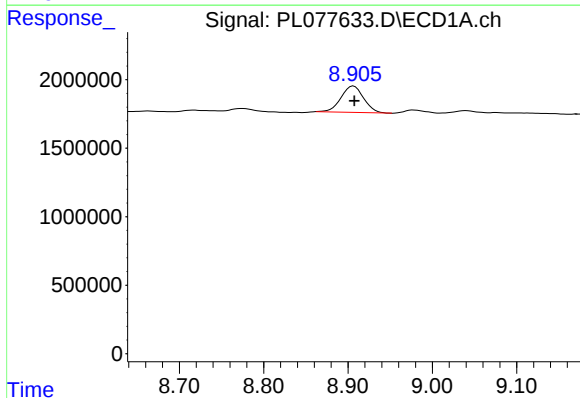

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.001 min
Response: 3591944
Conc: 2.39 ng/ml

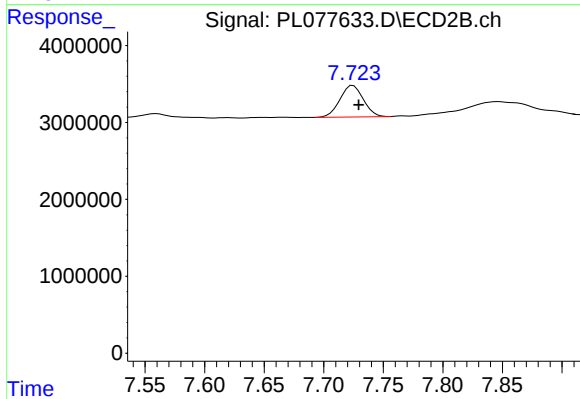

#28 Decachlorobiphenyl

R.T.: 7.725 min
Delta R.T.: -0.005 min
Response: 5595741
Conc: 2.84 ng/ml