

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
 Data File : PL091577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 16:52
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 17:23:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 17:19:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.783	108.3E6	168.0E6	74.566	74.929
28)	SA Decachlor...	9.061	7.925	82899124	133.6E6	73.670	74.214
Target Compounds							
23)	Chlordane-1	4.706	3.782	45211603	49999002	746.016	744.885
24)	Chlordane-2	5.236	4.359	51124678	53816651	732.005	744.369
25)	Chlordane-3	5.946	4.990	179.6E6	171.0E6	740.428	752.942
26)	Chlordane-4	6.027	5.052	215.7E6	152.8E6	741.579	731.167
27)	Chlordane-5	6.876	5.949	41009743	53827664	742.757	745.683



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
Data File : PL091577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 16:52
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 17:23:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 17:19:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

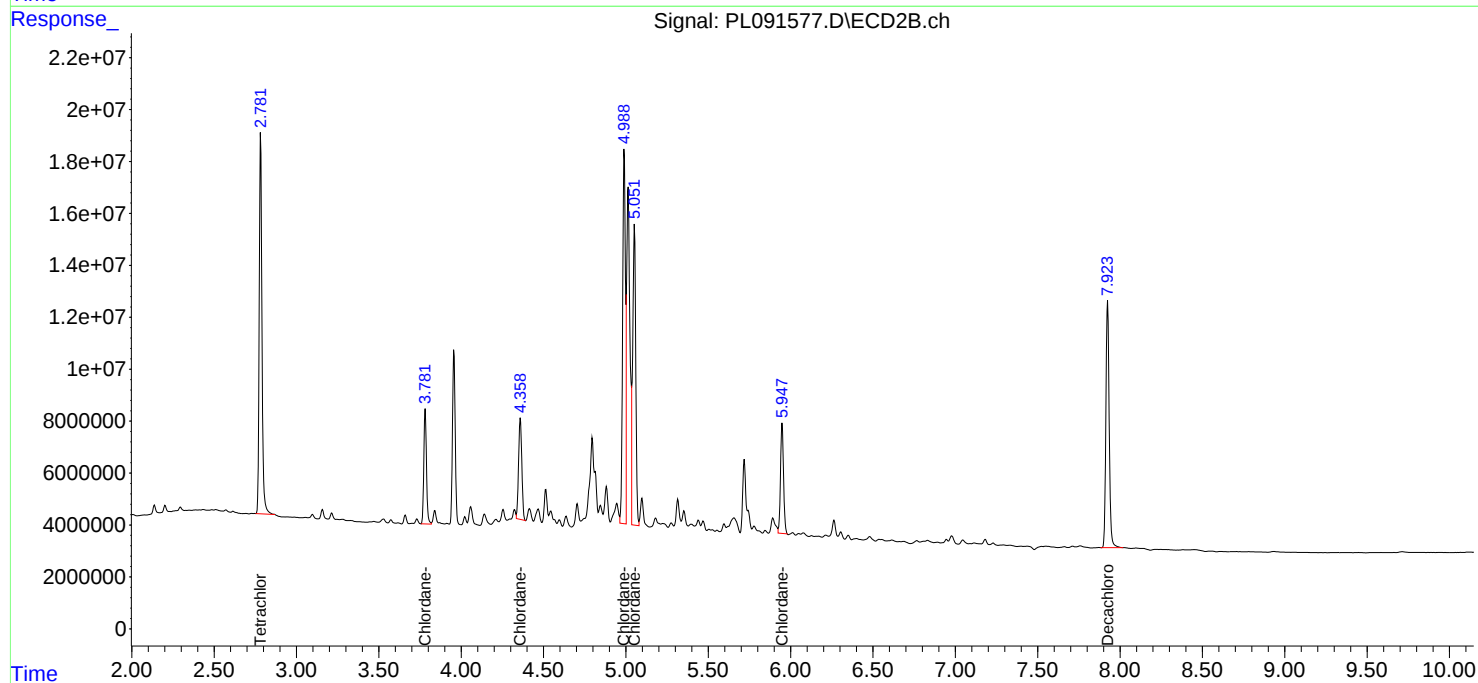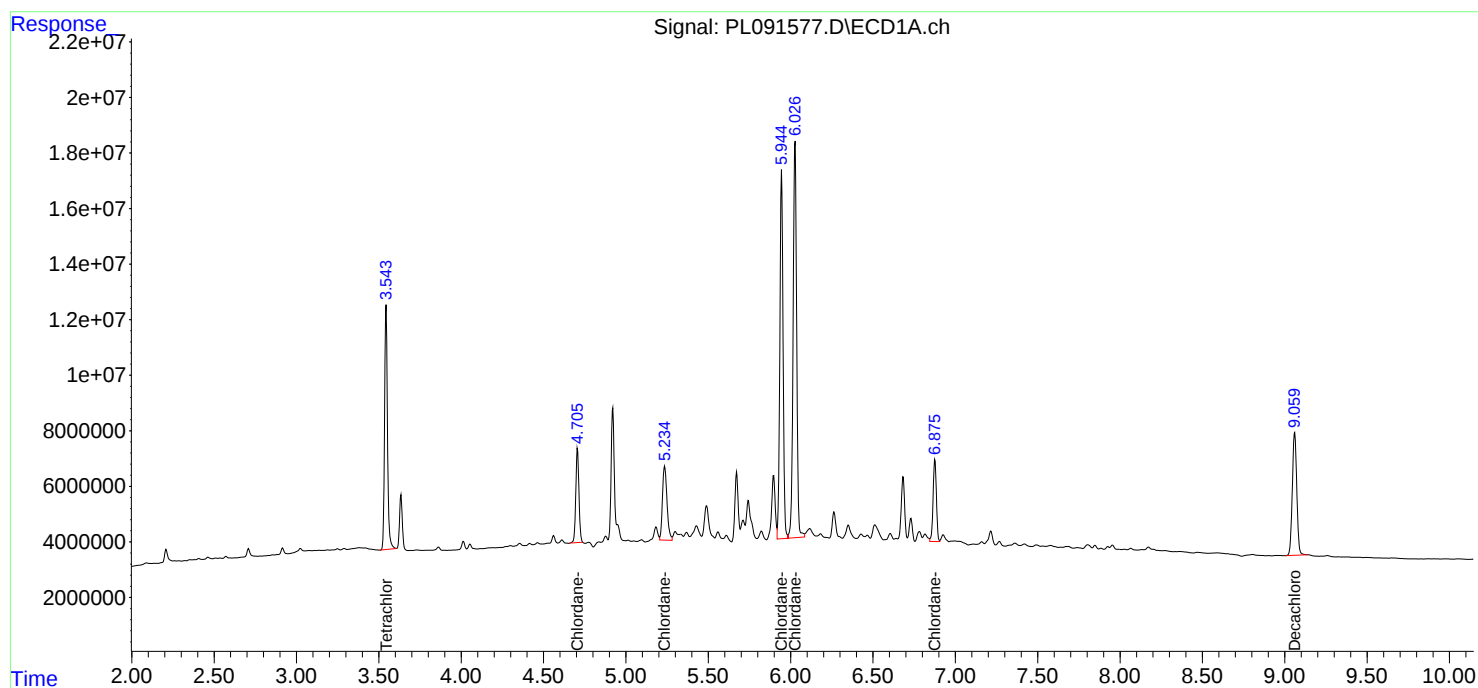


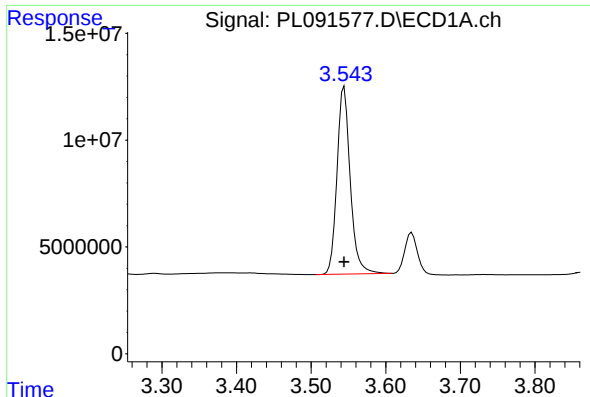

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 108297429
Conc: 74.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

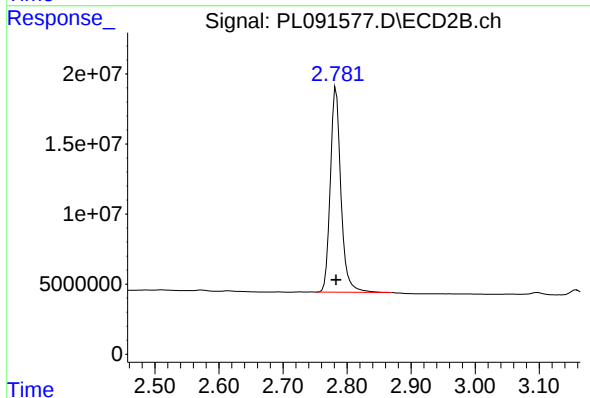


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 167956592
Conc: 74.93 ng/ml

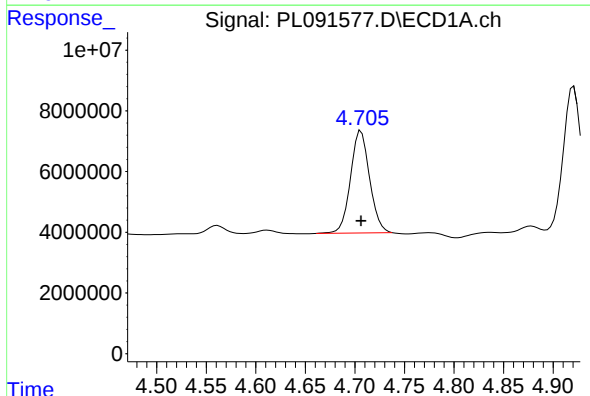


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 45211603
Conc: 746.02 ng/ml

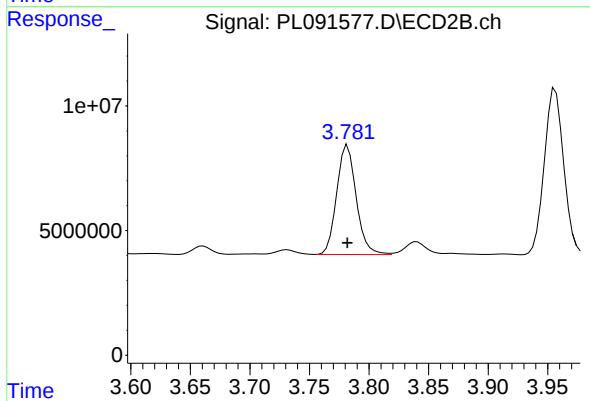

#23 Chlordane-1


R.T.: 3.782 min
Delta R.T.: 0.000 min
Response: 49999002
Conc: 744.89 ng/ml

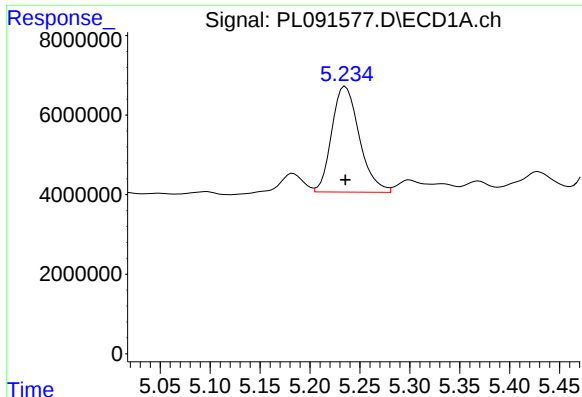

#24 Chlordane-2


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 51124678
Conc: 732.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

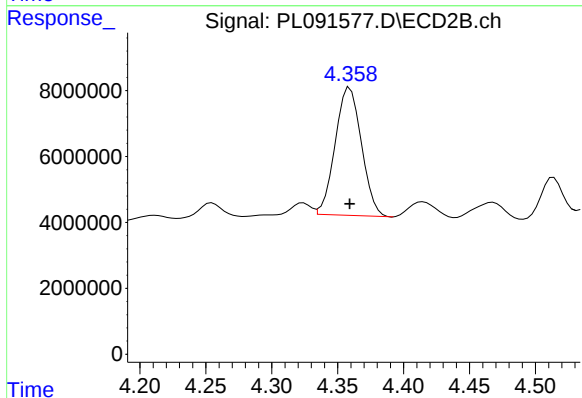


#24 Chlordane-2

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 53816651
Conc: 744.37 ng/ml

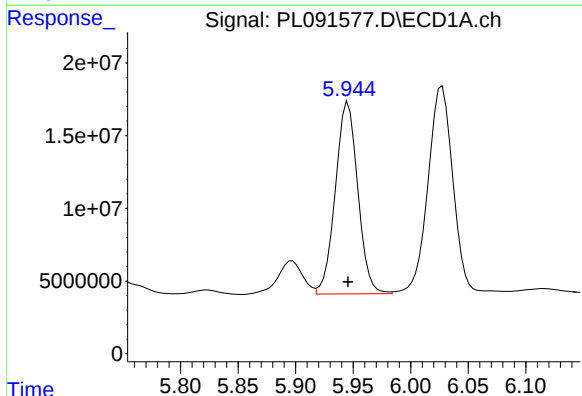


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 179575342
Conc: 740.43 ng/ml

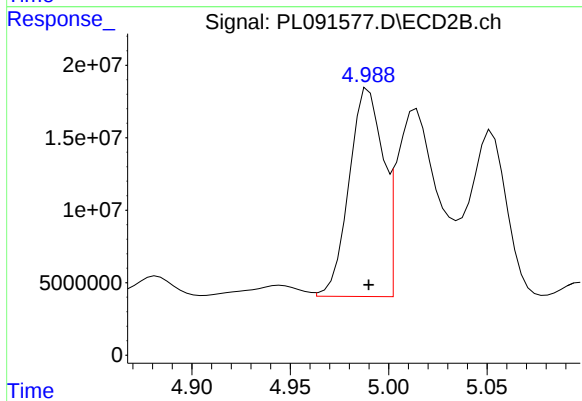

#25 Chlordane-3


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 171003436
Conc: 752.94 ng/ml

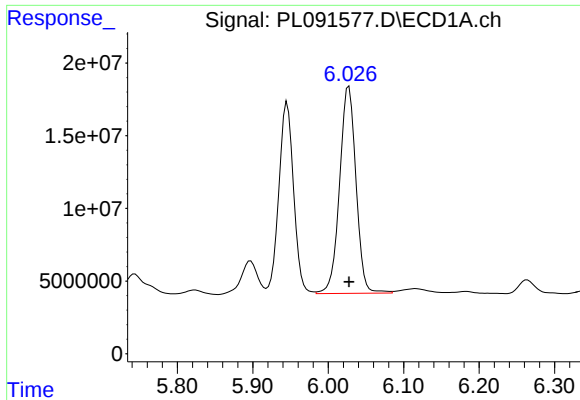

#26 Chlordane-4


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 215654872
Conc: 741.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

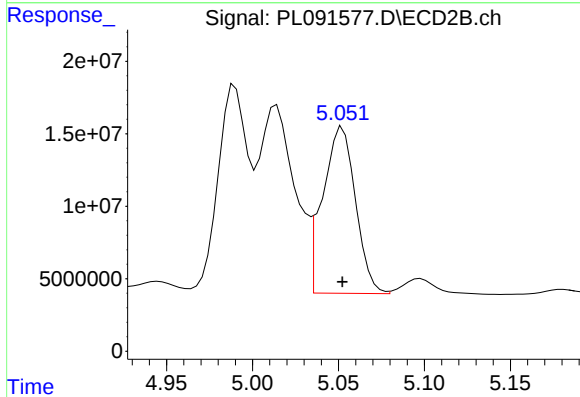


#26 Chlordane-4

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 152827566
Conc: 731.17 ng/ml

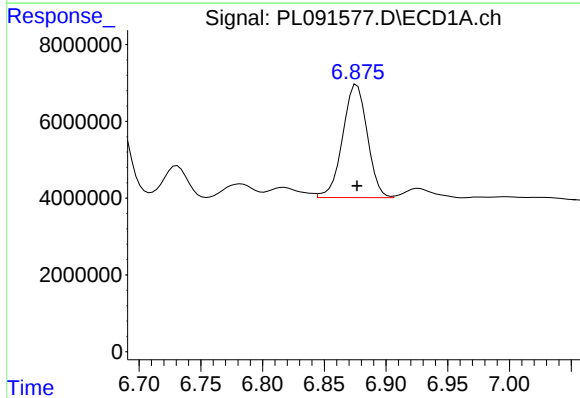


#27 Chlordane-5

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 41009743
Conc: 742.76 ng/ml

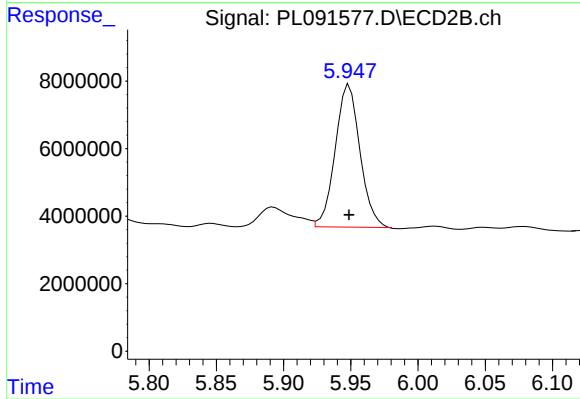

#27 Chlordane-5


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 53827664
Conc: 745.68 ng/ml

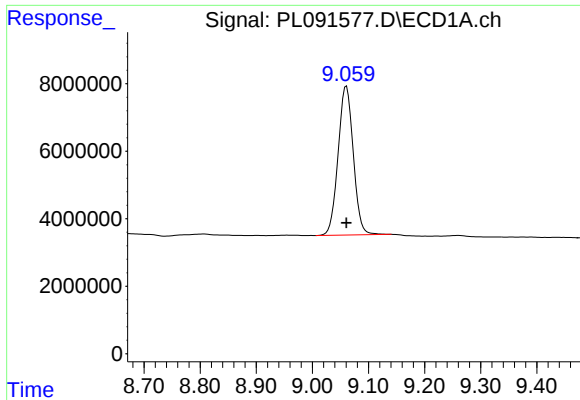

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 82899124
Conc: 73.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

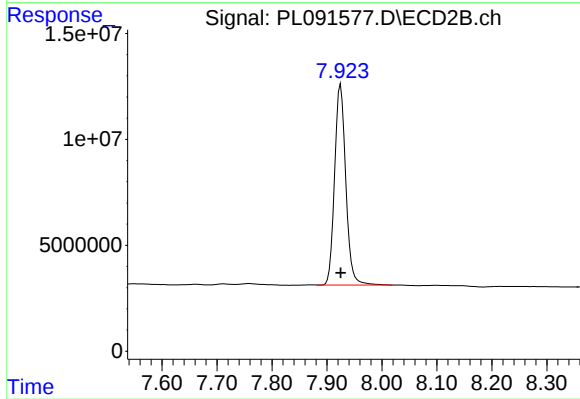

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 133577467
Conc: 74.21 ng/ml