

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
 Data File : PL091578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 17:06
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 17:20:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 17:19:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.783	72968528	111.2E6	50.000	50.000
28) SA Decachlor...	9.060	7.925	58081135	91176732	50.000	50.000
Target Compounds						
23) Chlordane-1	4.706	3.782	30713014	33545288	500.000	500.000
24) Chlordane-2	5.236	4.360	36841024	36440792	500.000	500.000
25) Chlordane-3	5.945	4.990	122.5E6	111.5E6	500.000	500.000
26) Chlordane-4	6.027	5.053	146.6E6	104.3E6	500.000	500.000
27) Chlordane-5	6.876	5.948	28162351	35427383	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
Data File : PL091578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 17:06
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 17:20:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 17:19:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

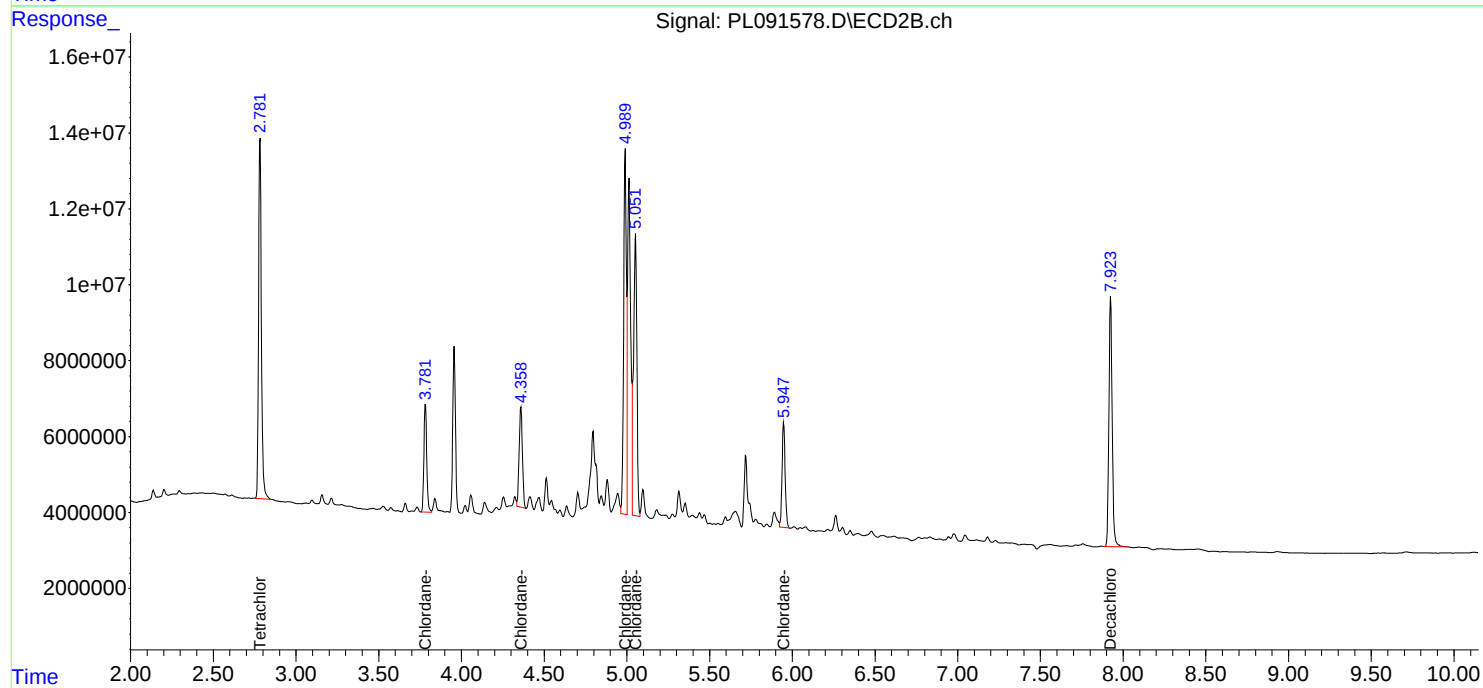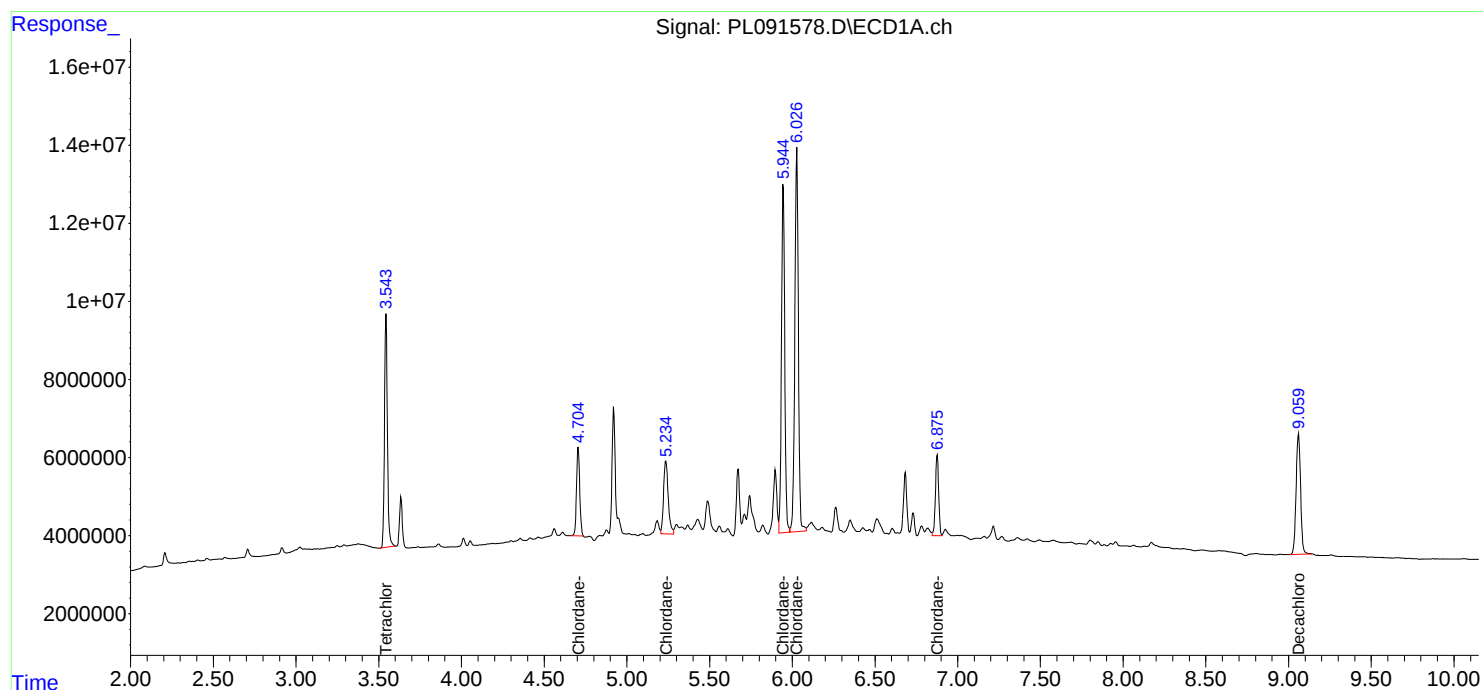


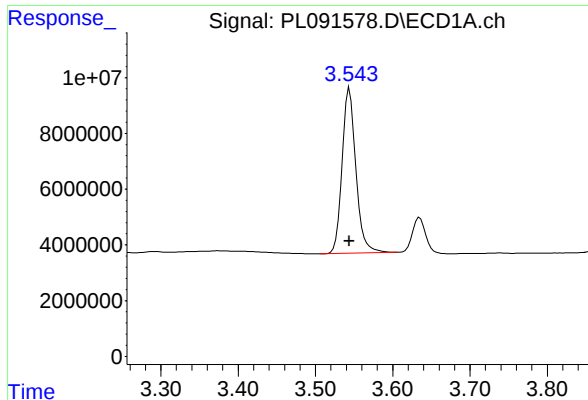

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 72968528
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

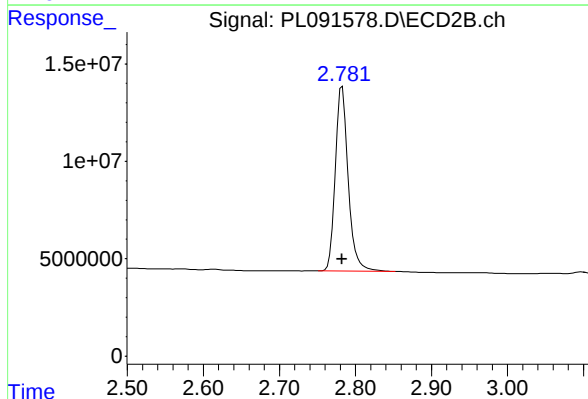


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 111183553
Conc: 50.00 ng/ml

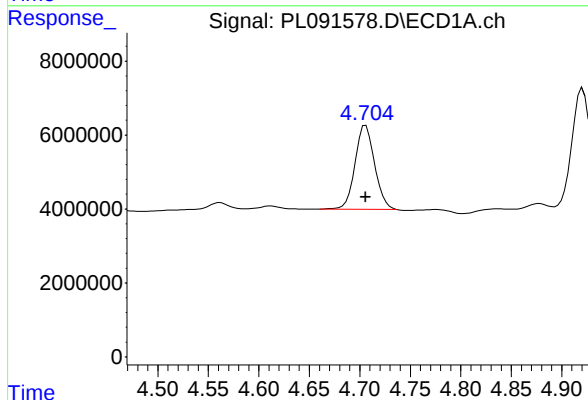


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 30713014
Conc: 500.00 ng/ml

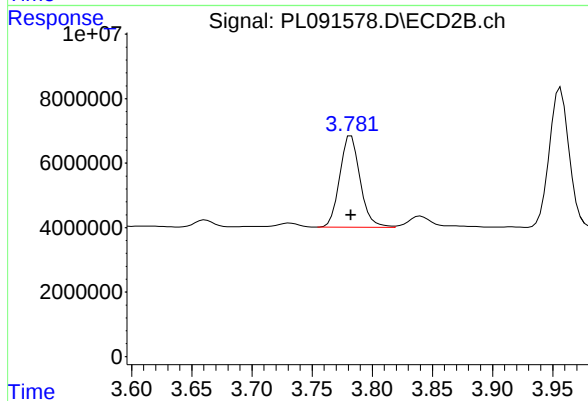

#23 Chlordane-1


R.T.: 3.782 min
Delta R.T.: 0.000 min
Response: 33545288
Conc: 500.00 ng/ml

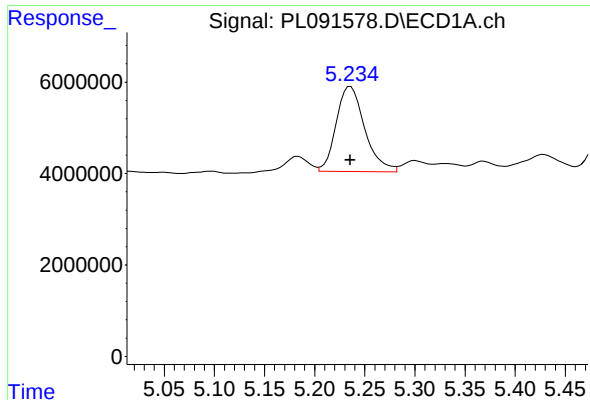

#24 Chlordane-2


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 36841024
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

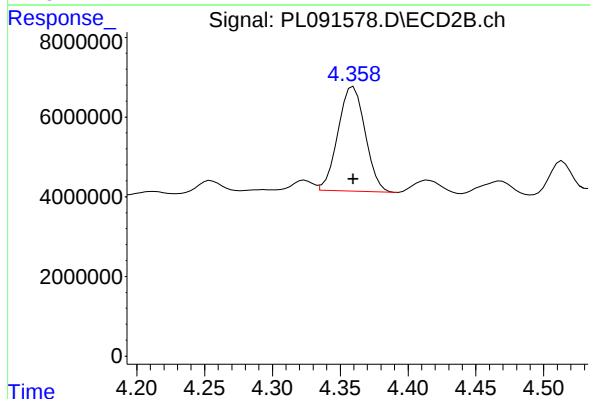


#24 Chlordane-2

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 36440792
Conc: 500.00 ng/ml

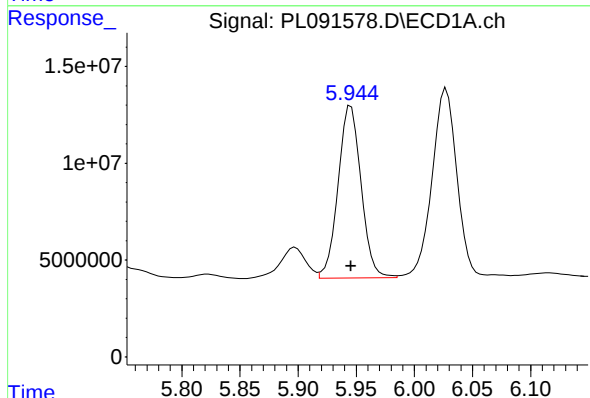


#25 Chlordane-3

R.T.: 5.945 min
Delta R.T.: 0.000 min
Response: 122538160
Conc: 500.00 ng/ml

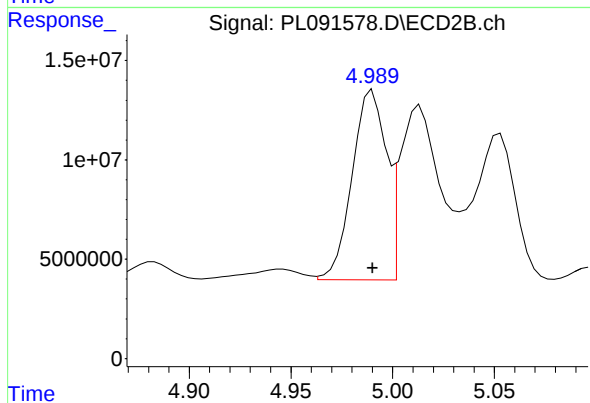

#25 Chlordane-3


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 111507436
Conc: 500.00 ng/ml

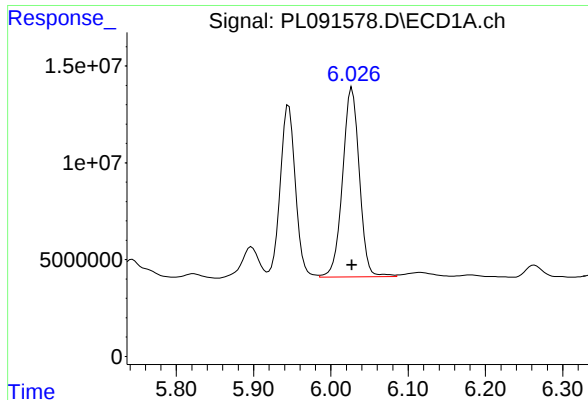

#26 Chlordane-4


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 146612440
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

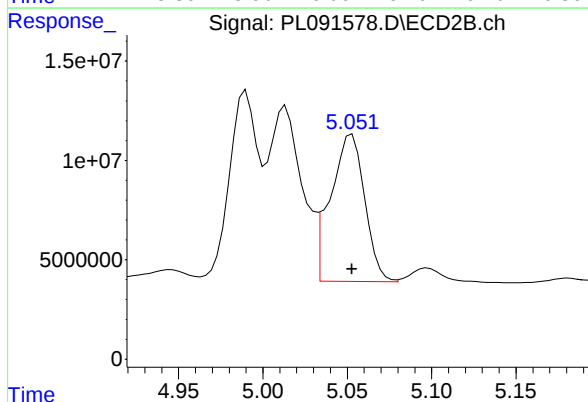


#26 Chlordane-4

R.T.: 5.053 min
Delta R.T.: 0.000 min
Response: 104269708
Conc: 500.00 ng/ml

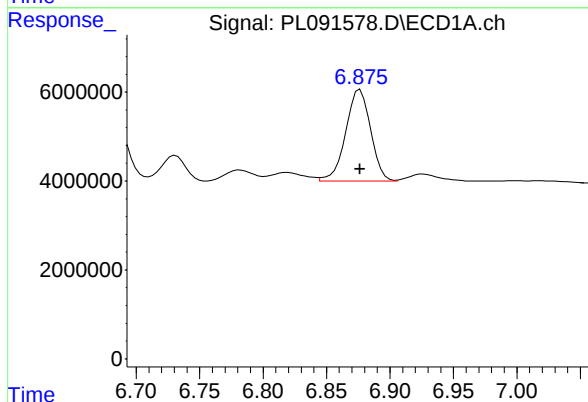


#27 Chlordane-5

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 28162351
Conc: 500.00 ng/ml

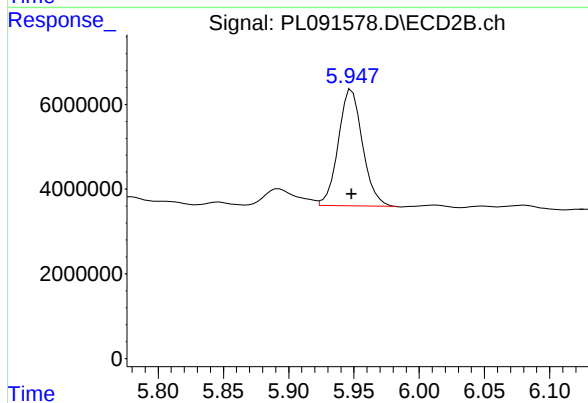

#27 Chlordane-5


R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 35427383
Conc: 500.00 ng/ml

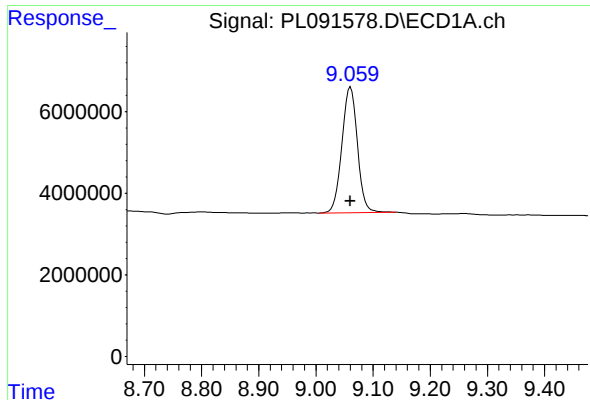

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 58081135
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

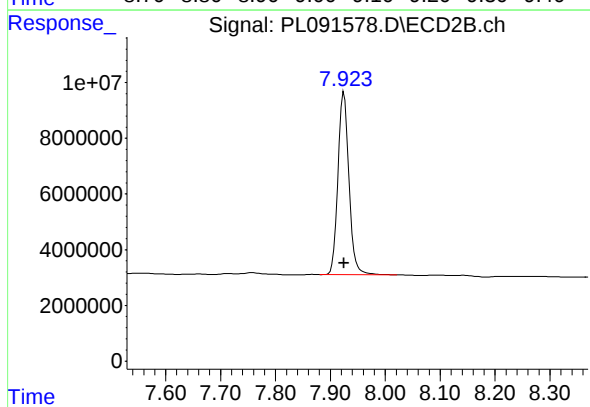

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 91176732
Conc: 50.00 ng/ml