

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091018\
 Data File : PL039794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2018 17:38
 Operator : AJ\SJ
 Sample : J4821-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:18:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.905	101.6E6	43938036	14.530	16.389
28)	SA Decachlor...	7.955	8.891	84139948	37428536	11.980	16.129 #
Target Compounds							
8)	B Heptachlo...	4.908f	5.771	3341497	4893642	0.350	1.455 #
23)	Chlordane-1	4.209	0.000	17828695	0	56.315	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091018\
Data File : PL039794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2018 17:38
Operator : AJ\SJ
Sample : J4821-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 05:18:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

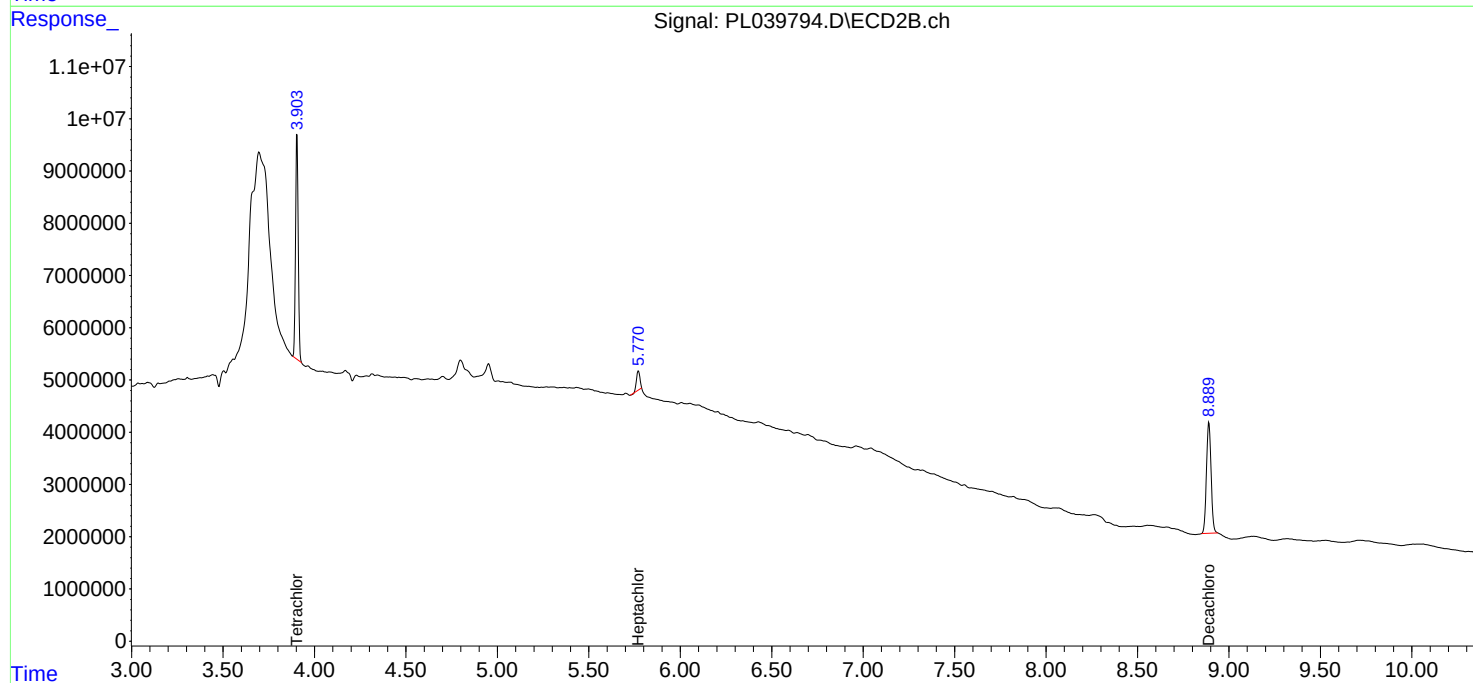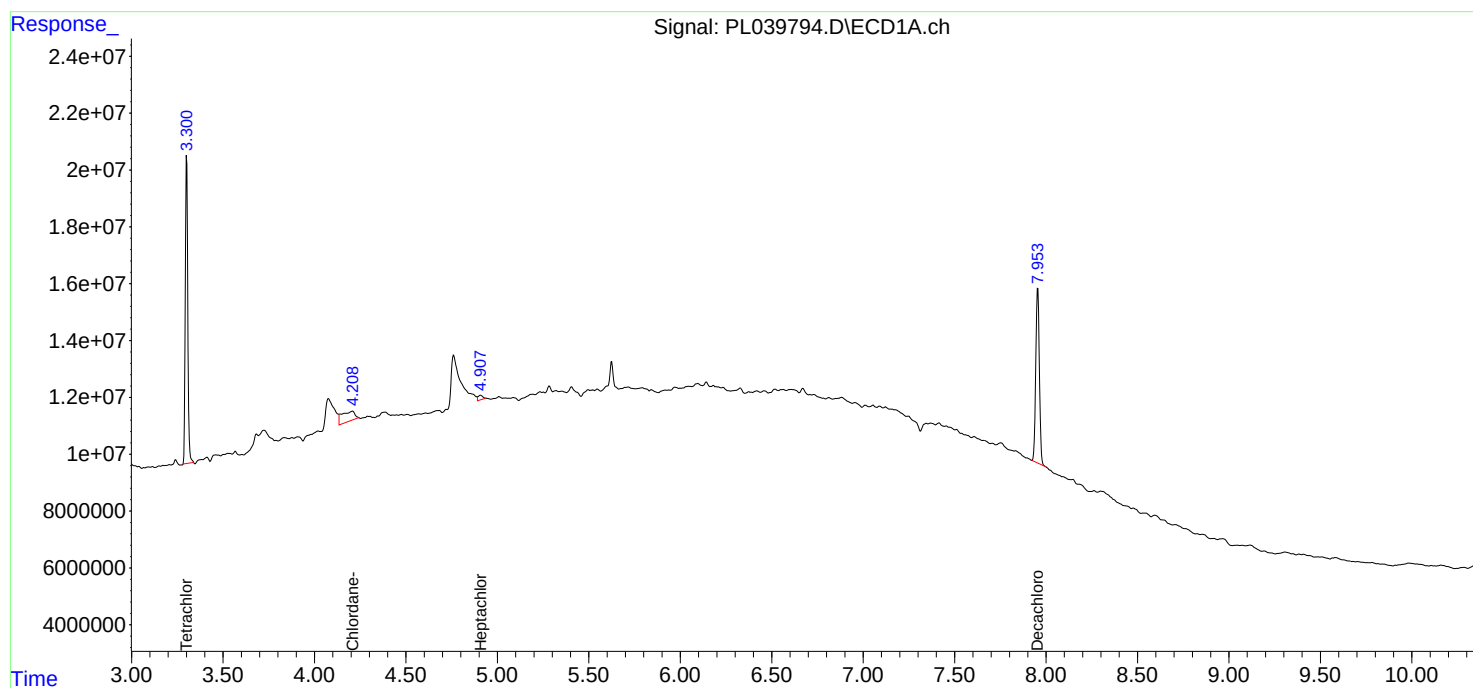


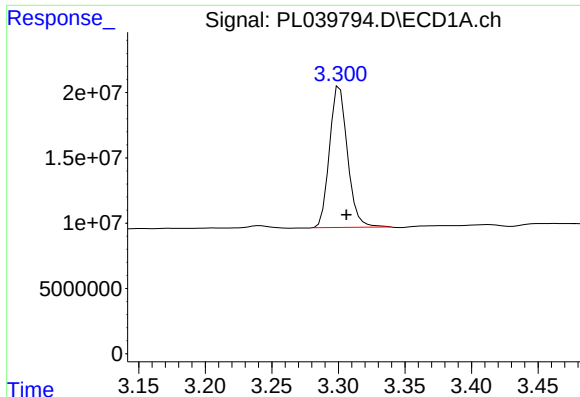

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: -0.005 min
Response: 101569186
Conc: 14.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

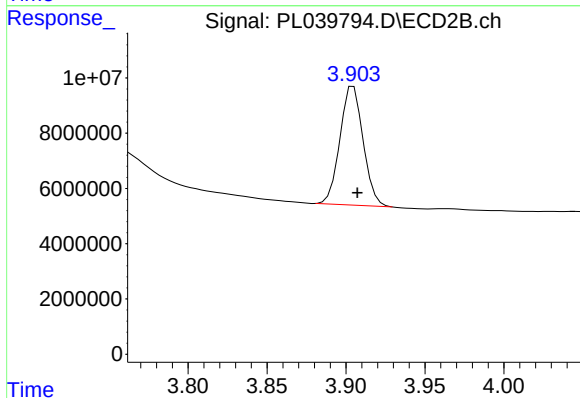


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.003 min
Response: 43938036
Conc: 16.39 ng/ml

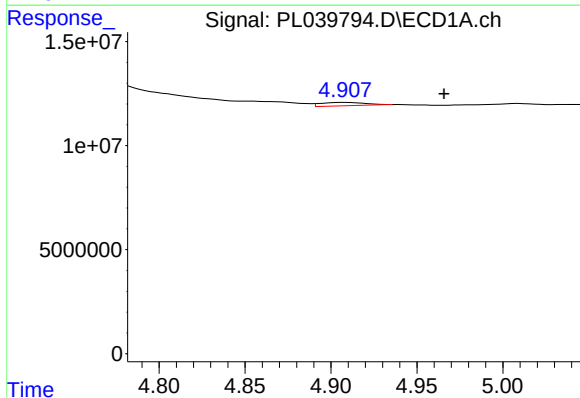


#8 Heptachlor epoxide

R.T.: 4.908 min
Delta R.T.: -0.058 min
Response: 3341497
Conc: 0.35 ng/ml

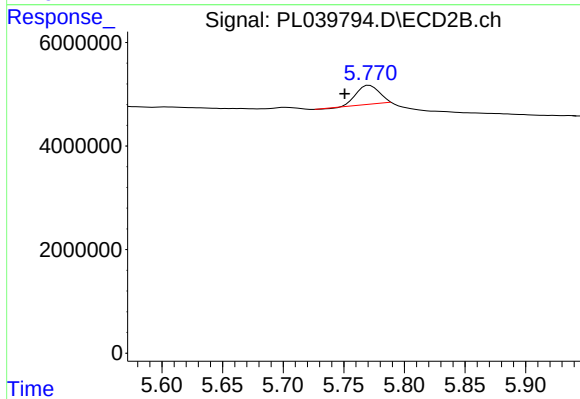

#8 Heptachlor epoxide


R.T.: 5.771 min
Delta R.T.: 0.020 min
Response: 4893642
Conc: 1.46 ng/ml

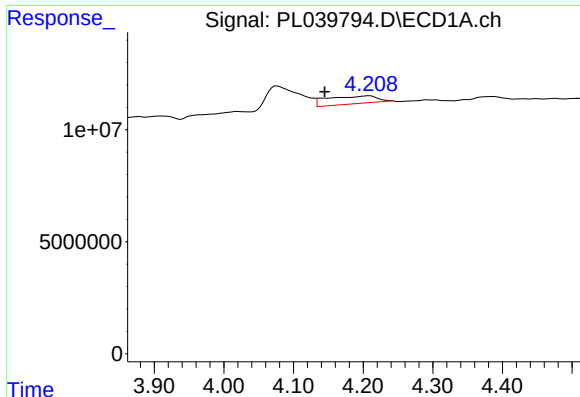

#23 Chlordane-1


R.T.: 4.209 min
Delta R.T.: 0.064 min
Response: 17828695
Conc: 56.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

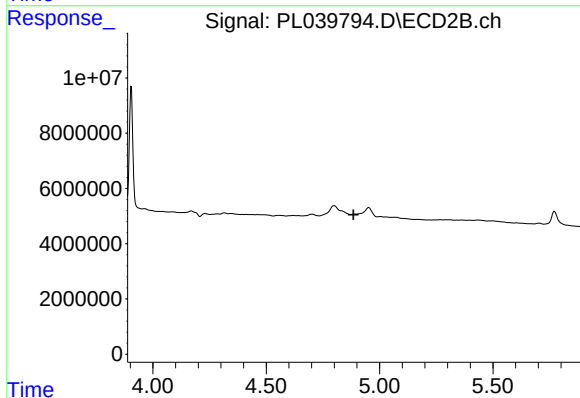


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

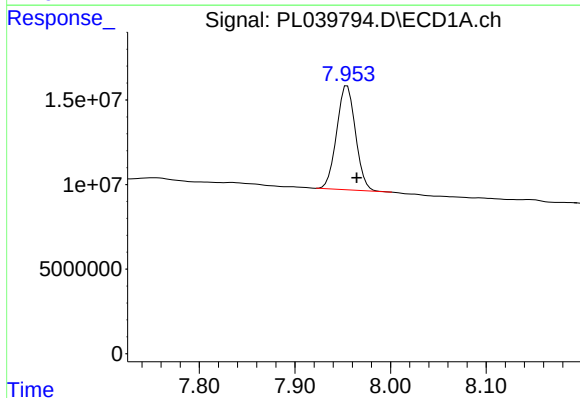

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: -0.010 min
Response: 84139948
Conc: 11.98 ng/ml

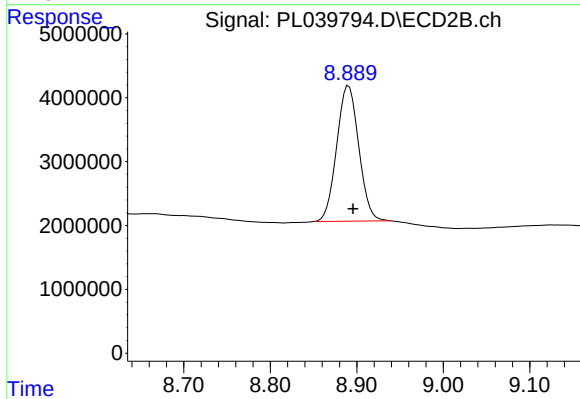

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: -0.005 min
Response: 37428536
Conc: 16.13 ng/ml