

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091018\
 Data File : PL039826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2018 02:08
 Operator : AJ\SJ
 Sample : J4777-07 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:24:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.905	12176978	4498383	1.742	1.678
28)	SA Decachlor...	7.954	0.000	10849384	0	1.545	N.D. #
Target Compounds							
8)	B Heptachlo...	4.921f	5.773	3015274	6315417	0.316	1.878 #
9)	A Endosulfan I	5.316	0.000	13363763	0	1.526	N.D. #
23)	Chlordane-1	4.140	0.000	4850417	0	15.321	N.D. #
24)	Chlordane-2	4.662	0.000	6092249	0	17.427	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091018\
Data File : PL039826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2018 02:08
Operator : AJ\SJ
Sample : J4777-07 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 05:24:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

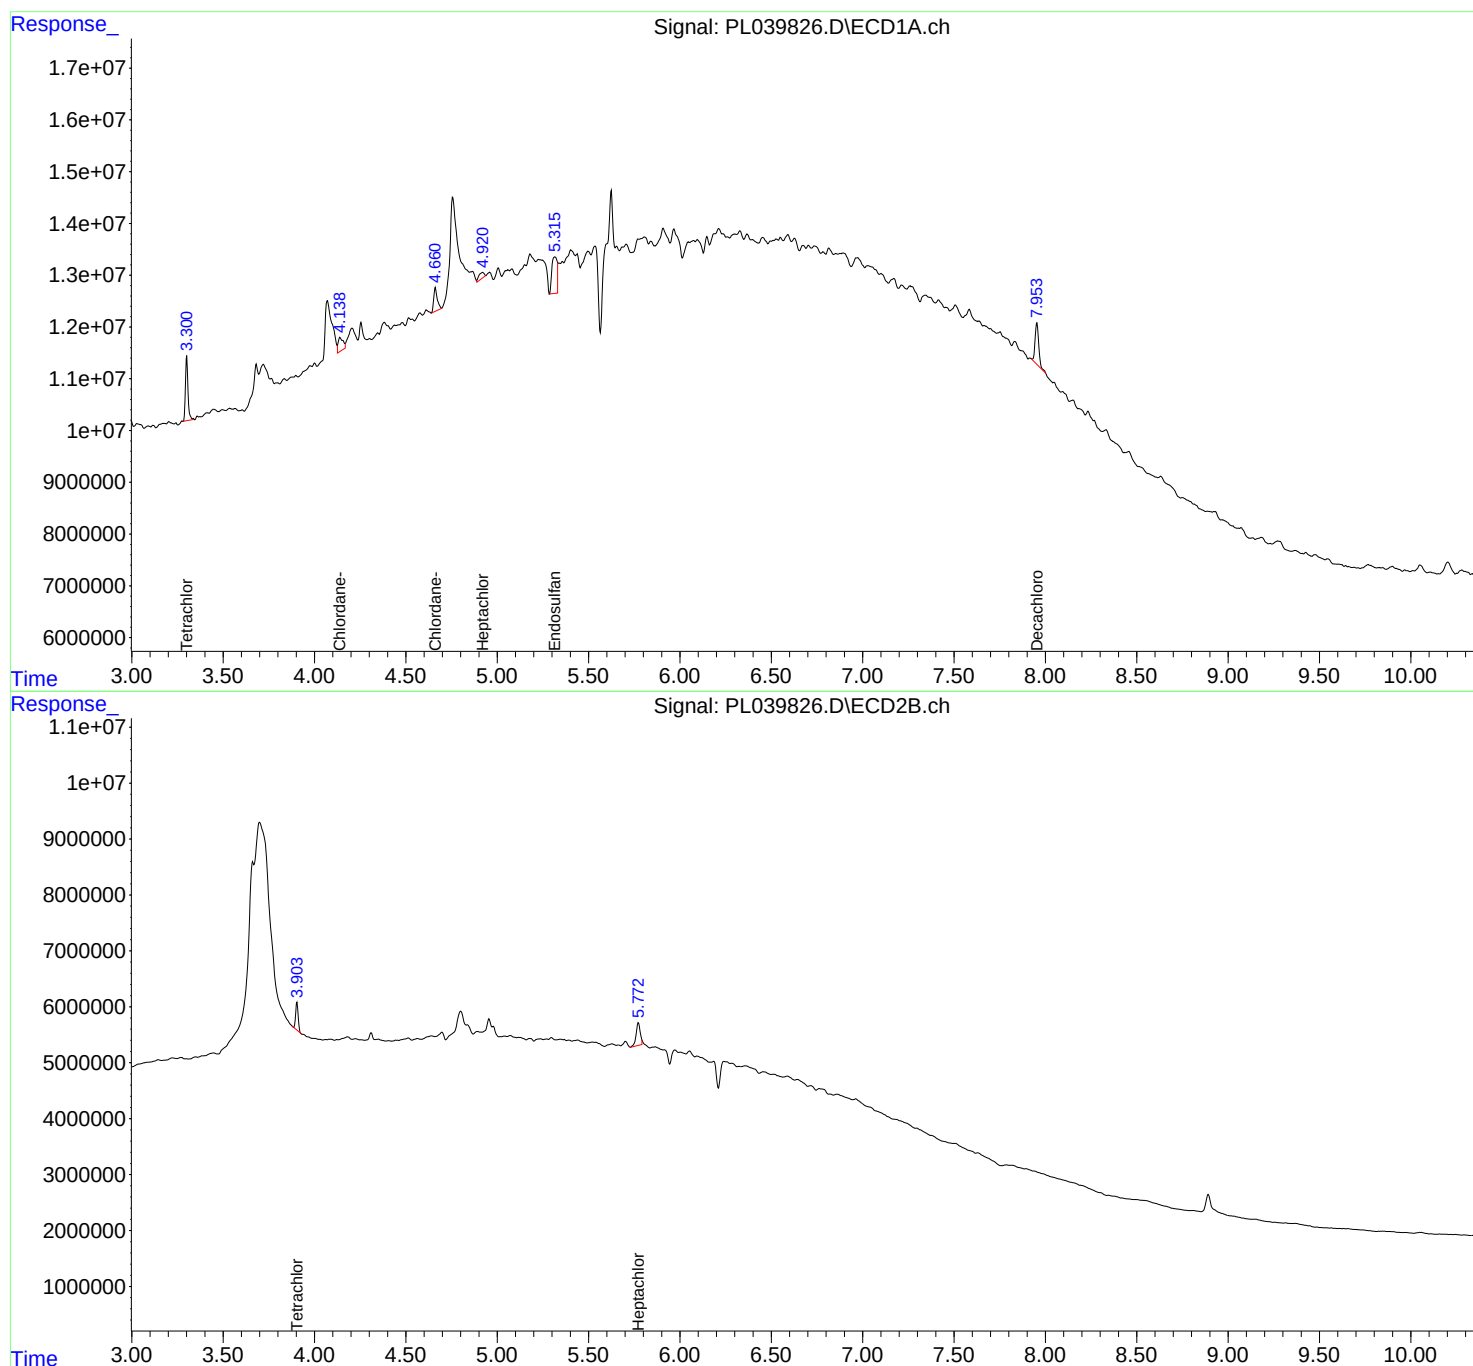


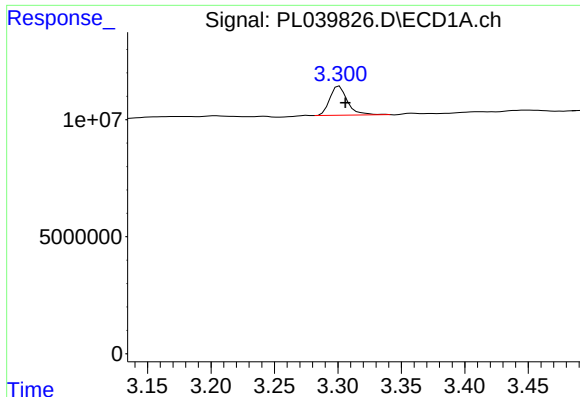

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: -0.005 min
Response: 12176978
Conc: 1.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

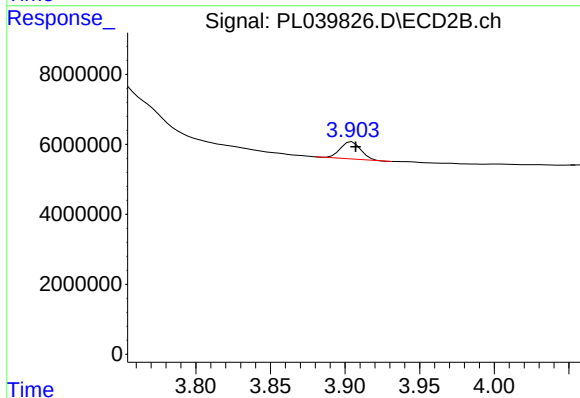


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 4498383
Conc: 1.68 ng/ml

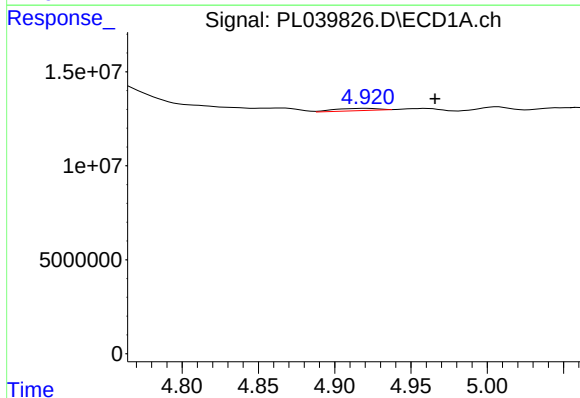


#8 Heptachlor epoxide

R.T.: 4.921 min
Delta R.T.: -0.045 min
Response: 3015274
Conc: 0.32 ng/ml

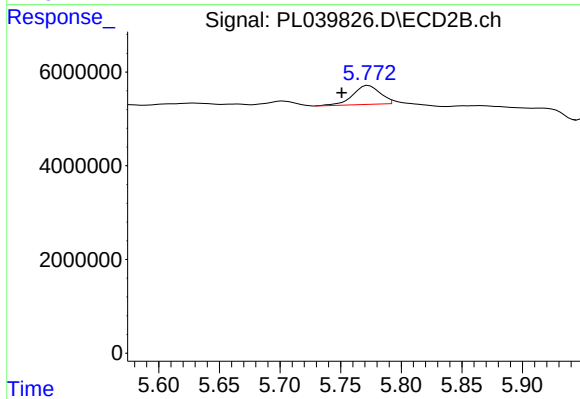

#8 Heptachlor epoxide


R.T.: 5.773 min
Delta R.T.: 0.022 min
Response: 6315417
Conc: 1.88 ng/ml

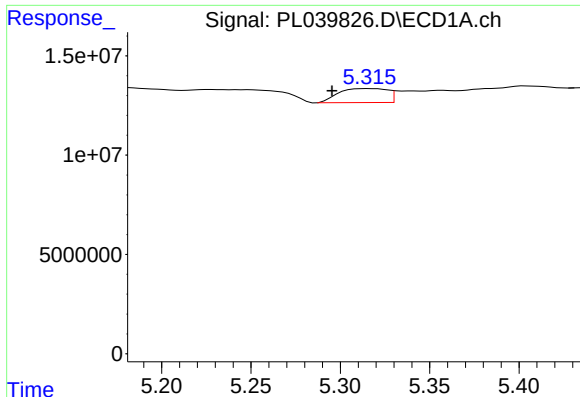

#9 Endosulfan I


R.T.: 5.316 min
Delta R.T.: 0.021 min
Response: 13363763
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

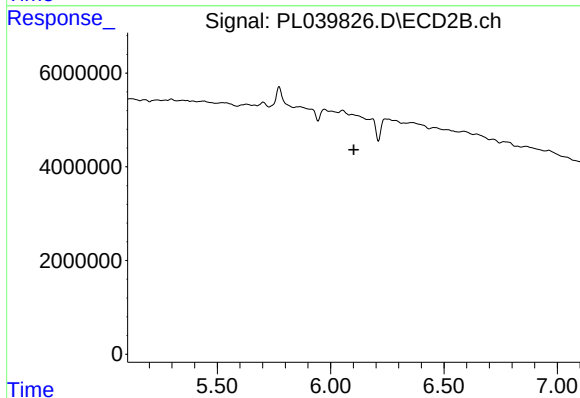


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

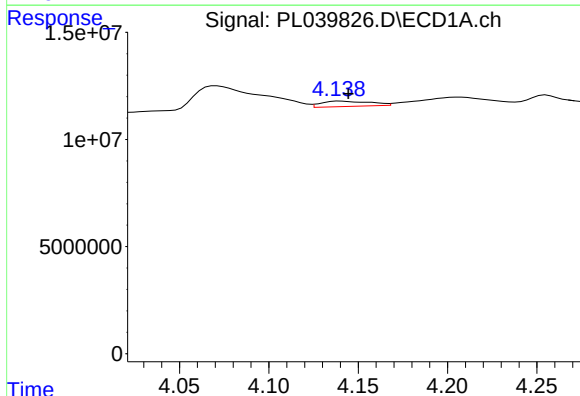


#23 Chlordane-1

R.T.: 4.140 min
Delta R.T.: -0.005 min
Response: 4850417
Conc: 15.32 ng/ml

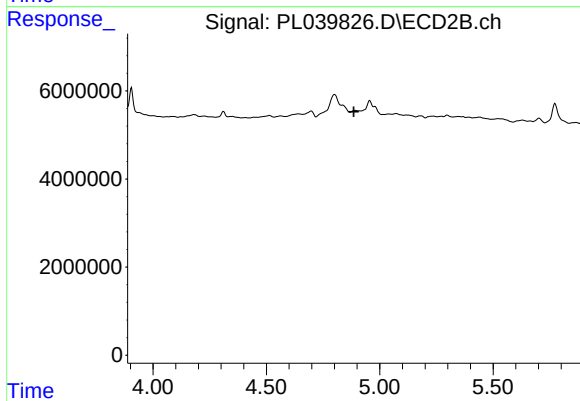

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

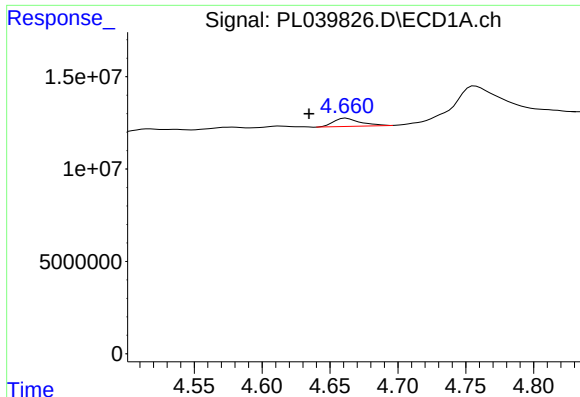

#24 Chlordane-2

R.T.: 4.662 min
Delta R.T.: 0.027 min
Response: 6092249
Conc: 17.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

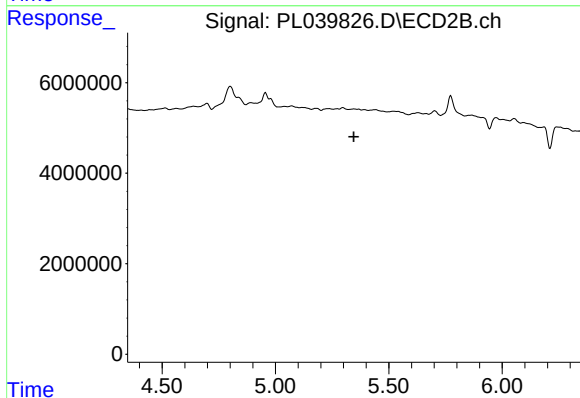


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: -0.010 min
Response: 10849384
Conc: 1.54 ng/ml

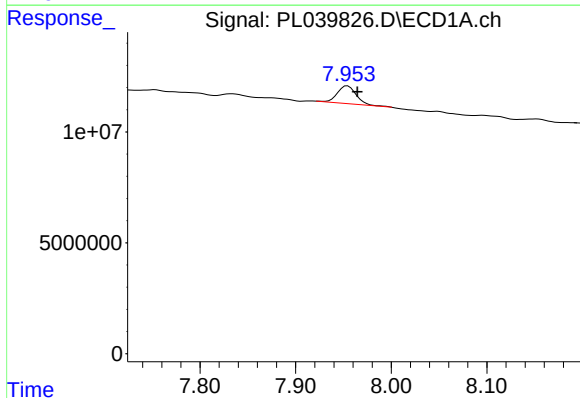

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.