

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091018\
 Data File : PL039828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2018 02:36
 Operator : AJ\SJ
 Sample : J4769-03 2X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:28:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.905	44627006	16133287	6.384	6.018
28)	SA Decachlor...	7.954	8.891	44562976	19766326	6.345	8.518 #
Target Compounds							
9)	A Endosulfan I	5.235f	0.000	11372850	0	1.299	N.D. #
10)	B gamma-Chl...	5.180	0.000	7772555	0	0.787	N.D. #
11)	B alpha-Chl...	5.235	0.000	11372850	0	1.184	N.D. #
12)	B 4,4'-DDE	5.405	0.000	6880681	0	0.719	N.D. #
23)	Chlordane-1	4.138	0.000	6522882	0	20.604	N.D. #
24)	Chlordane-2	4.628	0.000	12514945	0	35.799	N.D. #
25)	Chlordane-3	5.180	0.000	7772555	0	7.116	N.D. #
26)	Chlordane-4	5.235	0.000	11372850	0	11.380	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091018\
Data File : PL039828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2018 02:36
Operator : AJ\SJ
Sample : J4769-03 2X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 05:28:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

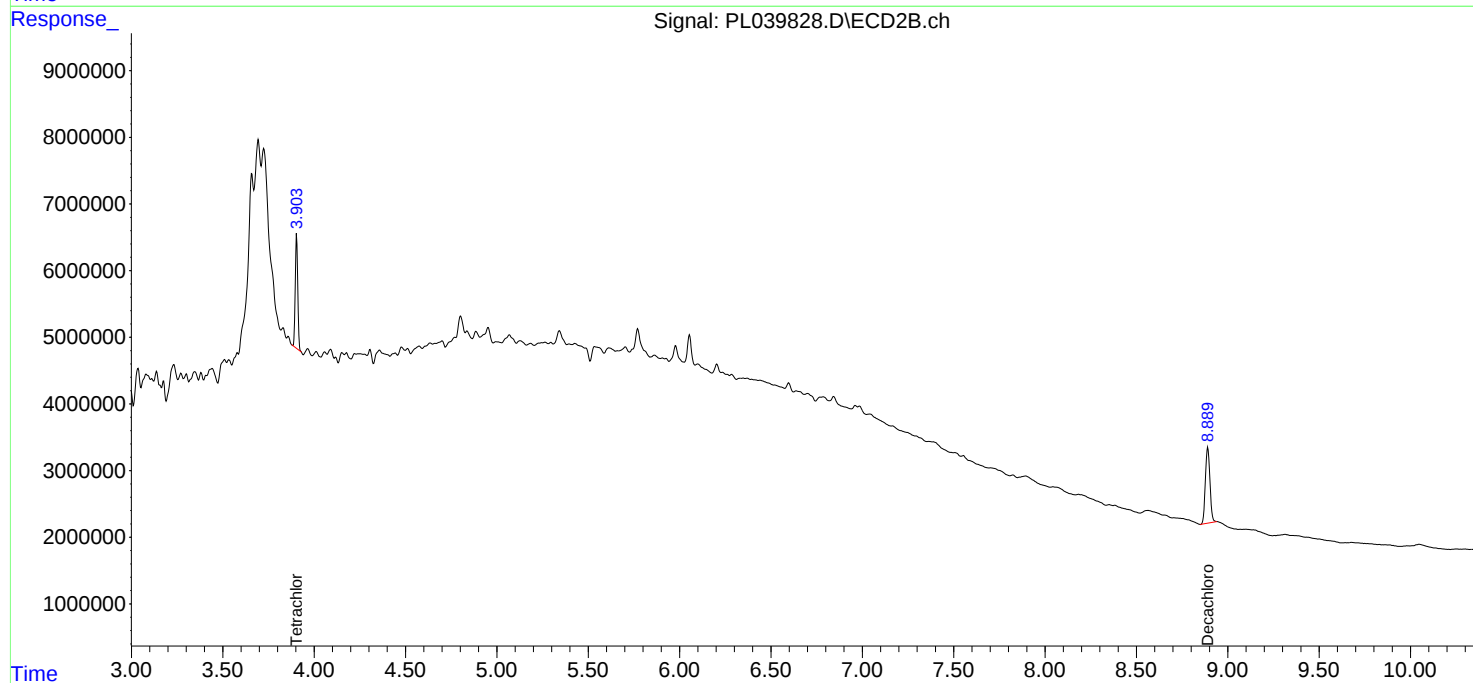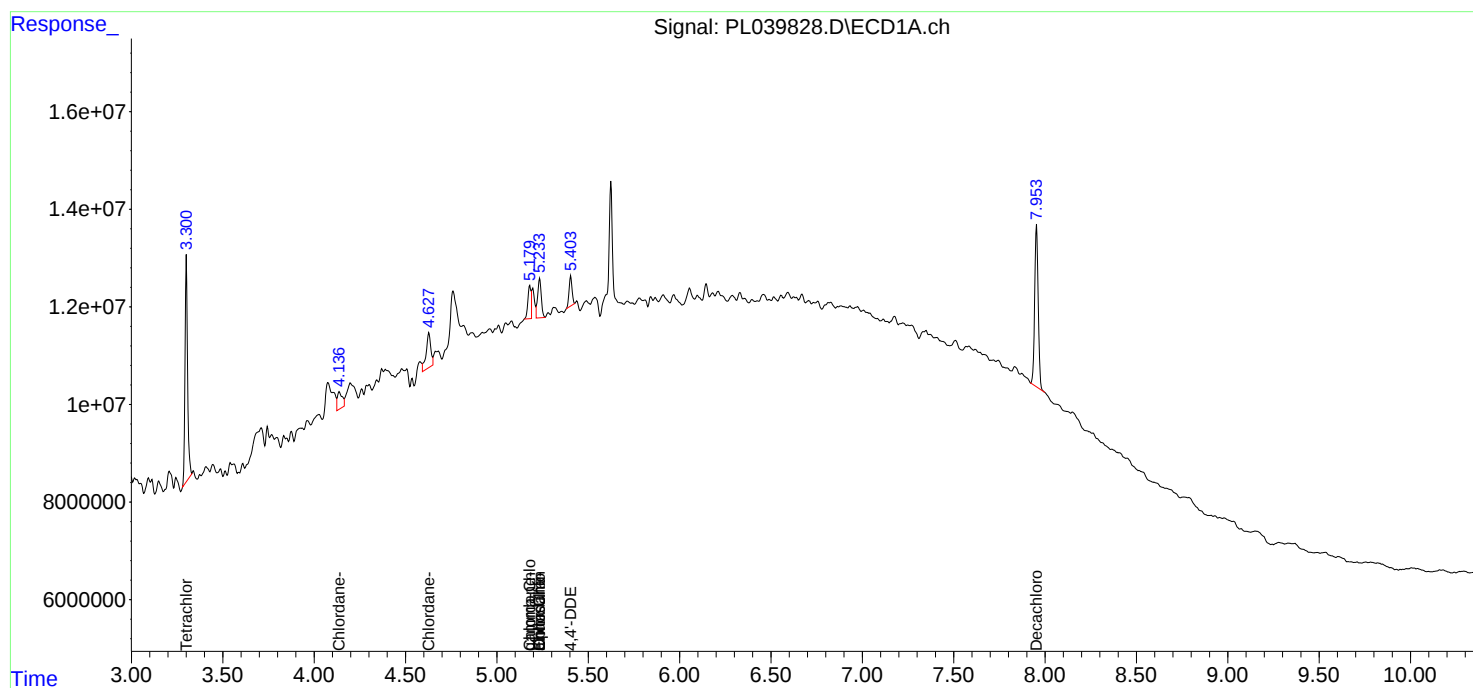


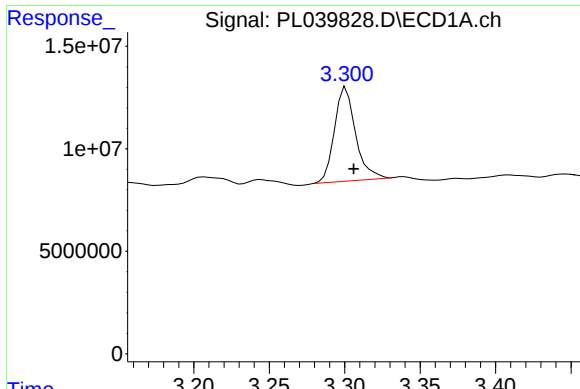

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: -0.005 min
Response: 44627006
Conc: 6.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

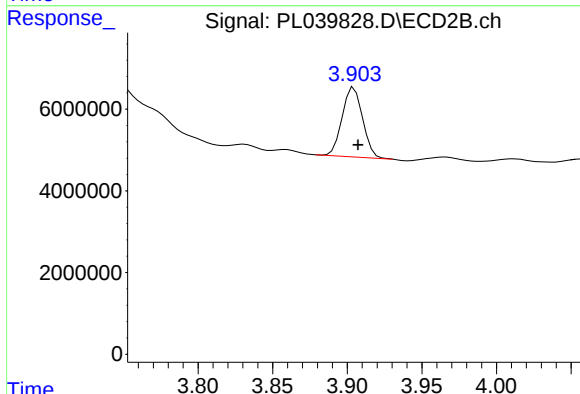


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.003 min
Response: 16133287
Conc: 6.02 ng/ml

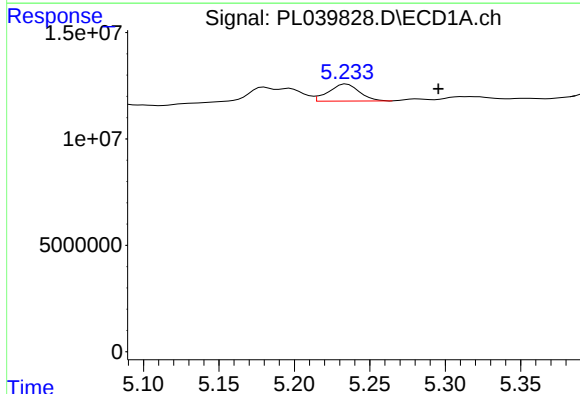


#9 Endosulfan I

R.T.: 5.235 min
Delta R.T.: -0.061 min
Response: 11372850
Conc: 1.30 ng/ml

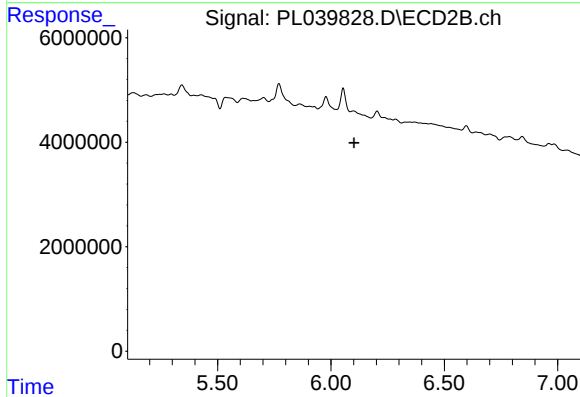

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.102 min
Response: 0
Conc: N.D.

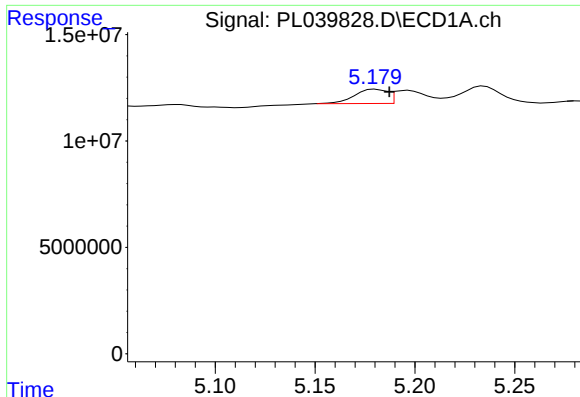

#10 gamma-Chlordane


R.T.: 5.180 min
Delta R.T.: -0.007 min
Response: 7772555
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

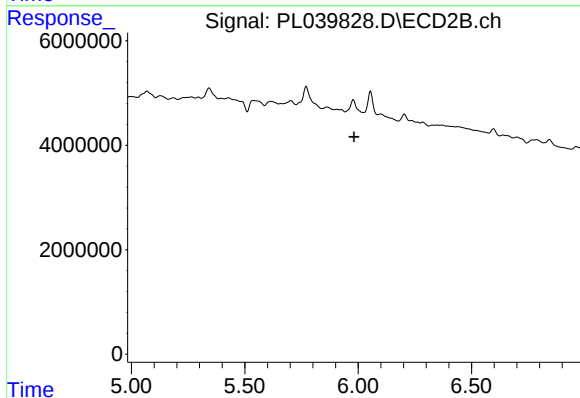


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

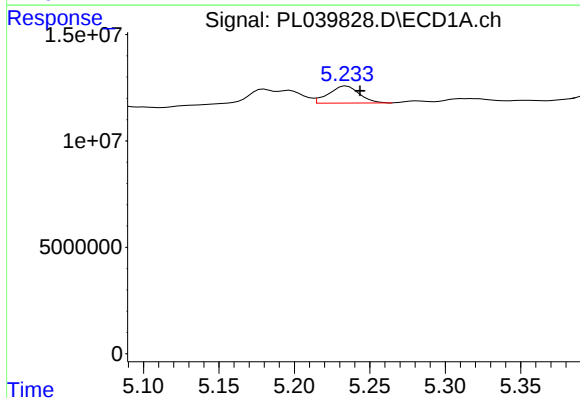


#11 alpha-Chlordane

R.T.: 5.235 min
Delta R.T.: -0.009 min
Response: 11372850
Conc: 1.18 ng/ml

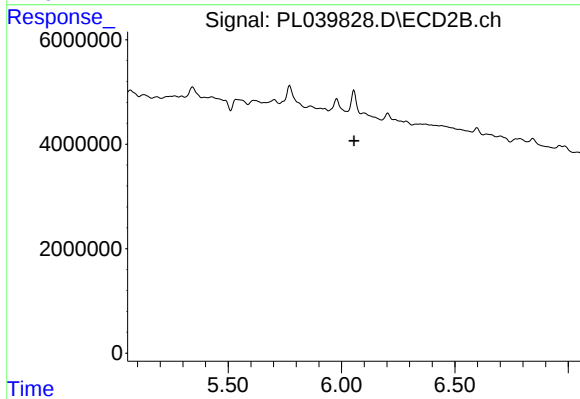

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

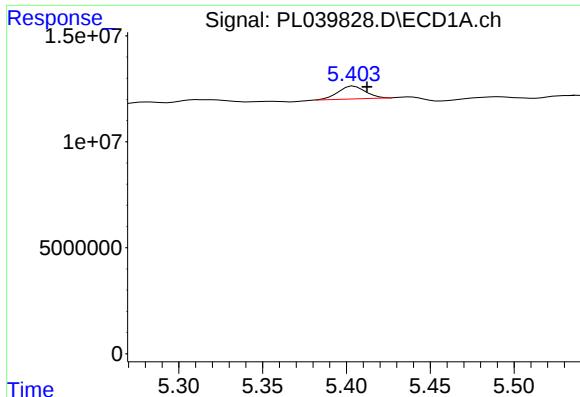

#12 4,4'-DDE


R.T.: 5.405 min
Delta R.T.: -0.008 min
Response: 6880681
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

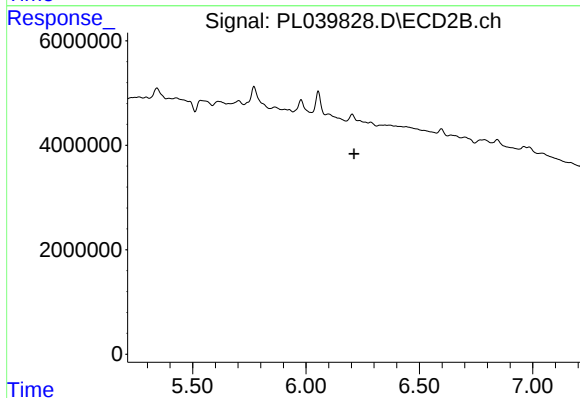


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

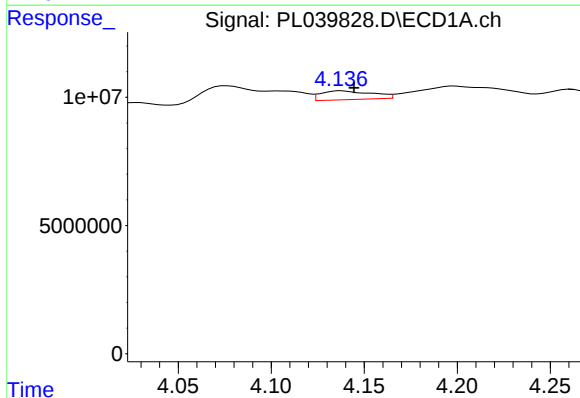


#23 Chlordane-1

R.T.: 4.138 min
Delta R.T.: -0.007 min
Response: 6522882
Conc: 20.60 ng/ml

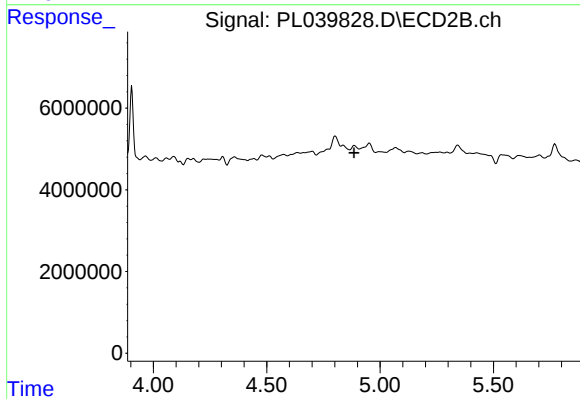

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

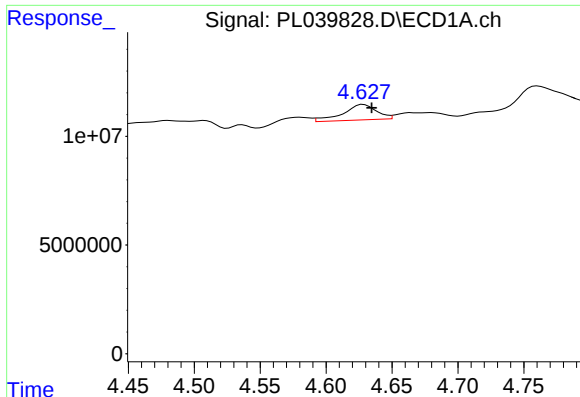

#24 Chlordane-2


R.T.: 4.628 min
Delta R.T.: -0.006 min
Response: 12514945
Conc: 35.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

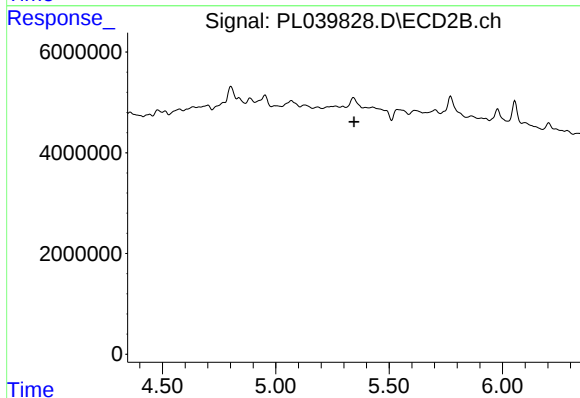


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

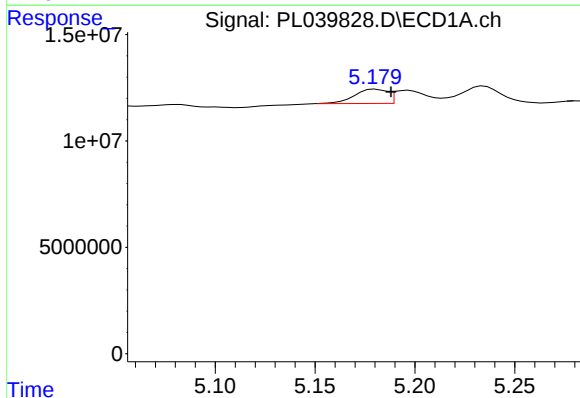


#25 Chlordane-3

R.T.: 5.180 min
Delta R.T.: -0.008 min
Response: 7772555
Conc: 7.12 ng/ml

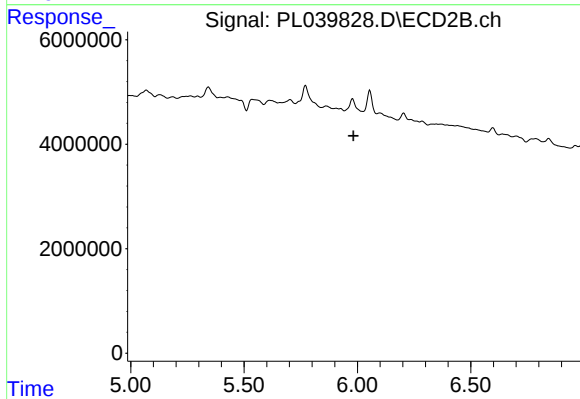

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

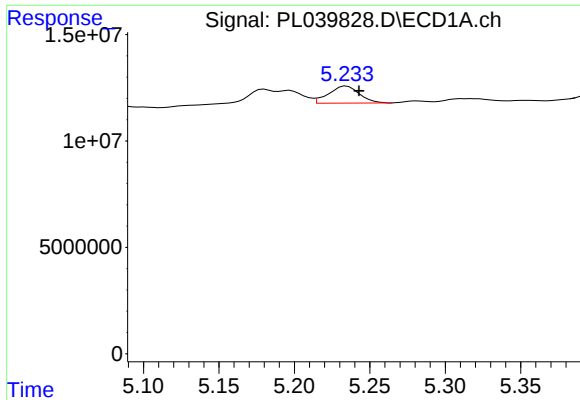

#26 Chlordane-4


R.T.: 5.235 min
Delta R.T.: -0.008 min
Response: 11372850
Conc: 11.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

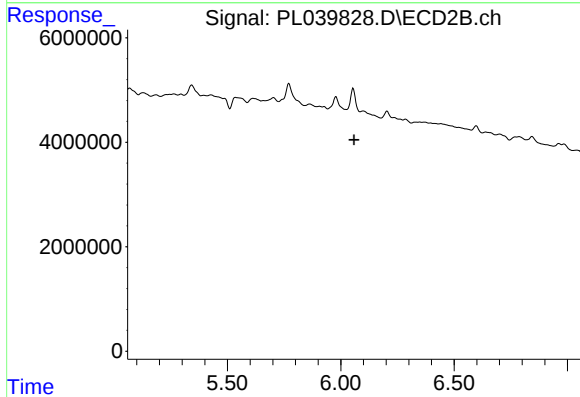


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

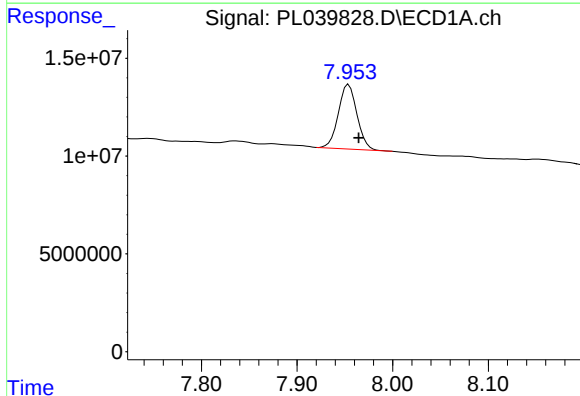

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: -0.010 min
Response: 44562976
Conc: 6.34 ng/ml

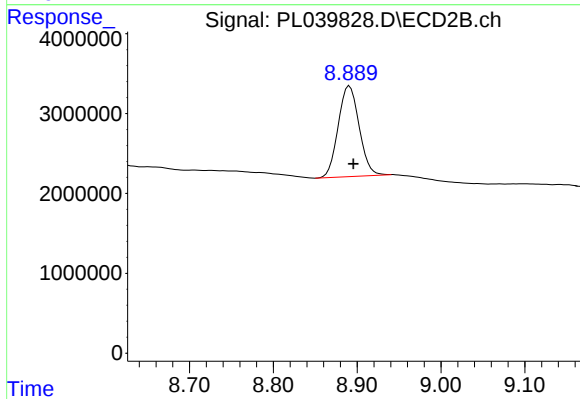

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: -0.005 min
Response: 19766326
Conc: 8.52 ng/ml