

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091019\
 Data File : PL052334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 13:44
 Operator : SG\AJ
 Sample : PB122962BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 00:47:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.922	179.8E6	44460050	21.004	20.350
28)	SA Decachlor...	7.969	8.944	248.5E6	52885064	20.471	17.374
Target Compounds							
6)	B beta-BHC	0.000	4.794f	0	1707444	N.D.	1.172 #
8)	B Heptachlo...	0.000	5.797	0	926018	N.D.	0.274 #
9)	A Endosulfan I	5.325f	0.000	8919442	0	0.663	N.D. #
15)	B Endosulfa...	0.000	6.842	0	2810289	N.D.	0.853 #
27)	Chlordane-5	0.000	6.873f	0	284428	N.D.	2.885 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091019\
Data File : PL052334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 13:44
Operator : SG\AJ
Sample : PB122962BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 00:47:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

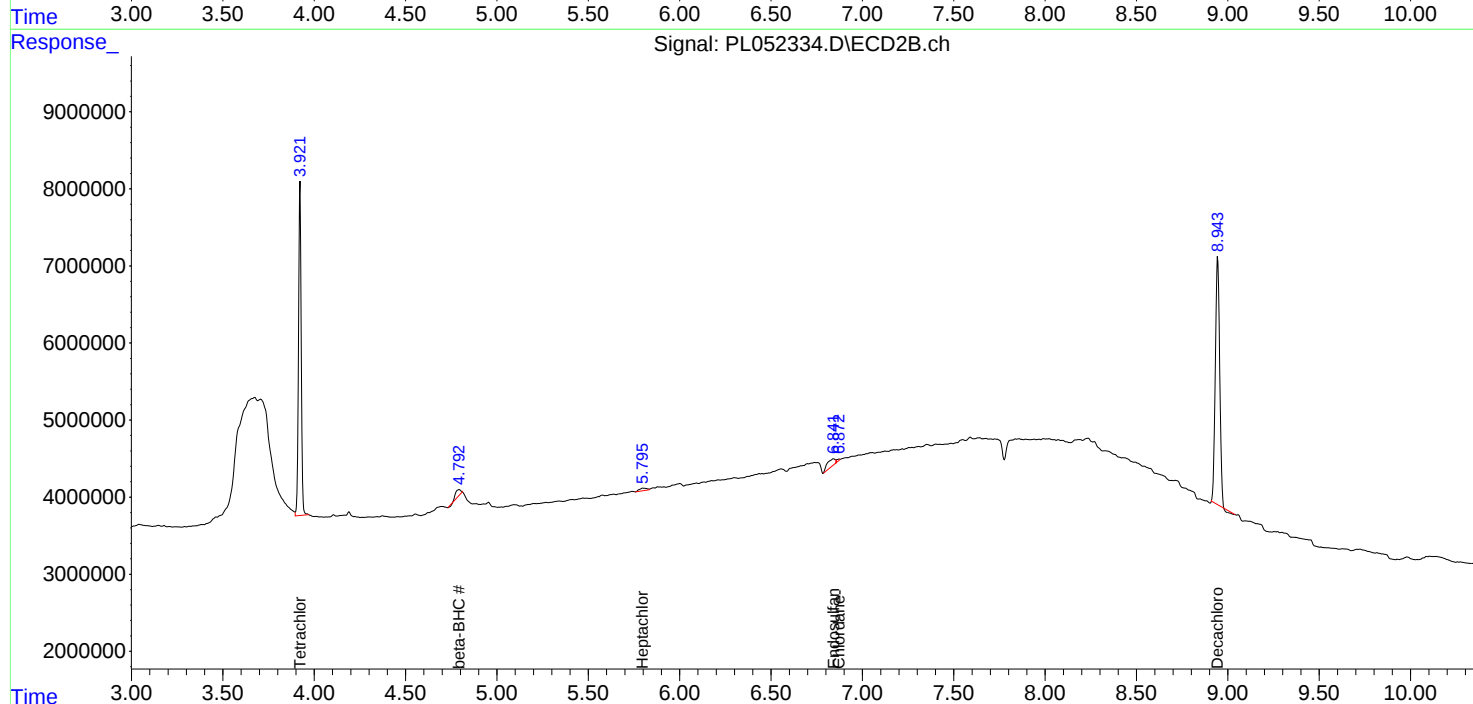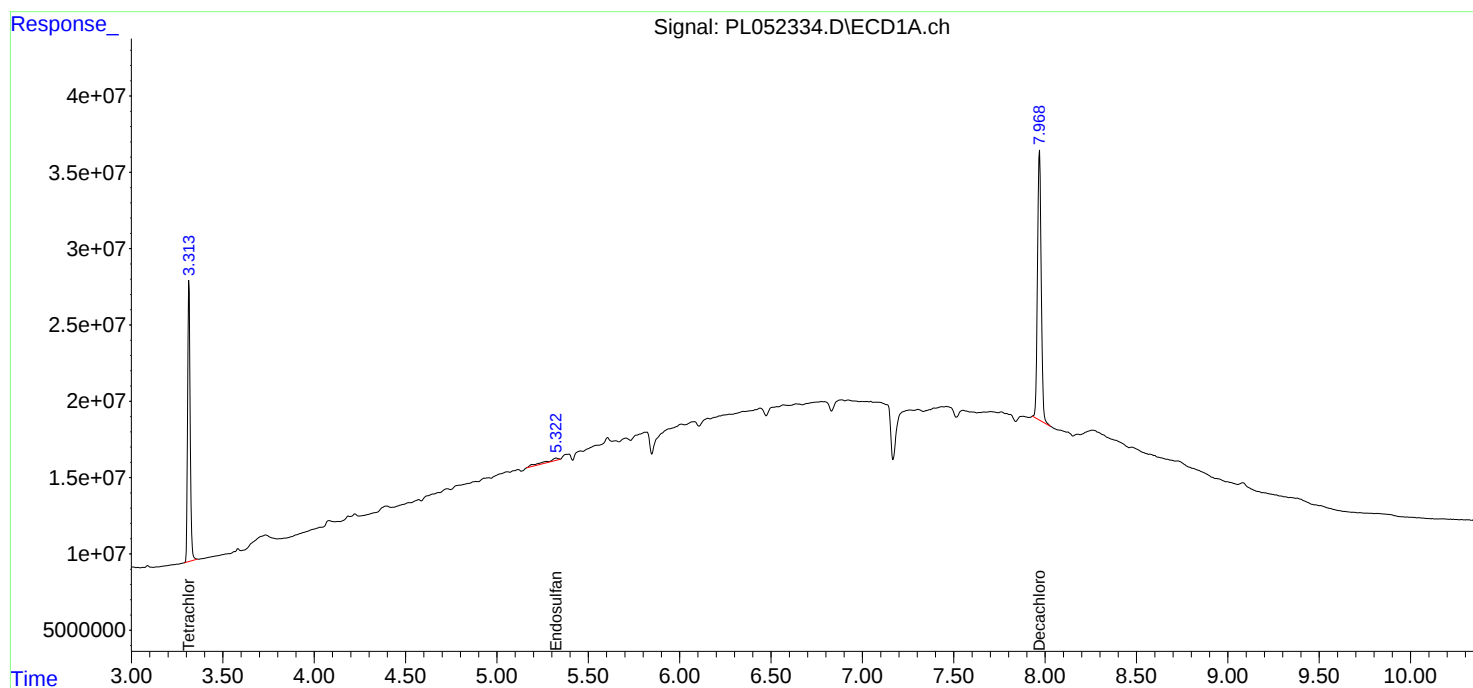


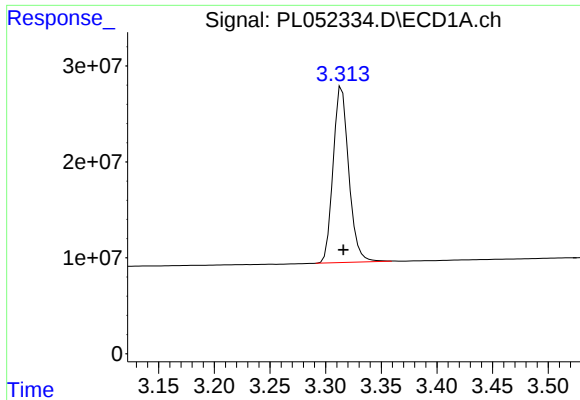

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.001 min
Response: 179763545
Conc: 21.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

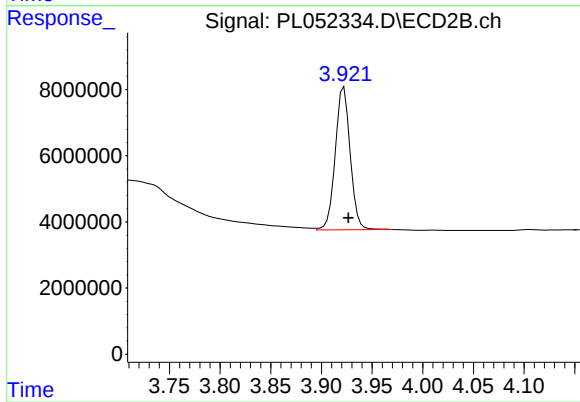


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.004 min
Response: 44460050
Conc: 20.35 ng/ml

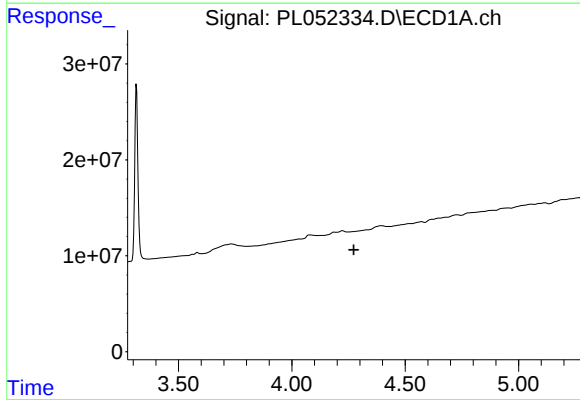


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

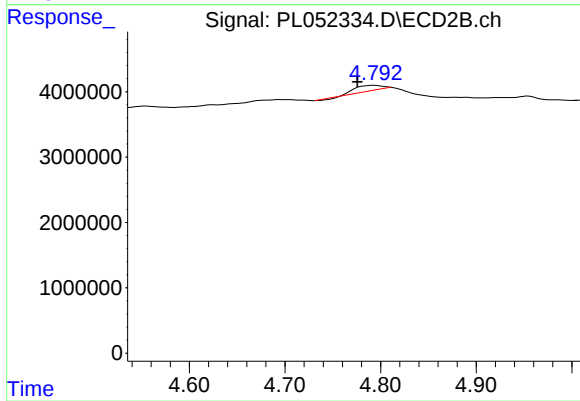

#6 beta-BHC


R.T.: 4.794 min
Delta R.T.: 0.018 min
Response: 1707444
Conc: 1.17 ng/ml

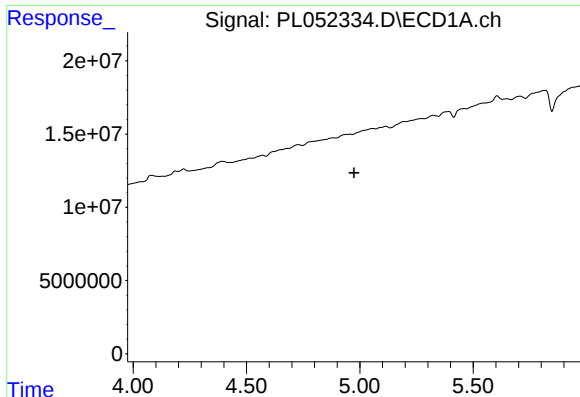

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

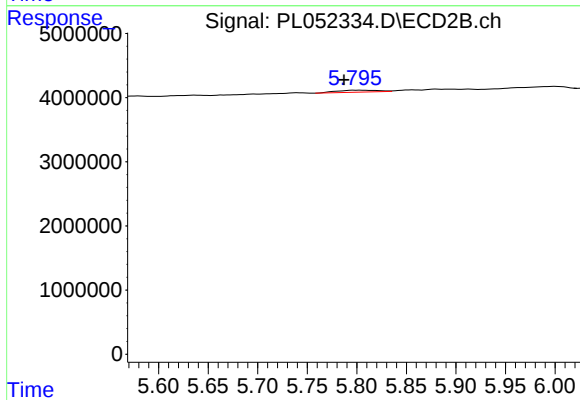


#8 Heptachlor epoxide

R.T.: 5.797 min
Delta R.T.: 0.010 min
Response: 926018
Conc: 0.27 ng/ml

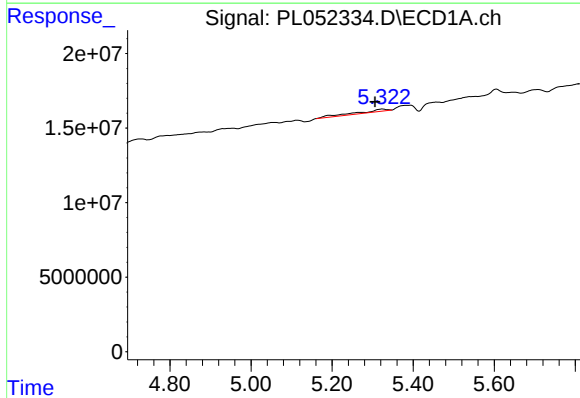


#9 Endosulfan I

R.T.: 5.325 min
Delta R.T.: 0.019 min
Response: 8919442
Conc: 0.66 ng/ml

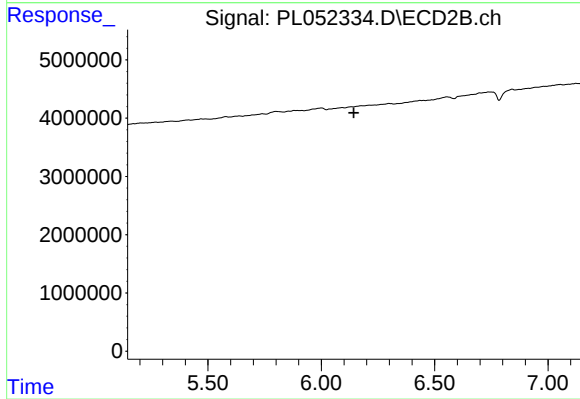

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

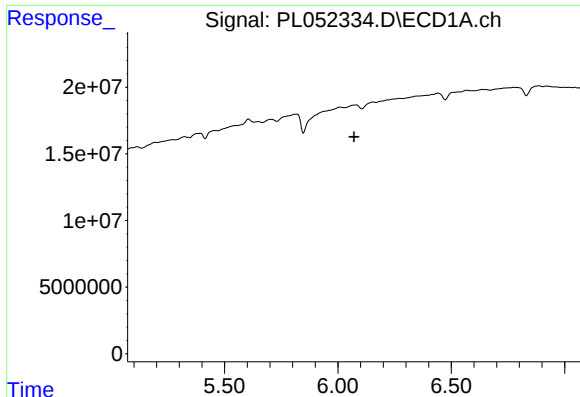

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

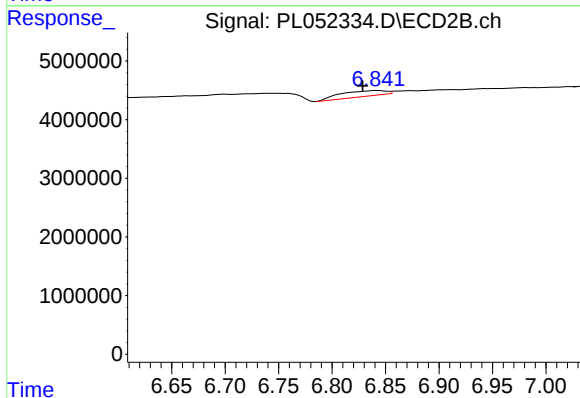


#15 Endosulfan II

R.T.: 6.842 min
Delta R.T.: 0.013 min
Response: 2810289
Conc: 0.85 ng/ml

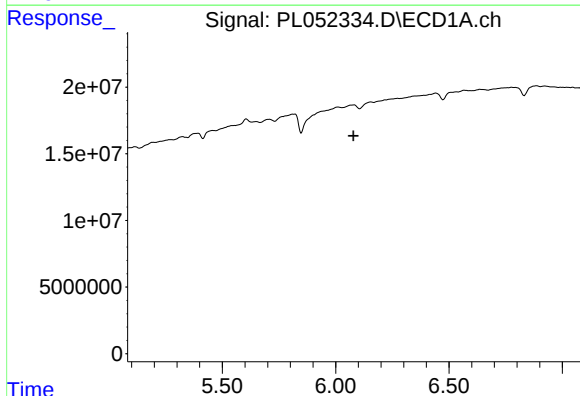


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

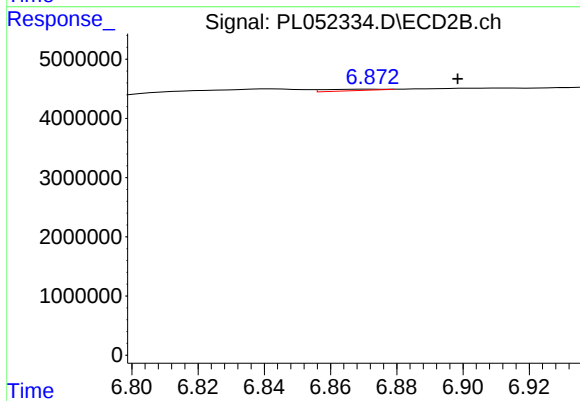

#27 Chlordane-5


R.T.: 6.873 min
Delta R.T.: -0.025 min
Response: 284428
Conc: 2.89 ng/ml

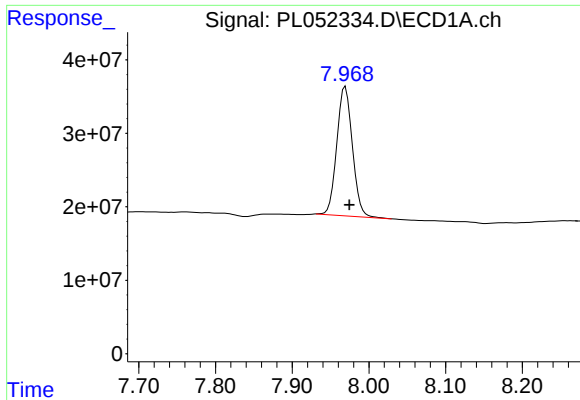

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: -0.005 min
Response: 248467487
Conc: 20.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

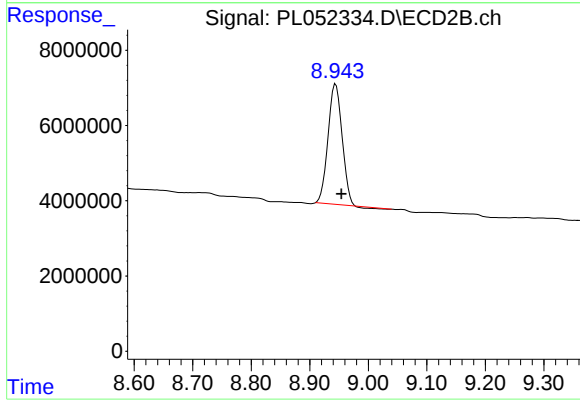

#28 Decachlorobiphenyl

R.T.: 8.944 min
Delta R.T.: -0.010 min
Response: 52885064
Conc: 17.37 ng/ml