

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091019\
 Data File : PL052359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 20:18
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 00:53:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.922	226.1E6	53992767	26.420	24.713
28)	SA Decachlor...	7.967	8.945	236.9E6	52209643	19.514	17.152
Target Compounds							
6)	B beta-BHC	0.000	4.800f	0	390814	N.D.	0.268 #
8)	B Heptachlo...	0.000	5.782	0	17345154	N.D.	5.140 #
9)	A Endosulfan I	5.323f	6.151	12760842	1176481	0.949	0.364 #
11)	B alpha-Chl...	5.256	0.000	49425865	0	3.415	N.D. #
13)	MA Dieldrin	5.539	0.000	17306317	0	1.138	N.D. #
14)	MA Endrin	5.806	6.616	7165950	-1348910	0.491	N.D. #
15)	B Endosulfa...	6.082	0.000	2457819	0	0.177	N.D. #
18)	B Endrin al...	0.000	6.932f	0	792450	N.D.	0.280 #
19)	B Endosulfa...	0.000	7.182	0	487963	N.D.	0.158 #
26)	Chlordane-4	5.256	0.000	49425865	0	40.534	N.D. #
27)	Chlordane-5	6.082	0.000	2457819	0	5.009	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091019\
Data File : PL052359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 20:18
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 00:53:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

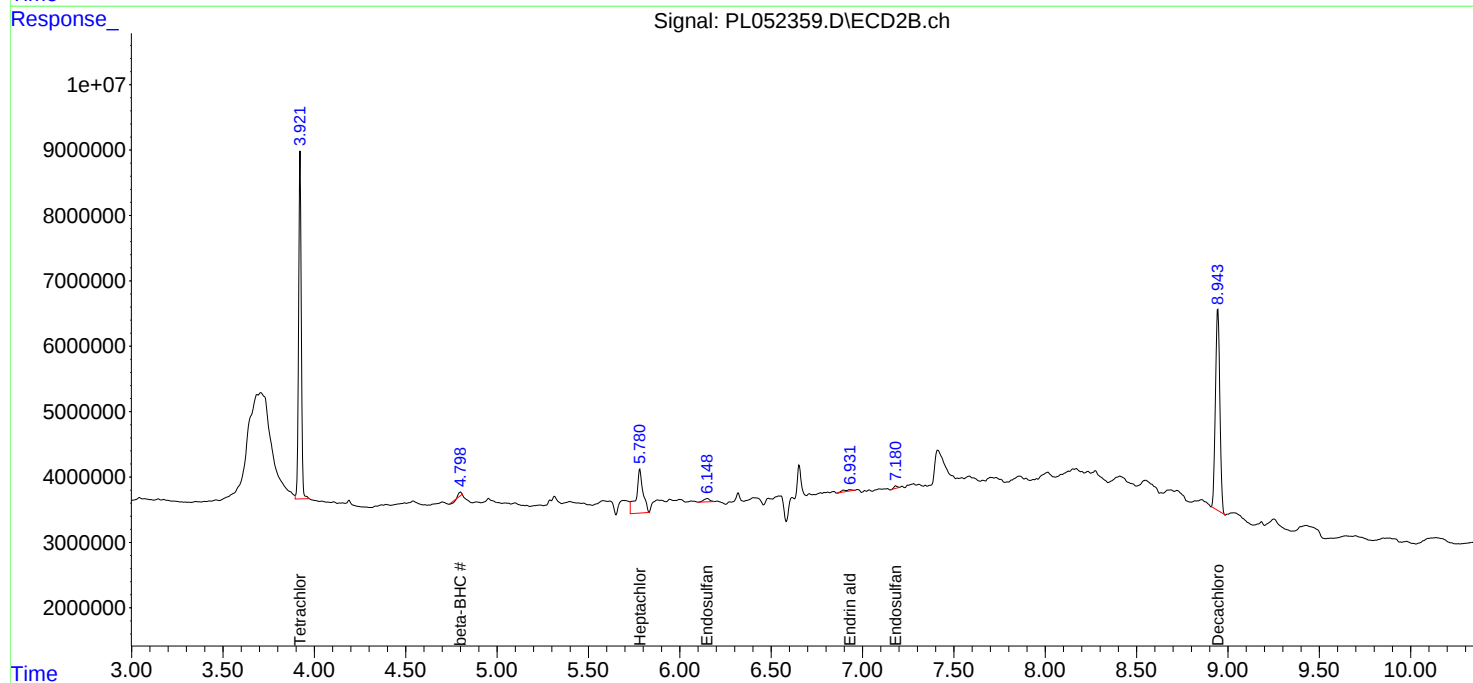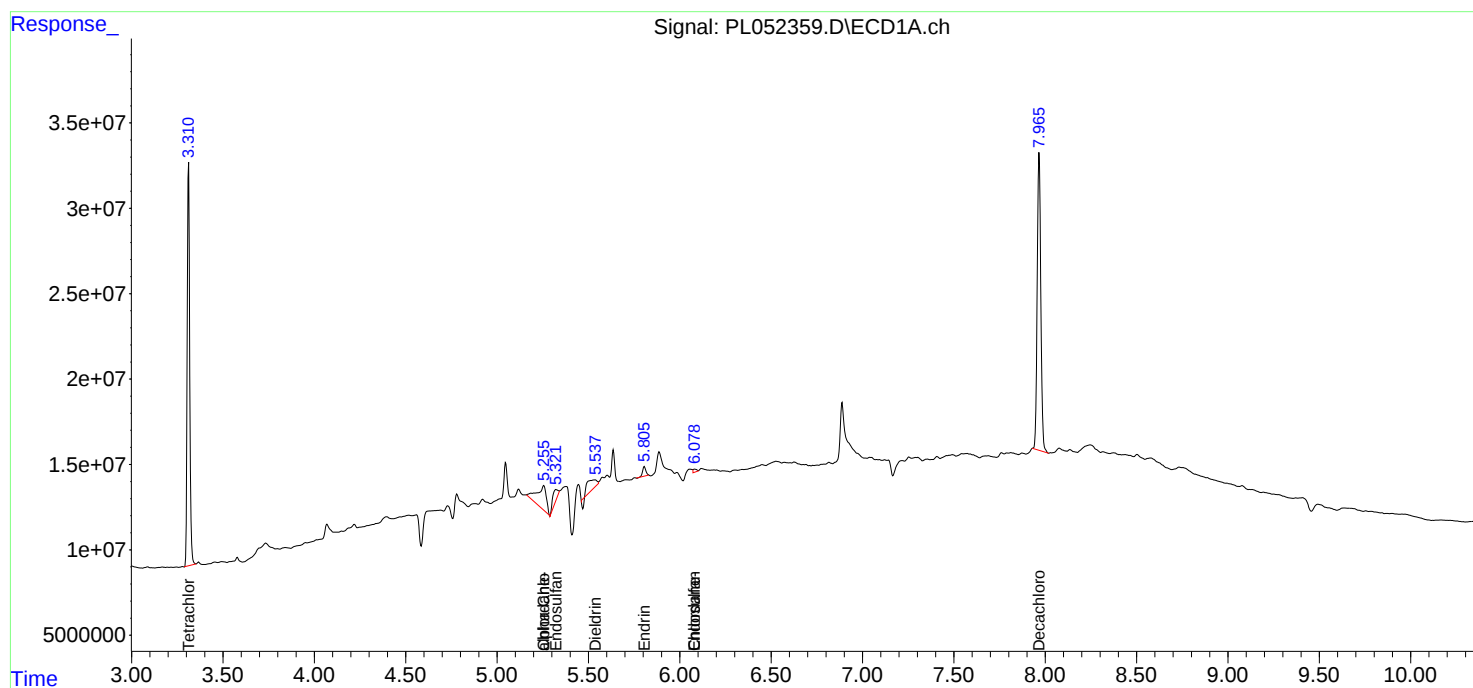


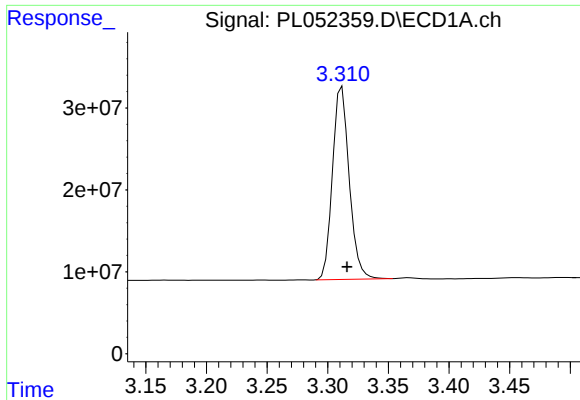

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 226122725
Conc: 26.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

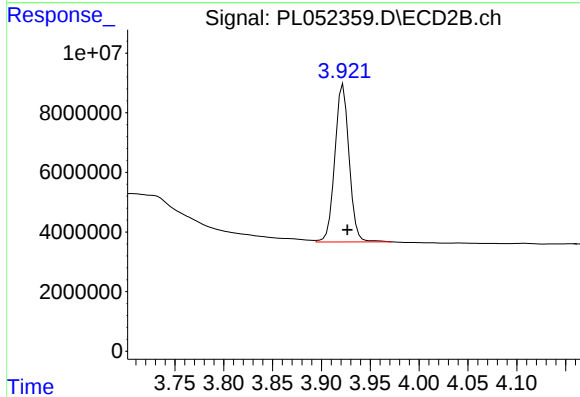


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.004 min
Response: 53992767
Conc: 24.71 ng/ml

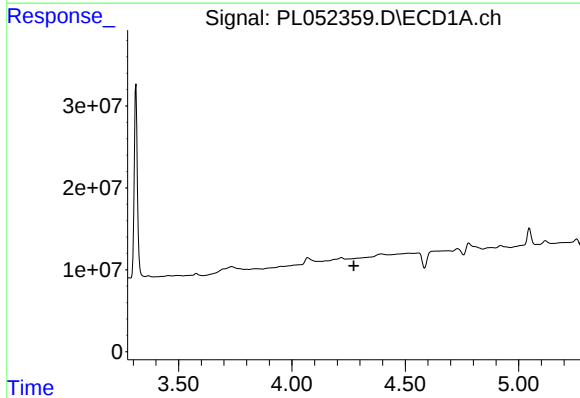


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

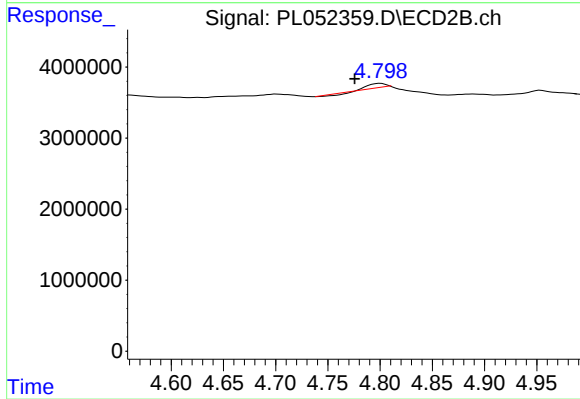

#6 beta-BHC


R.T.: 4.800 min
Delta R.T.: 0.024 min
Response: 390814
Conc: 0.27 ng/ml

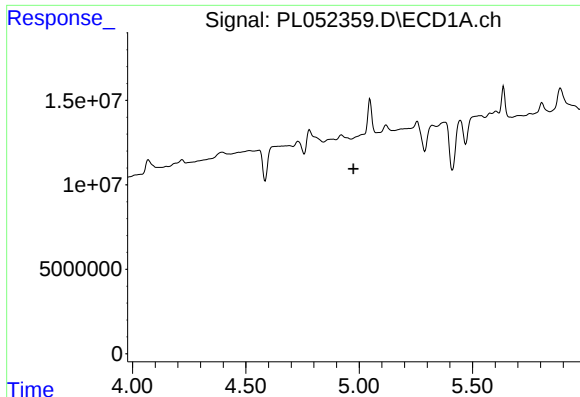

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

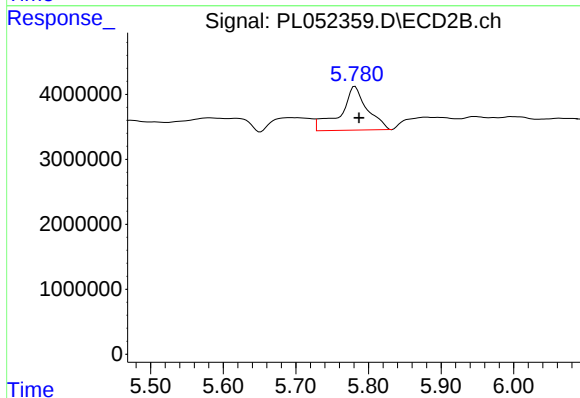


#8 Heptachlor epoxide

R.T.: 5.782 min
Delta R.T.: -0.005 min
Response: 17345154
Conc: 5.14 ng/ml

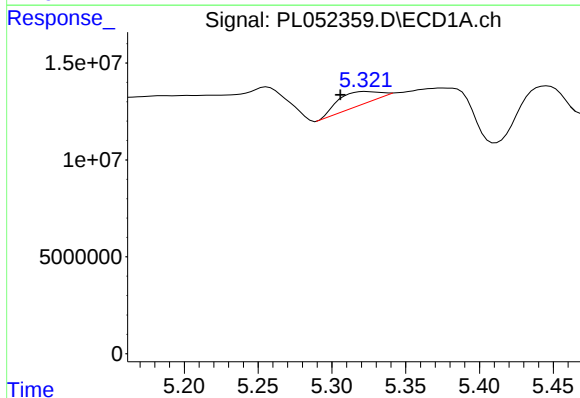


#9 Endosulfan I

R.T.: 5.323 min
Delta R.T.: 0.017 min
Response: 12760842
Conc: 0.95 ng/ml

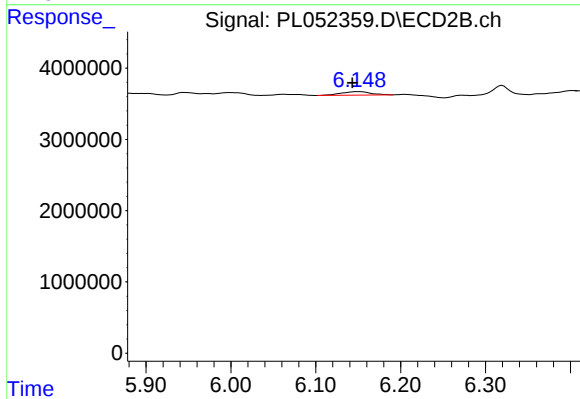

#9 Endosulfan I


R.T.: 6.151 min
Delta R.T.: 0.008 min
Response: 1176481
Conc: 0.36 ng/ml

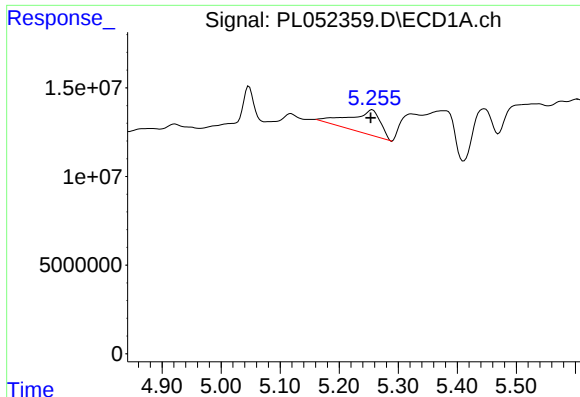

#11 alpha-Chlordane


R.T.: 5.256 min
Delta R.T.: 0.003 min
Response: 49425865
Conc: 3.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

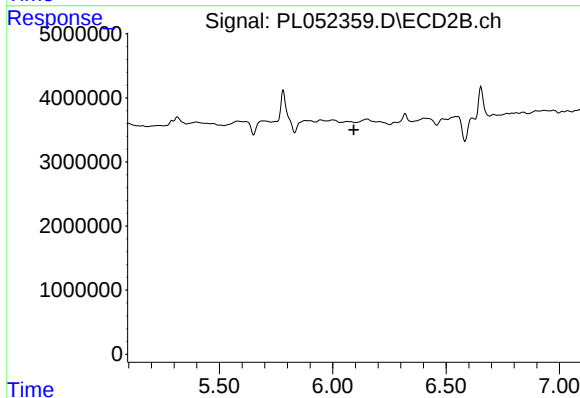


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

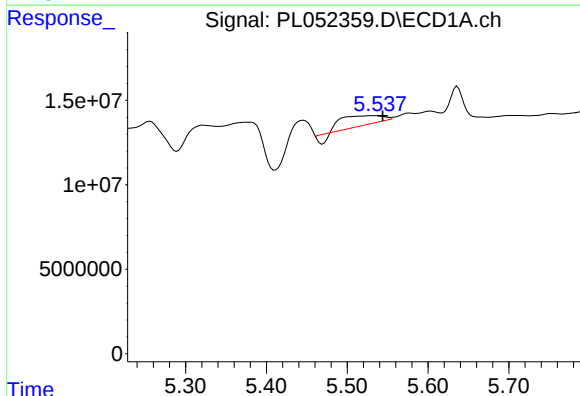


#13 Dieldrin

R.T.: 5.539 min
Delta R.T.: -0.005 min
Response: 17306317
Conc: 1.14 ng/ml

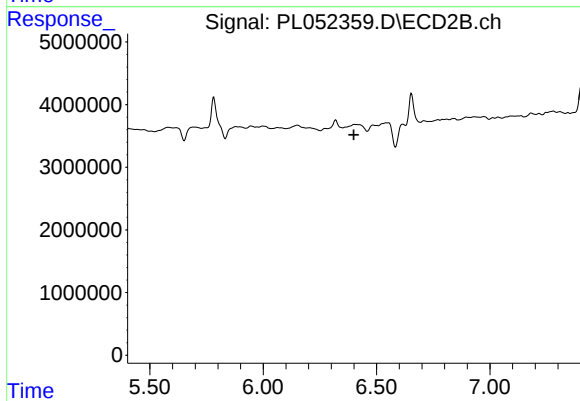

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

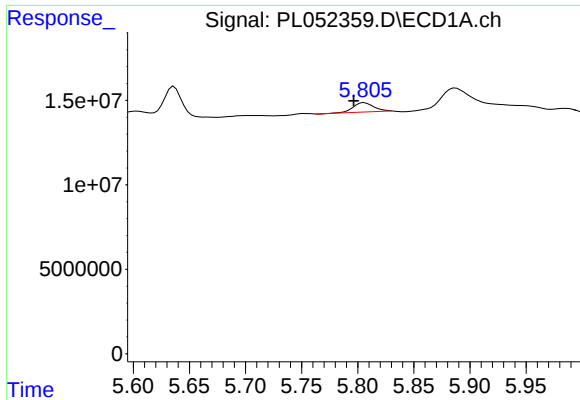

#14 Endrin


R.T.: 5.806 min
Delta R.T.: 0.010 min
Response: 7165950
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

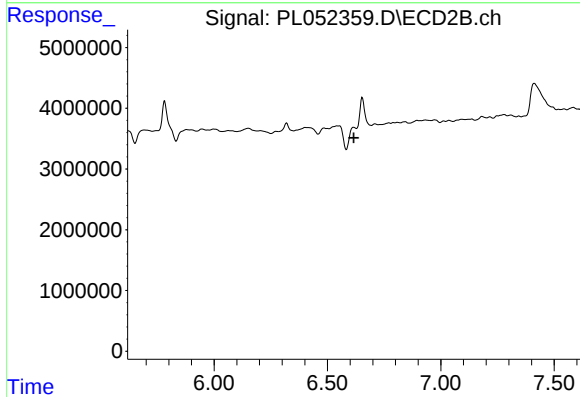


#14 Endrin

R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: -1348910
Conc: N.D.

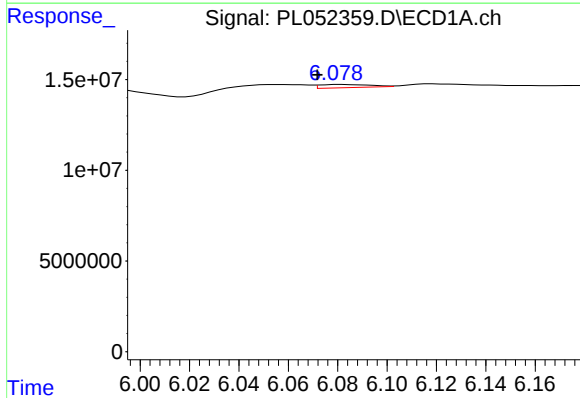


#15 Endosulfan II

R.T.: 6.082 min
Delta R.T.: 0.010 min
Response: 2457819
Conc: 0.18 ng/ml

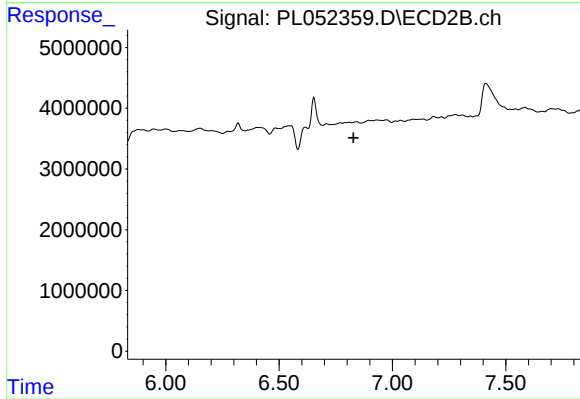

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.829 min
Response: 0
Conc: N.D.

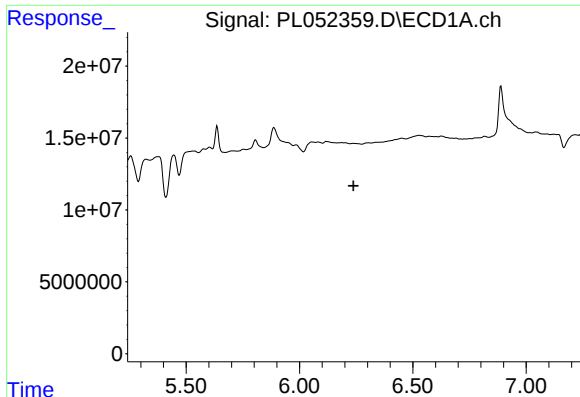

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

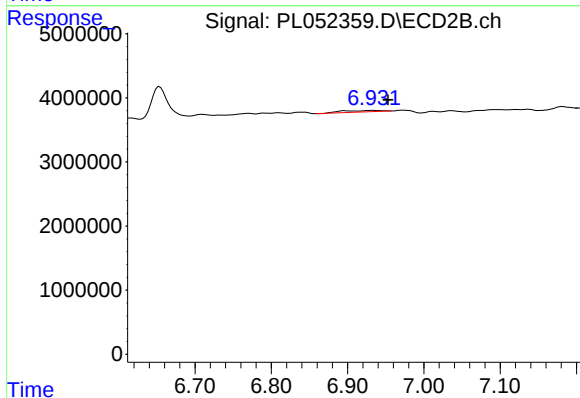


#18 Endrin aldehyde

R.T.: 6.932 min
Delta R.T.: -0.021 min
Response: 792450
Conc: 0.28 ng/ml

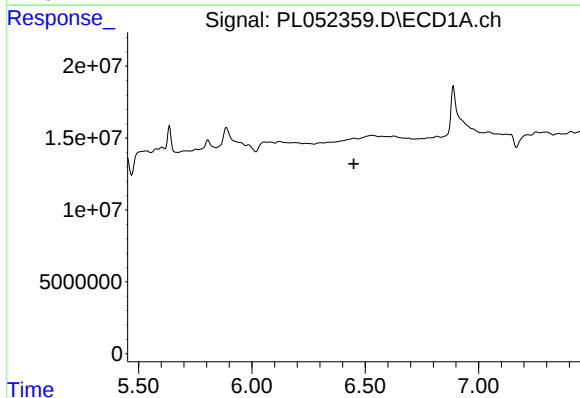


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.449 min
Response: 0
Conc: N.D.

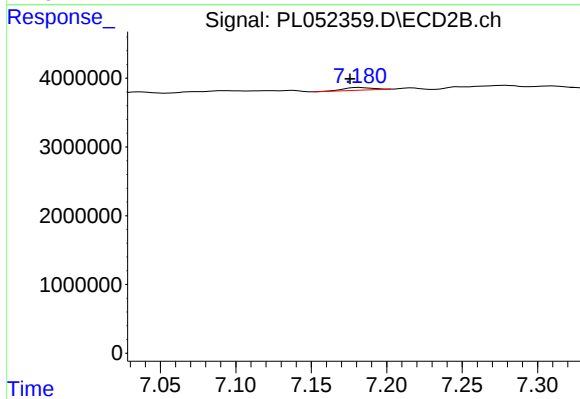

#19 Endosulfan Sulfate


R.T.: 7.182 min
Delta R.T.: 0.006 min
Response: 487963
Conc: 0.16 ng/ml

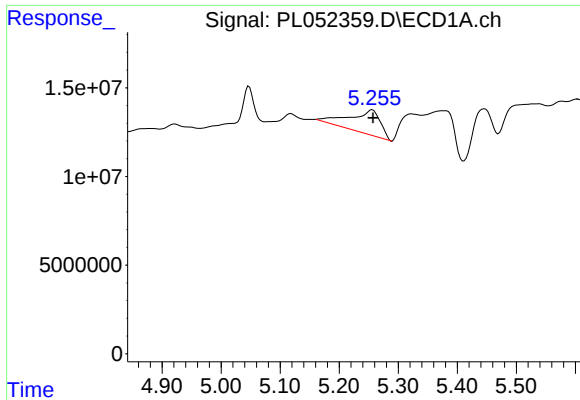

#26 Chlordane-4


R.T.: 5.256 min
Delta R.T.: -0.001 min
Response: 49425865
Conc: 40.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

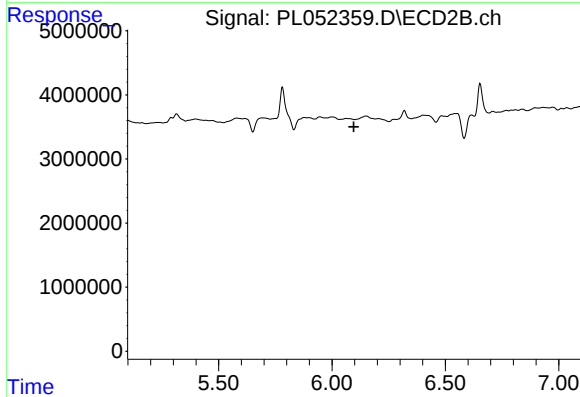


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

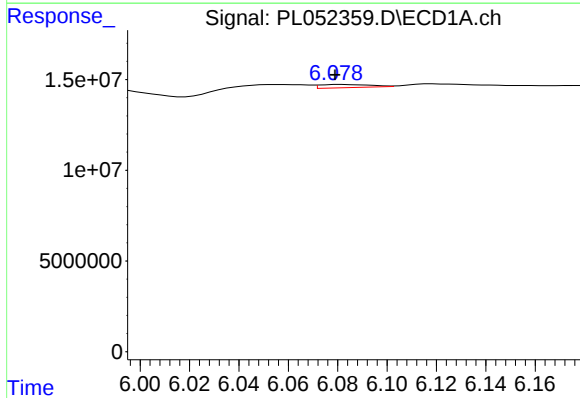


#27 Chlordane-5

R.T.: 6.082 min
Delta R.T.: 0.003 min
Response: 2457819
Conc: 5.01 ng/ml

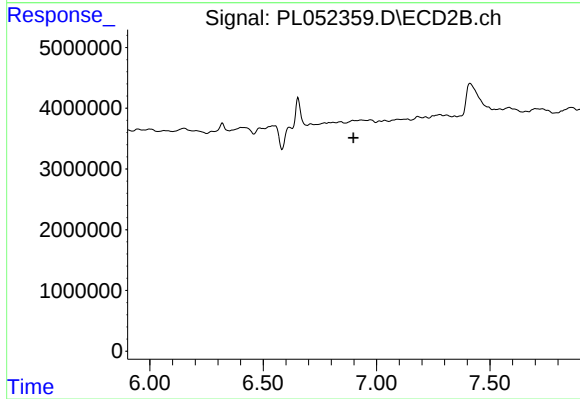

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.898 min
Response: 0
Conc: N.D.

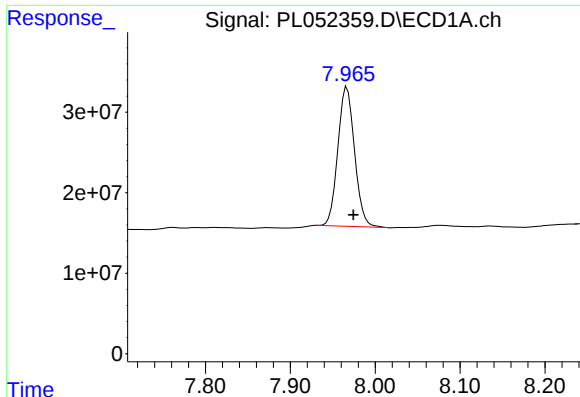

#28 Decachlorobiphenyl


R.T.: 7.967 min

Delta R.T.: -0.008 min

Response: 236860094

Conc: 19.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

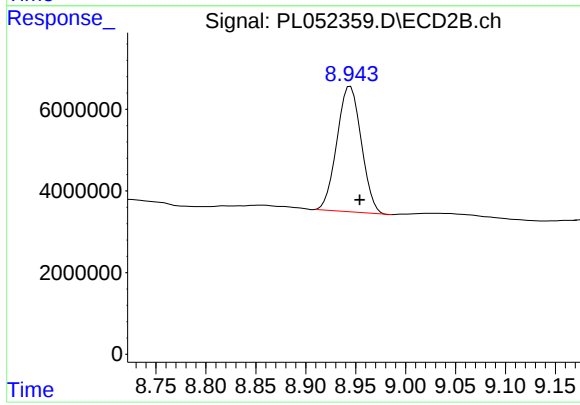

#28 Decachlorobiphenyl

R.T.: 8.945 min

Delta R.T.: -0.009 min

Response: 52209643

Conc: 17.15 ng/ml