

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091019\
 Data File : PL052343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 16:27
 Operator : SG\AJ
 Sample : K4738-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-01-H02-H03-H02A-H03A

Manual Integrations
 APPROVED

Ankita
 9/11/2019 11:04:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 00:49:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.922	212.3E6	54707826	24.804	25.040
28)	SA Decachlor...	7.967	8.943	250.5E6	57611199	20.636	18.927m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091019\
Data File : PL052343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 16:27
Operator : SG\AJ
Sample : K4738-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-H02-H03-H02A-H03A


Manual Integrations
APPROVED

Ankita
9/11/2019 11:04:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 00:49:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

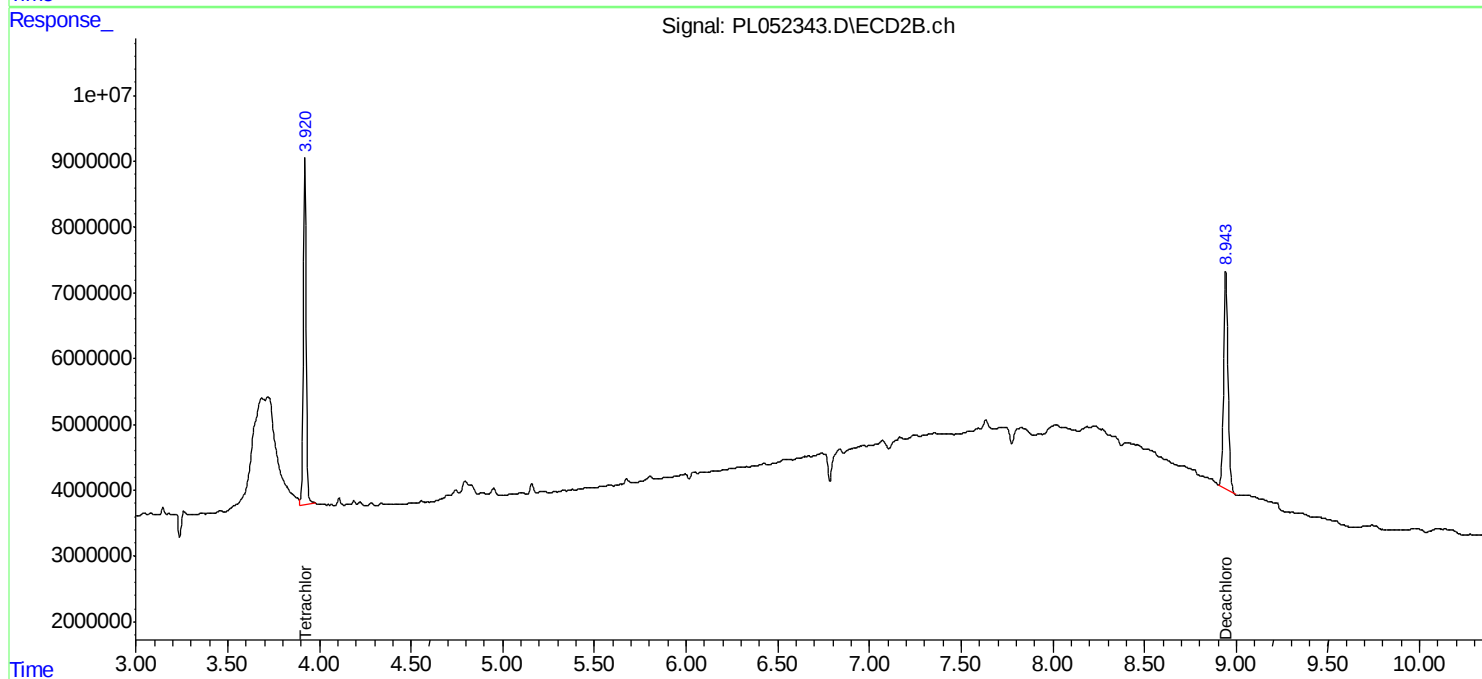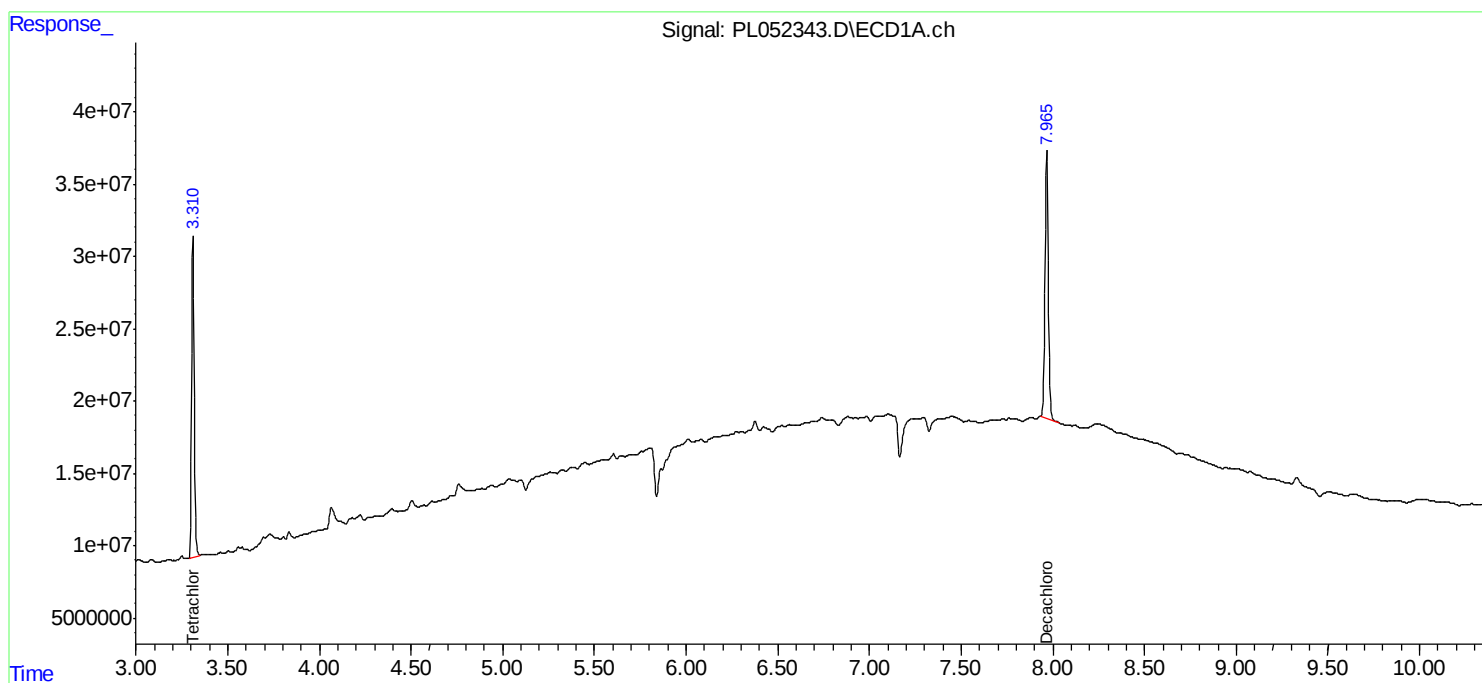

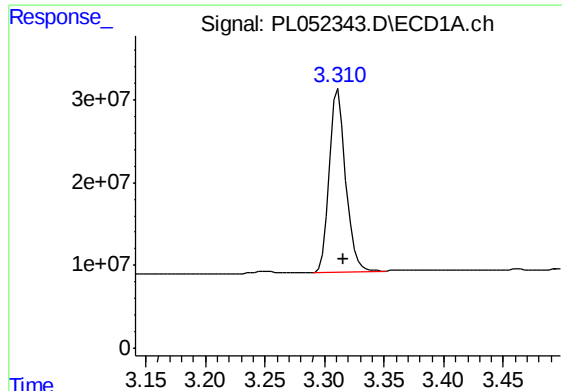


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 212288448
Conc: 24.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-H02-H03-H02A-H03A


Manual Integrations
APPROVED

Ankita
9/11/2019 11:04:20 AM

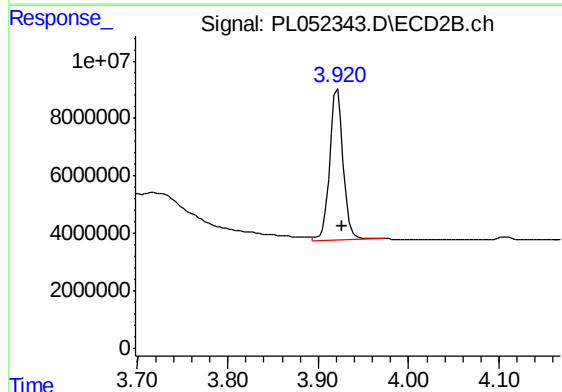


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.005 min
Response: 54707826
Conc: 25.04 ng/ml

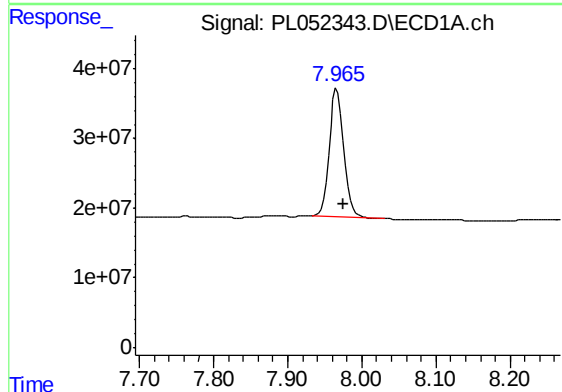

#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.008 min
Response: 250477345
Conc: 20.64 ng/ml

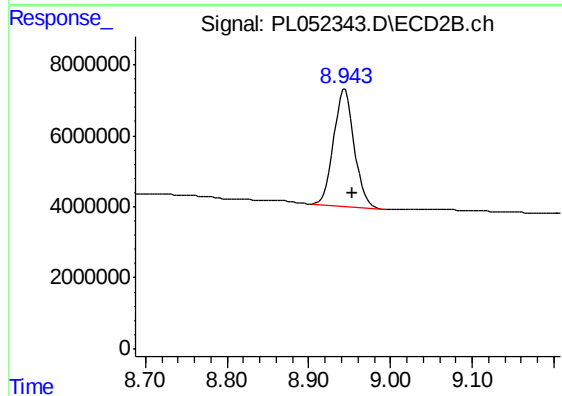

#28 Decachlorobiphenyl

R.T.: 8.943 min
Delta R.T.: -0.011 min
Response: 57611199
Conc: 18.93 ng/ml m