

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091021\
 Data File : PL069794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 13:25
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 15:16:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 10 15:15:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.563	54290580	131.4E6	108.708	106.040
28)	SA Decachlor...	10.402	11.491	64720980	110.4E6	92.109	98.631
Target Compounds							
23)	Chlordane-1	5.962	6.949	16971812	45930850	1107.811	1117.877
24)	Chlordane-2	6.651	7.541	22636295	50926549	1004.064	1034.839
25)	Chlordane-3	7.352	8.299	65136254	193.5E6	1074.357	1053.766
26)	Chlordane-4	7.420	8.382	69340211	238.6E6	1070.655	1063.606
27)	Chlordane-5	8.369	9.270	24178119	40882220	1035.554	1050.943



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091021\
Data File : PL069794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 13:25
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 15:16:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Fri Sep 10 15:15:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

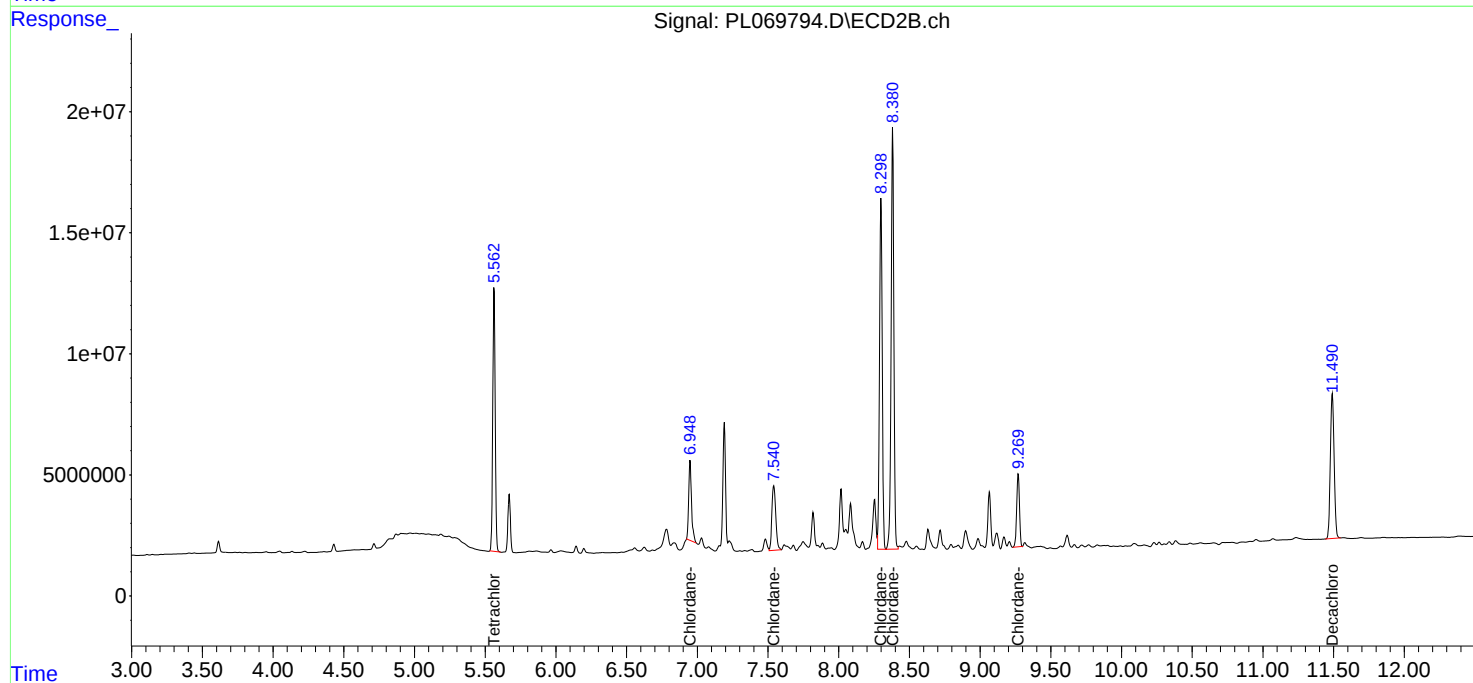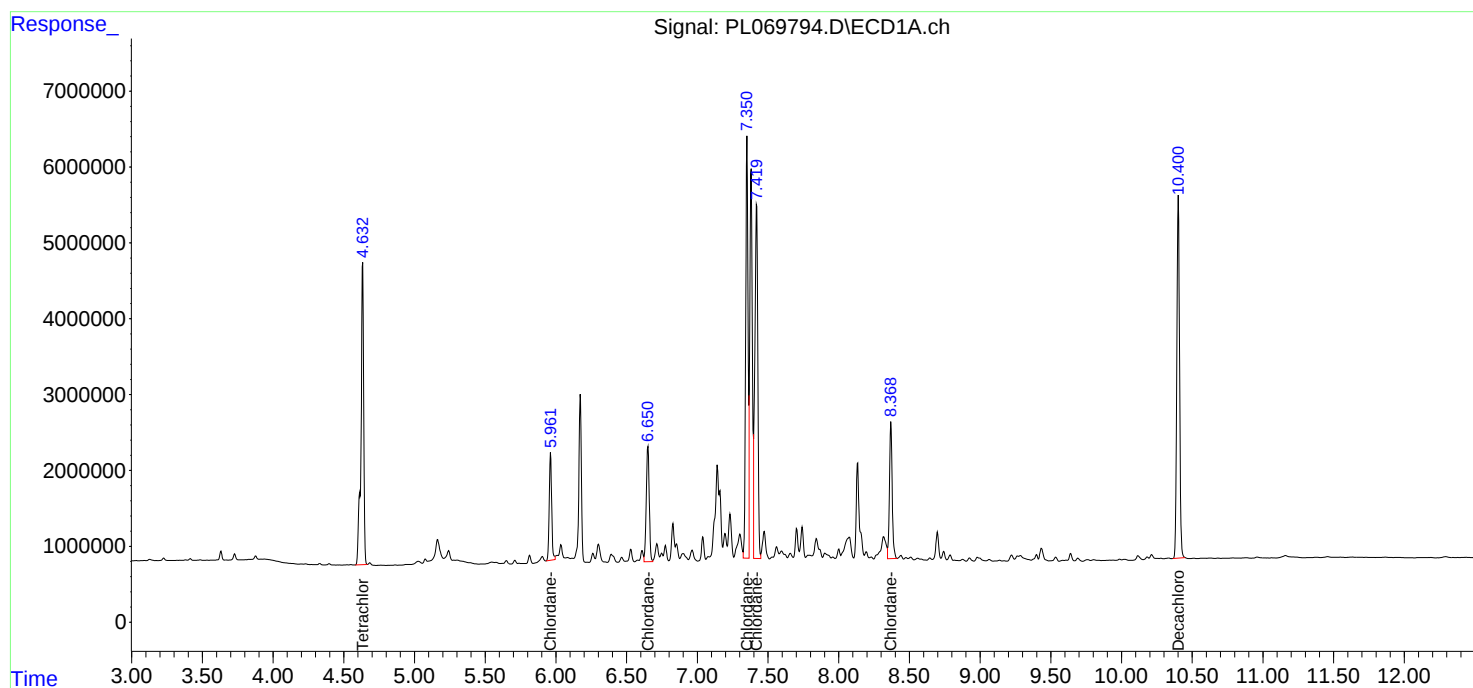


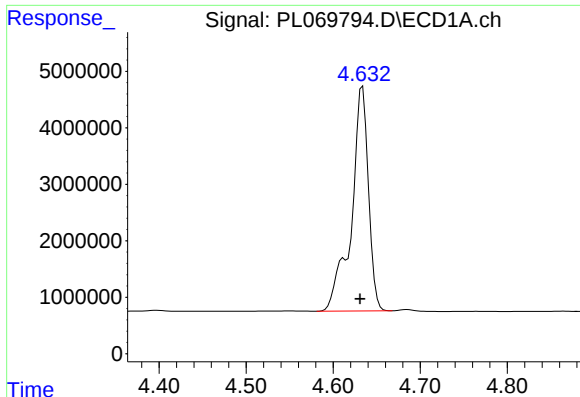

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.003 min
Response: 54290580
Conc: 108.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

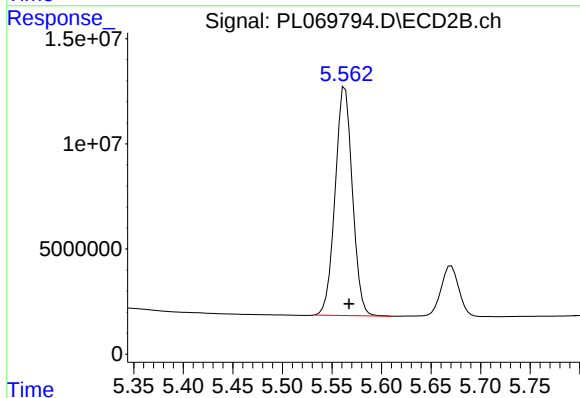


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 131415005
Conc: 106.04 ng/ml

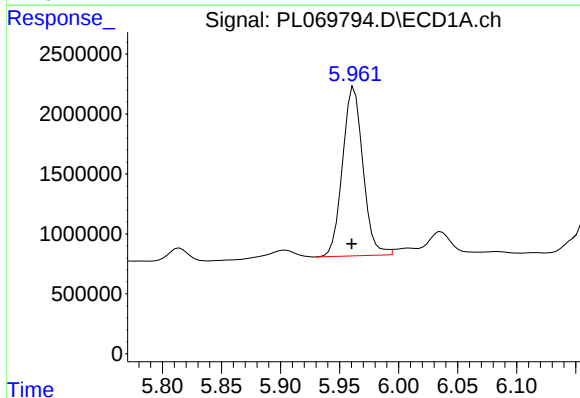


#23 Chlordane-1

R.T.: 5.962 min
Delta R.T.: 0.002 min
Response: 16971812
Conc: 1107.81 ng/ml

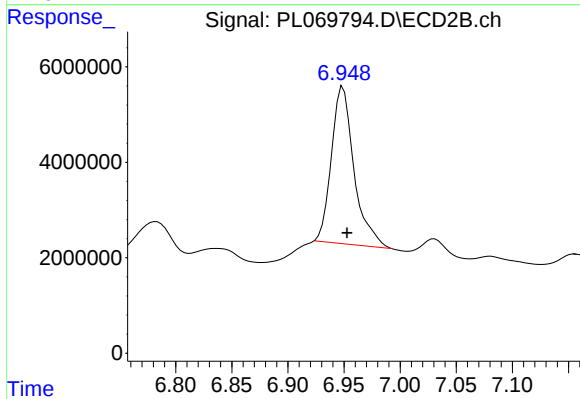

#23 Chlordane-1


R.T.: 6.949 min
Delta R.T.: -0.003 min
Response: 45930850
Conc: 1117.88 ng/ml

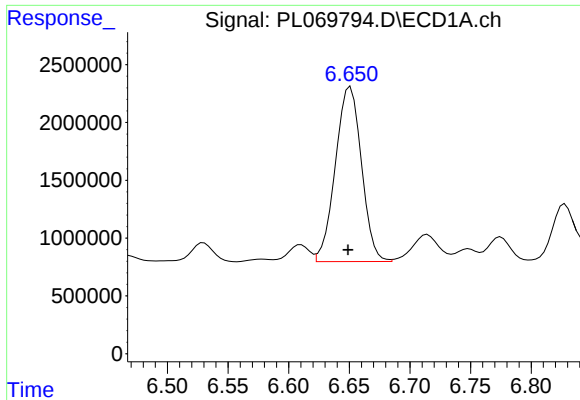

#24 Chlordane-2


R.T.: 6.651 min
Delta R.T.: 0.002 min
Response: 22636295
Conc: 1004.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

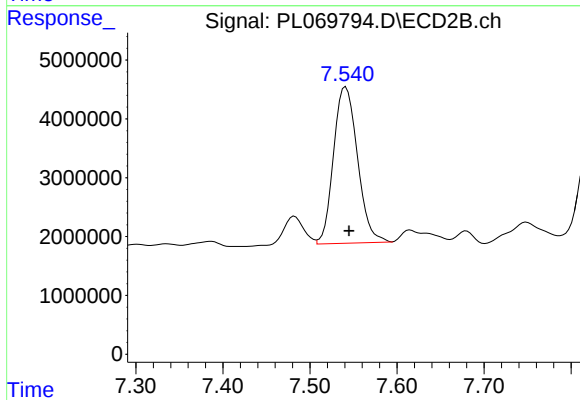


#24 Chlordane-2

R.T.: 7.541 min
Delta R.T.: -0.003 min
Response: 50926549
Conc: 1034.84 ng/ml

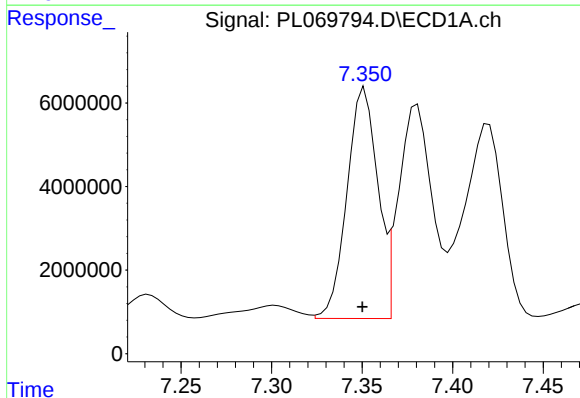


#25 Chlordane-3

R.T.: 7.352 min
Delta R.T.: 0.001 min
Response: 65136254
Conc: 1074.36 ng/ml

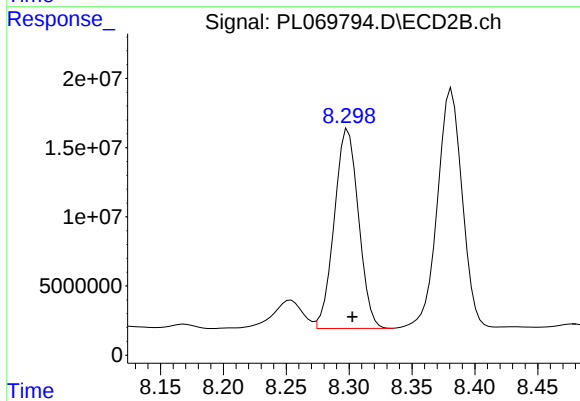

#25 Chlordane-3


R.T.: 8.299 min
Delta R.T.: -0.003 min
Response: 193460022
Conc: 1053.77 ng/ml

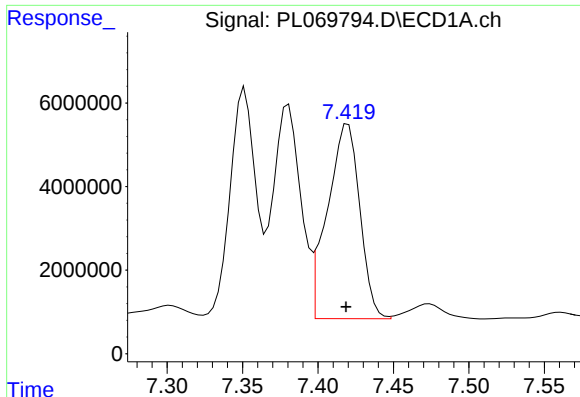

#26 Chlordane-4


R.T.: 7.420 min
Delta R.T.: 0.001 min
Response: 69340211
Conc: 1070.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

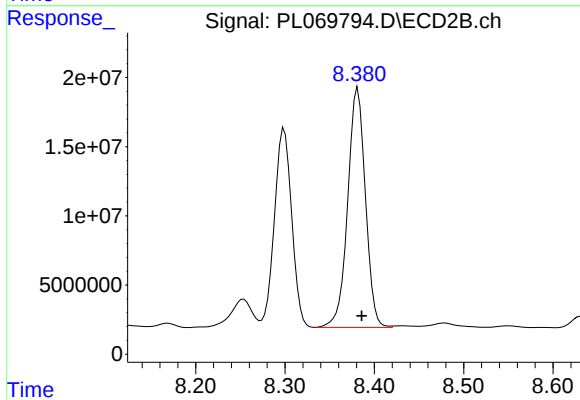


#26 Chlordane-4

R.T.: 8.382 min
Delta R.T.: -0.004 min
Response: 238639575
Conc: 1063.61 ng/ml

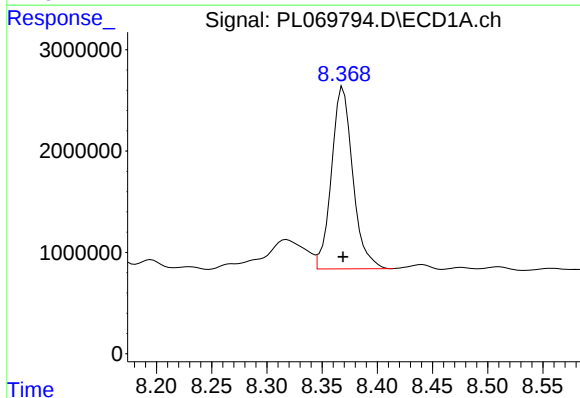


#27 Chlordane-5

R.T.: 8.369 min
Delta R.T.: 0.000 min
Response: 24178119
Conc: 1035.55 ng/ml

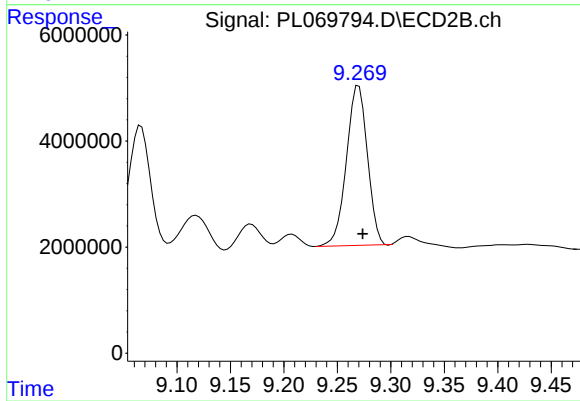

#27 Chlordane-5


R.T.: 9.270 min
Delta R.T.: -0.004 min
Response: 40882220
Conc: 1050.94 ng/ml

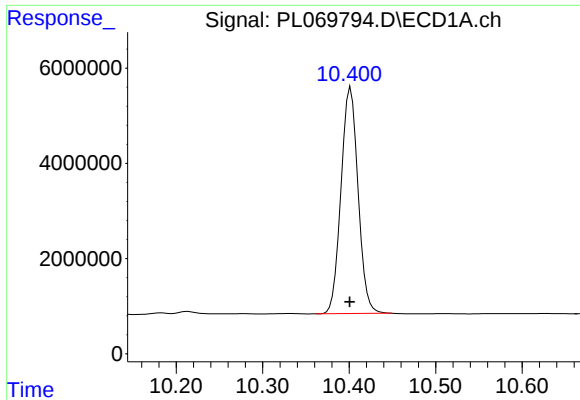

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 64720980
Conc: 92.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

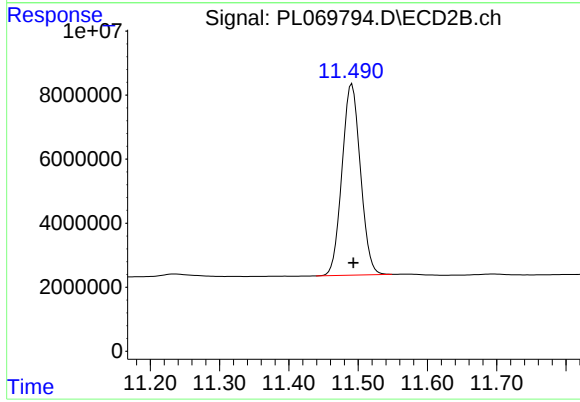

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.002 min
Response: 110389146
Conc: 98.63 ng/ml