

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091021\
 Data File : PL069795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 13:41
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 15:16:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 10 15:15:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.631	5.567	36426223	91824974	72.938	74.094
28)	SA Decachlor...	10.400	11.494	49889583	83076582	71.001	74.228
Target Compounds							
23)	Chlordane-1	5.961	6.953	11320583	31987487	738.935	778.520
24)	Chlordane-2	6.650	7.545	16319045	36758032	723.853	746.932
25)	Chlordane-3	7.351	8.303	45666392	141.2E6	753.221	768.841
26)	Chlordane-4	7.420	8.386	48602307	171.0E6	750.449	762.277
27)	Chlordane-5	8.370	9.274	17379310	29535107	744.360	759.247



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091021\
Data File : PL069795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 13:41
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 15:16:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Fri Sep 10 15:15:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

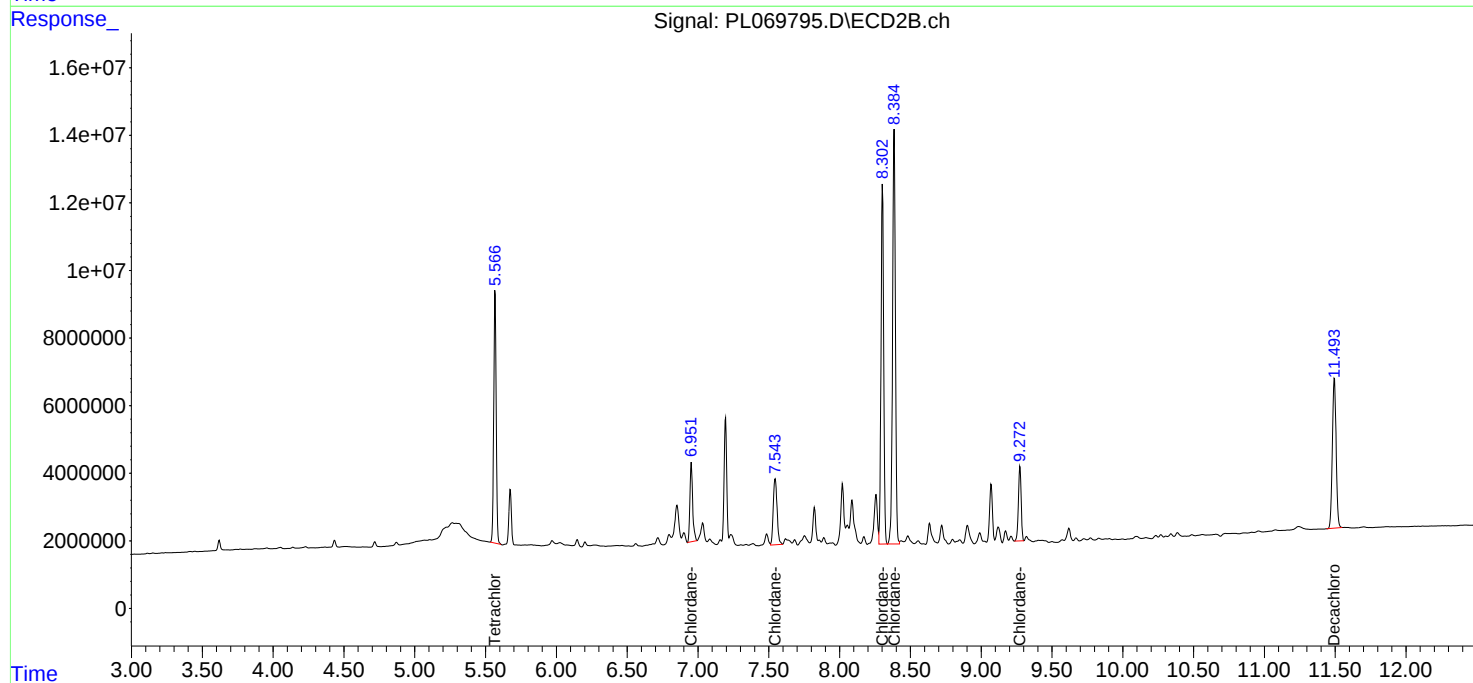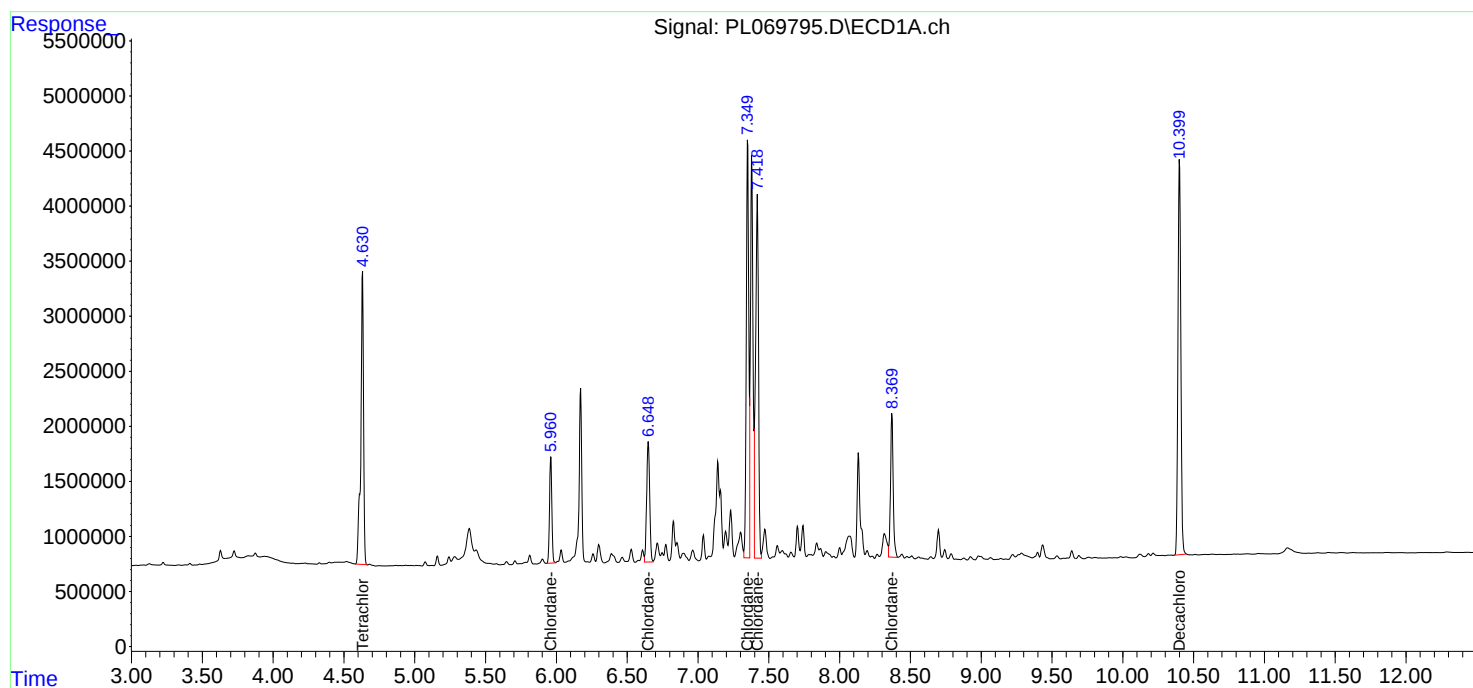


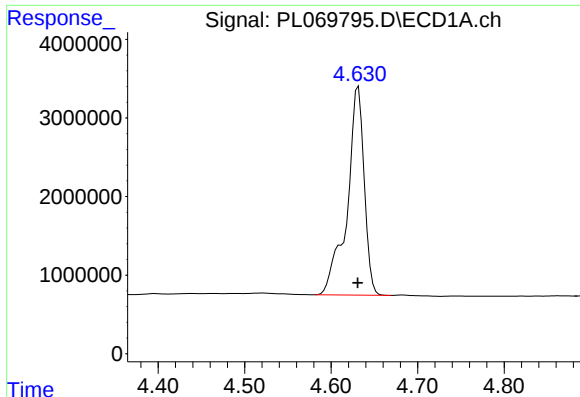

#1 Tetrachloro-m-xylene


R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 36426223
Conc: 72.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

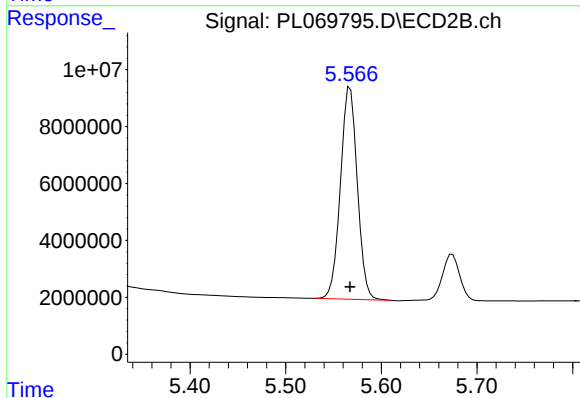


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 91824974
Conc: 74.09 ng/ml

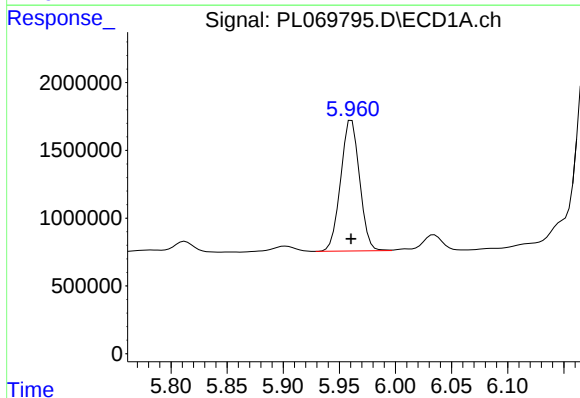


#23 Chlordane-1

R.T.: 5.961 min
Delta R.T.: 0.000 min
Response: 11320583
Conc: 738.94 ng/ml

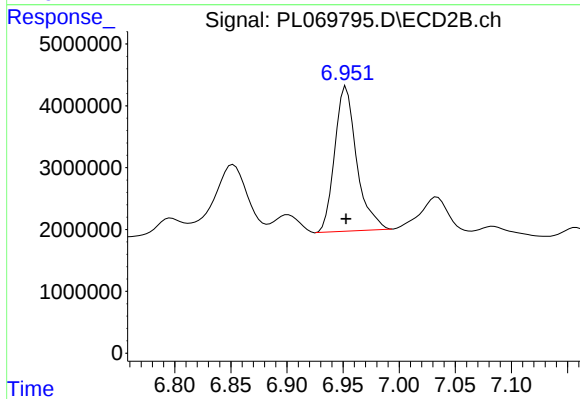

#23 Chlordane-1


R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 31987487
Conc: 778.52 ng/ml

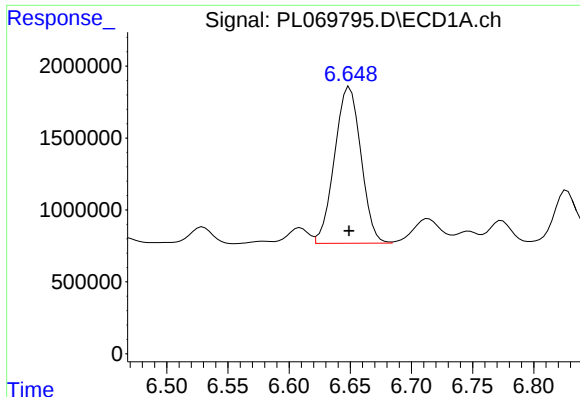

#24 Chlordane-2


R.T.: 6.650 min
Delta R.T.: 0.000 min
Response: 16319045
Conc: 723.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

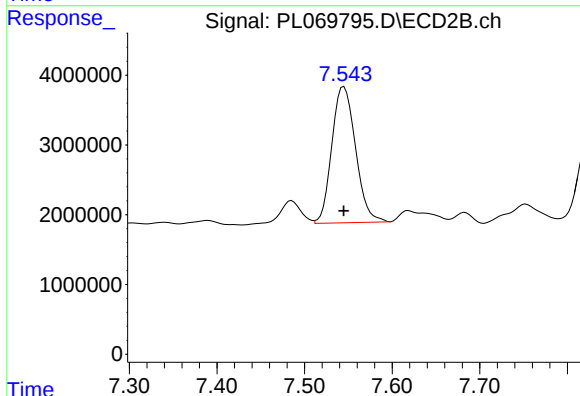


#24 Chlordane-2

R.T.: 7.545 min
Delta R.T.: 0.000 min
Response: 36758032
Conc: 746.93 ng/ml

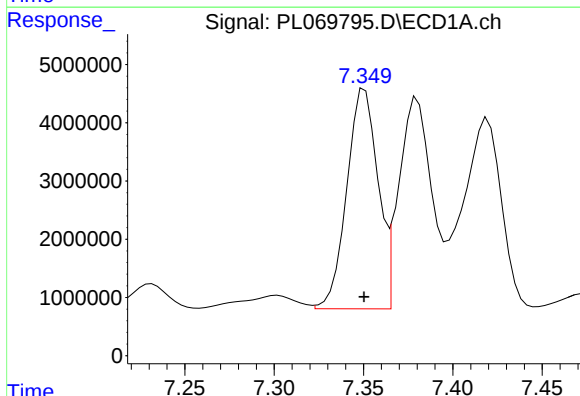


#25 Chlordane-3

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 45666392
Conc: 753.22 ng/ml

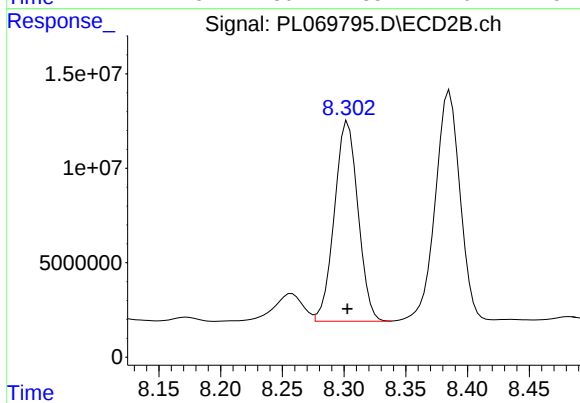

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 141150978
Conc: 768.84 ng/ml

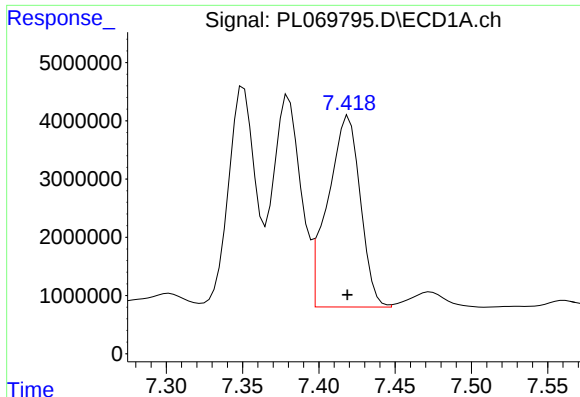

#26 Chlordane-4


R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 48602307
Conc: 750.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

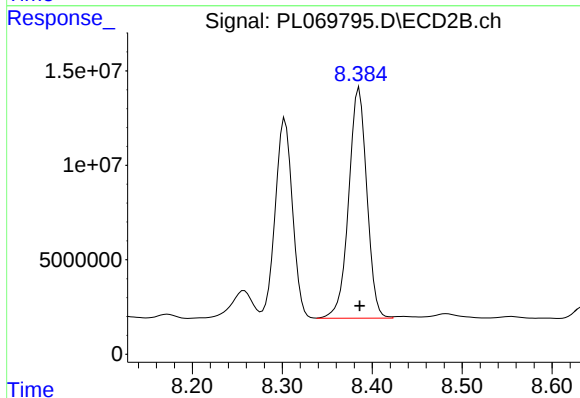


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 171030829
Conc: 762.28 ng/ml

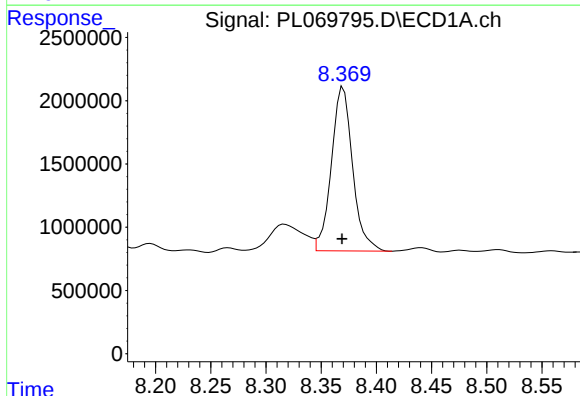


#27 Chlordane-5

R.T.: 8.370 min
Delta R.T.: 0.000 min
Response: 17379310
Conc: 744.36 ng/ml

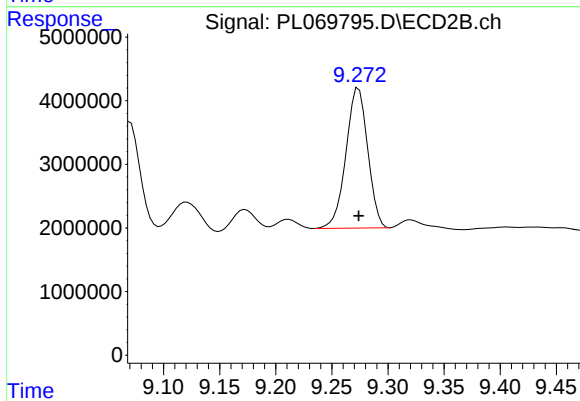

#27 Chlordane-5


R.T.: 9.274 min
Delta R.T.: 0.000 min
Response: 29535107
Conc: 759.25 ng/ml

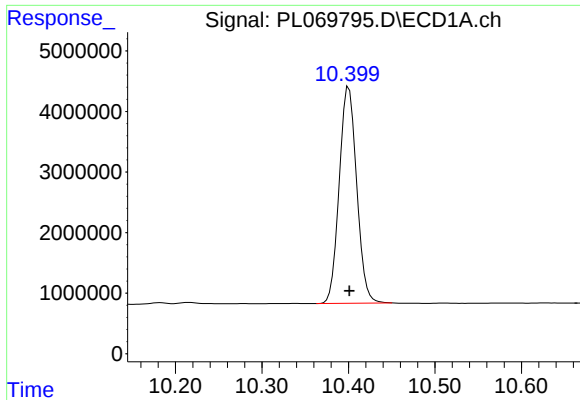

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: 0.000 min
Response: 49889583
Conc: 71.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

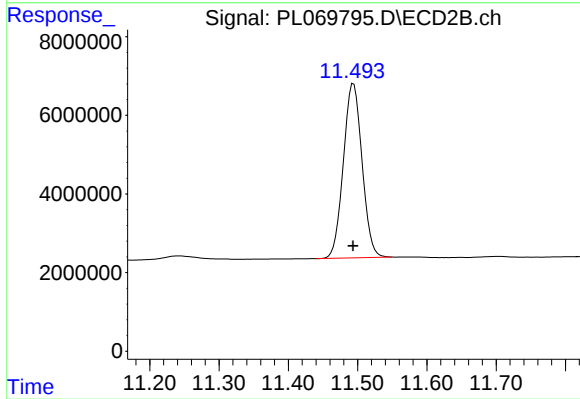

#28 Decachlorobiphenyl

R.T.: 11.494 min
Delta R.T.: 0.000 min
Response: 83076582
Conc: 74.23 ng/ml