

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091021\
 Data File : PL069805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 17:01
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL091021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 17:20:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 10 17:20:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.629	5.564	25489661	65293698	48.679	50.585
28)	SA Decachlor...	10.397	11.486	35011982	59744039	46.950	51.258
Target Compounds							
23)	Chlordane-1	5.957	6.949	7805100	22870436	483.831	557.178
24)	Chlordane-2	6.646	7.540	11585079	26065336	488.058	502.925
25)	Chlordane-3	7.346	8.298	31085918	99766462	496.369	525.944
26)	Chlordane-4	7.416	8.381	33310355	120.5E6	494.547	517.353
27)	Chlordane-5	8.365	9.269	11983875	20849217	483.568	495.800



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091021\
Data File : PL069805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 17:01
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL091021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 17:20:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Fri Sep 10 17:20:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

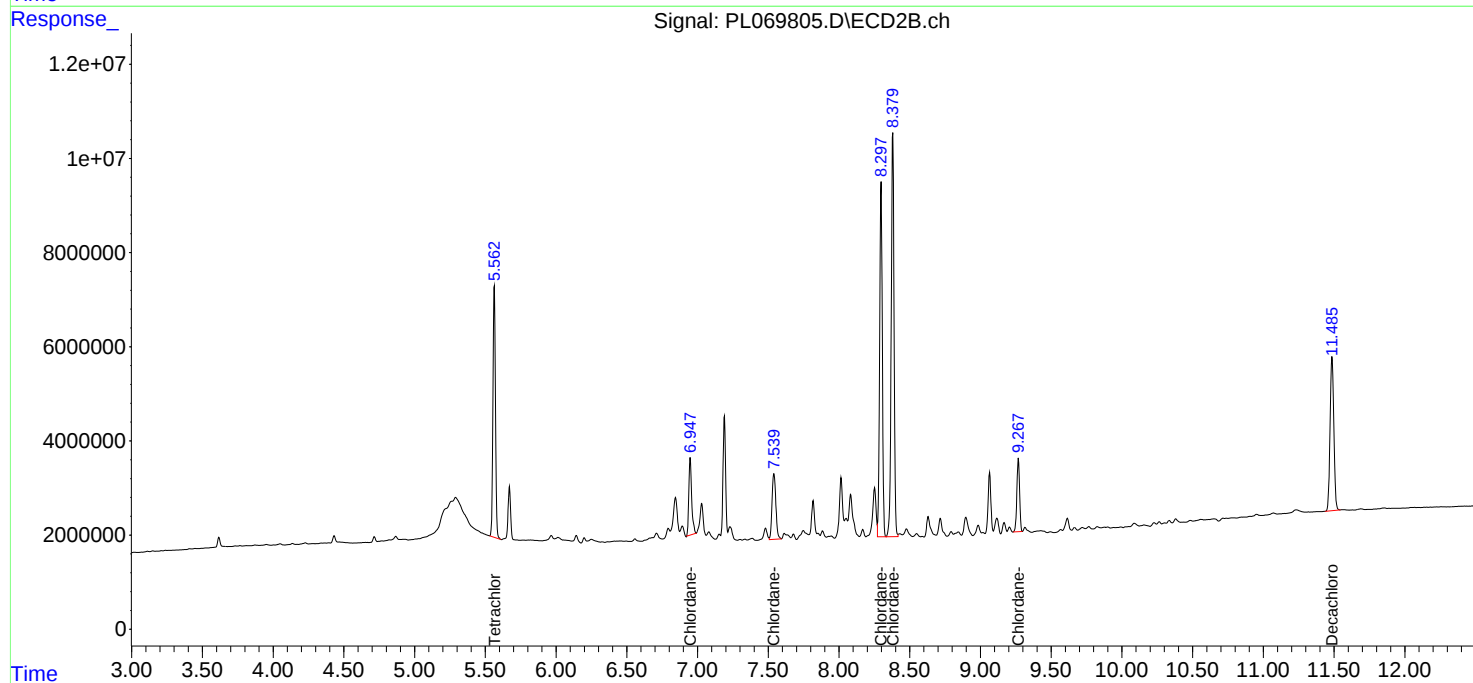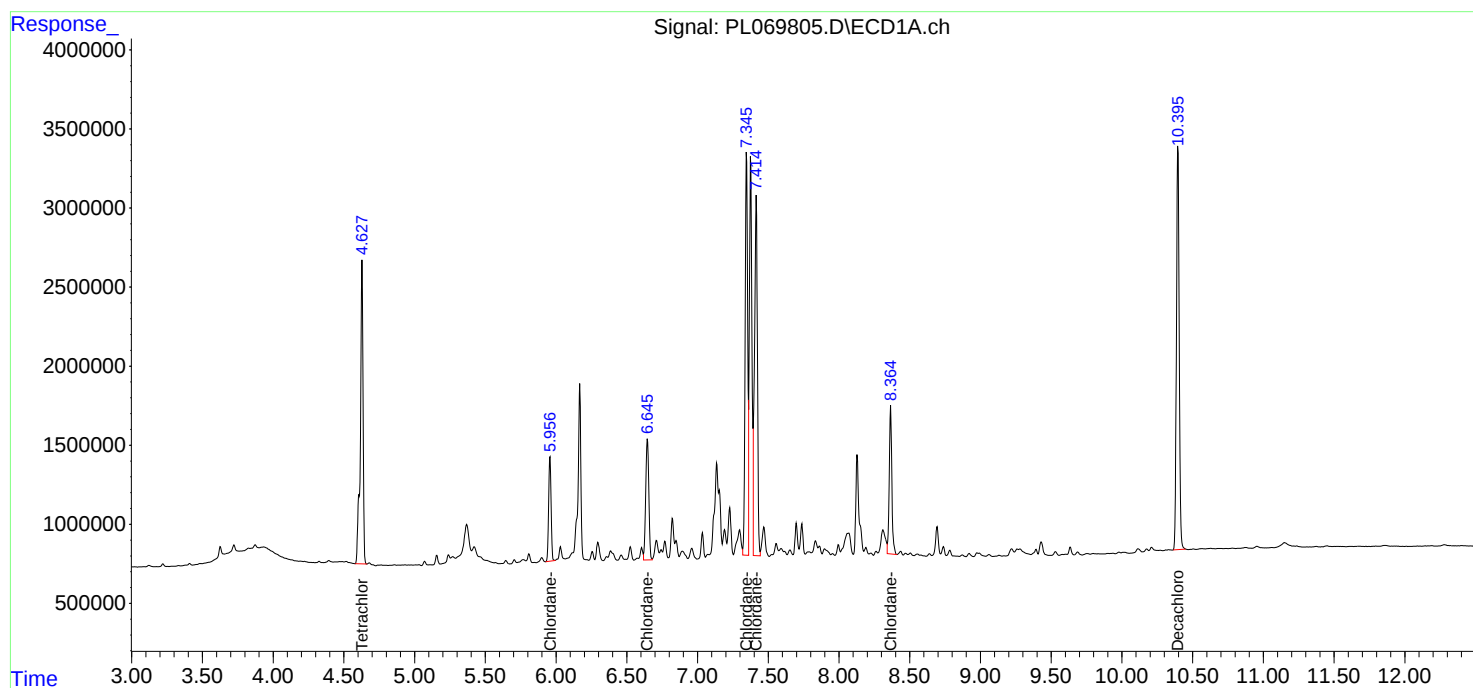


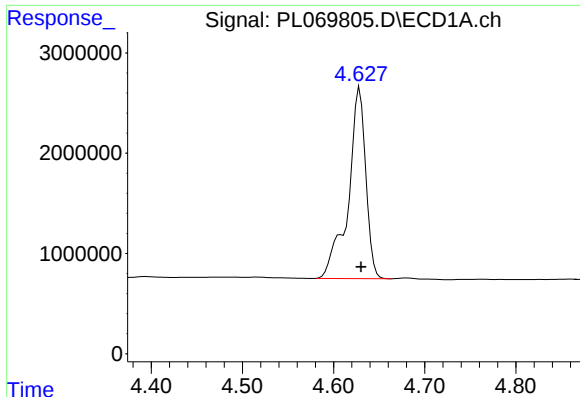

#1 Tetrachloro-m-xylene


R.T.: 4.629 min
Delta R.T.: -0.001 min
Response: 25489661
Conc: 48.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091021

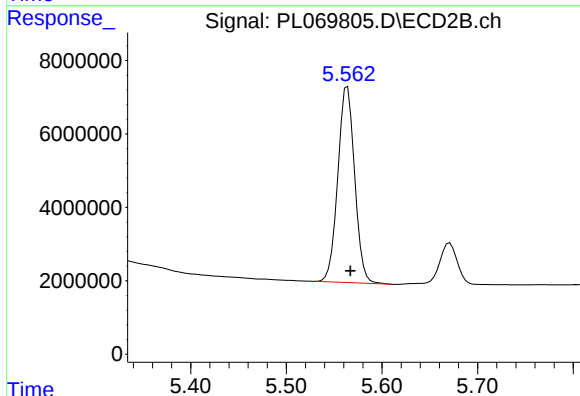


#1 Tetrachloro-m-xylene

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 65293698
Conc: 50.58 ng/ml

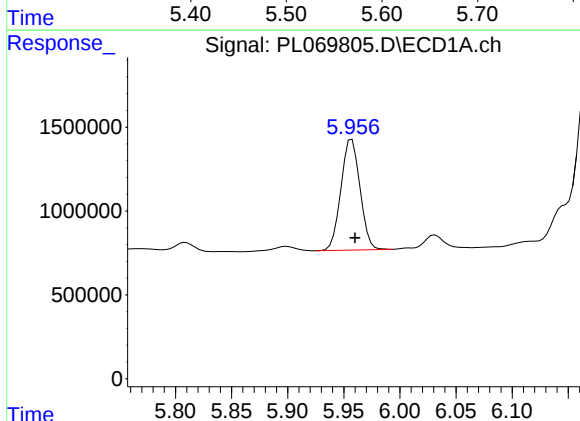


#23 Chlordane-1

R.T.: 5.957 min
Delta R.T.: -0.003 min
Response: 7805100
Conc: 483.83 ng/ml

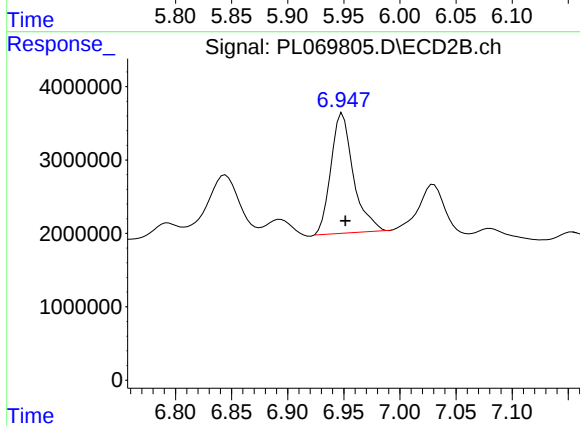

#23 Chlordane-1


R.T.: 6.949 min
Delta R.T.: -0.002 min
Response: 22870436
Conc: 557.18 ng/ml

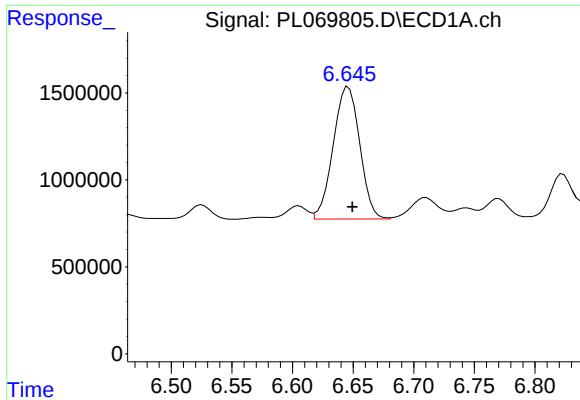

#24 Chlordane-2


R.T.: 6.646 min
Delta R.T.: -0.003 min
Response: 11585079
Conc: 488.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091021

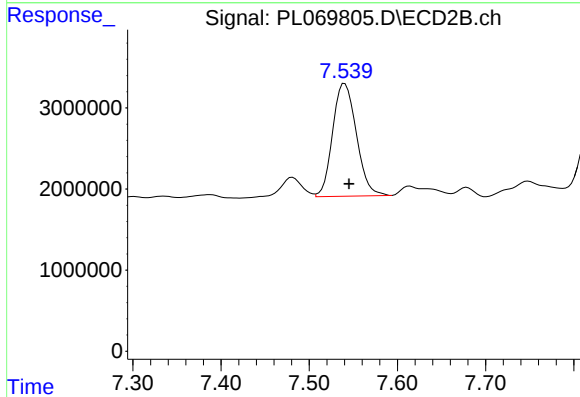


#24 Chlordane-2

R.T.: 7.540 min
Delta R.T.: -0.005 min
Response: 26065336
Conc: 502.92 ng/ml

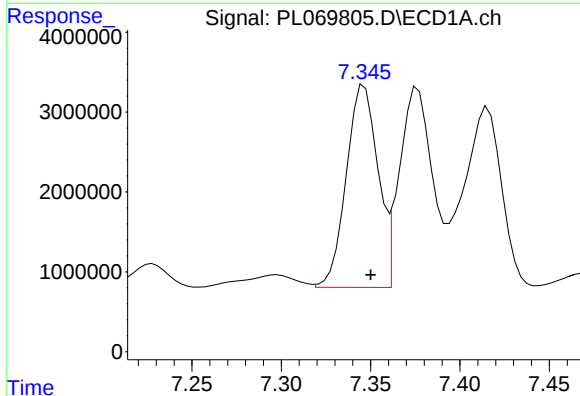


#25 Chlordane-3

R.T.: 7.346 min
Delta R.T.: -0.004 min
Response: 31085918
Conc: 496.37 ng/ml

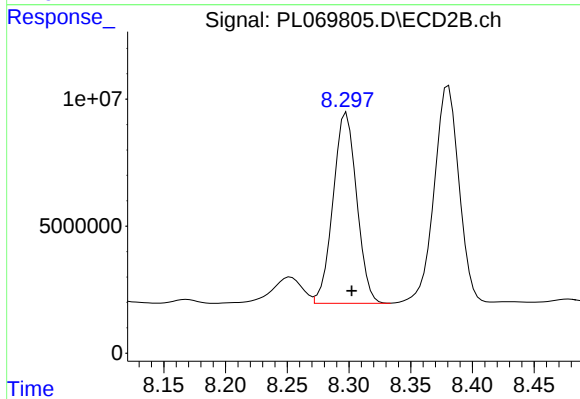

#25 Chlordane-3


R.T.: 8.298 min
Delta R.T.: -0.004 min
Response: 99766462
Conc: 525.94 ng/ml

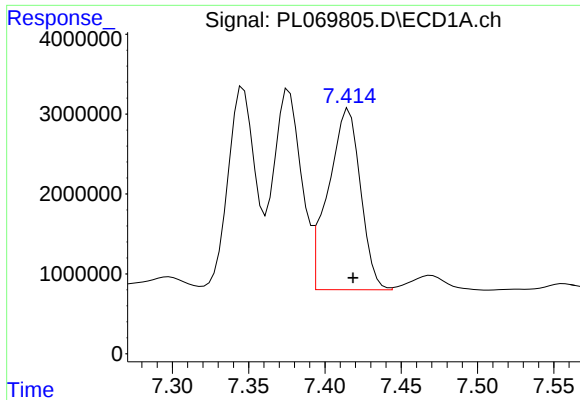

#26 Chlordane-4


R.T.: 7.416 min
Delta R.T.: -0.003 min
Response: 33310355
Conc: 494.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091021

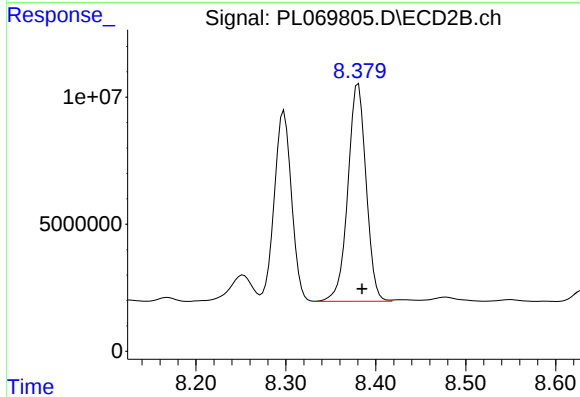


#26 Chlordane-4

R.T.: 8.381 min
Delta R.T.: -0.004 min
Response: 120471290
Conc: 517.35 ng/ml

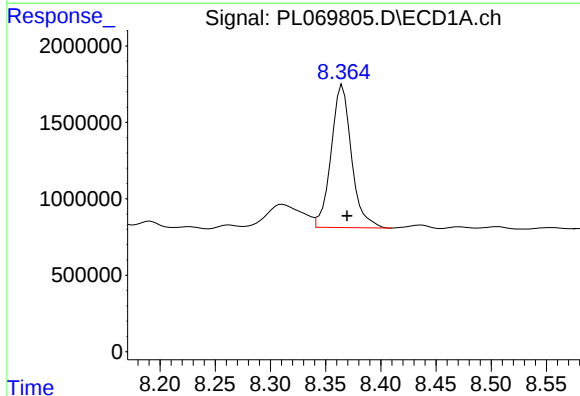


#27 Chlordane-5

R.T.: 8.365 min
Delta R.T.: -0.004 min
Response: 11983875
Conc: 483.57 ng/ml

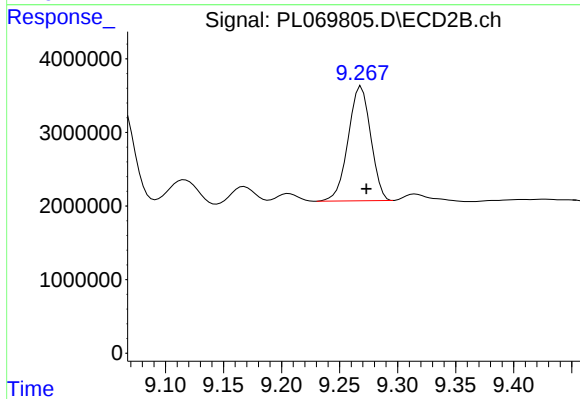

#27 Chlordane-5


R.T.: 9.269 min
Delta R.T.: -0.004 min
Response: 20849217
Conc: 495.80 ng/ml

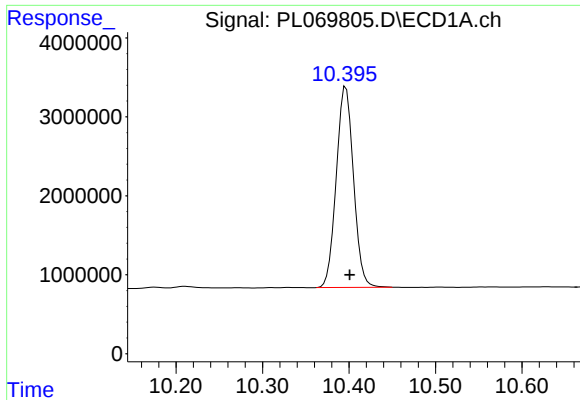

#28 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: -0.004 min
Response: 35011982
Conc: 46.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091021

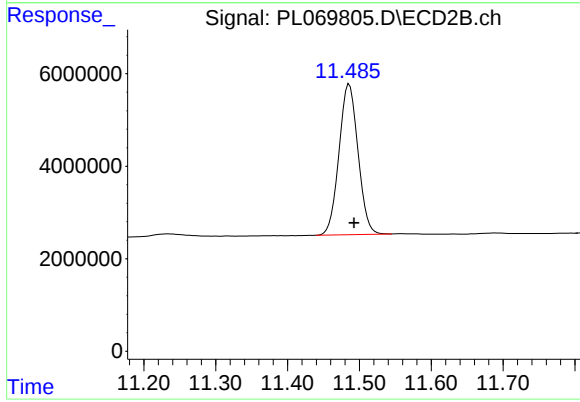

#28 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: -0.007 min
Response: 59744039
Conc: 51.26 ng/ml