

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091023\
 Data File : PL085205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 14:56
 Operator : AR\AJ
 Sample : PB155404BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB155404BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/11/2023
 Supervised By :Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 22:48:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.487	2.686	42727247	20506575	17.469	18.049
2) SA Decachlor...	9.040	7.870	33975726	24116294	21.128m	18.118

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091023\
Data File : PL085205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 14:56
Operator : AR\AJ
Sample : PB155404BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB155404BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/11/2023
Supervised By : Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 22:48:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

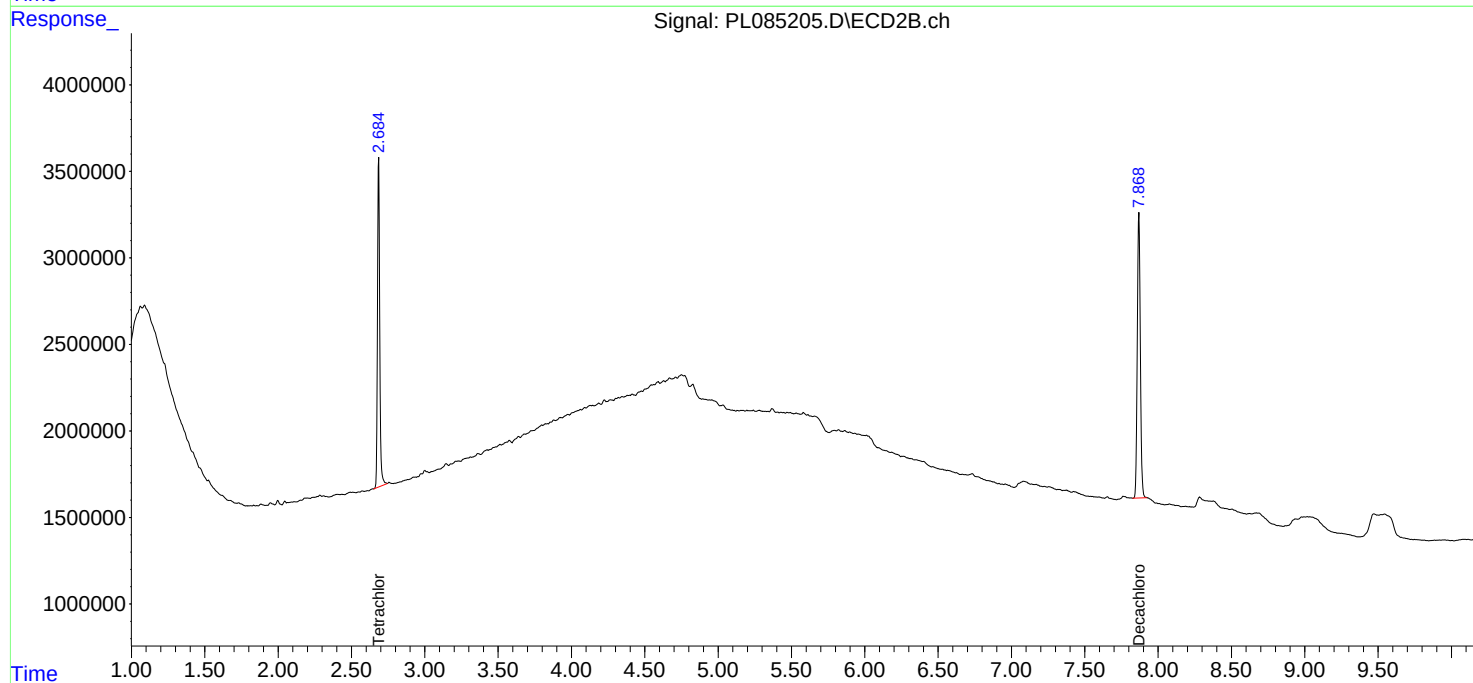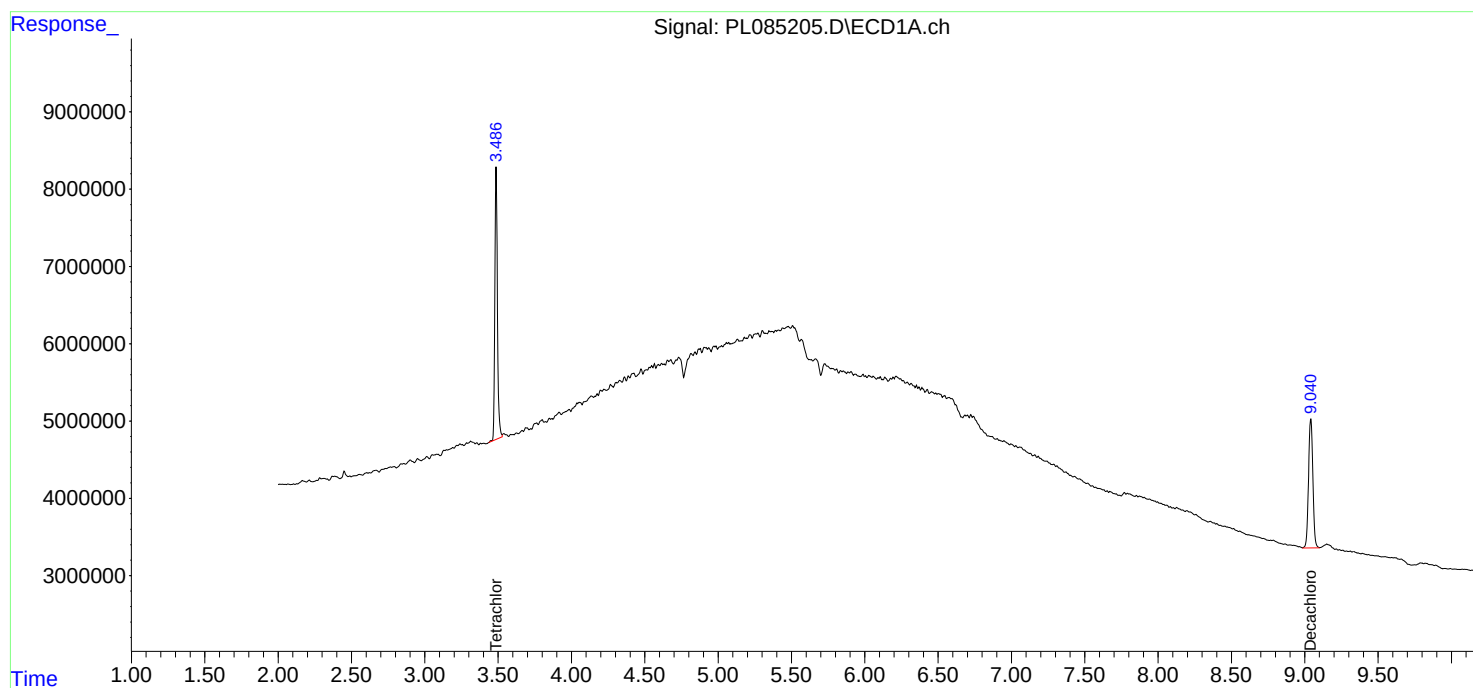

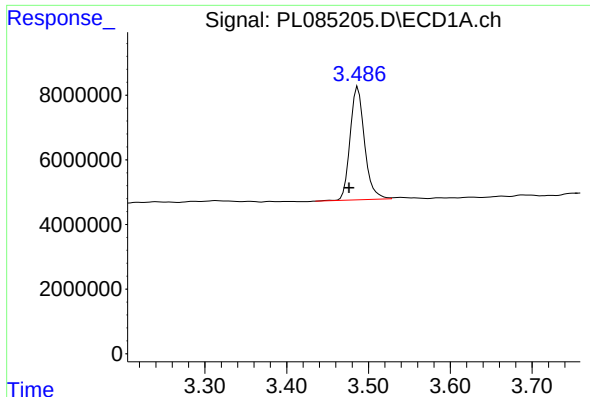


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.011 min
Response: 42727247
Conc: 17.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB155404BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/11/2023
Supervised By :Ankita Jodhani 09/11/2023

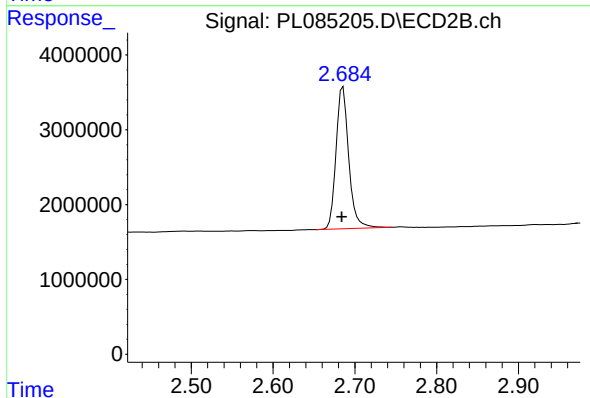


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.001 min
Response: 20506575
Conc: 18.05 ng/ml

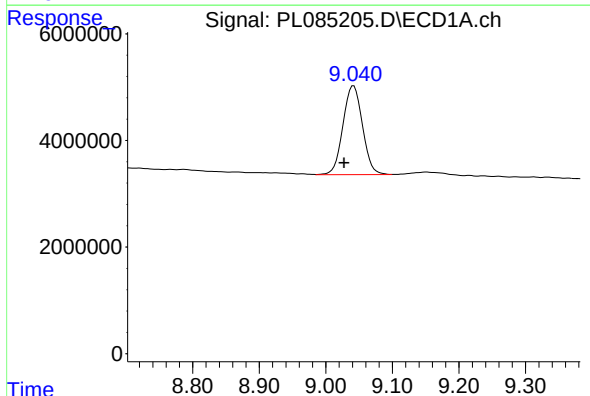

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.013 min
Response: 33975726
Conc: 21.13 ng/ml m

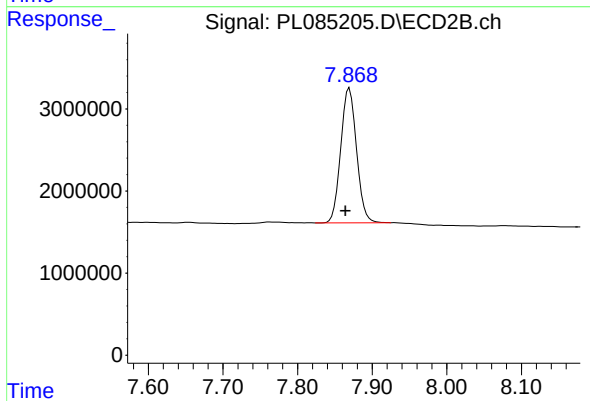

#28 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: 0.005 min
Response: 24116294
Conc: 18.12 ng/ml