

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091024\
 Data File : PL091622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2024 16:43
 Operator : AR\AJ
 Sample : P3845-13DL2 100X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-TXP-WPDL2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:36:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.783	0	895697	N.D.	0.479 #
28)	SA Decachlor...	0.000	7.921	0	1090215	N.D.	0.590 #
Target Compounds							
3)	MA gamma-BHC...	0.000	3.631	0	38319	N.D.	0.016 #
4)	MA Heptachlor	4.920	0.000	7095137	0	3.788	N.D. #
7)	B delta-BHC	0.000	4.145	0	265716	N.D.	0.115 #
8)	B Heptachlo...	0.000	4.736	0	133032	N.D.	0.063 #
9)	A Endosulfan I	0.000	5.130f	0	334939	N.D.	0.174 #
10)	B gamma-Chl...	0.000	4.984	0	699606	N.D.	0.317 #
12)	B 4,4'-DDE	0.000	5.232	0	989945	N.D.	0.522 #
13)	MA Dieldrin	0.000	5.363	0	522282	N.D.	0.254 #
14)	MA Endrin	0.000	5.662	0	561381	N.D.	0.297 #
15)	B Endosulfa...	6.769f	0.000	2731932	0	1.763	N.D. #
17)	MA 4,4'-DDT	0.000	6.052	0	2232339	N.D.	1.389 #
18)	B Endrin al...	0.000	6.139f	0	248291	N.D.	0.182 #
19)	B Endosulfa...	0.000	6.344	0	537998	N.D.	0.313 #
20)	A Methoxychlor	0.000	6.603f	0	1222565	N.D.	1.380 #
21)	B Endrin ke...	0.000	6.871f	0	143211	N.D.	0.071 #
22)	Mirex	0.000	7.041	0	4288530	N.D.	2.418 #
23)	Chlordane-1	0.000	3.765	0	487692	N.D.	7.011 #
25)	Chlordane-3	0.000	4.984	0	699606	N.D.	3.001 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091024\
Data File : PL091622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2024 16:43
Operator : AR\AJ
Sample : P3845-13DL2 100X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 05:36:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

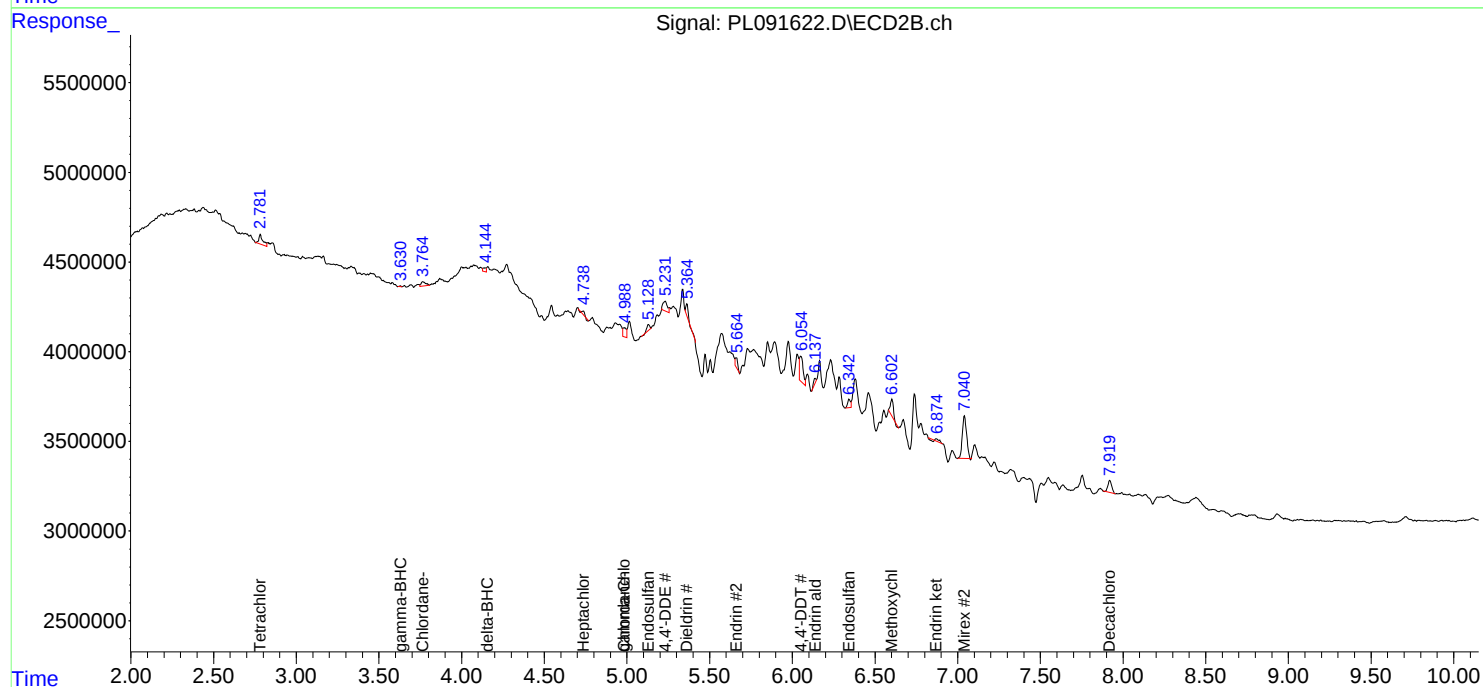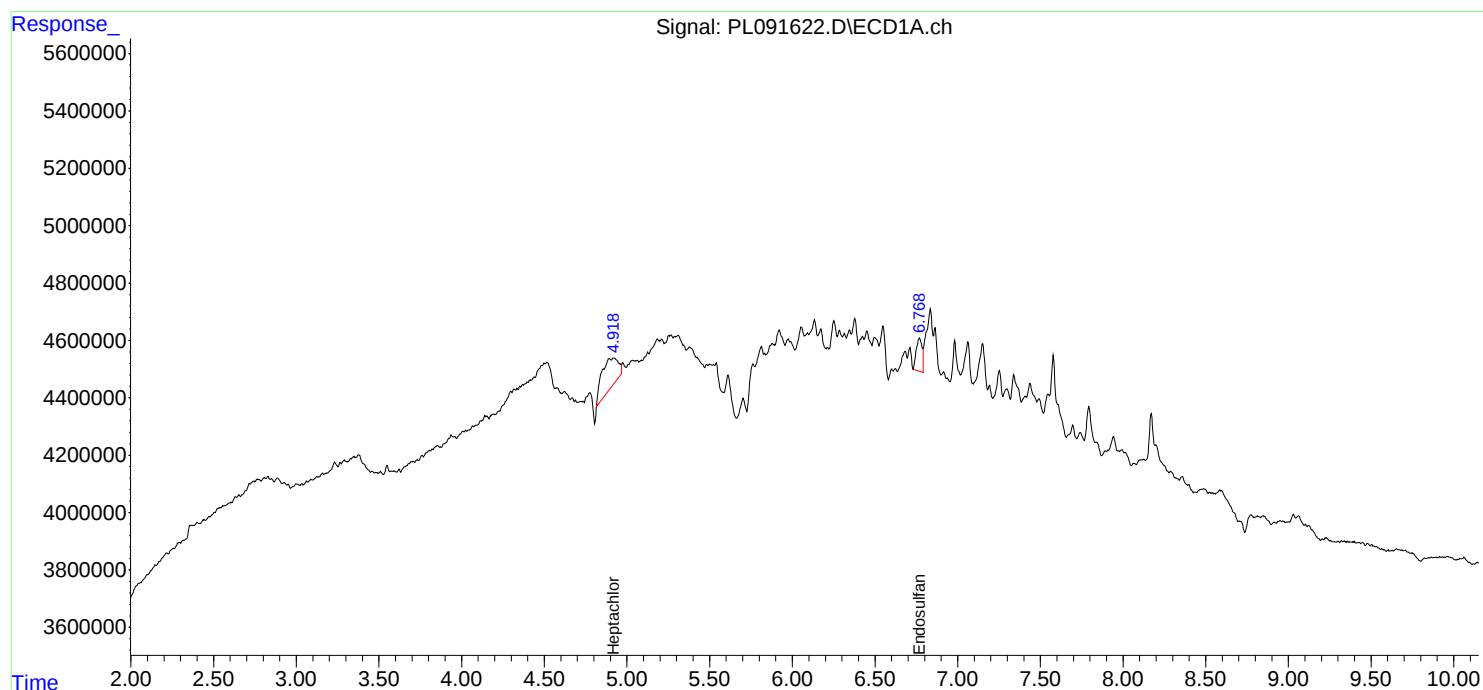


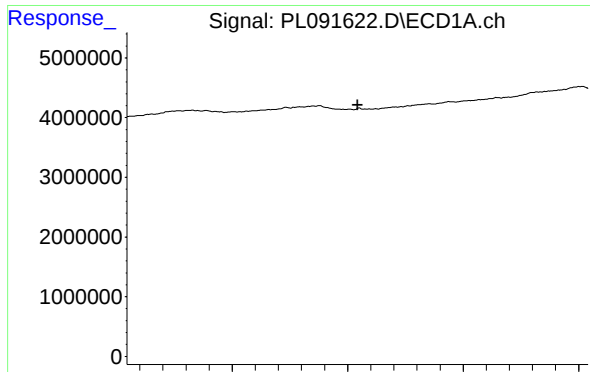

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

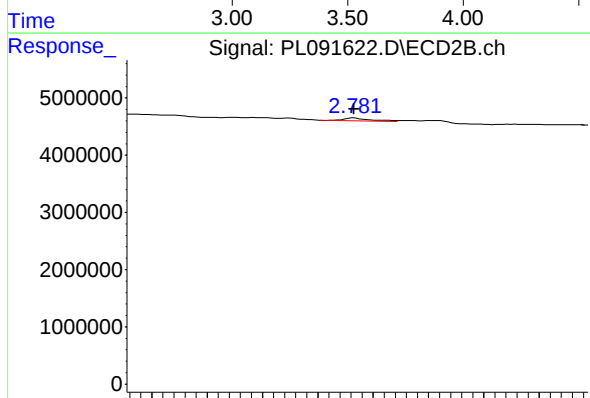


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 895697
Conc: 0.48 ng/ml

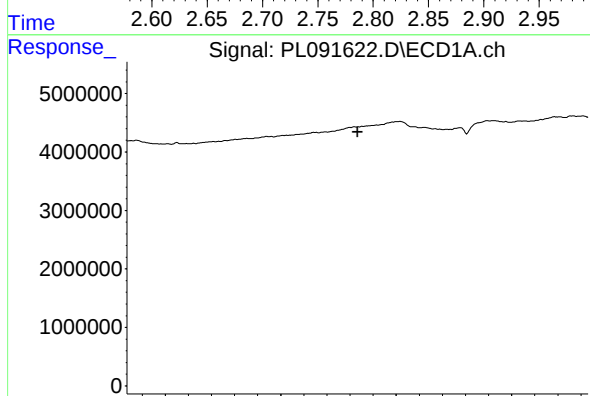


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.332 min
Response: 0
Conc: N.D.

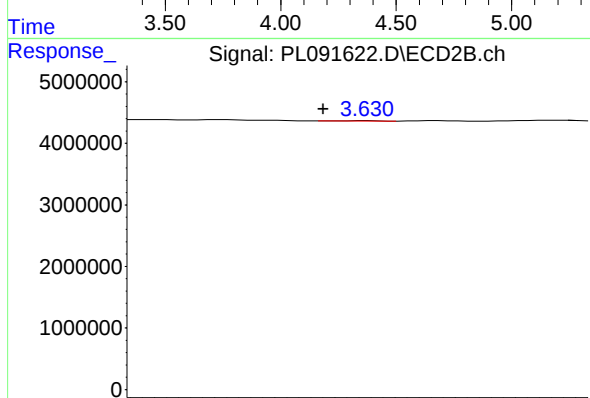

#3 gamma-BHC (Lindane)


R.T.: 3.631 min
Delta R.T.: 0.014 min
Response: 38319
Conc: 0.02 ng/ml

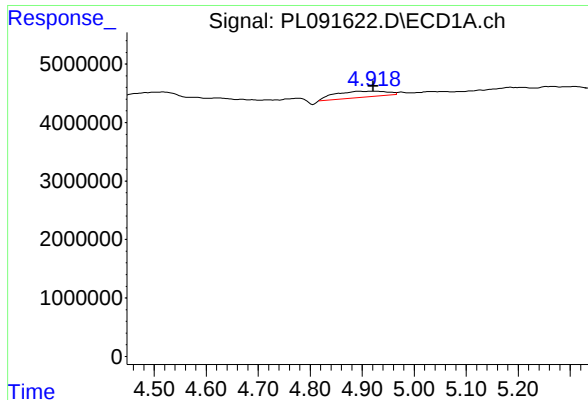

#4 Heptachlor


R.T.: 4.920 min
Delta R.T.: 0.000 min
Response: 7095137
Conc: 3.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

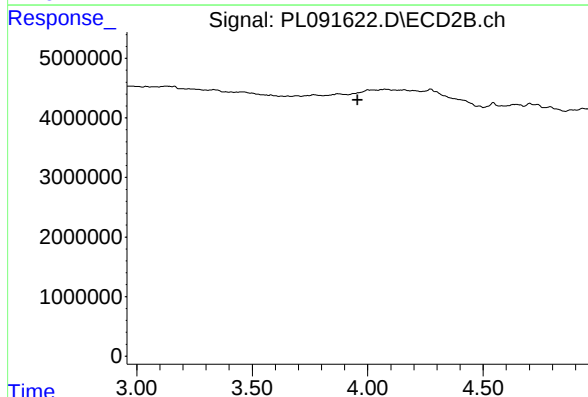


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.956 min
Response: 0
Conc: N.D.

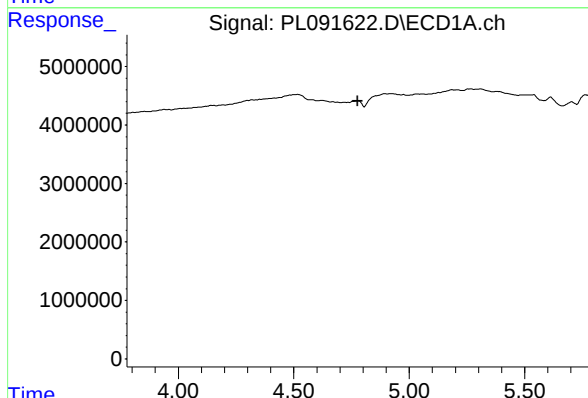


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.776 min
Response: 0
Conc: N.D.

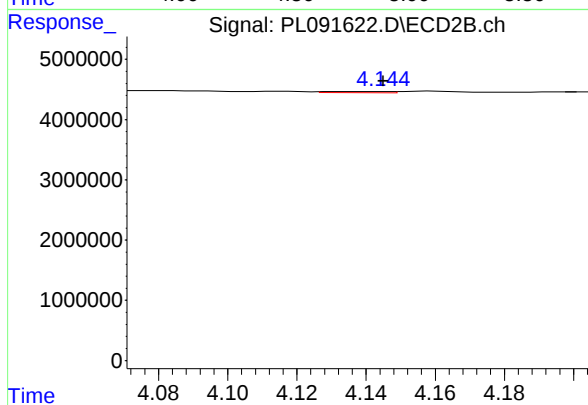

#7 delta-BHC


R.T.: 4.145 min
Delta R.T.: 0.000 min
Response: 265716
Conc: 0.12 ng/ml

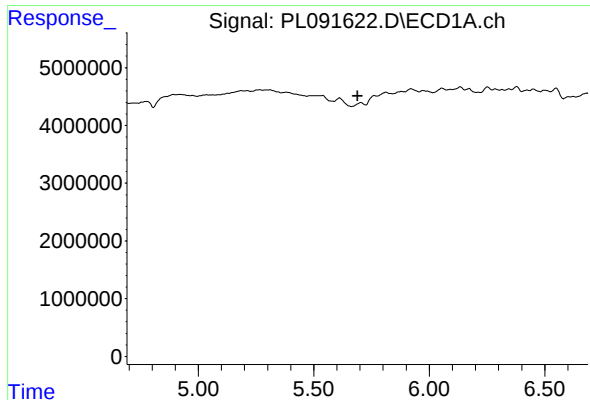

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.689 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

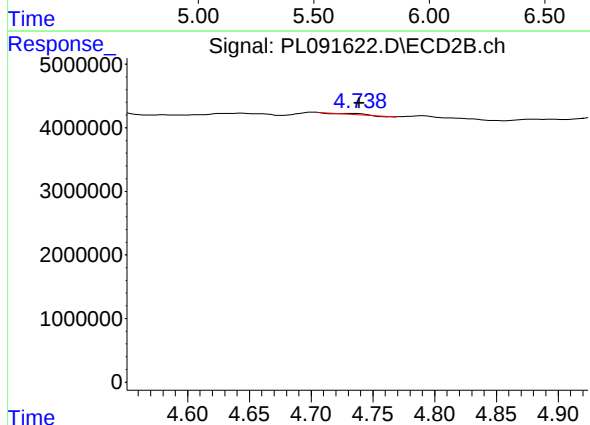


#8 Heptachlor epoxide

R.T.: 4.736 min
Delta R.T.: -0.003 min
Response: 133032
Conc: 0.06 ng/ml

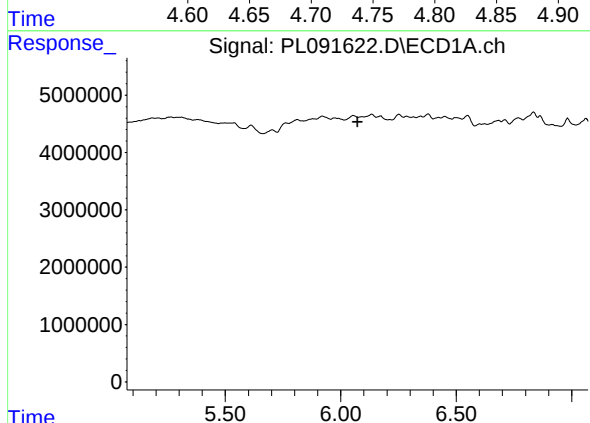


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.074 min
Response: 0
Conc: N.D.

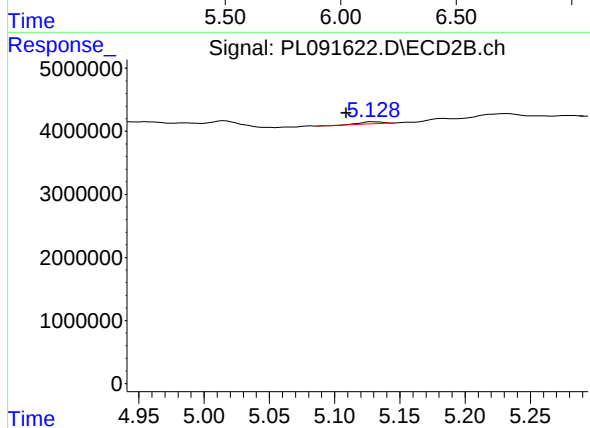

#9 Endosulfan I


R.T.: 5.130 min
Delta R.T.: 0.021 min
Response: 334939
Conc: 0.17 ng/ml

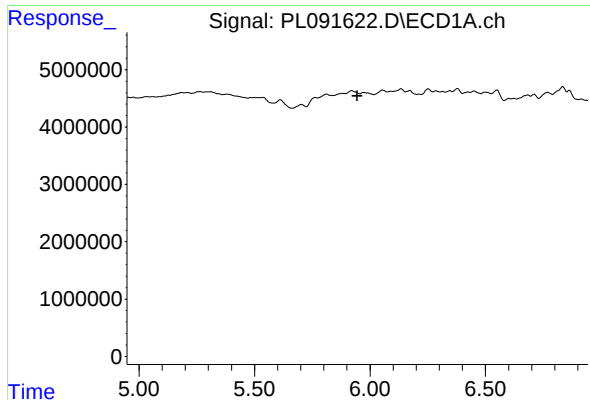

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

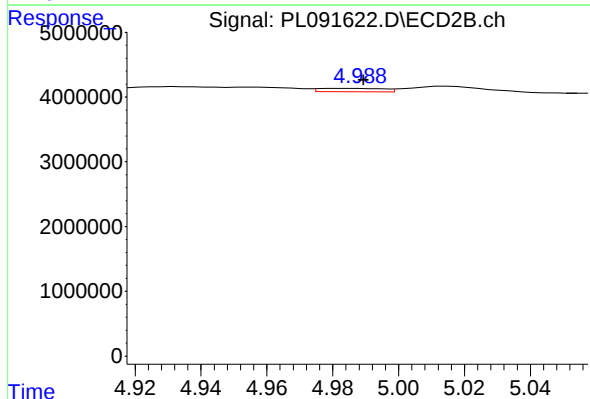


#10 gamma-Chlordane

R.T.: 4.984 min
Delta R.T.: -0.005 min
Response: 699606
Conc: 0.32 ng/ml

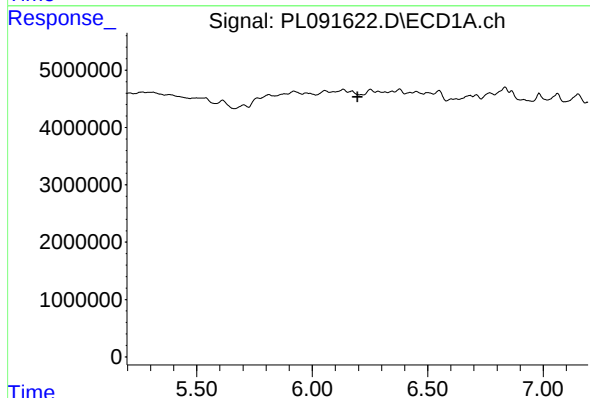


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

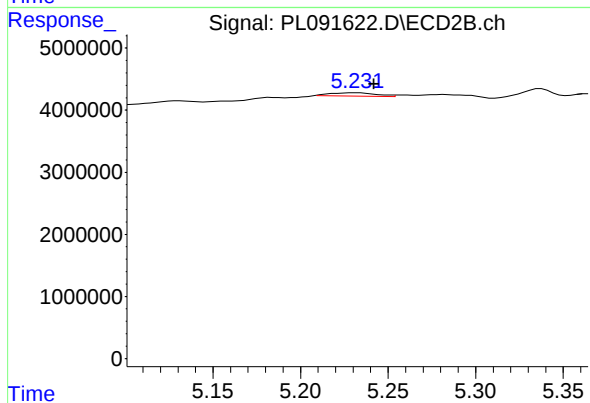

#12 4,4'-DDE


R.T.: 5.232 min
Delta R.T.: -0.010 min
Response: 989945
Conc: 0.52 ng/ml

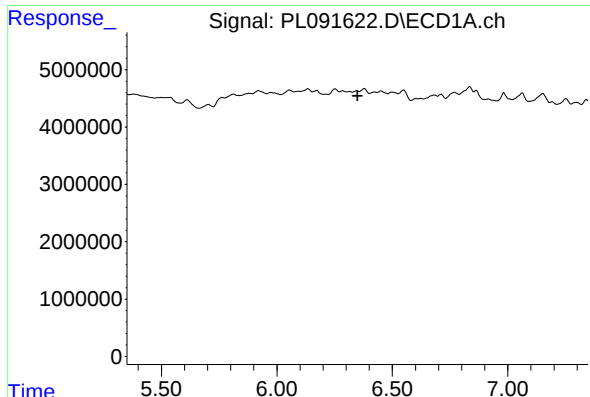

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

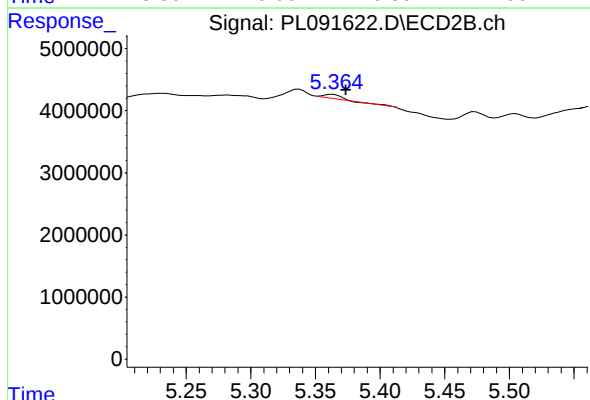


#13 Dieldrin

R.T.: 5.363 min
Delta R.T.: -0.010 min
Response: 522282
Conc: 0.25 ng/ml

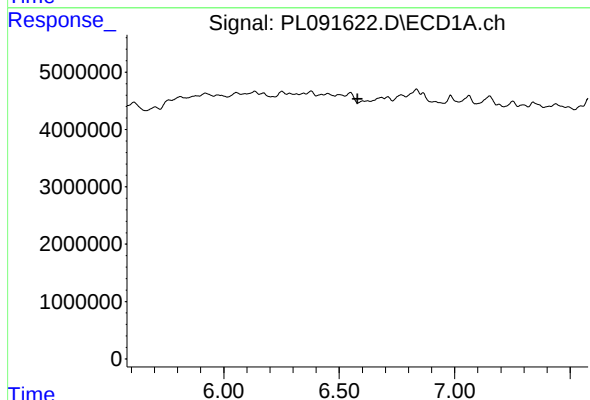


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.579 min
Response: 0
Conc: N.D.

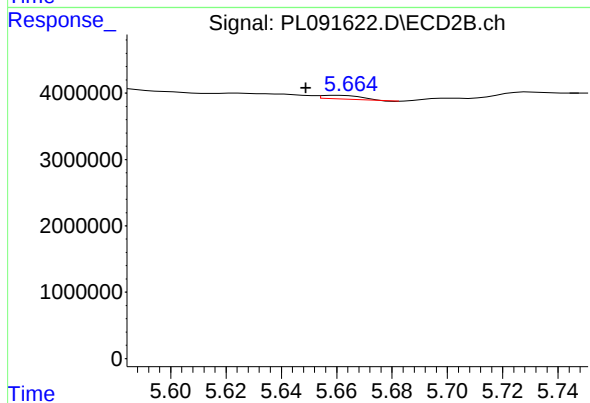

#14 Endrin


R.T.: 5.662 min
Delta R.T.: 0.013 min
Response: 561381
Conc: 0.30 ng/ml

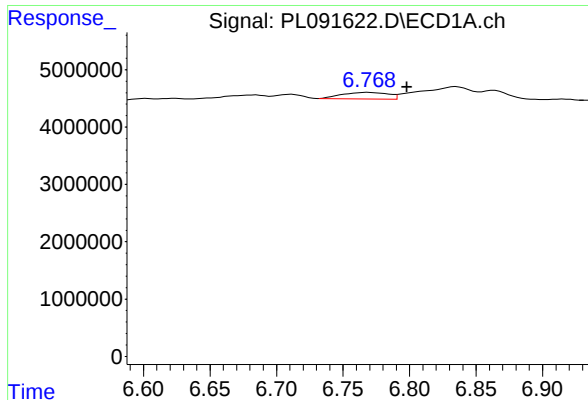

#15 Endosulfan II


R.T.: 6.769 min
Delta R.T.: -0.029 min
Response: 2731932
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

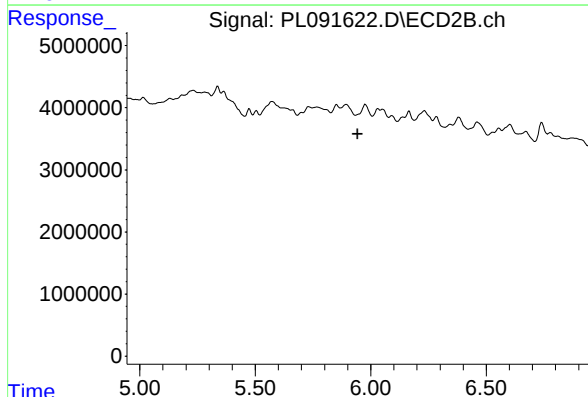


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

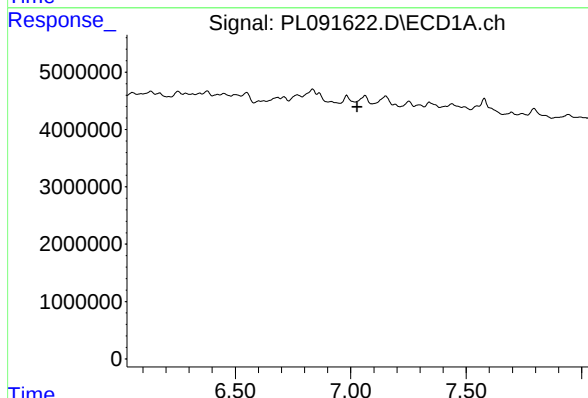


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.028 min
Response: 0
Conc: N.D.

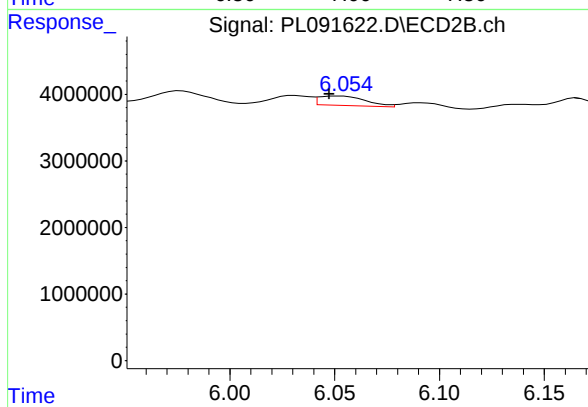

#17 4,4'-DDT


R.T.: 6.052 min
Delta R.T.: 0.004 min
Response: 2232339
Conc: 1.39 ng/ml

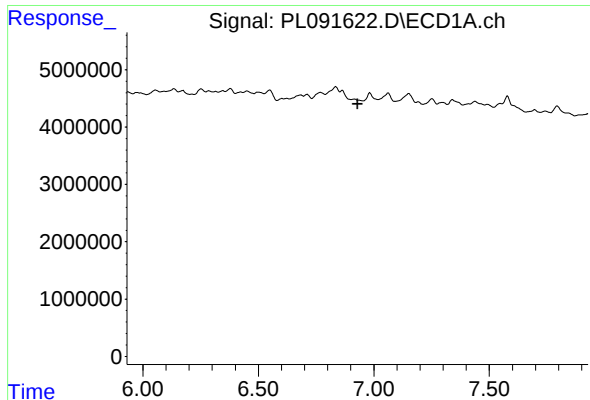

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

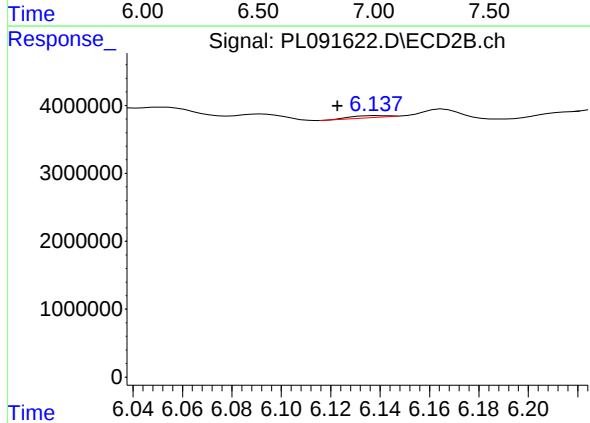


#18 Endrin aldehyde

R.T.: 6.139 min
Delta R.T.: 0.016 min
Response: 248291
Conc: 0.18 ng/ml

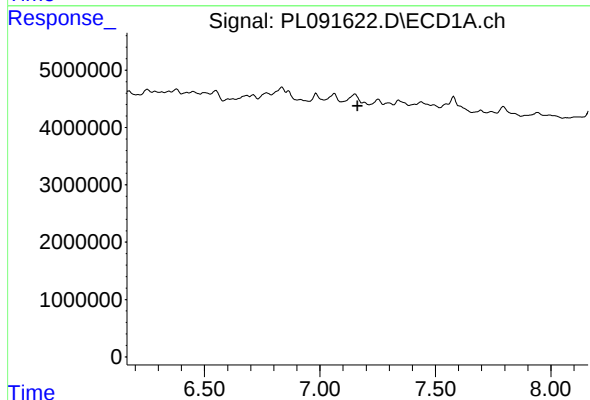


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.162 min
Response: 0
Conc: N.D.

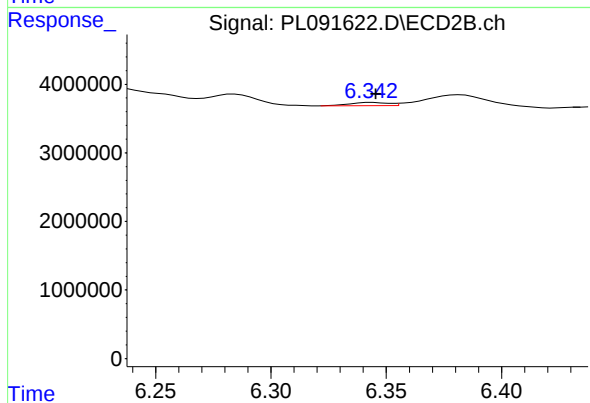

#19 Endosulfan Sulfate


R.T.: 6.344 min
Delta R.T.: -0.002 min
Response: 537998
Conc: 0.31 ng/ml

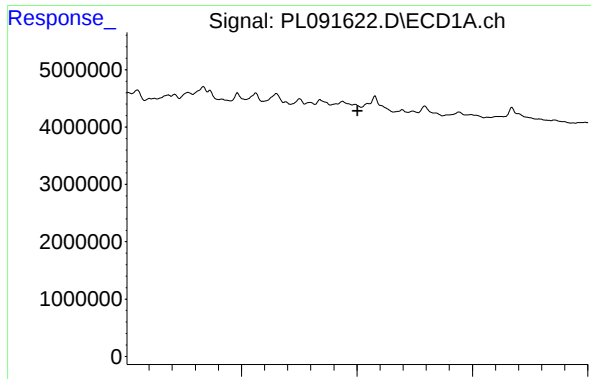

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

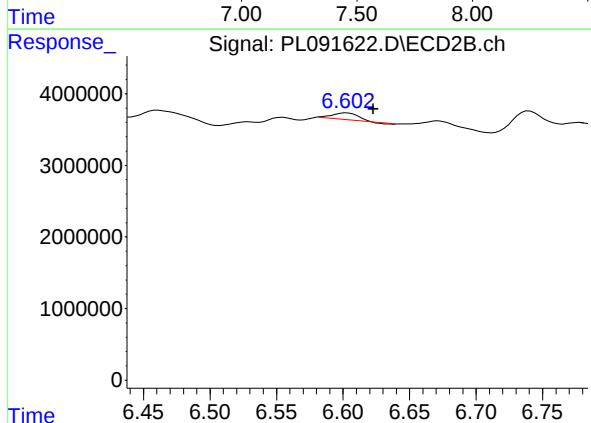


#20 Methoxychlor

R.T.: 6.603 min
Delta R.T.: -0.020 min
Response: 1222565
Conc: 1.38 ng/ml

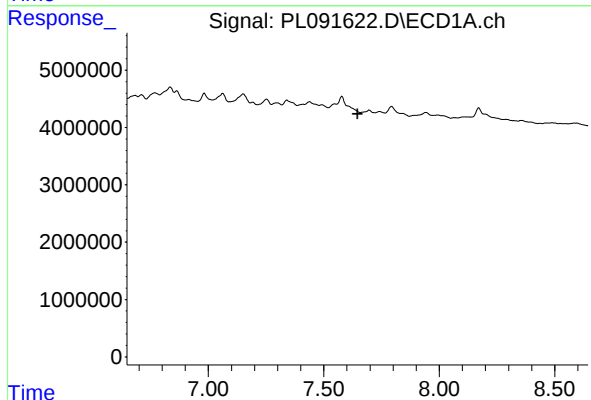


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.647 min
Response: 0
Conc: N.D.

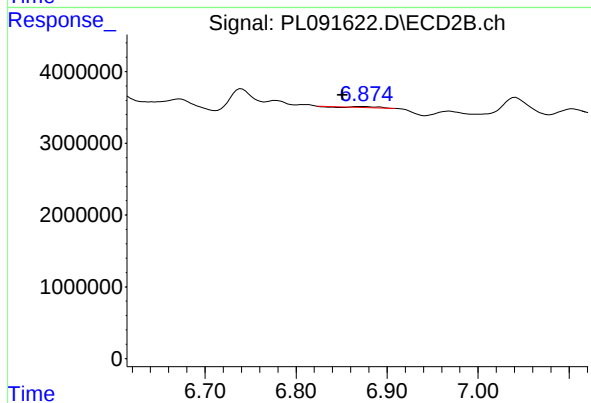

#21 Endrin ketone


R.T.: 6.871 min
Delta R.T.: 0.020 min
Response: 143211
Conc: 0.07 ng/ml

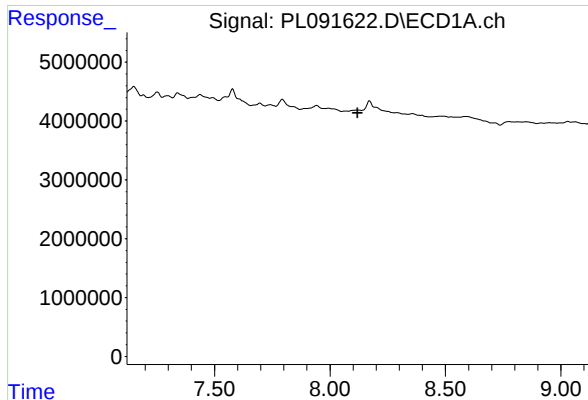

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

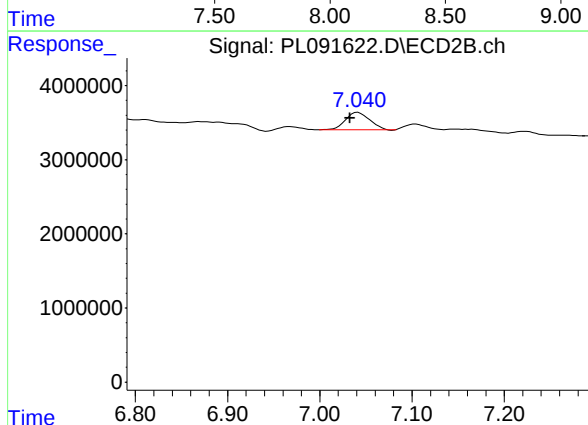


#22 Mirex

R.T.: 7.041 min
Delta R.T.: 0.008 min
Response: 4288530
Conc: 2.42 ng/ml

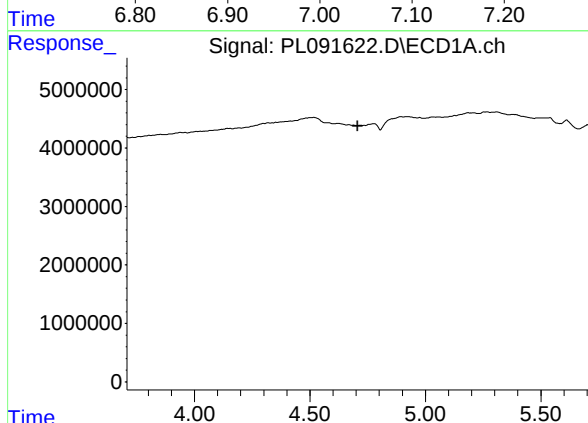


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.706 min
Response: 0
Conc: N.D.

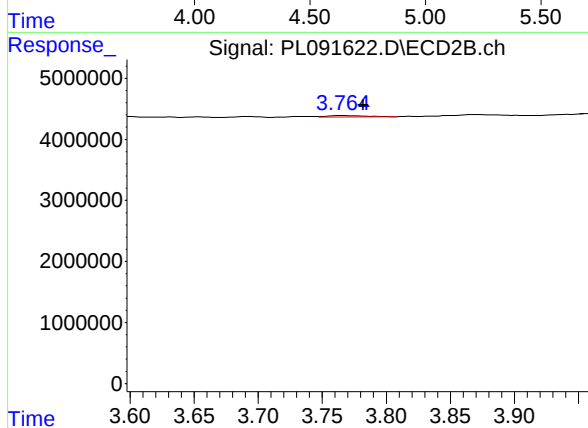

#23 Chlordane-1


R.T.: 3.765 min
Delta R.T.: -0.017 min
Response: 487692
Conc: 7.01 ng/ml

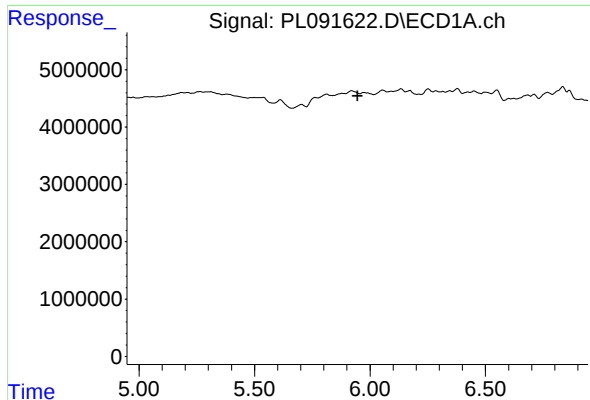

#25 Chlorine-3


R.T.: 0.000 min
Exp R.T.: 5.946 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-TXP-WPDL2

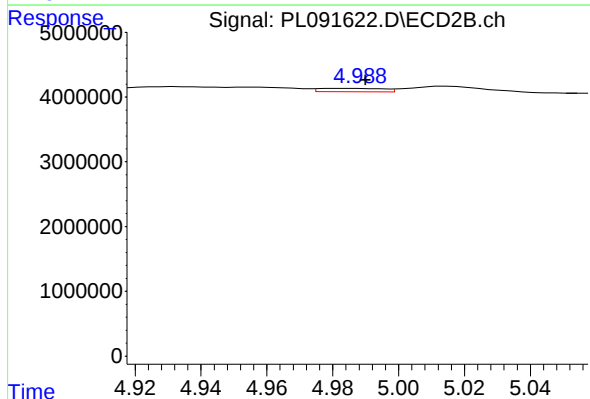


#25 Chlorine-3

R.T.: 4.984 min
Delta R.T.: -0.006 min
Response: 699606
Conc: 3.00 ng/ml

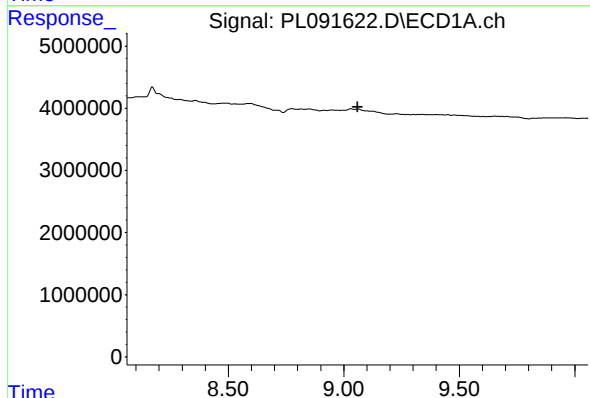

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.060 min
Response: 0
Conc: N.D.

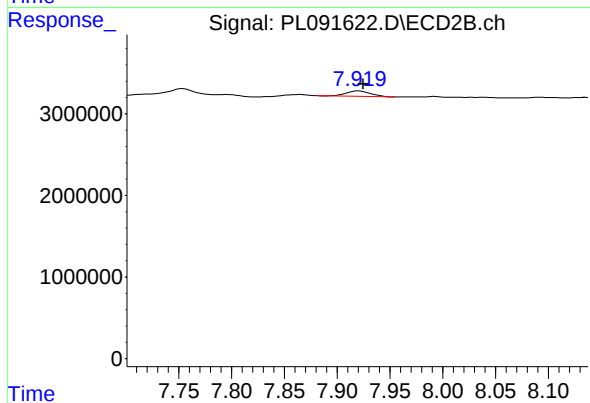

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.004 min
Response: 1090215
Conc: 0.59 ng/ml