

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091119\
 Data File : PL052370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2019 19:26
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 03:25:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 12 03:24:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	516.6E6	103.4E6	50.000	50.000
28)	SA Decachlor...	7.969	8.949	651.1E6	137.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.151	4.908	162.7E6	44060871	500.000	500.000
24)	Chlordane-2	4.641	5.374	214.1E6	50525635	500.000	500.000
25)	Chlordane-3	5.195	6.018	665.7E6	218.3E6	500.000	500.000
26)	Chlordane-4	5.249	6.090	629.9E6	262.1E6	500.000	500.000
27)	Chlordane-5	6.070	6.893	258.5E6	47607405	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091119\
Data File : PL052370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2019 19:26
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 03:25:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
Quant Title : GC Extractables
QLast Update : Thu Sep 12 03:24:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

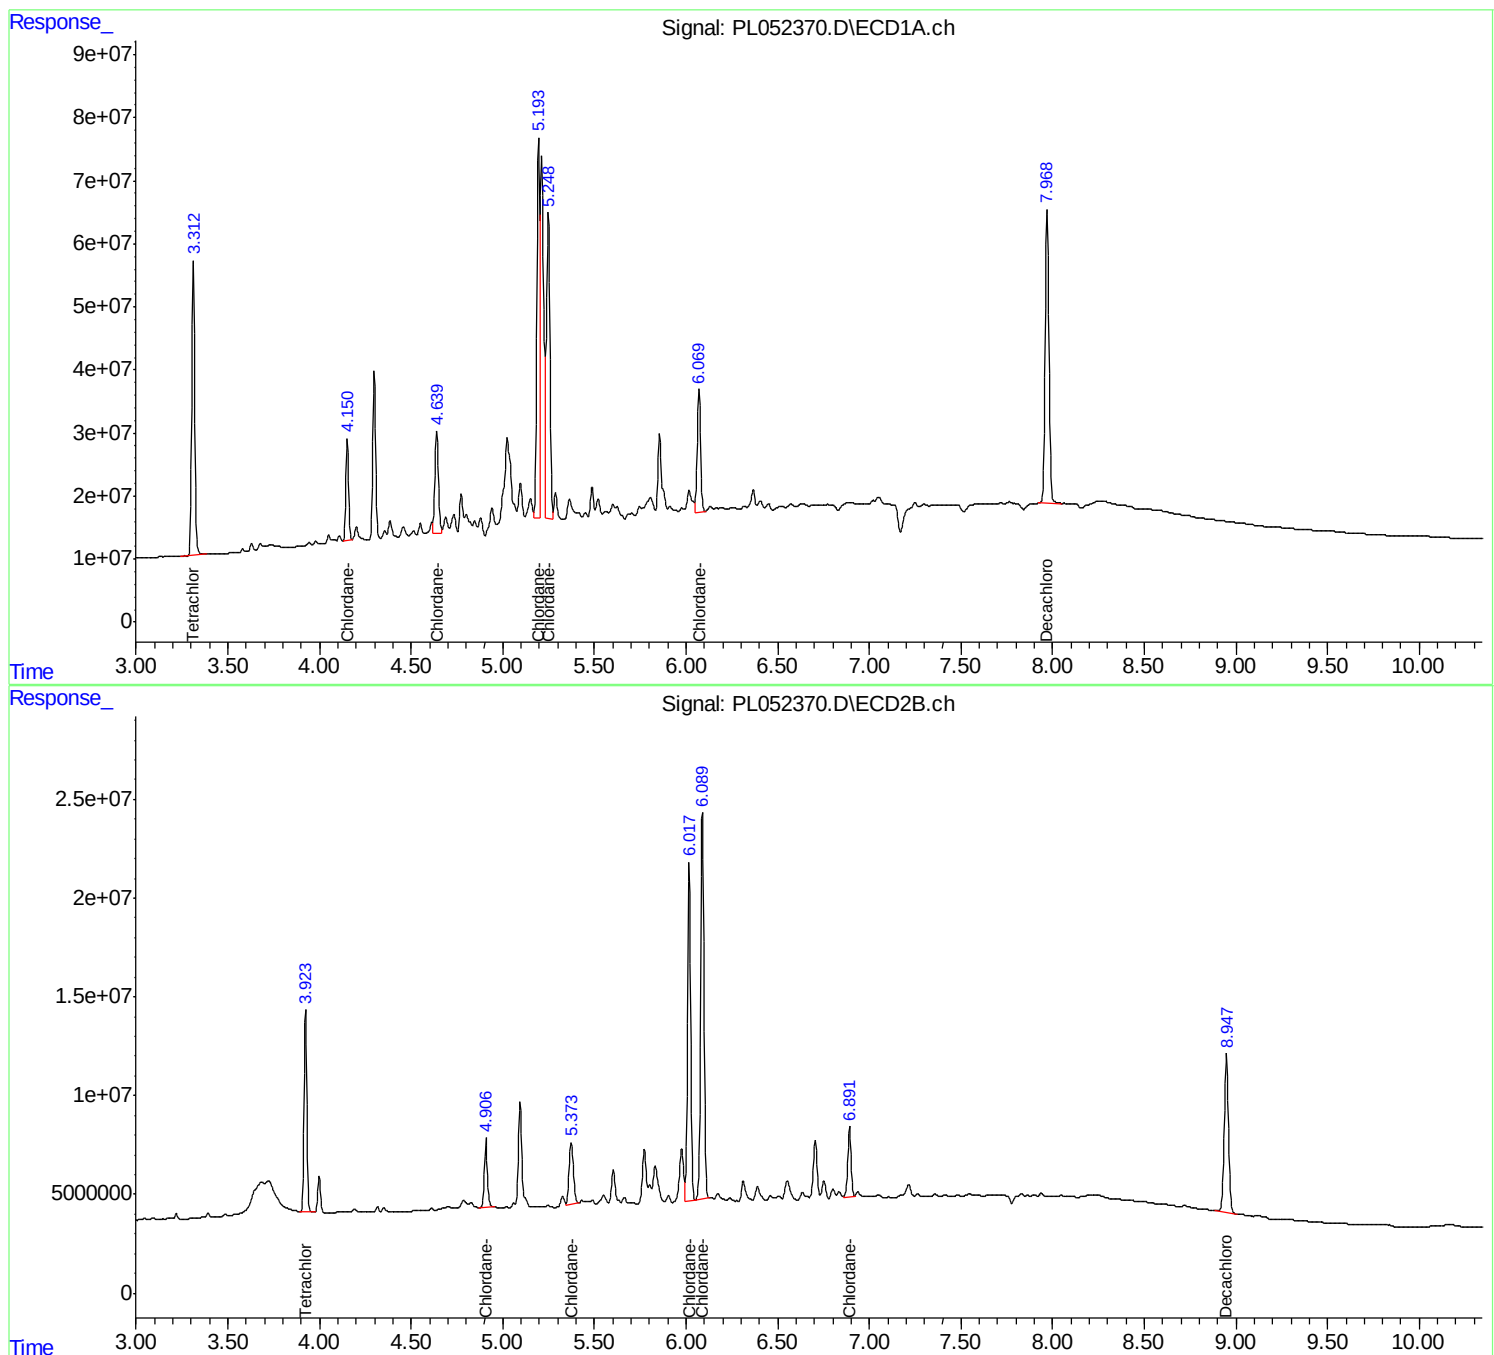


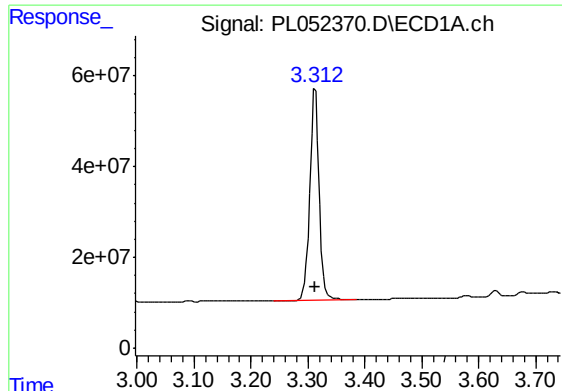

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 516590287
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

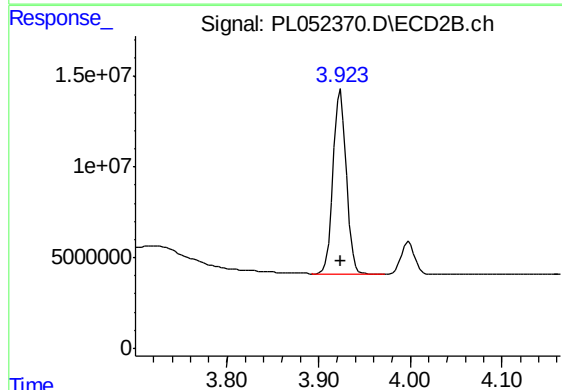


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 103408457
Conc: 50.00 ng/ml

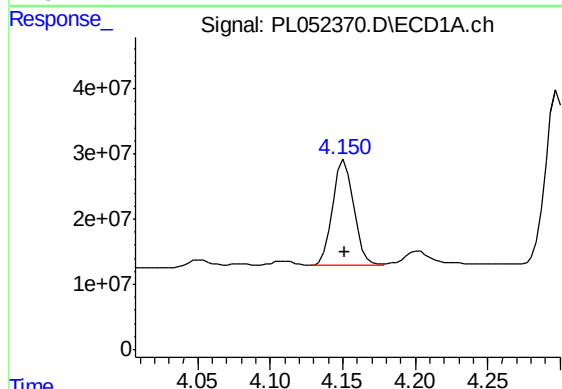


#23 Chlordane-1

R.T.: 4.151 min
Delta R.T.: 0.000 min
Response: 162659982
Conc: 500.00 ng/ml

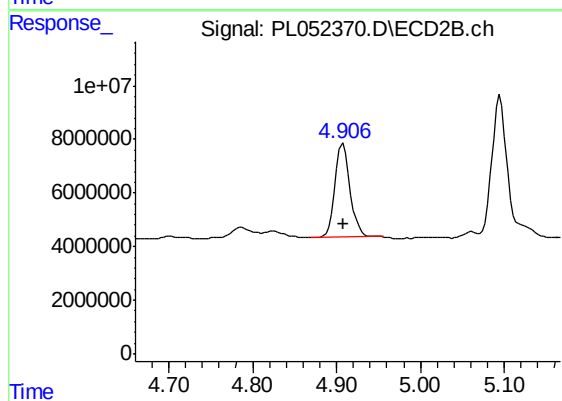

#23 Chlordane-1


R.T.: 4.908 min
Delta R.T.: 0.000 min
Response: 44060871
Conc: 500.00 ng/ml

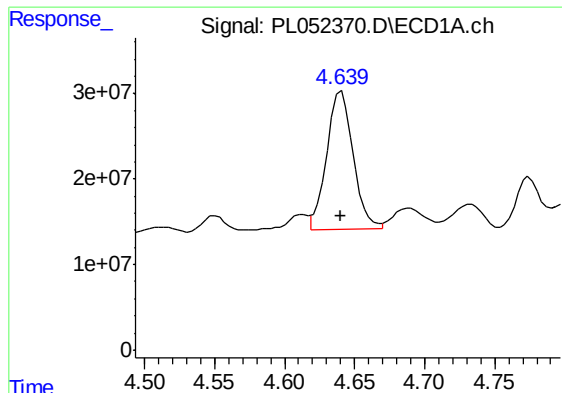

#24 Chlordane-2


R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 214106505
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

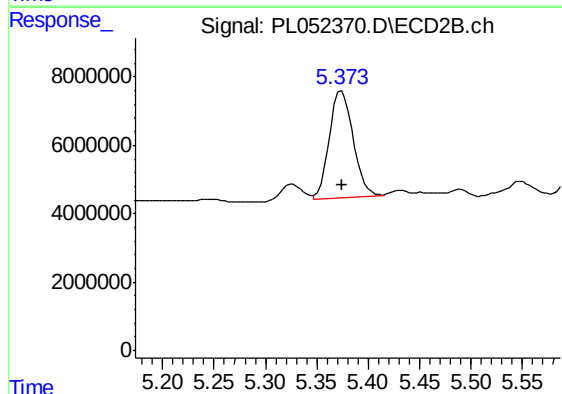


#24 Chlordane-2

R.T.: 5.374 min
Delta R.T.: 0.000 min
Response: 50525635
Conc: 500.00 ng/ml

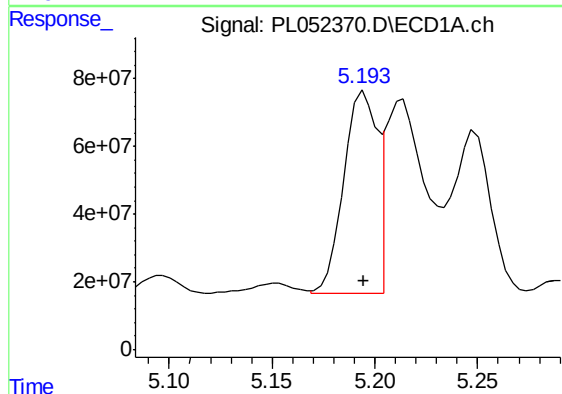


#25 Chlordane-3

R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 665691122
Conc: 500.00 ng/ml

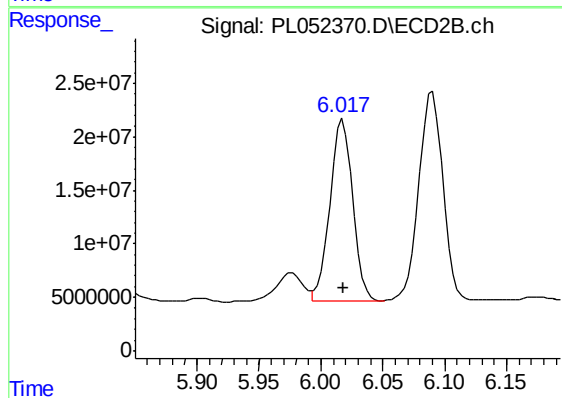

#25 Chlordane-3


R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 218332985
Conc: 500.00 ng/ml

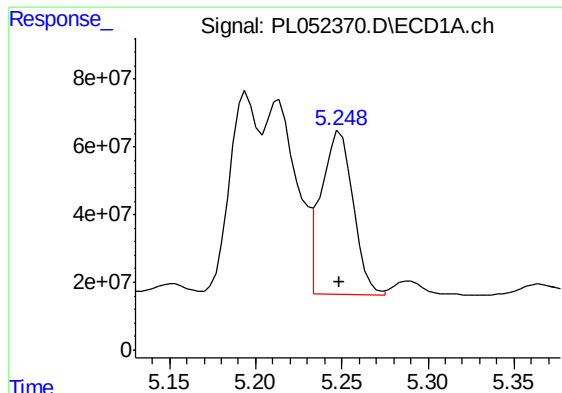

#26 Chlordane-4


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 629931456
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

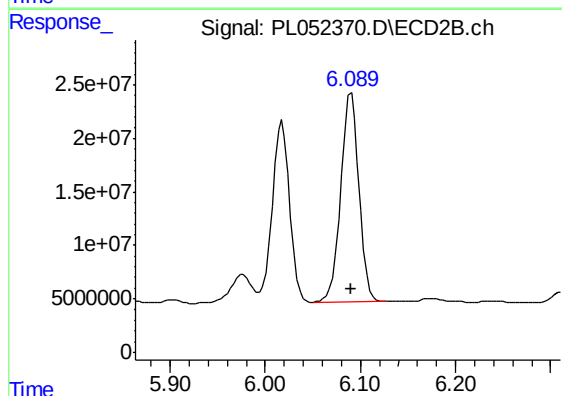


#26 Chlordane-4

R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 262051676
Conc: 500.00 ng/ml

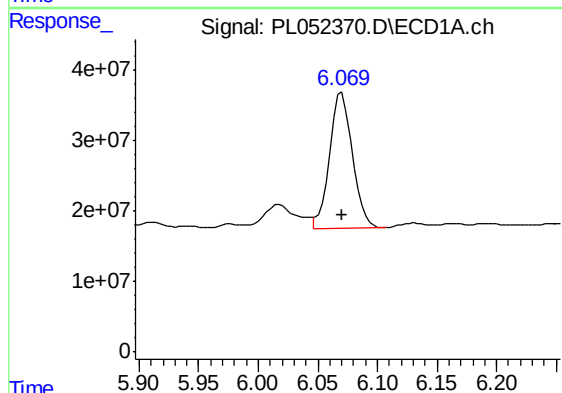


#27 Chlordane-5

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 258490317
Conc: 500.00 ng/ml

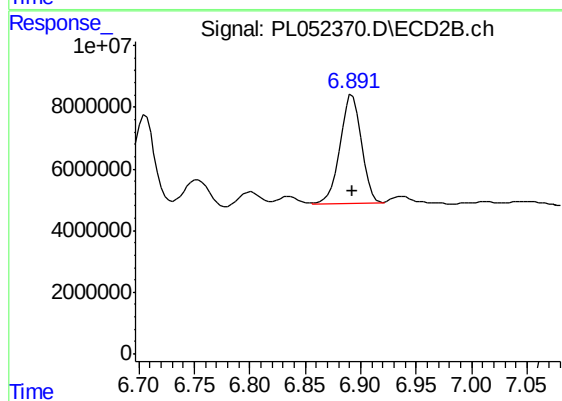

#27 Chlordane-5


R.T.: 6.893 min
Delta R.T.: 0.000 min
Response: 47607405
Conc: 500.00 ng/ml

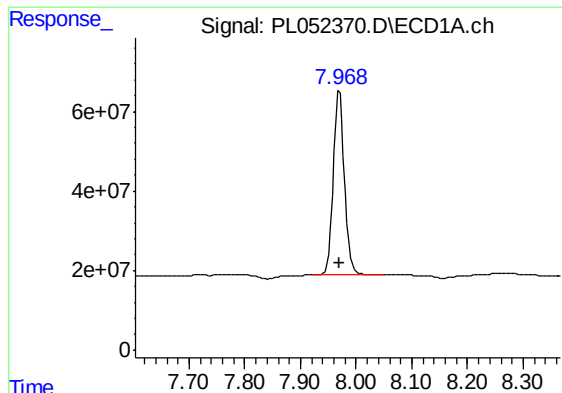

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 651082583
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

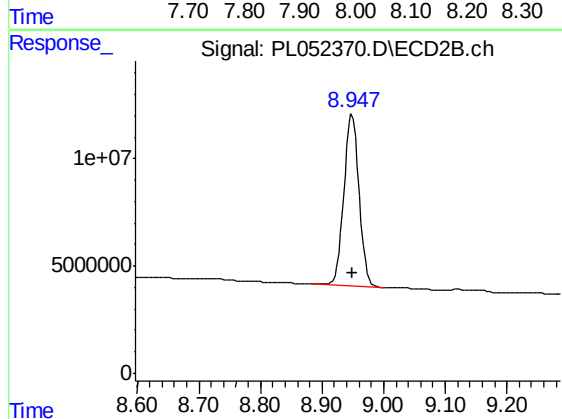

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 136959881
Conc: 50.00 ng/ml