

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
 Data File : PL061382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 14:31
 Operator : DD\AJ
 Sample : L3975-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 17:44:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	28640998	52821028	16.606	17.172
28)	SA Decachlor...	8.209	9.093	24201975	28014978	14.507	11.848
Target Compounds							
2)	A alpha-BHC	0.000	4.423f	0	33198207	N.D.	7.189 #
9)	A Endosulfan I	0.000	6.242	0	9531958	N.D.	2.971 #
10)	B gamma-Chl...	0.000	6.127	0	12459204	N.D.	3.614 #
11)	B alpha-Chl...	0.000	6.195	0	20142353	N.D.	5.788 #
16)	A 4,4'-DDD	0.000	6.842	0	3308154	N.D.	1.288 #
17)	MA 4,4'-DDT	6.375	0.000	1170285	0	0.852	N.D. #
25)	Chlordane-3	0.000	6.127	0	12459204	N.D.	28.842 #
26)	Chlordane-4	0.000	6.195	0	20142353	N.D.	38.478 #
27)	Chlordane-5	6.314f	0.000	8540635	0	151.950	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
Data File : PL061382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 14:31
Operator : DD\AJ
Sample : L3975-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 17:44:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

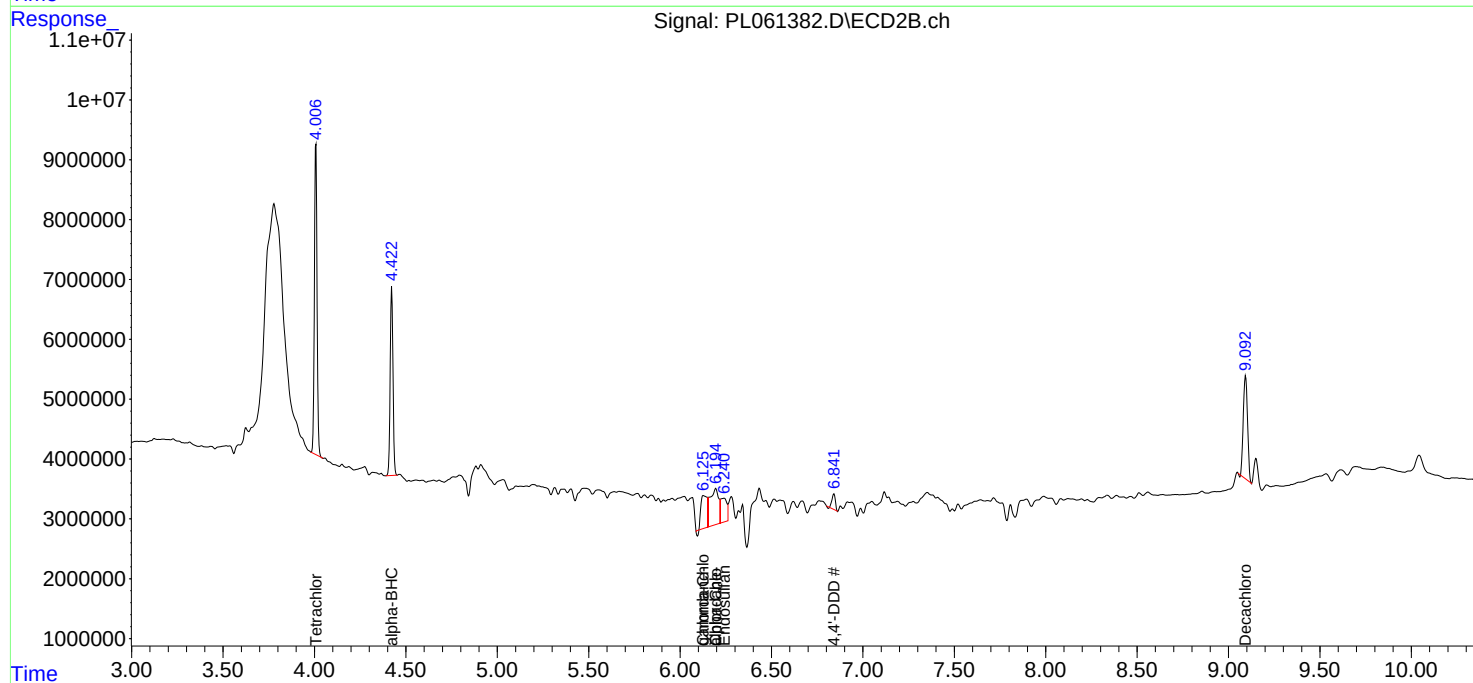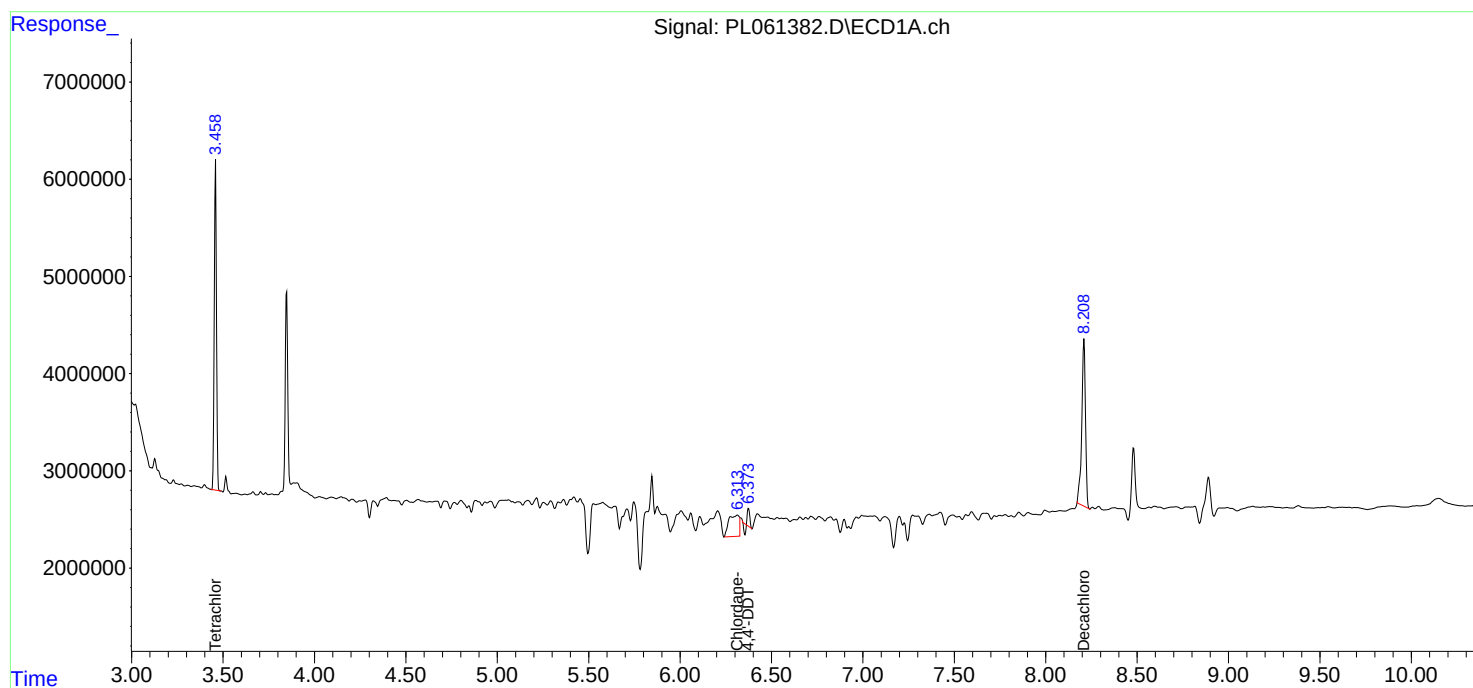


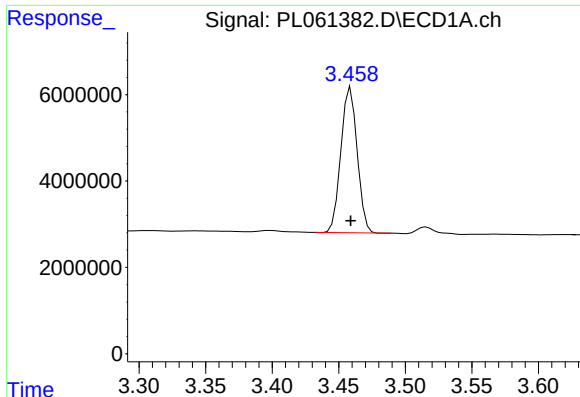

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 28640998
Conc: 16.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

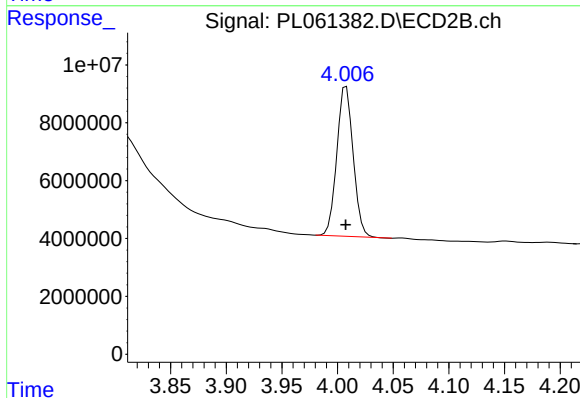


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 52821028
Conc: 17.17 ng/ml

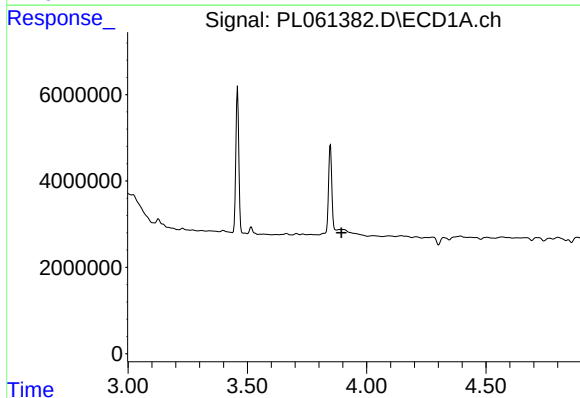


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.895 min
Response: 0
Conc: N.D.

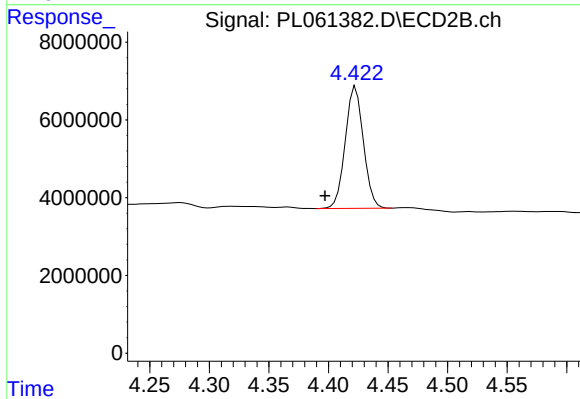

#2 alpha-BHC


R.T.: 4.423 min
Delta R.T.: 0.026 min
Response: 33198207
Conc: 7.19 ng/ml

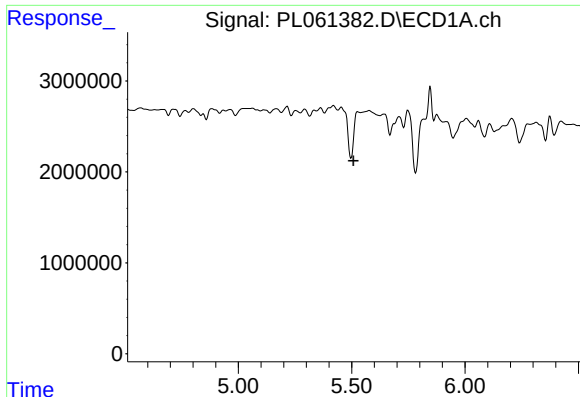

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

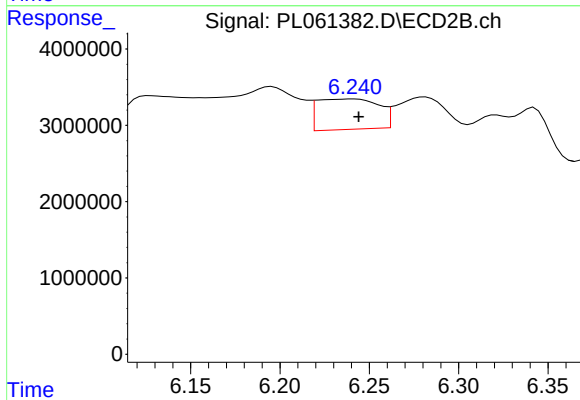


#9 Endosulfan I

R.T.: 6.242 min
Delta R.T.: -0.002 min
Response: 9531958
Conc: 2.97 ng/ml

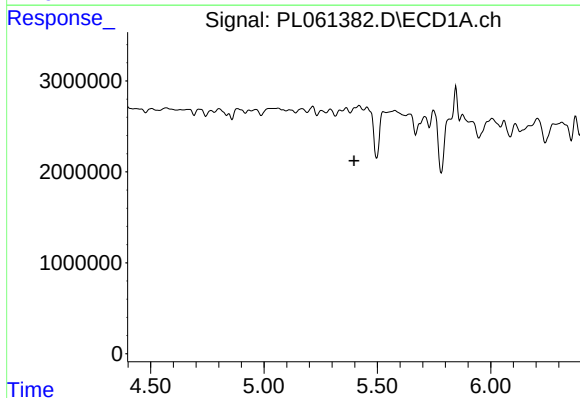


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

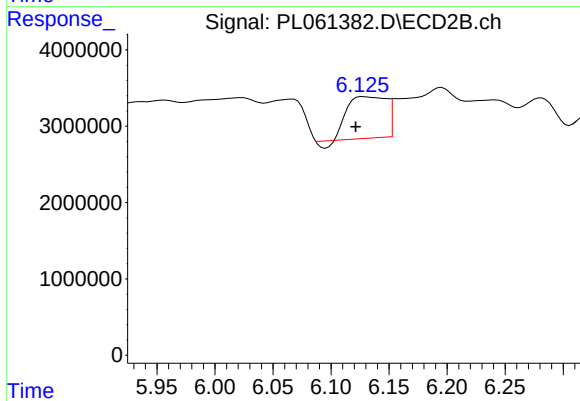

#10 gamma-Chlordane


R.T.: 6.127 min
Delta R.T.: 0.006 min
Response: 12459204
Conc: 3.61 ng/ml

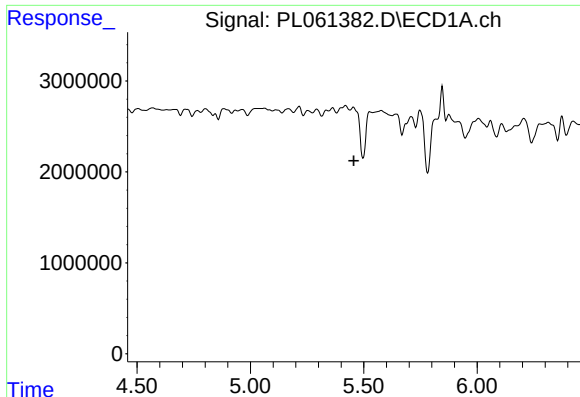

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

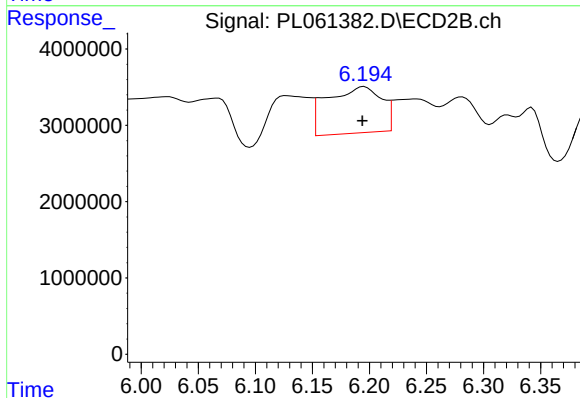


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.001 min
Response: 20142353
Conc: 5.79 ng/ml

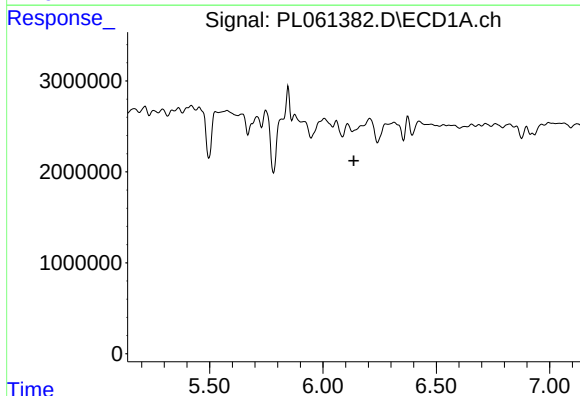


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.136 min
Response: 0
Conc: N.D.

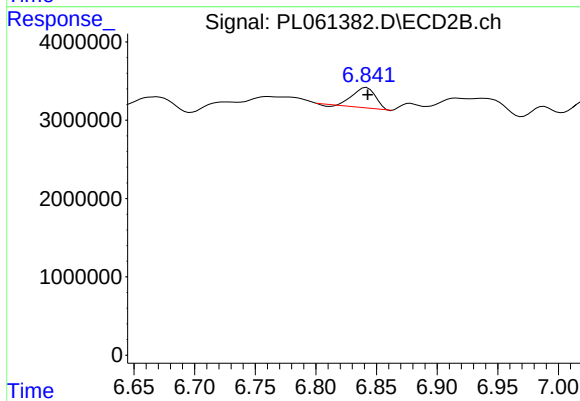

#16 4,4'-DDD


R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 3308154
Conc: 1.29 ng/ml

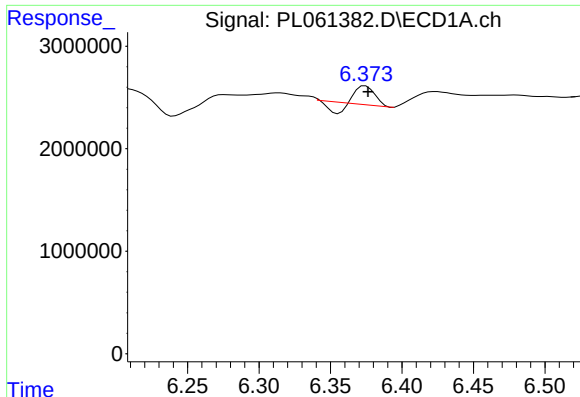

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: -0.002 min
Response: 1170285
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

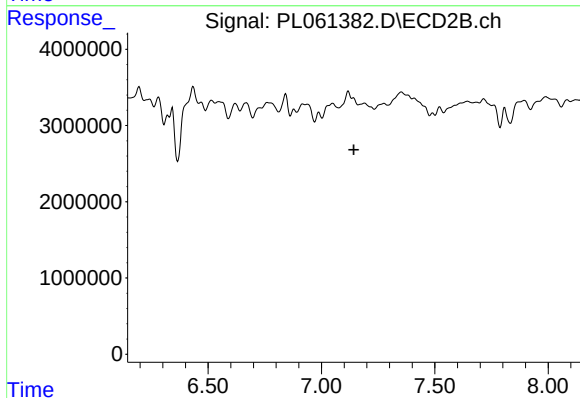


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.143 min
Response: 0
Conc: N.D.

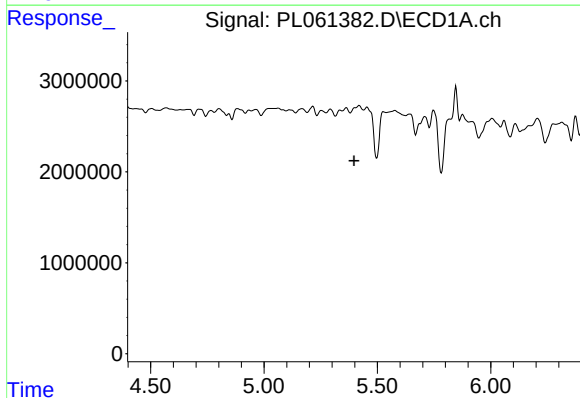


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

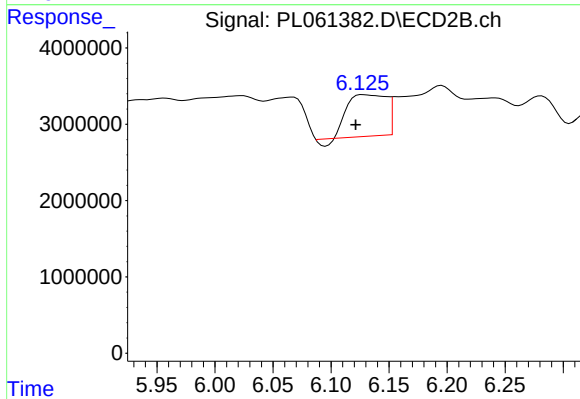

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.006 min
Response: 12459204
Conc: 28.84 ng/ml

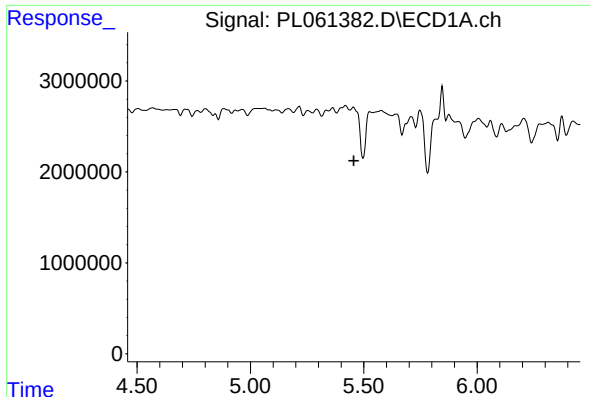

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

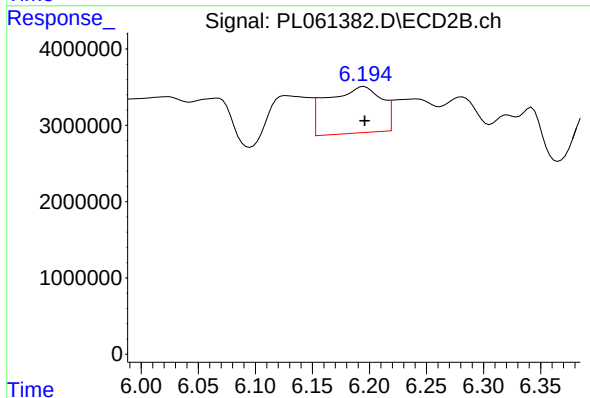


#26 Chlordane-4

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 20142353
Conc: 38.48 ng/ml

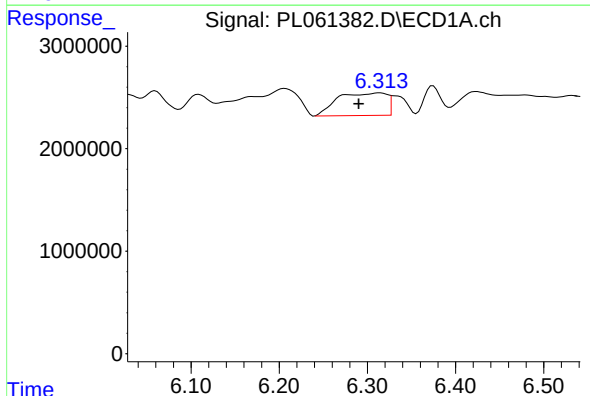


#27 Chlordane-5

R.T.: 6.314 min
Delta R.T.: 0.024 min
Response: 8540635
Conc: 151.95 ng/ml

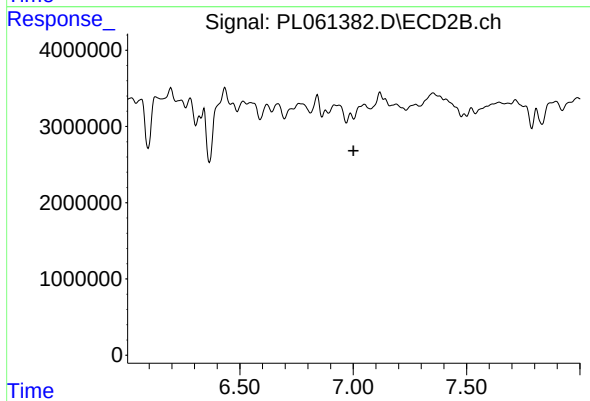

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.002 min
Response: 0
Conc: N.D.

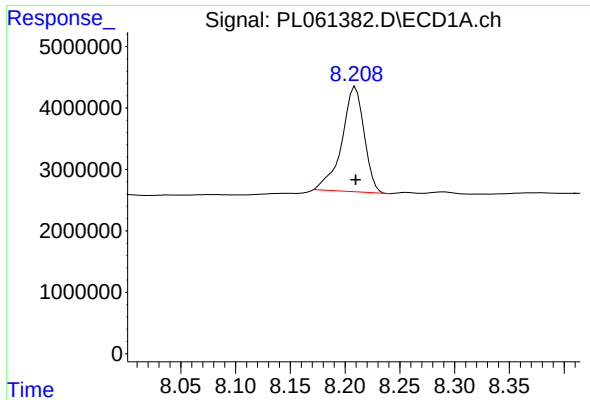

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 24201975
Conc: 14.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

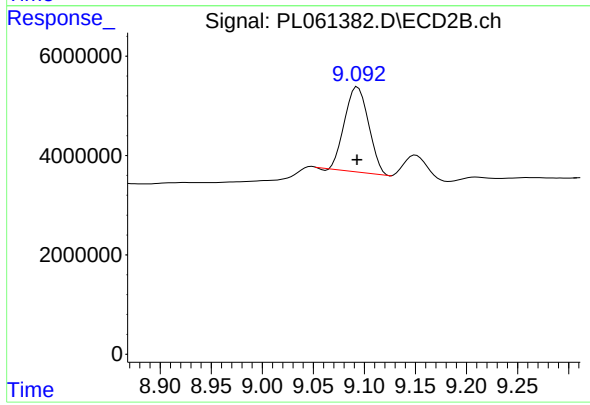

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 28014978
Conc: 11.85 ng/ml