

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
 Data File : PL061389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 16:12
 Operator : DD\AJ
 Sample : L3953-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N2930S

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:03:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 17:46:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.005	37656123	46709316	21.834m	15.185m#
28)	SA Decachlor...	8.209	9.092	14082112	24261338	8.441m	10.260m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
Data File : PL061389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 16:12
Operator : DD\AJ
Sample : L3953-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
N2930S


Manual Integrations
APPROVED

Ankita
9/14/2020 11:03:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 17:46:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

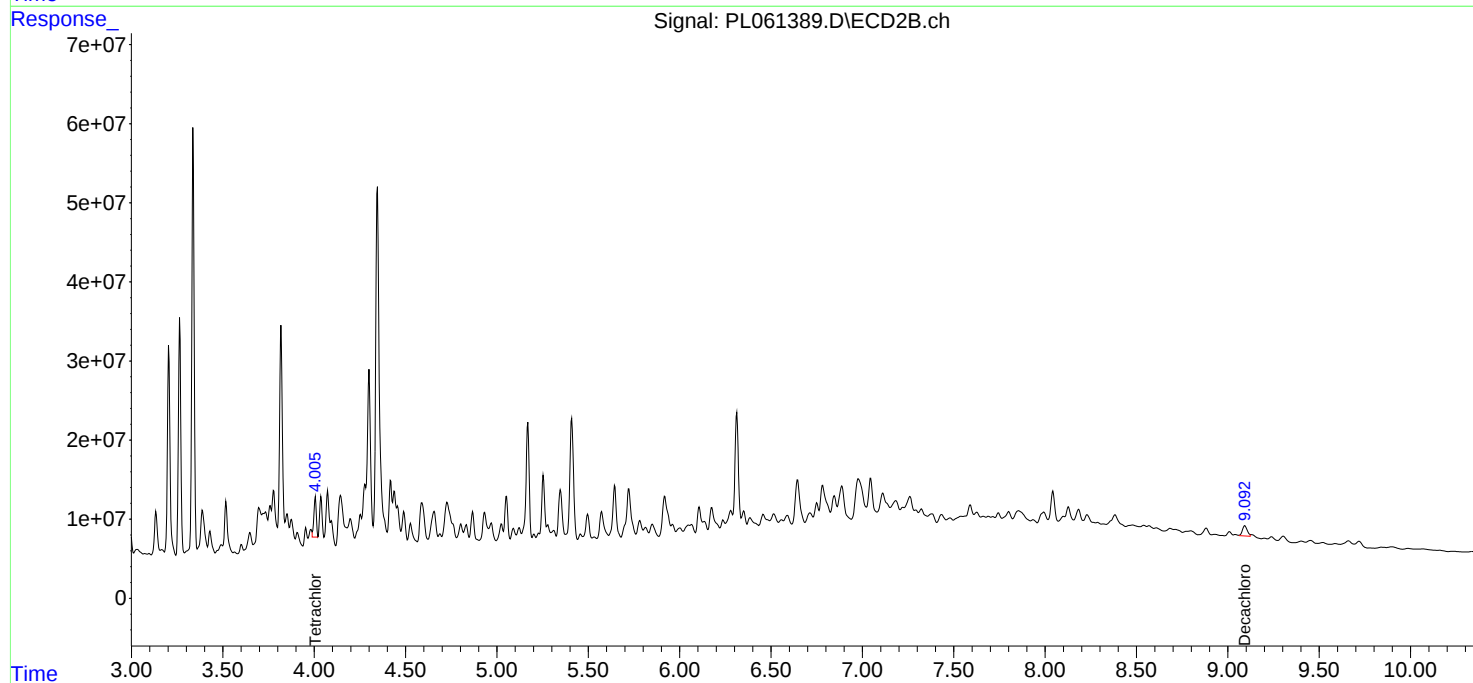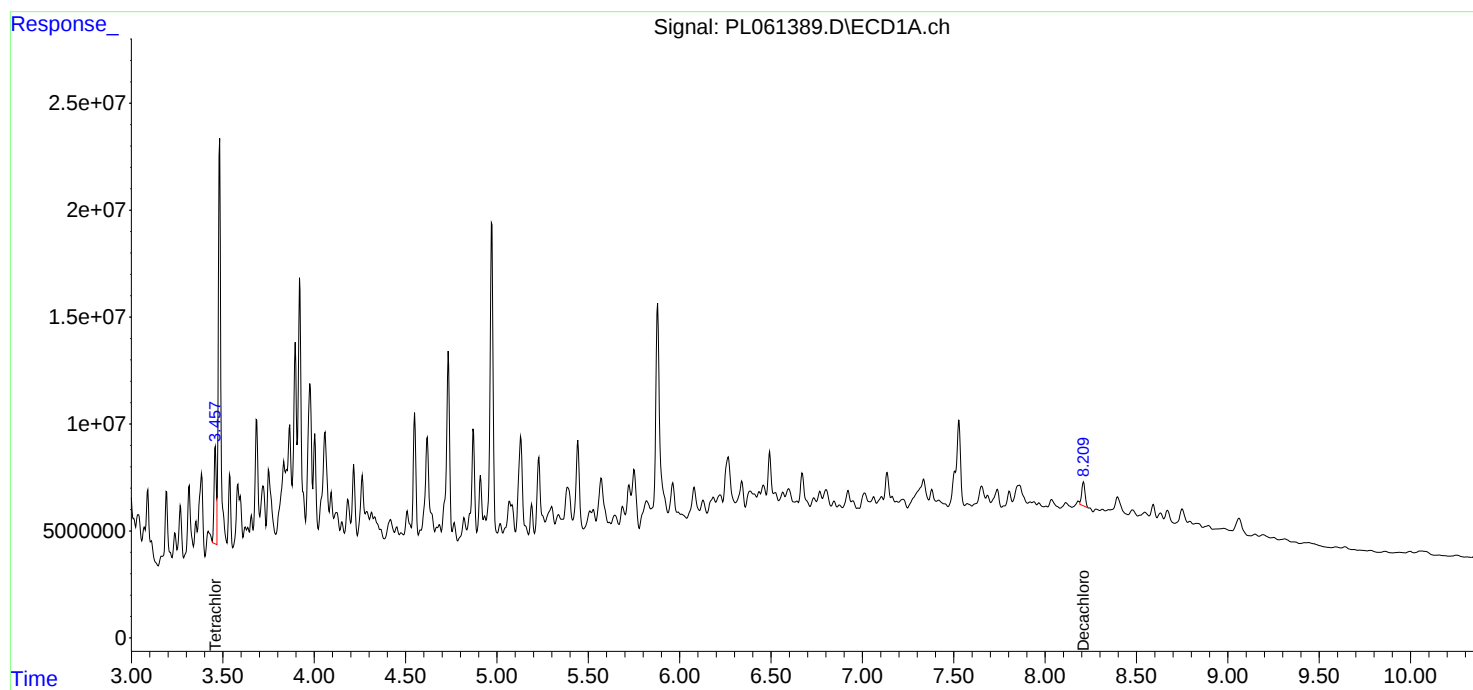

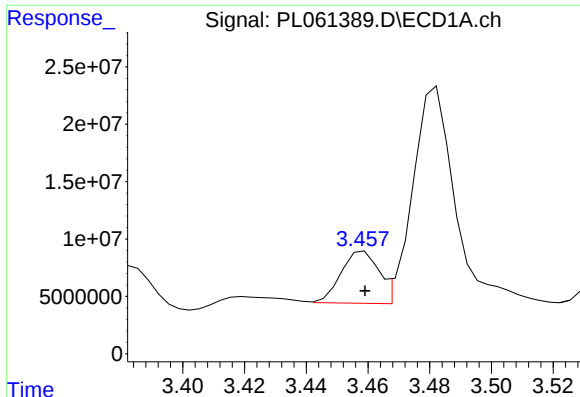


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.002 min
Response: 37656123
Conc: 21.83 ng/ml m

Instrument :
ECD_L
ClientSampleId :
N2930S


Manual Integrations
APPROVED

Ankita
9/14/2020 11:03:25 AM

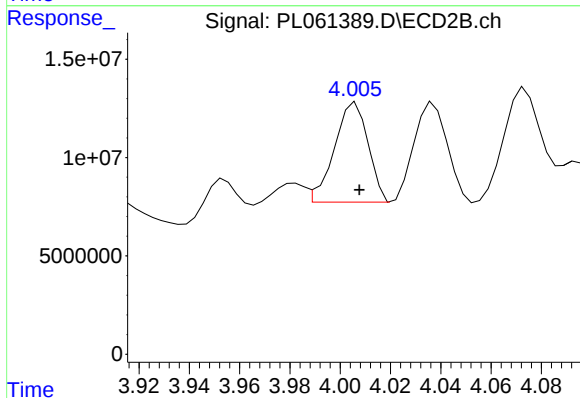


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 46709316
Conc: 15.19 ng/ml m

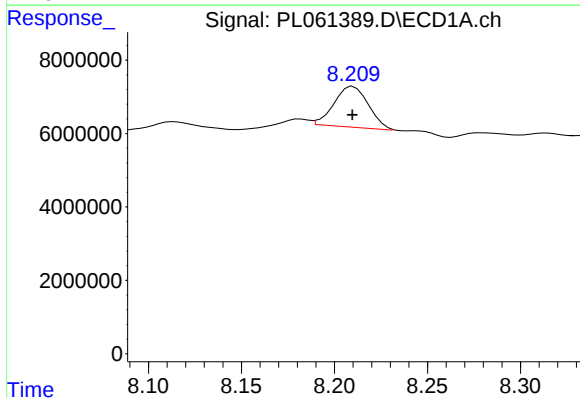

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 14082112
Conc: 8.44 ng/ml m

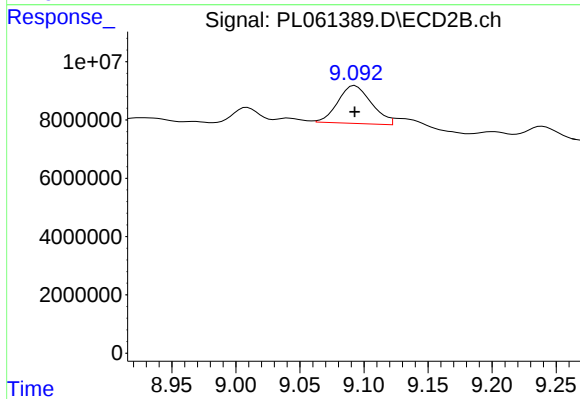

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.001 min
Response: 24261338
Conc: 10.26 ng/ml m