

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
 Data File : PL061390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 16:26
 Operator : DD\AJ
 Sample : L3976-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BSY-WC-WATER-DRUM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 17:46:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	36010812	59071106	20.880	19.204
28)	SA Decachlor...	8.210	9.093	24996541	36150824	14.983	15.289
Target Compounds							
4)	MA Heptachlor	4.484	5.193	4224372	6899224	1.969	1.765



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
Data File : PL061390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 16:26
Operator : DD\AJ
Sample : L3976-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BSY-WC-WATER-DRUM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 17:46:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

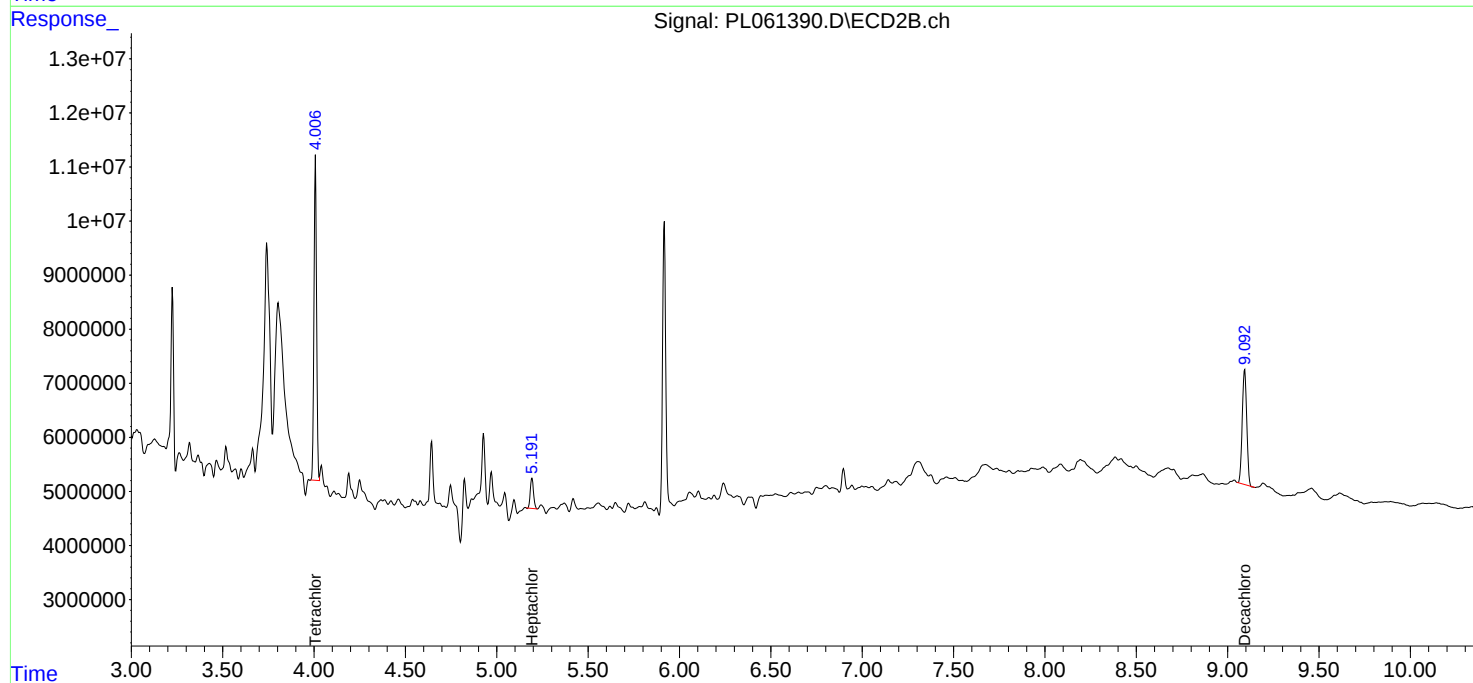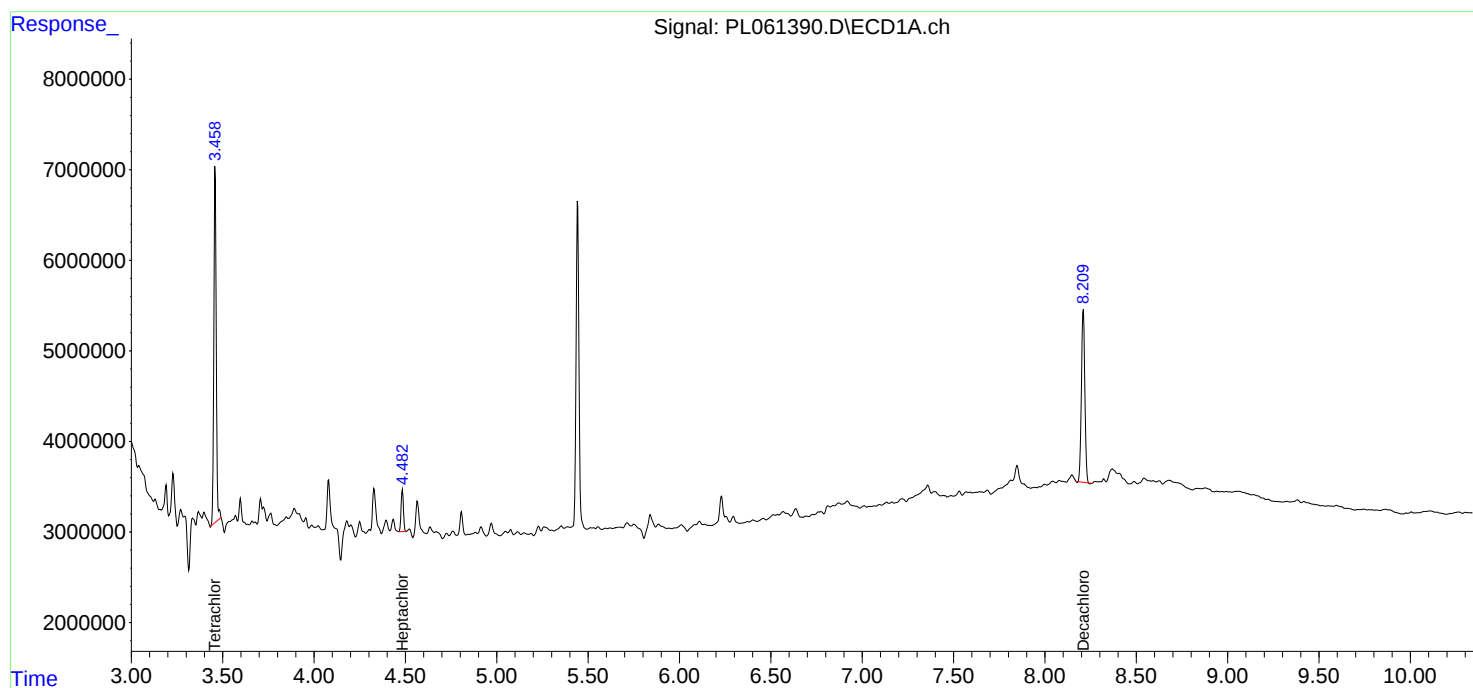


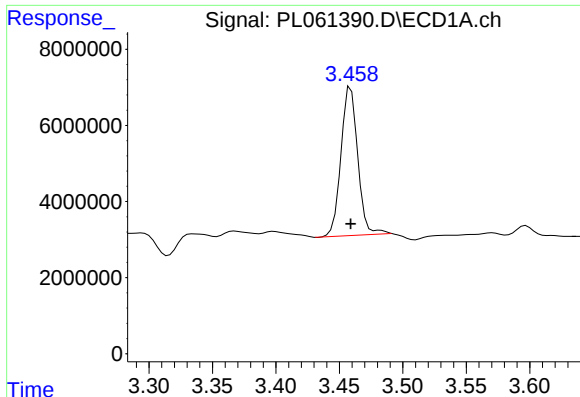

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 36010812
Conc: 20.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
BSY-WC-WATER-DRUM

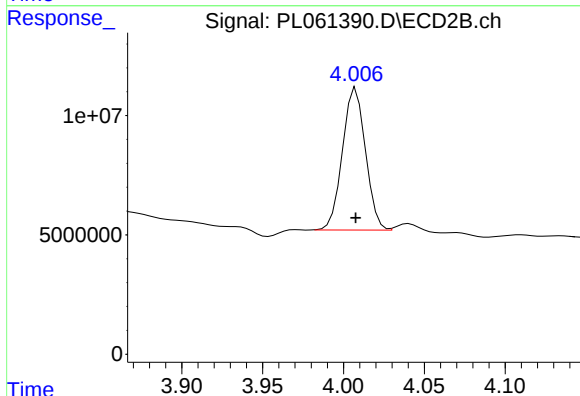


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 59071106
Conc: 19.20 ng/ml

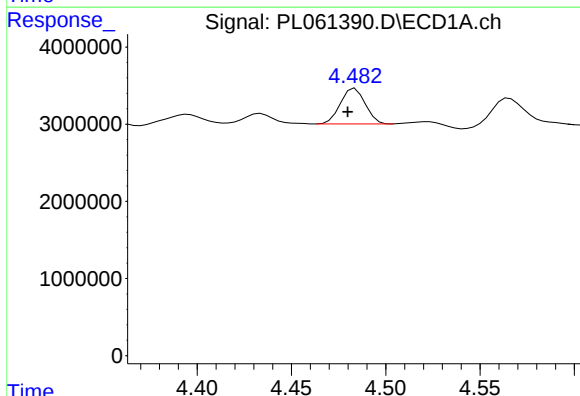


#4 Heptachlor

R.T.: 4.484 min
Delta R.T.: 0.004 min
Response: 4224372
Conc: 1.97 ng/ml

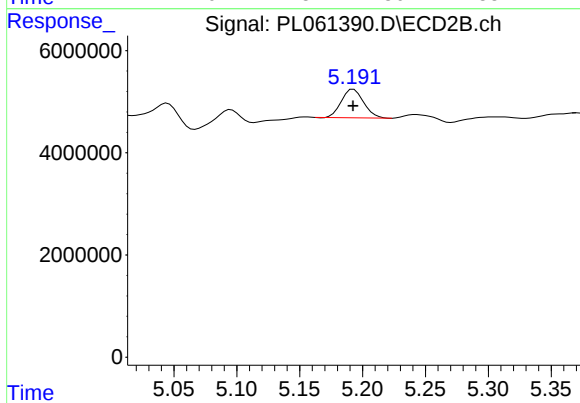

#4 Heptachlor


R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 6899224
Conc: 1.76 ng/ml

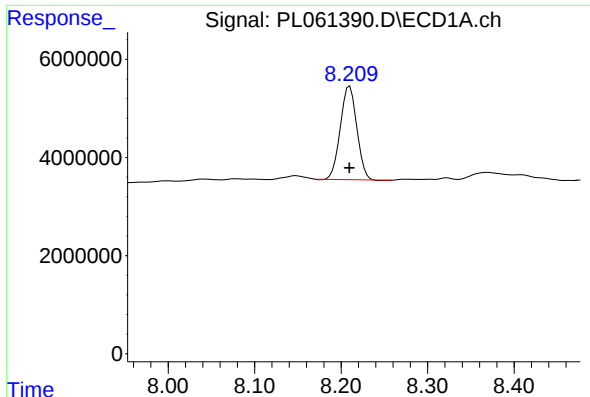

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 24996541
Conc: 14.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
BSY-WC-WATER-DRUM

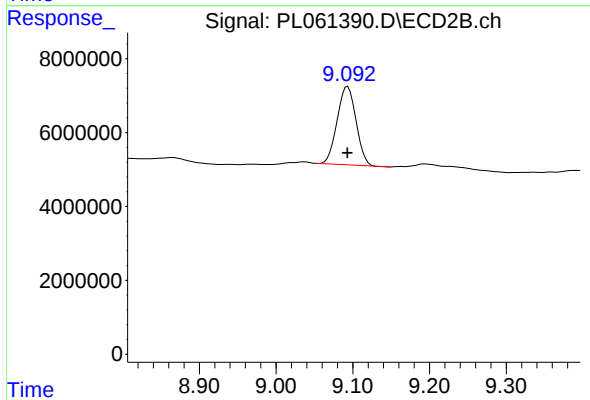

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 36150824
Conc: 15.29 ng/ml