

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
 Data File : PL061396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 17:51
 Operator : DD\AJ
 Sample : L3660-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VB25984

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:03:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 18:47:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.009	40390097	69017173	23.419m	22.438
28)	SA Decachlor...	8.210	9.094	39243224	56787099	23.522	24.016

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091120\
Data File : PL061396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 17:51
Operator : DD\AJ
Sample : L3660-14
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VB25984


Manual Integrations
APPROVED

Ankita
9/14/2020 11:03:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 18:47:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

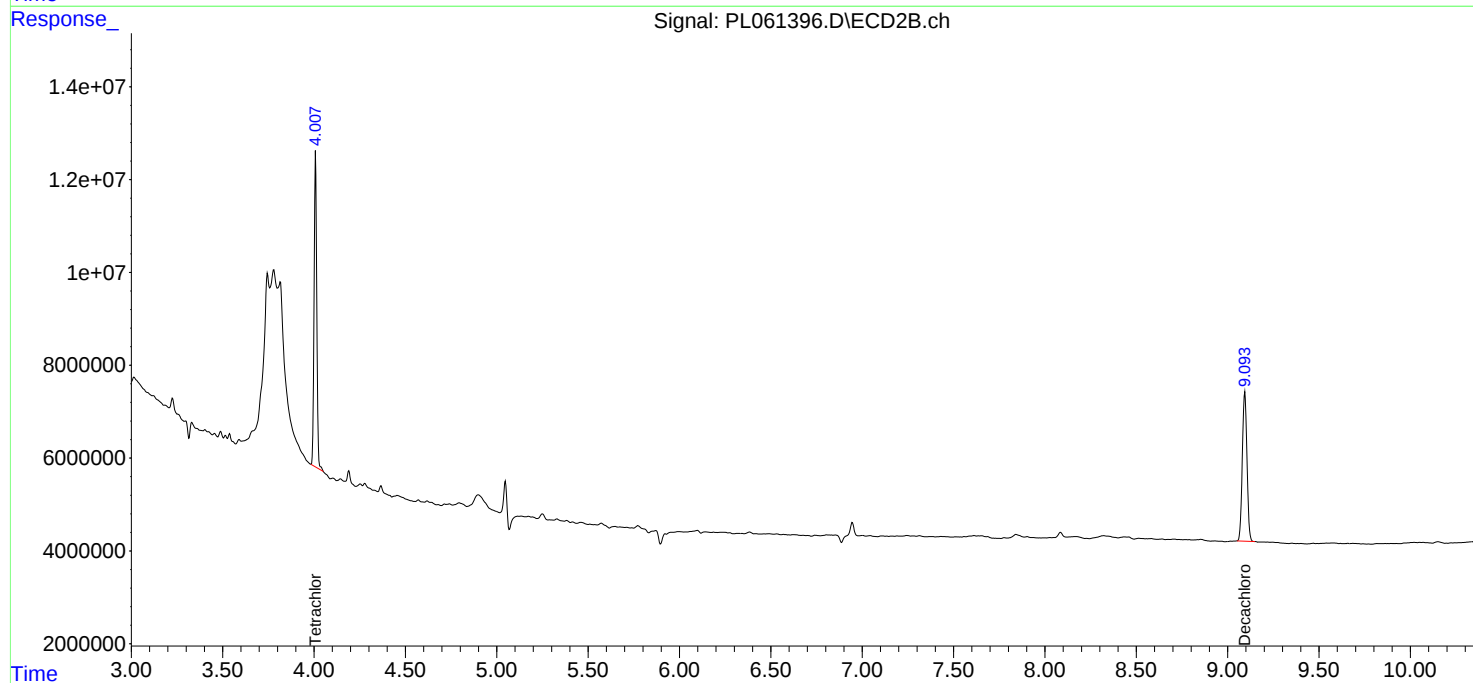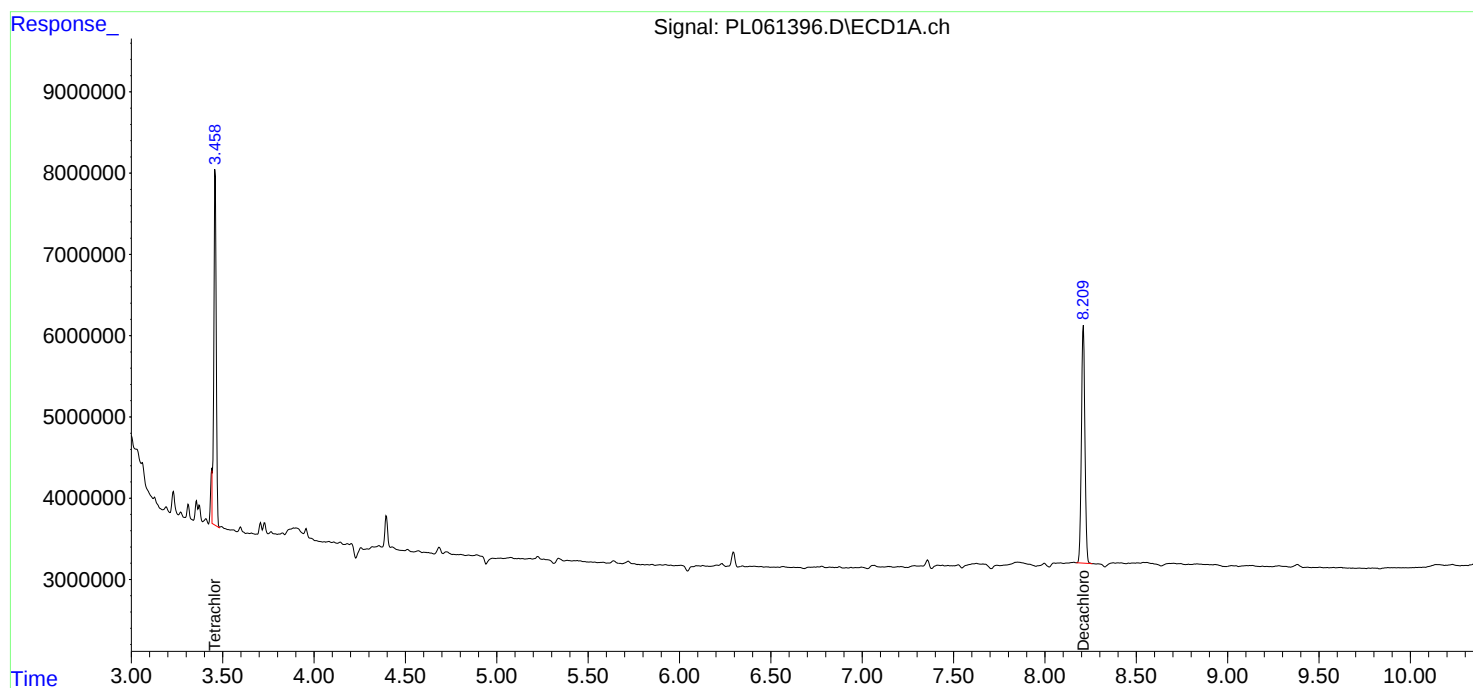

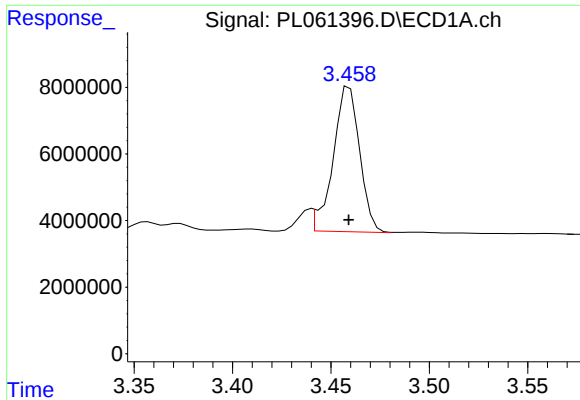


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 40390097
Conc: 23.42 ng/ml m

Instrument :
ECD_L
ClientSampleId :
VB25984


Manual Integrations
APPROVED

Ankita
9/14/2020 11:03:29 AM

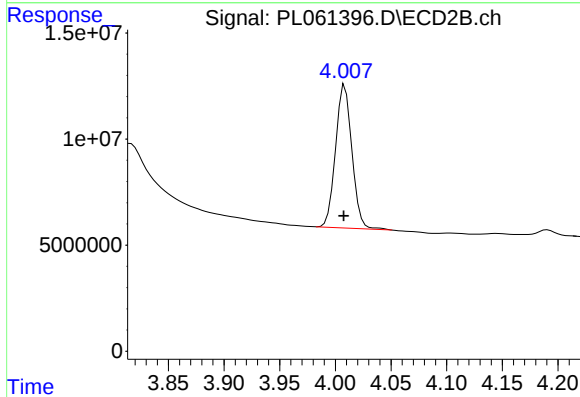


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.001 min
Response: 69017173
Conc: 22.44 ng/ml

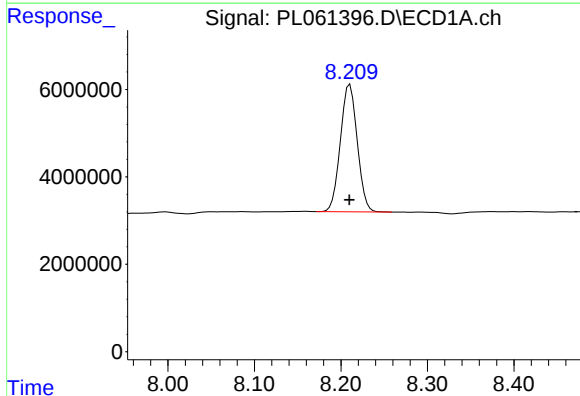

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 39243224
Conc: 23.52 ng/ml

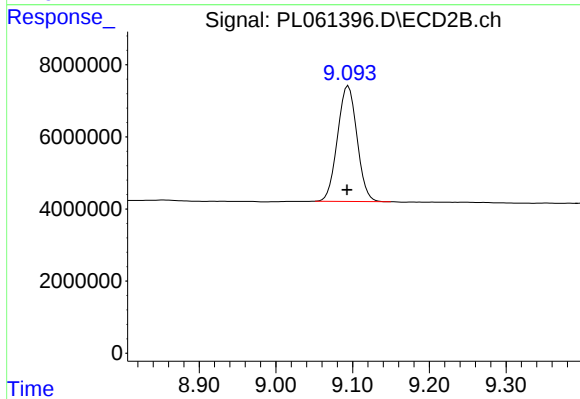

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.002 min
Response: 56787099
Conc: 24.02 ng/ml