

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091124\
 Data File : PL091632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2024 04:40
 Operator : AR\AJ
 Sample : P3861-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DN-B-37

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/11/2024
 Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 07:07:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.781	21904051	24660254	14.054	13.185
28) SA Decachlor...	9.054	7.920	20323250	30339661	16.723	16.430
Target Compounds						
17) MA 4,4'-DDT	7.022	6.043	3896043	4823687	2.970m	3.002

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091124\
Data File : PL091632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2024 04:40
Operator : AR\AJ
Sample : P3861-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DN-B-37


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/11/2024
Supervised By : Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 07:07:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

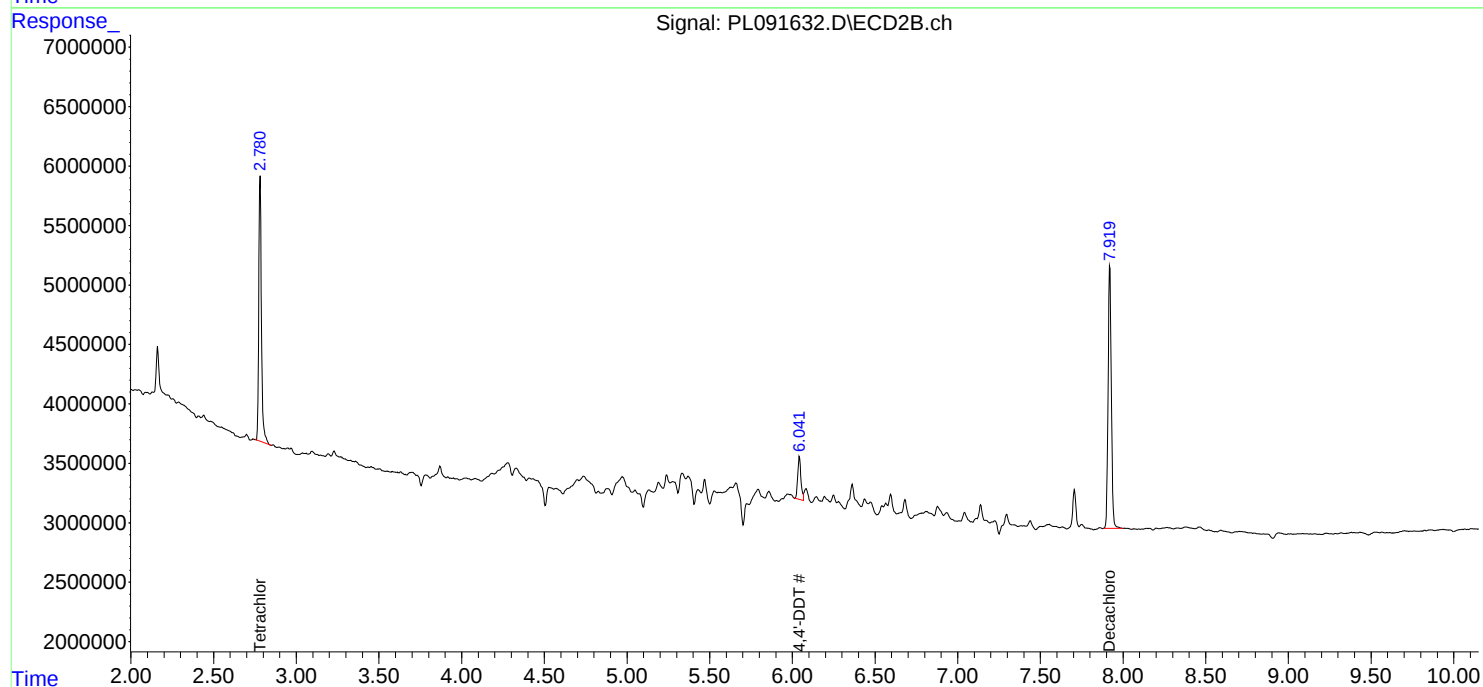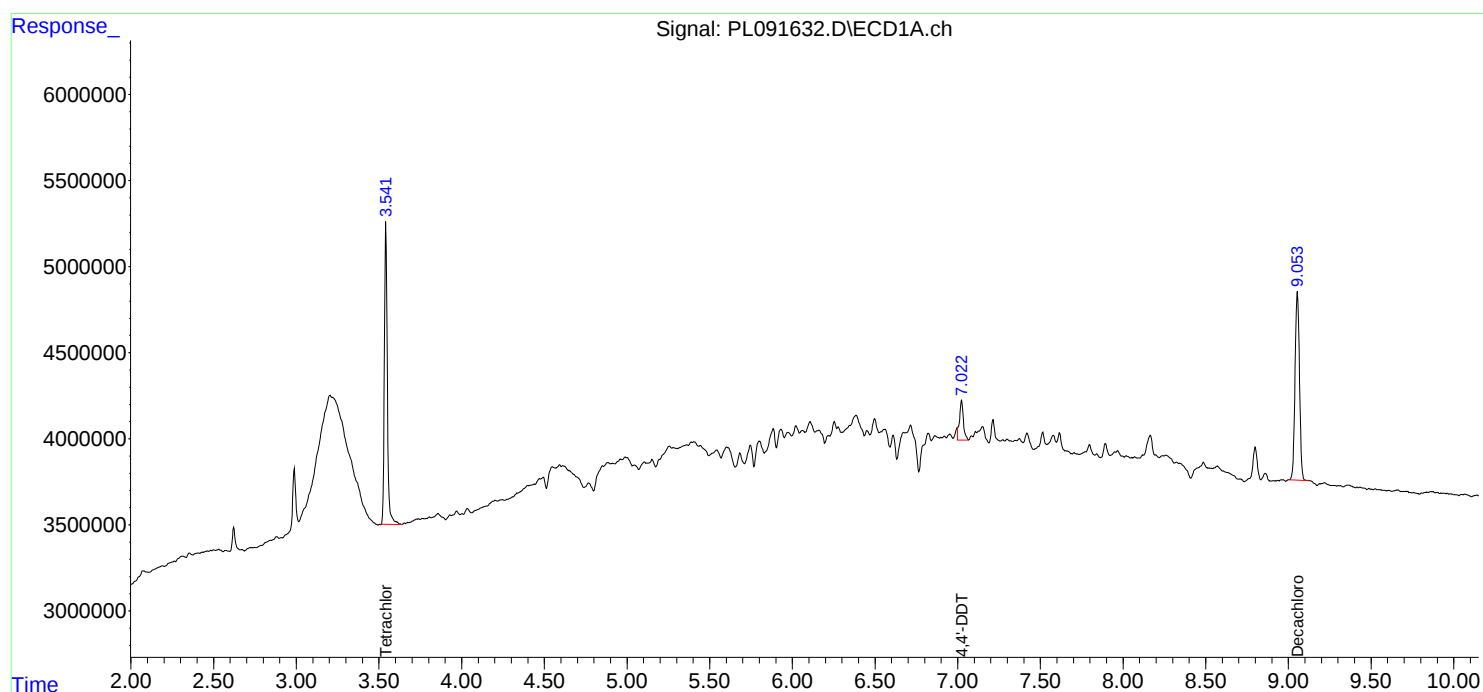

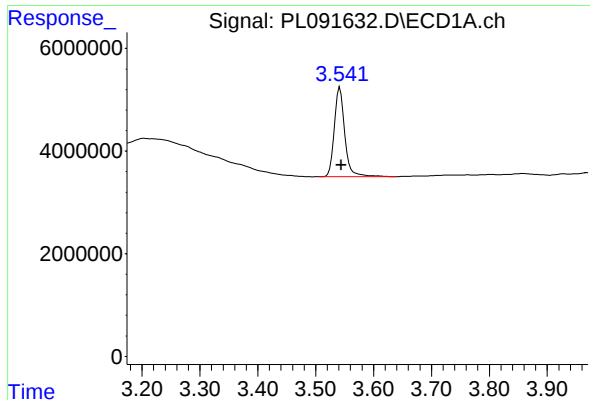


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 21904051
Conc: 14.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
DN-B-37


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/11/2024
Supervised By :Ankita Jodhani 09/12/2024

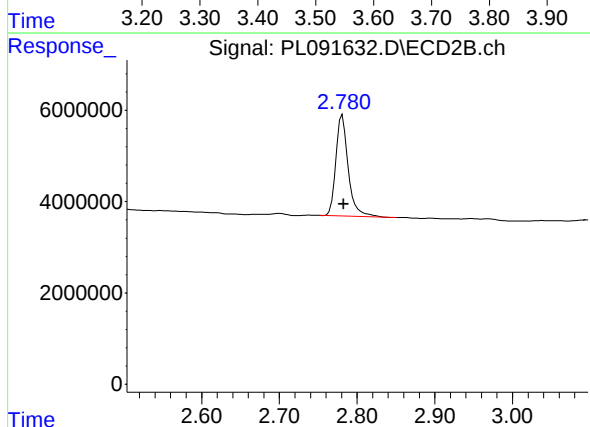


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: -0.002 min
Response: 24660254
Conc: 13.19 ng/ml

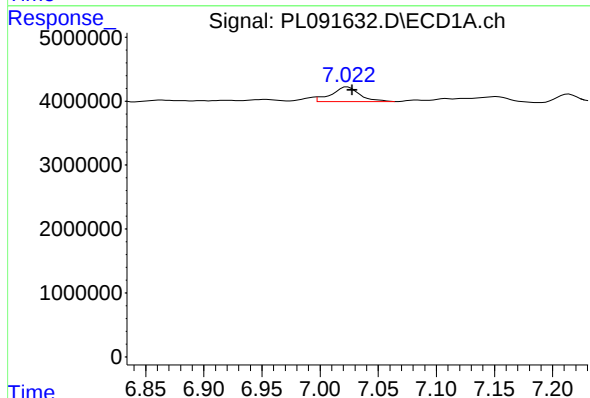


#17 4,4'-DDT

R.T.: 7.022 min
Delta R.T.: -0.005 min
Response: 3896043
Conc: 2.97 ng/ml m

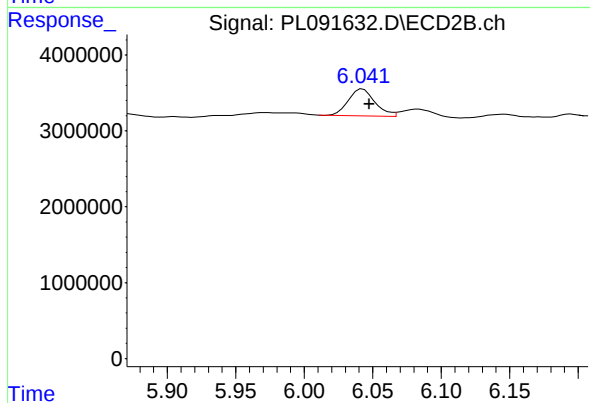

#17 4,4'-DDT

R.T.: 6.043 min
Delta R.T.: -0.005 min
Response: 4823687
Conc: 3.00 ng/ml

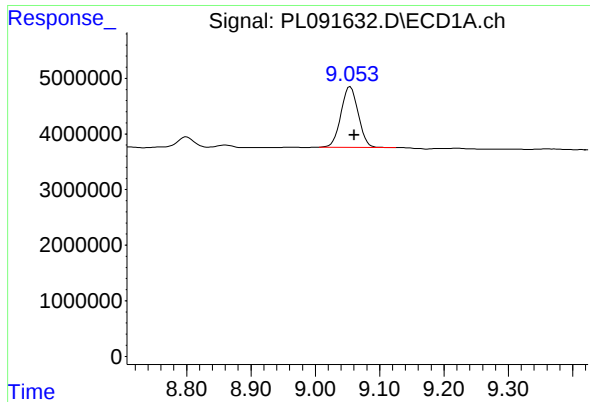


#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.006 min
Response: 20323250
Conc: 16.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
DN-B-37

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/11/2024
Supervised By :Ankita Jodhani 09/12/2024

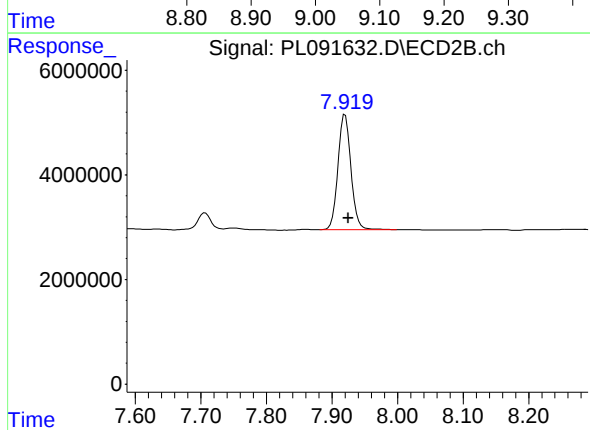

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: -0.005 min
Response: 30339661
Conc: 16.43 ng/ml