

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091124\
 Data File : PL091641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2024 08:09
 Operator : AR\AJ
 Sample : PB163261BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB163261BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/11/2024
 Supervised By : Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 09:12:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.783	31720892	35346759	20.352	18.899
28) SA Decachlor...	9.070	7.925	23907637	35614448	19.672	19.287m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091124\
Data File : PL091641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2024 08:09
Operator : AR\AJ
Sample : PB163261BL
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB163261BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/11/2024
Supervised By : Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 09:12:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

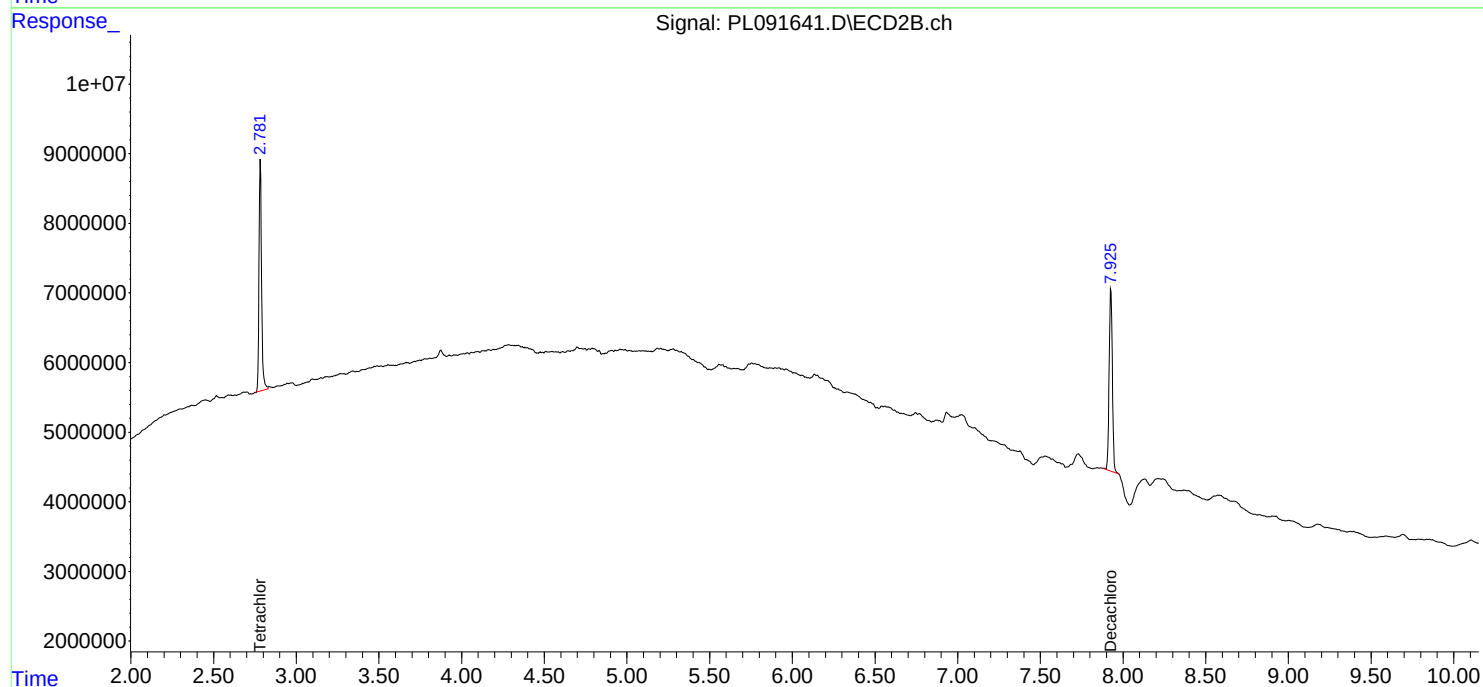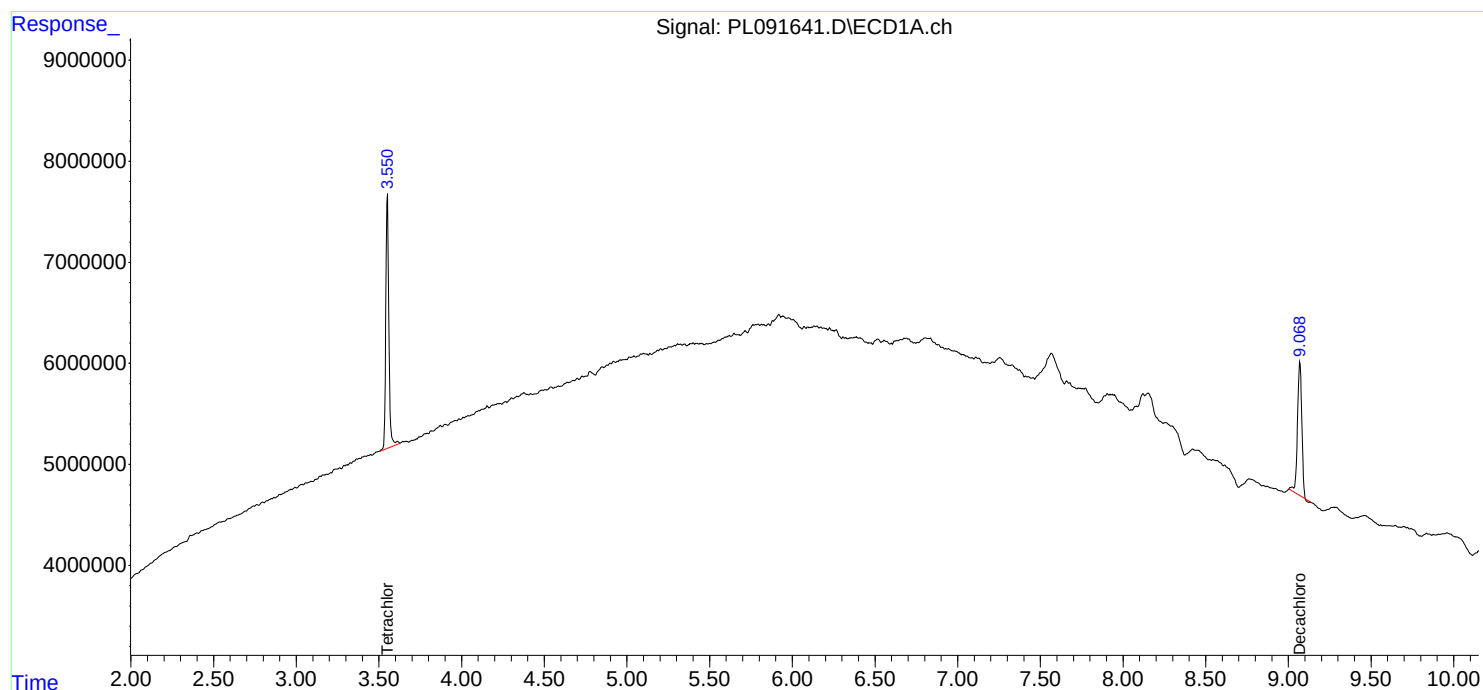

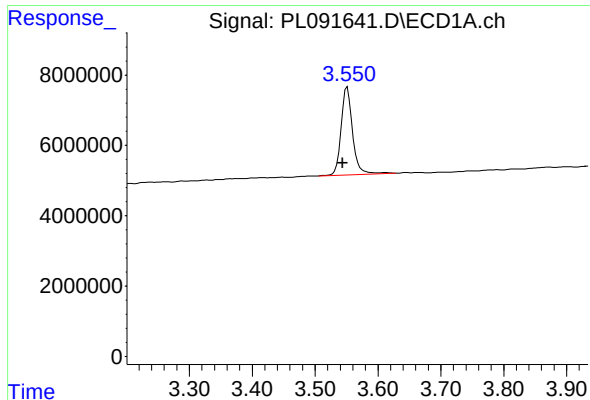


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.007 min
Response: 31720892
Conc: 20.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB163261BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/11/2024
Supervised By :Ankita Jodhani 09/12/2024

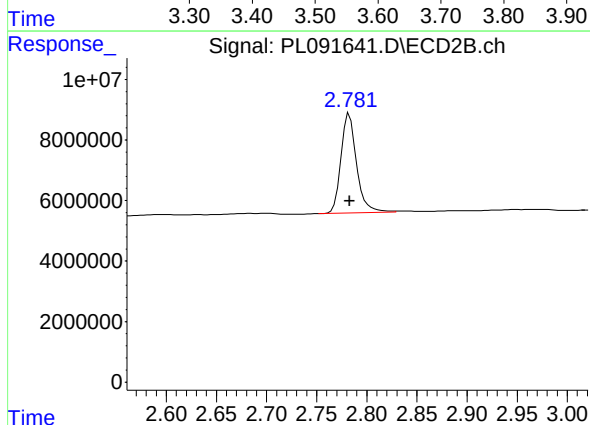


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 35346759
Conc: 18.90 ng/ml

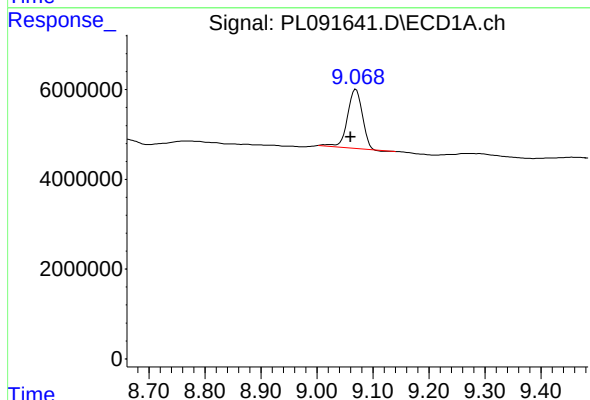

#28 Decachlorobiphenyl

R.T.: 9.070 min
Delta R.T.: 0.009 min
Response: 23907637
Conc: 19.67 ng/ml

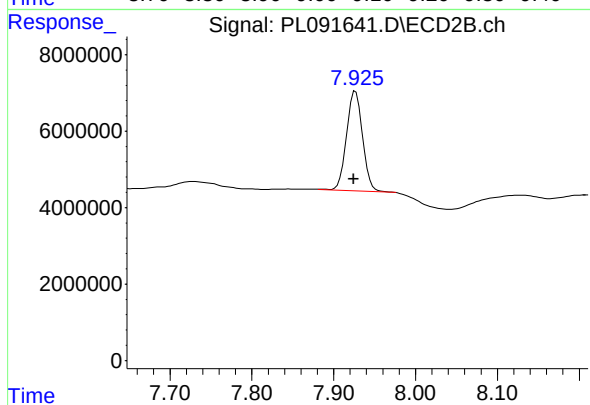

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 35614448
Conc: 19.29 ng/ml m