

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091125\
 Data File : PL097117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 10:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 07:09:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.823	68263670	101.2E6	17.309	17.963
28)	SA Decachlor...	8.998	7.982	53745318	99054732	18.153	20.655
Target Compounds							
8)	B Heptachlo...	5.643	0.000	39757485	0	7.726	N.D. #
13)	MA Dieldrin	0.000	5.412f	0	2773071	N.D.	0.423 #
14)	MA Endrin	0.000	5.710	0	30759502	N.D.	5.207 #
15)	B Endosulfa...	6.729f	0.000	29606129	0	6.721	N.D. #
16)	A 4,4'-DDD	6.659	0.000	10819444	0	3.428	N.D. #
18)	B Endrin al...	0.000	6.166	0	23121829	N.D.	1.123 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091125\
Data File : PL097117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 10:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 07:09:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

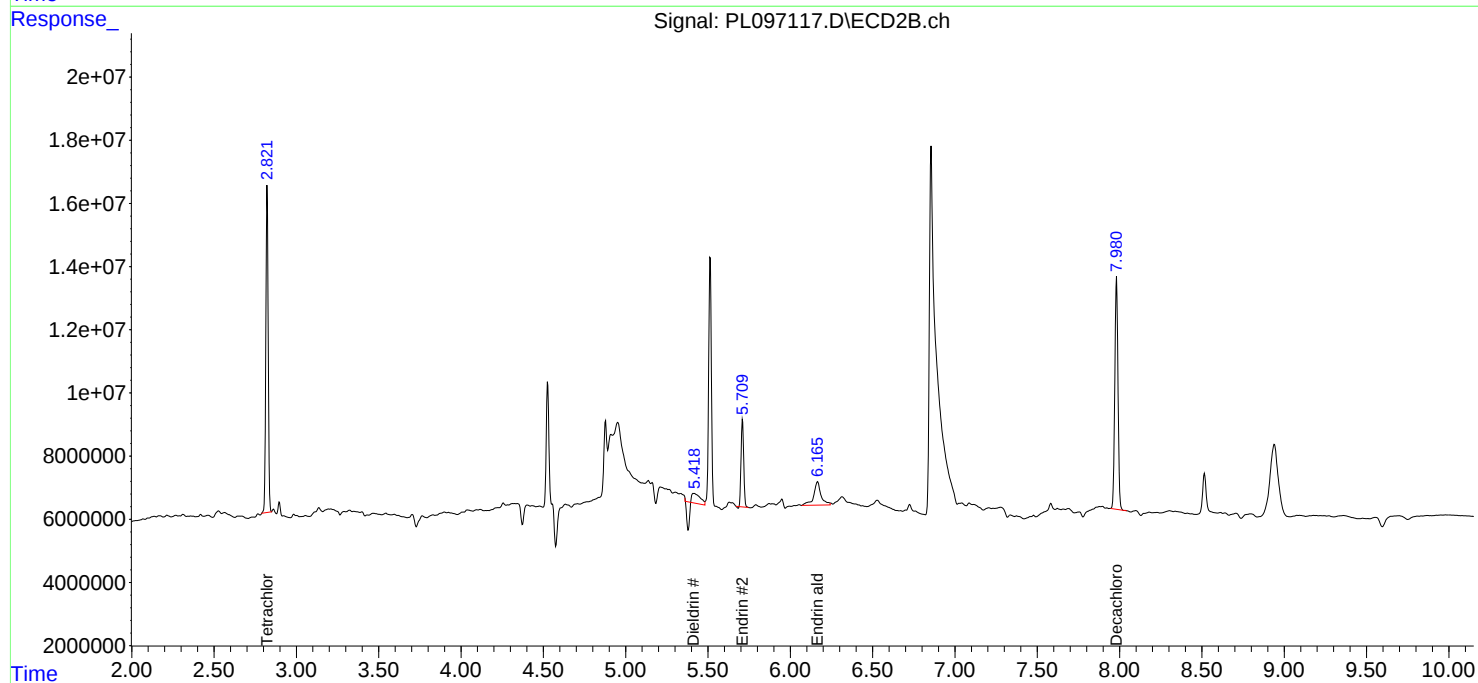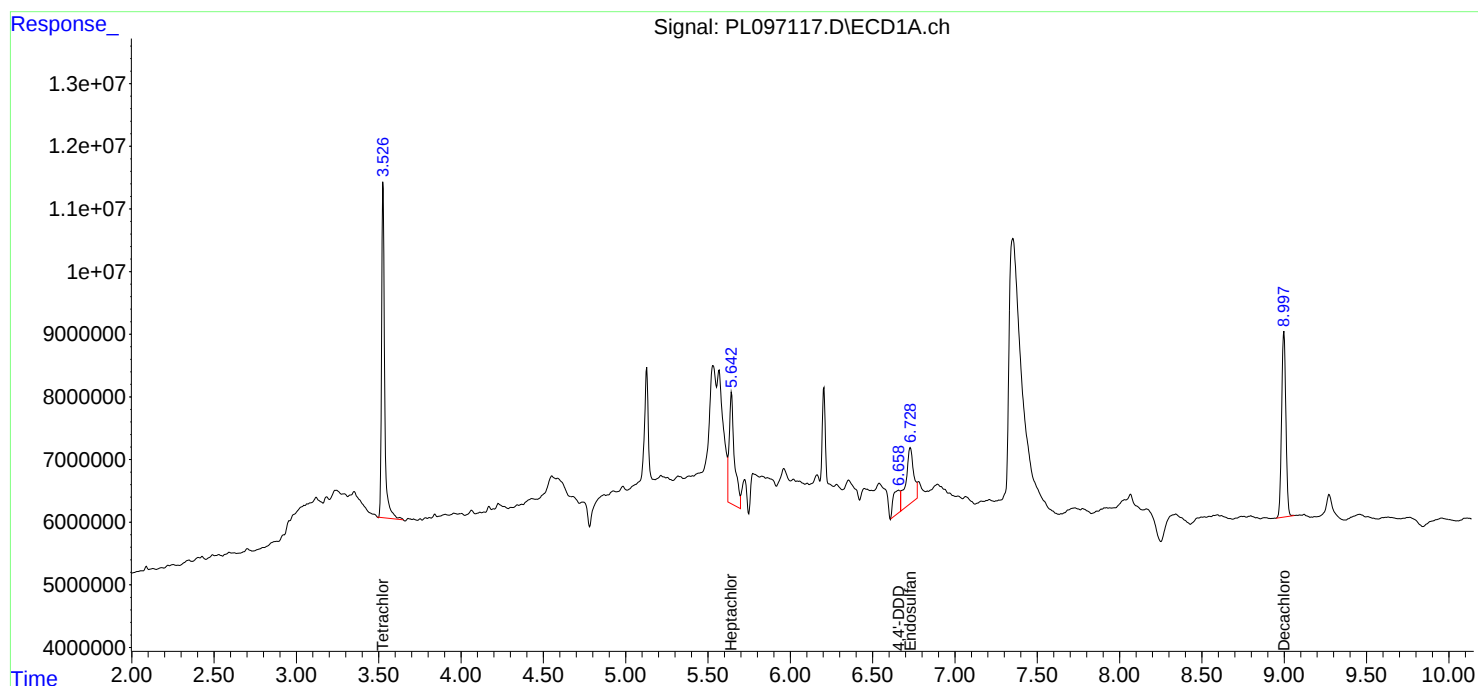


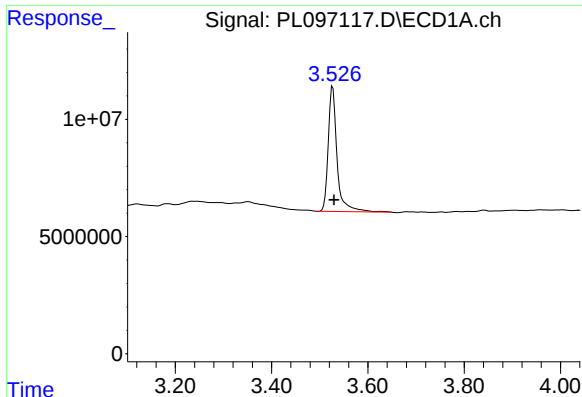

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: -0.003 min
Response: 68263670
Conc: 17.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

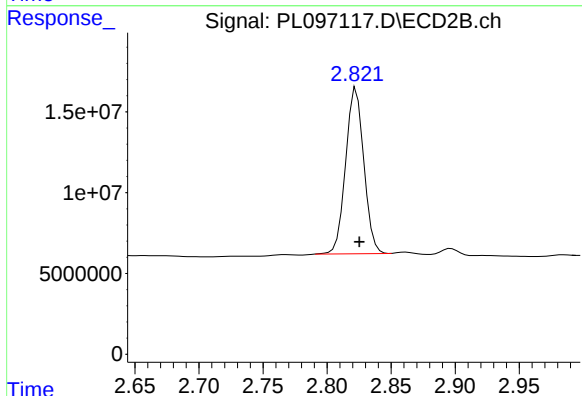


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: -0.003 min
Response: 101249169
Conc: 17.96 ng/ml

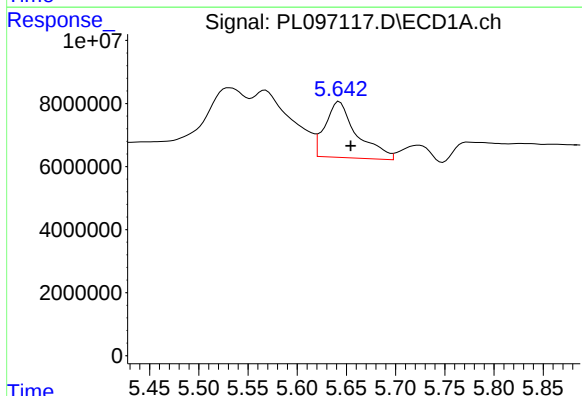


#8 Heptachlor epoxide

R.T.: 5.643 min
Delta R.T.: -0.012 min
Response: 39757485
Conc: 7.73 ng/ml

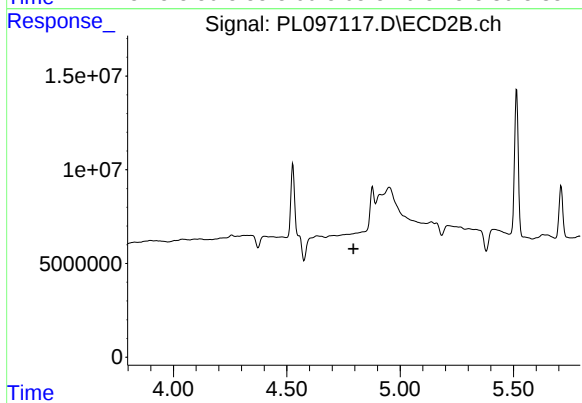

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.795 min
Response: 0
Conc: N.D.

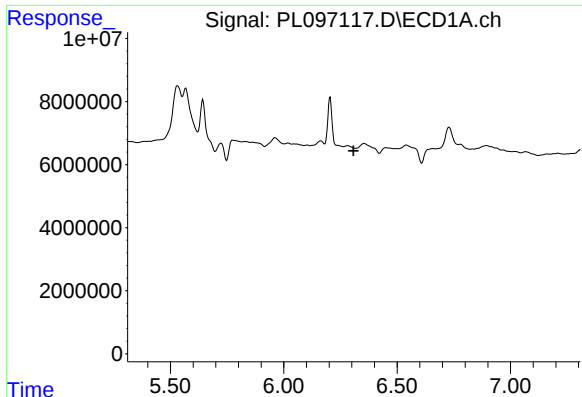

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.308 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

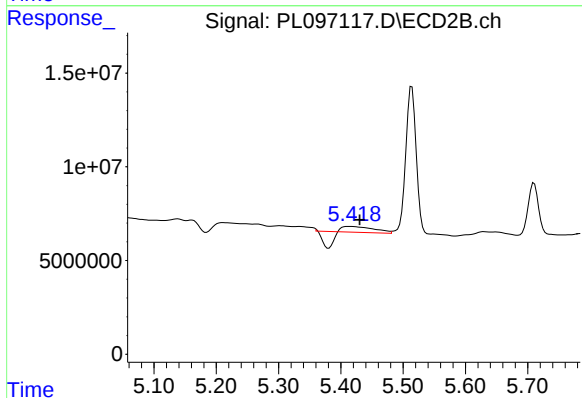


#13 Dieldrin

R.T.: 5.412 min
Delta R.T.: -0.018 min
Response: 2773071
Conc: 0.42 ng/ml

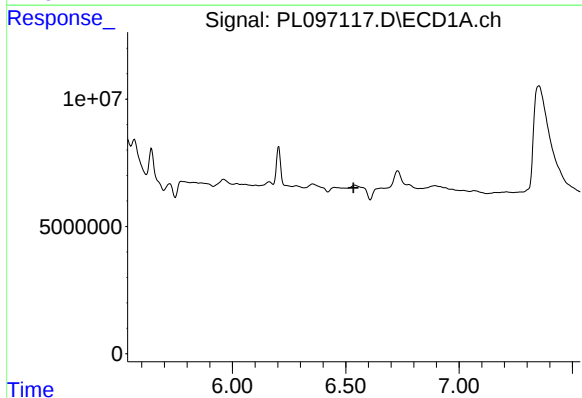


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.534 min
Response: 0
Conc: N.D.

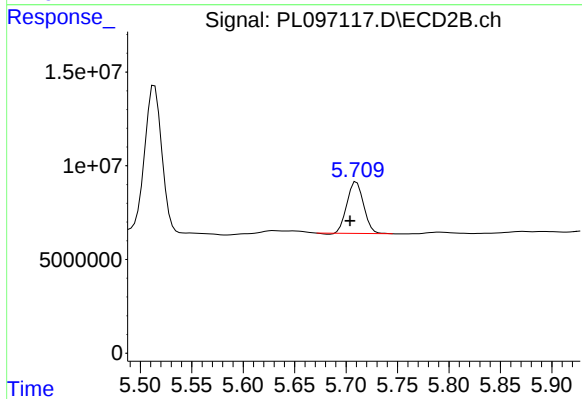

#14 Endrin


R.T.: 5.710 min
Delta R.T.: 0.006 min
Response: 30759502
Conc: 5.21 ng/ml

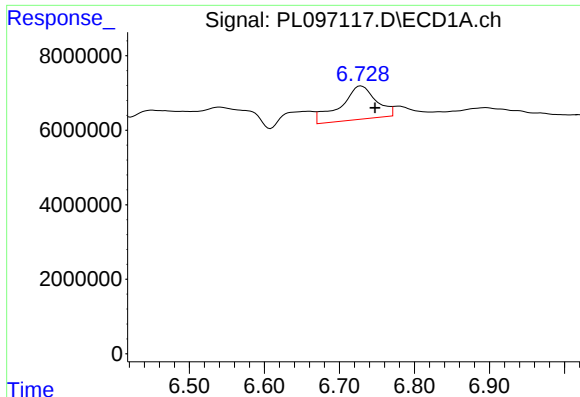

#15 Endosulfan II


R.T.: 6.729 min
Delta R.T.: -0.019 min
Response: 29606129
Conc: 6.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

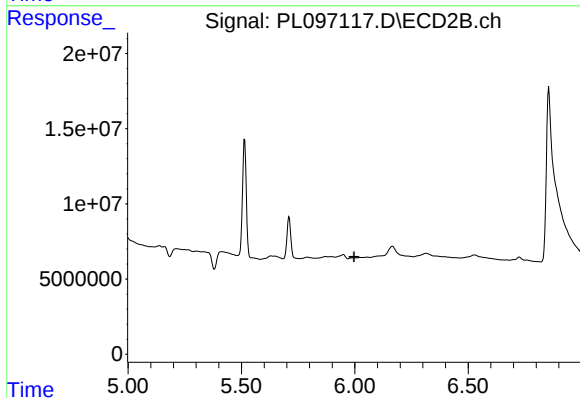


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

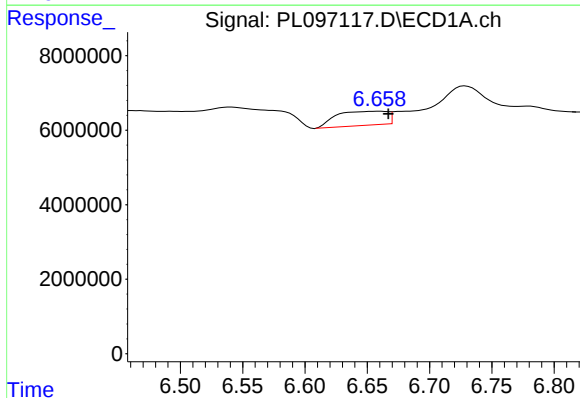


#16 4,4'-DDD

R.T.: 6.659 min
Delta R.T.: -0.008 min
Response: 10819444
Conc: 3.43 ng/ml

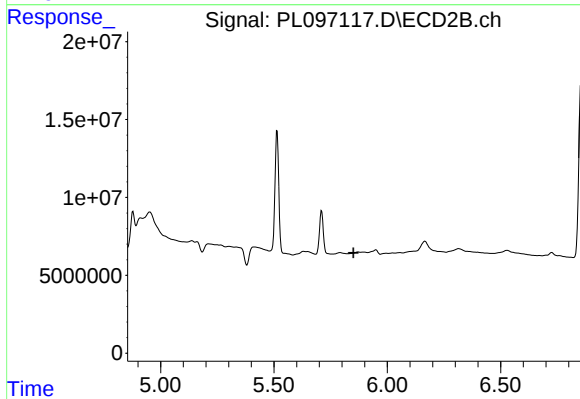

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.852 min
Response: 0
Conc: N.D.

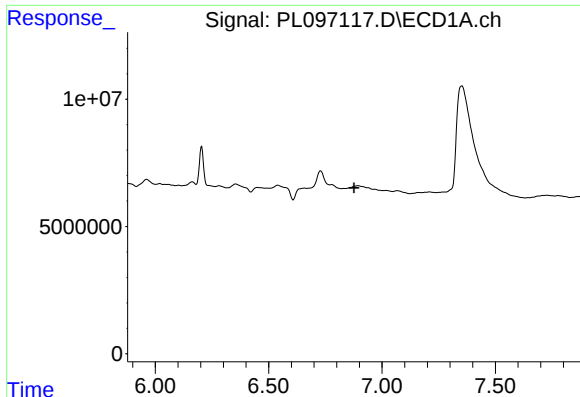

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.876 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

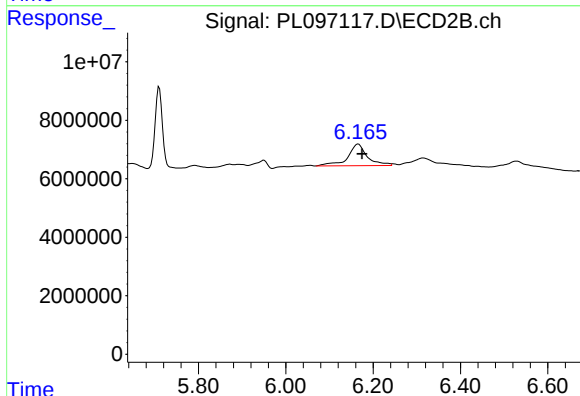


#18 Endrin aldehyde

R.T.: 6.166 min
Delta R.T.: -0.009 min
Response: 23121829
Conc: 1.12 ng/ml

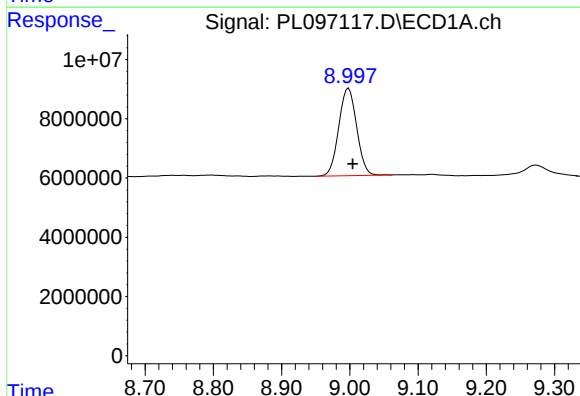

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: -0.006 min
Response: 53745318
Conc: 18.15 ng/ml

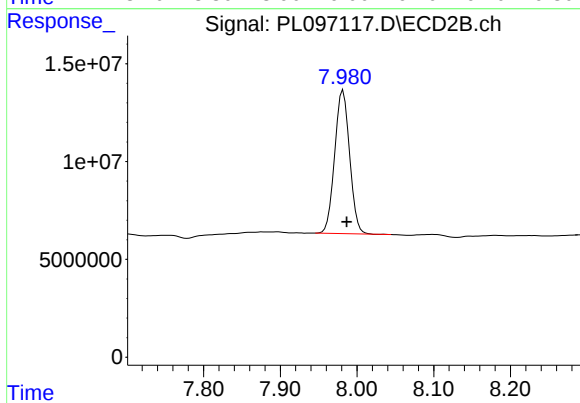

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.005 min
Response: 99054732
Conc: 20.65 ng/ml