

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091125\
 Data File : PL097135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 17:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 07:11:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.823	73797403	108.7E6	18.712	19.283
28)	SA Decachlor...	8.999	7.983	57382566	88176739	19.382	18.386
Target Compounds							
8)	B Heptachlo...	5.643	0.000	33152082	0	6.443	N.D. #
14)	MA Endrin	0.000	5.710	0	80592488	N.D.	13.643 #
15)	B Endosulfa...	6.734	0.000	1655156	0	0.376	N.D. #
24)	Chlordane-2	0.000	4.402	0	926592	N.D.	3.959 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091125\
Data File : PL097135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 17:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 07:11:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

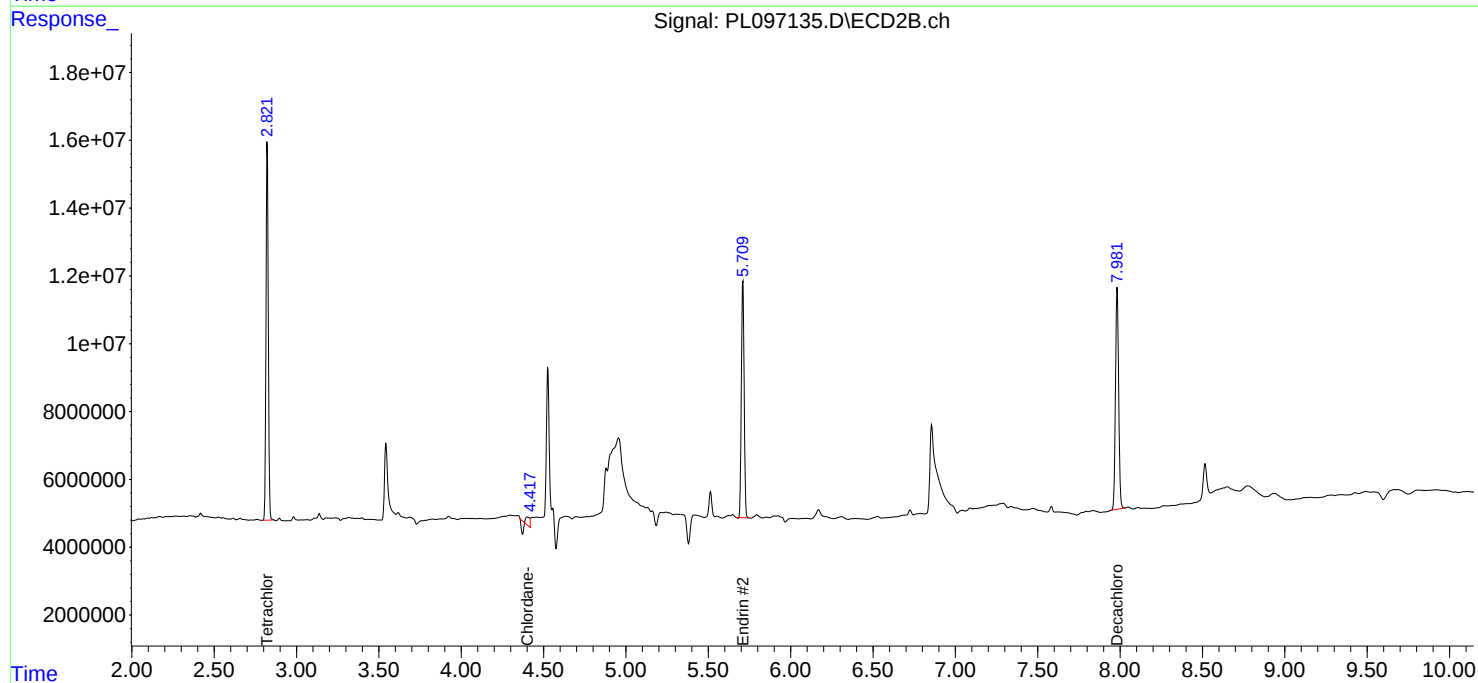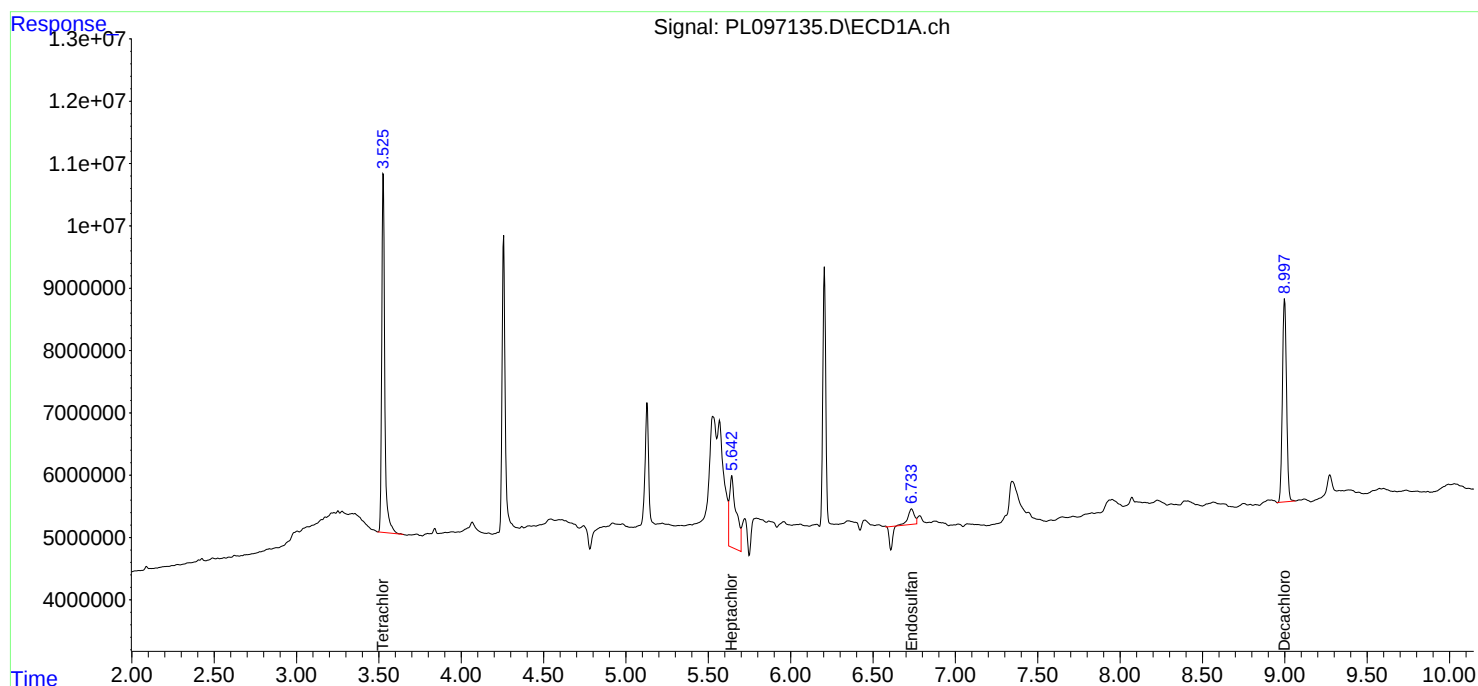


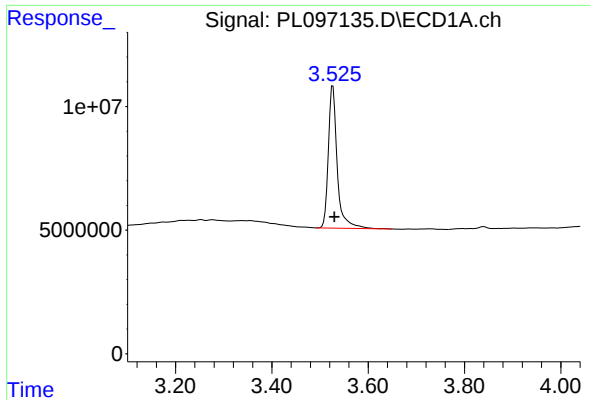

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: -0.003 min
Response: 73797403
Conc: 18.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

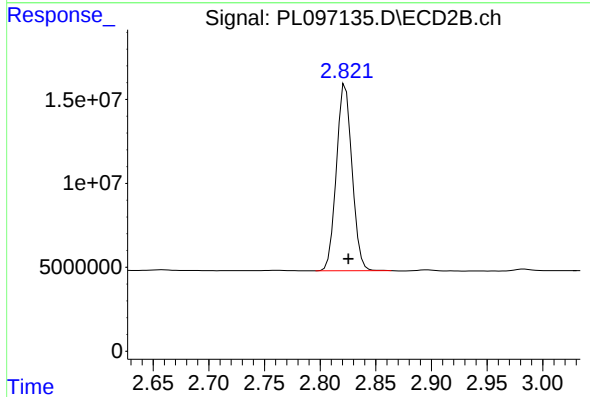


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: -0.003 min
Response: 108691003
Conc: 19.28 ng/ml

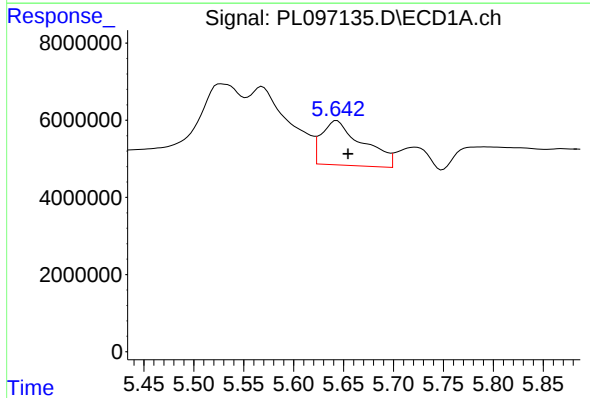


#8 Heptachlor epoxide

R.T.: 5.643 min
Delta R.T.: -0.011 min
Response: 33152082
Conc: 6.44 ng/ml

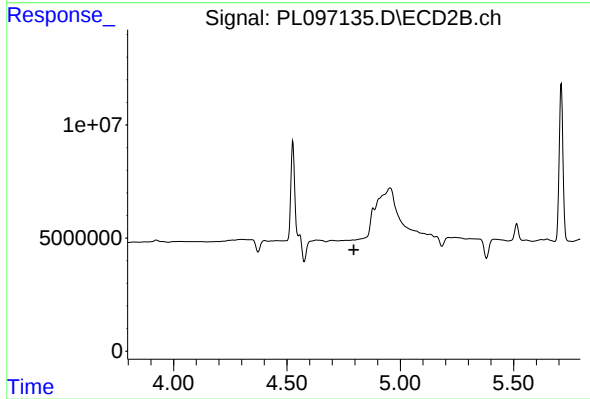

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.795 min
Response: 0
Conc: N.D.

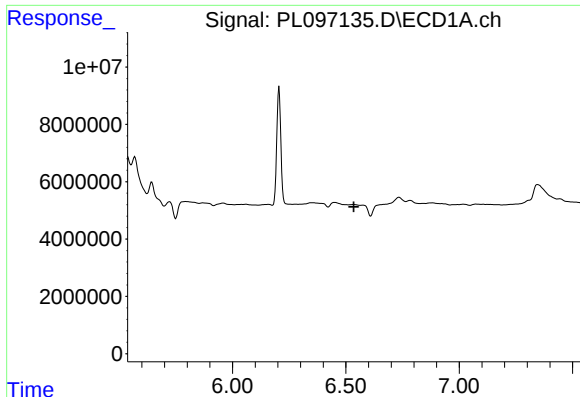

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

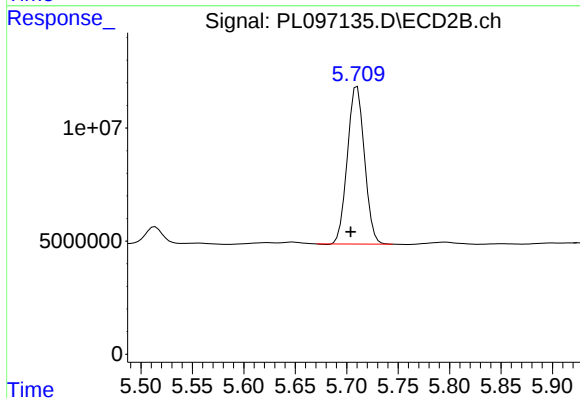


#14 Endrin

R.T.: 5.710 min
Delta R.T.: 0.006 min
Response: 80592488
Conc: 13.64 ng/ml

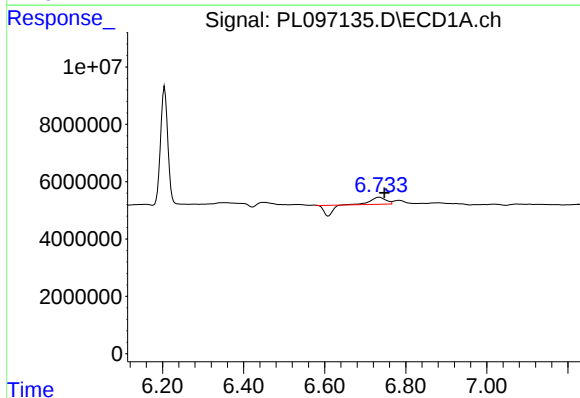


#15 Endosulfan II

R.T.: 6.734 min
Delta R.T.: -0.014 min
Response: 1655156
Conc: 0.38 ng/ml

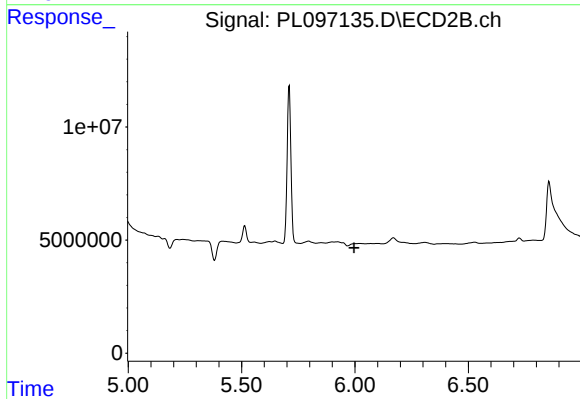

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

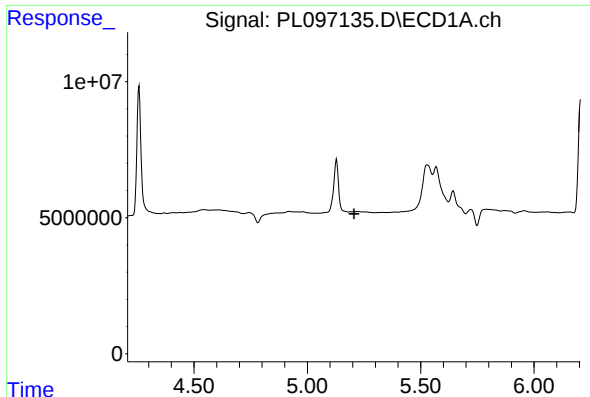

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

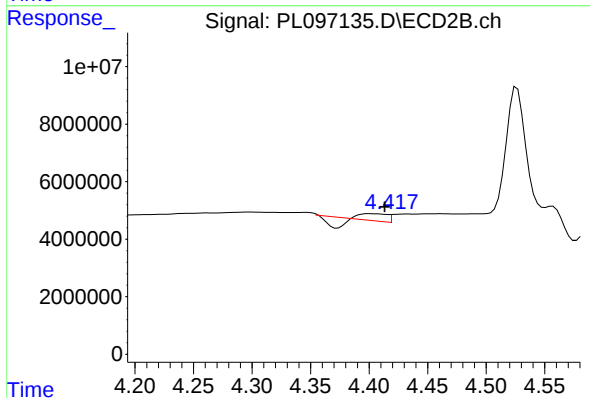


#24 Chlordane-2

R.T.: 4.402 min
Delta R.T.: -0.012 min
Response: 926592
Conc: 3.96 ng/ml

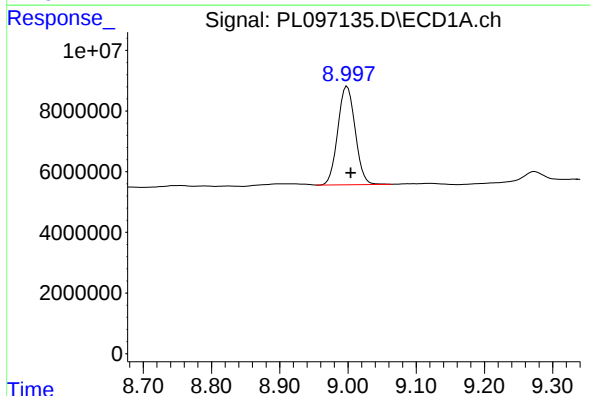

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.005 min
Response: 57382566
Conc: 19.38 ng/ml

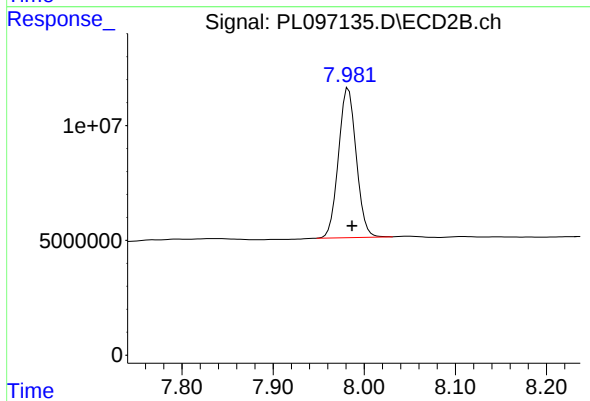

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.004 min
Response: 88176739
Conc: 18.39 ng/ml