

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091218\
 Data File : PL039855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2018 17:36
 Operator : AJ\SJ
 Sample : J4842-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 02:38:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.905	135.4E6	59381099	19.370	22.150
28)	SA Decachlor...	7.953	8.890	147.2E6	54604427	20.955	23.530
Target Compounds							
20)	A Methoxychlor	6.693	0.000	8754070	0	2.139	N.D. #
23)	Chlordane-1	4.190	0.000	5284988	0	16.694	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091218\
Data File : PL039855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2018 17:36
Operator : AJ\SJ
Sample : J4842-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 02:38:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

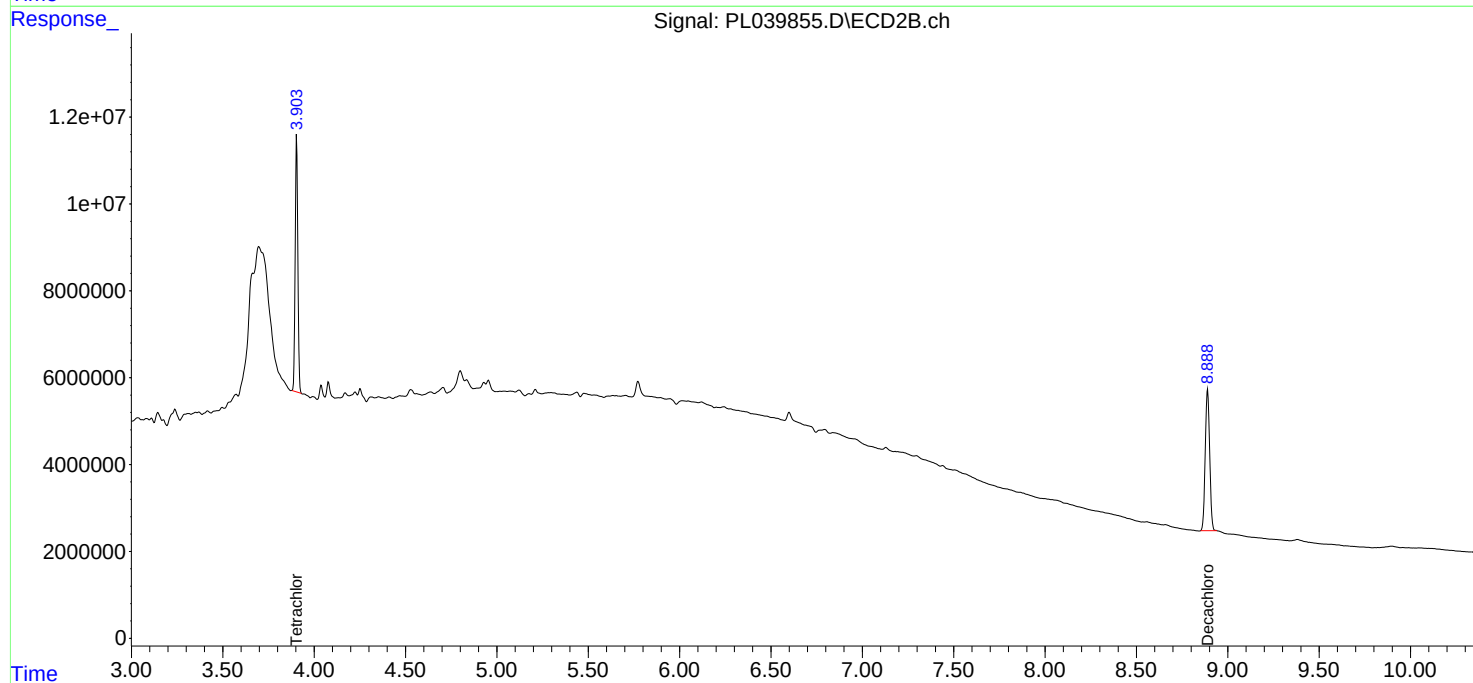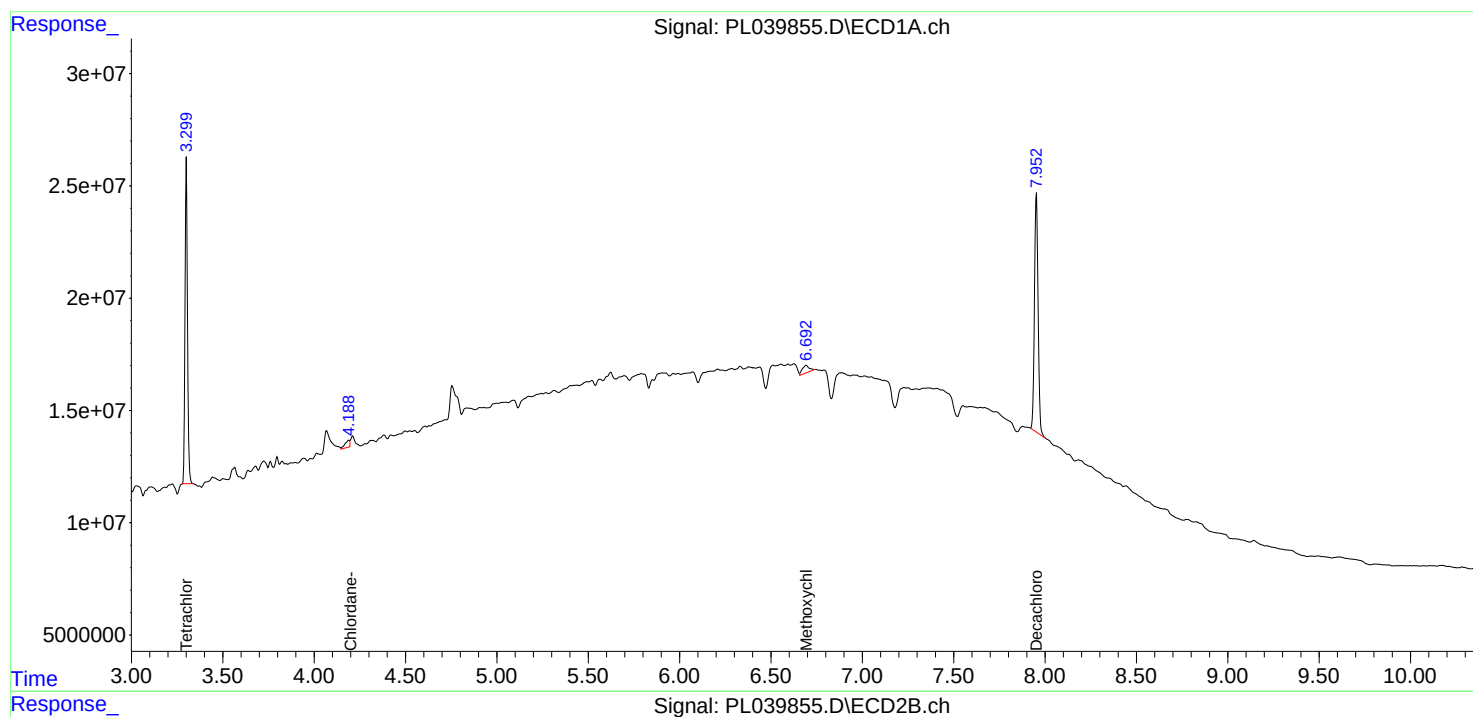


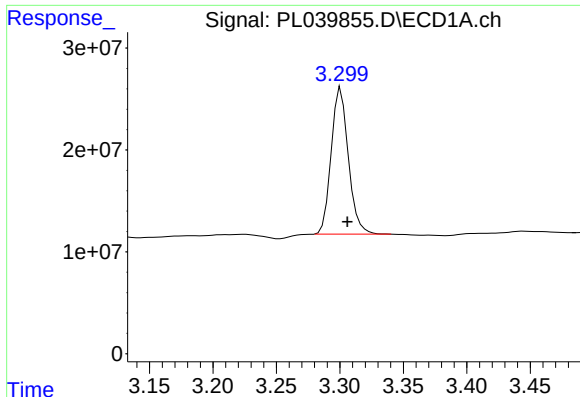

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: -0.005 min
Response: 135401005
Conc: 19.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

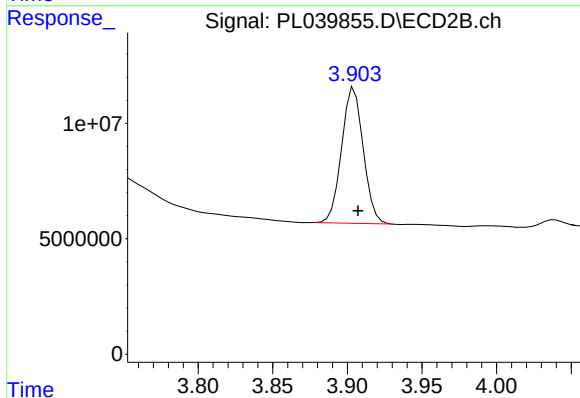


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.003 min
Response: 59381099
Conc: 22.15 ng/ml

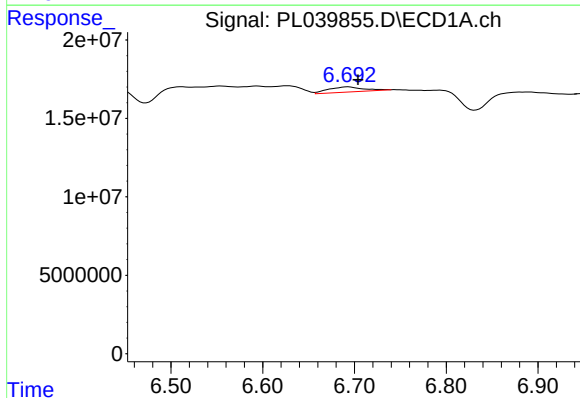


#20 Methoxychlor

R.T.: 6.693 min
Delta R.T.: -0.011 min
Response: 8754070
Conc: 2.14 ng/ml

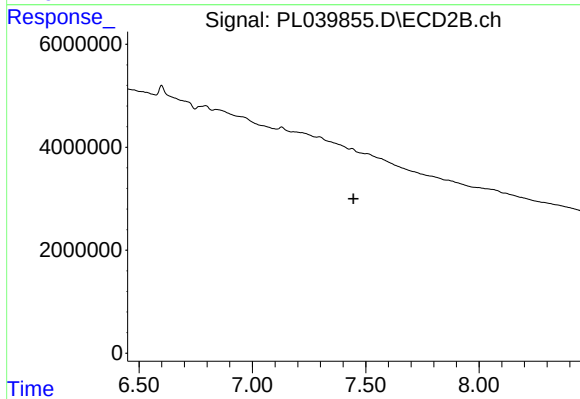

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

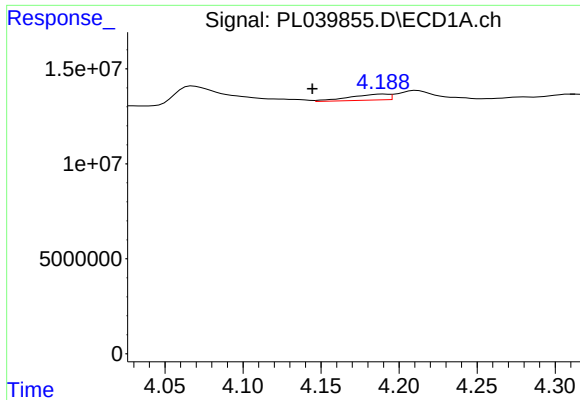

#23 Chlordane-1


R.T.: 4.190 min
Delta R.T.: 0.045 min
Response: 5284988
Conc: 16.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

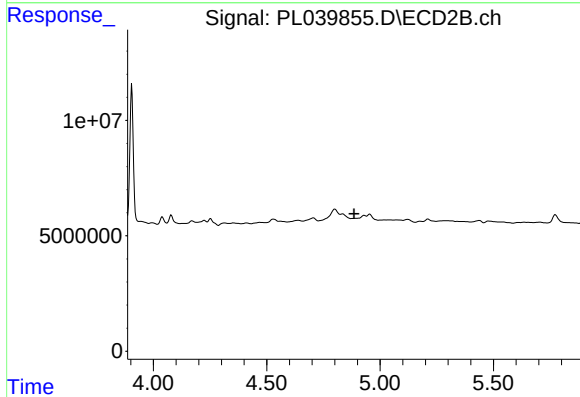


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

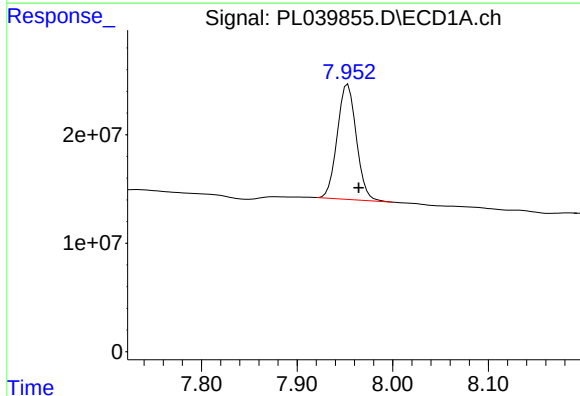

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: -0.011 min
Response: 147174476
Conc: 20.95 ng/ml

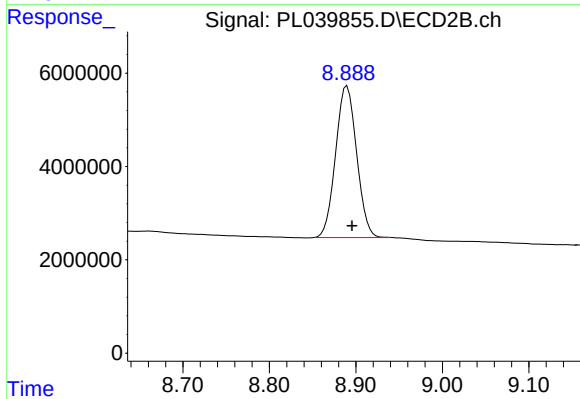

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: -0.006 min
Response: 54604427
Conc: 23.53 ng/ml