

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091218\
 Data File : PL039866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2018 09:51
 Operator : AJ\SJ
 Sample : J4856-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 10:07:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.306	3.903	175.8E6	76010049	25.146	28.352
28)	SA Decachlor...	7.958	8.890	161.8E6	61117510	23.043	26.337
Target Compounds							
6)	B beta-BHC	4.221f	0.000	7790866	0	1.677	N.D. #
8)	B Heptachlo...	4.916f	0.000	56897801	0	5.958	N.D. #
9)	A Endosulfan I	5.325	0.000	8812356	0	1.006	N.D. #
15)	B Endosulfa...	6.083	0.000	19321485	0	2.222	N.D. #
16)	A 4,4'-DDD	5.918	0.000	4366073	0	0.548	N.D. #
17)	MA 4,4'-DDT	6.152	0.000	3835055	0	0.506	N.D. #
23)	Chlordane-1	4.176	0.000	10137548	0	32.021	N.D. #
27)	Chlordane-5	6.083	0.000	19321485	0	59.574	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091218\
Data File : PL039866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2018 09:51
Operator : AJ\SJ
Sample : J4856-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 10:07:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

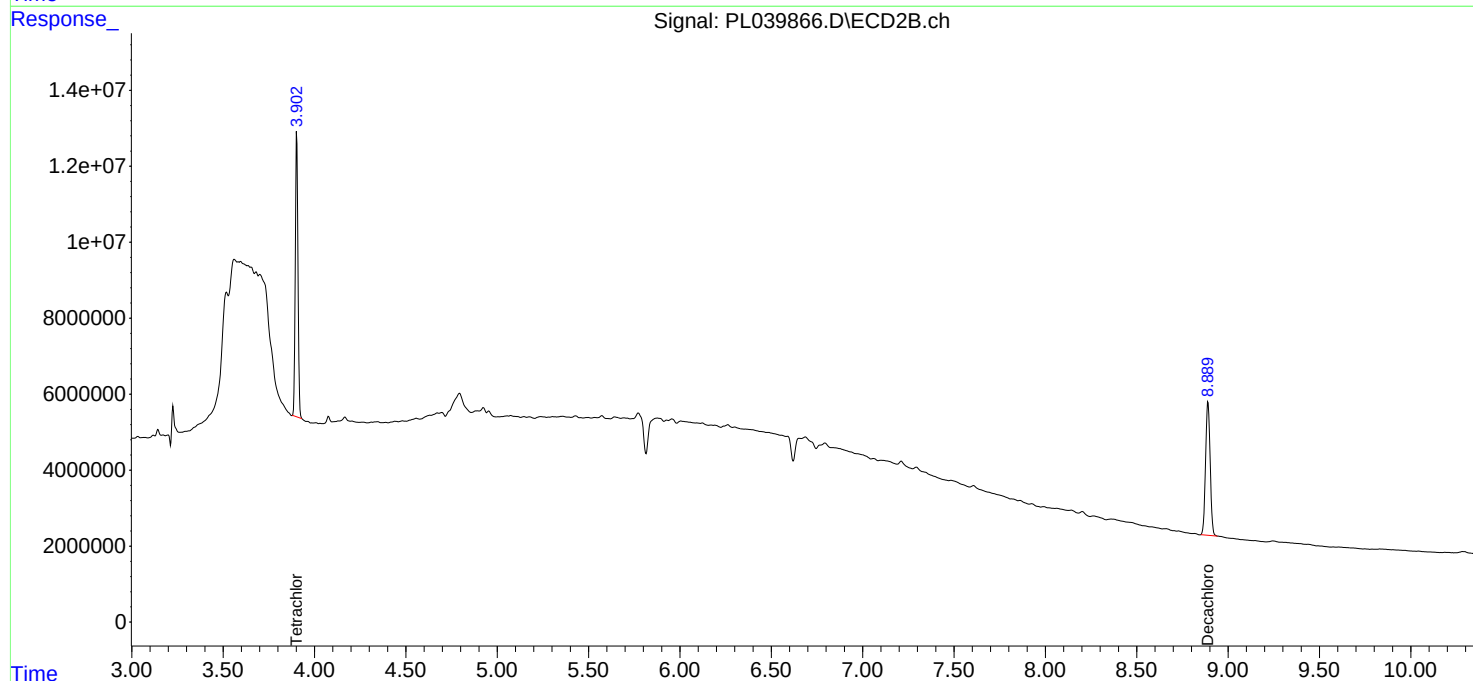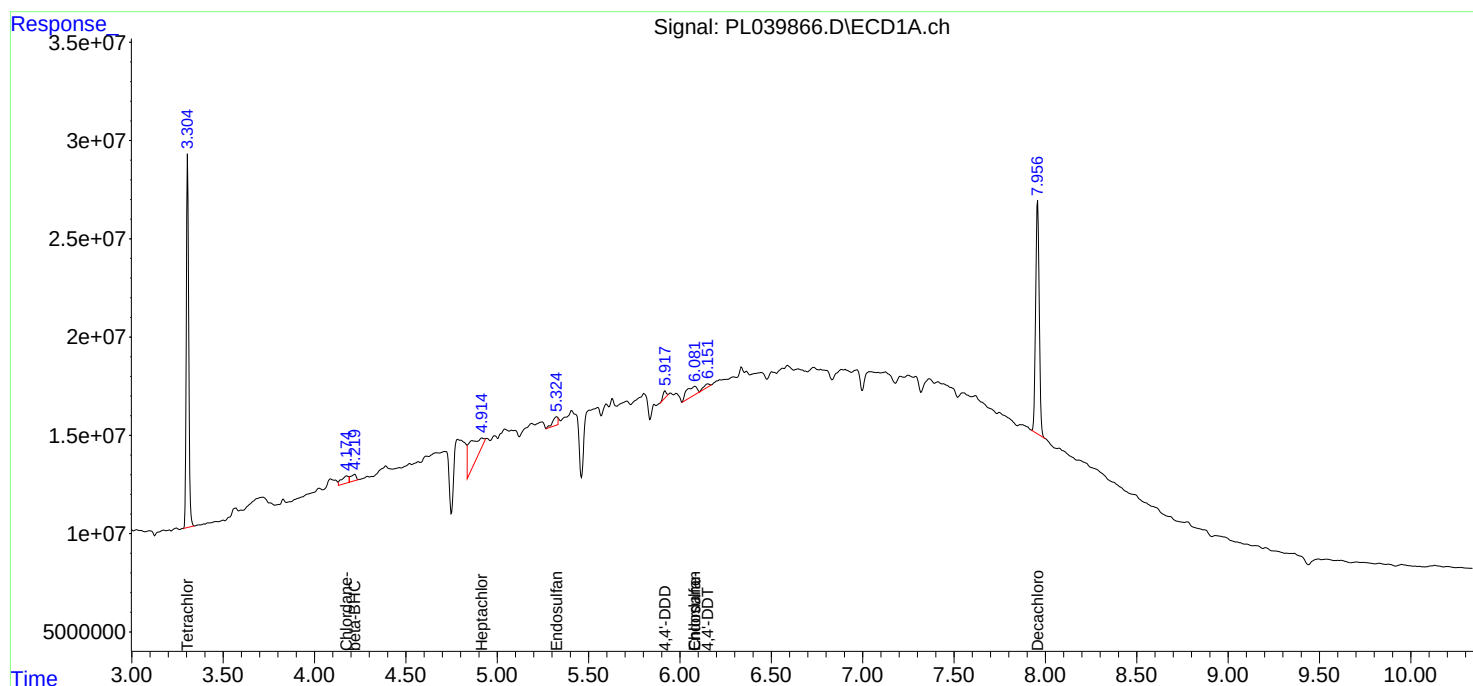


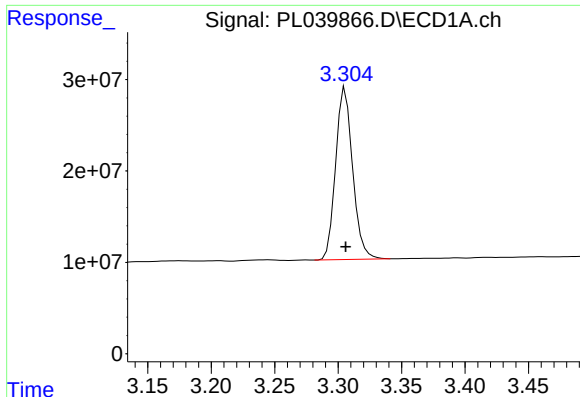

#1 Tetrachloro-m-xylene


R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 175778027
Conc: 25.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

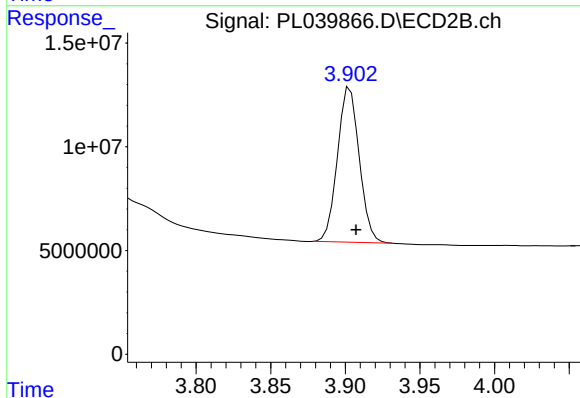


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: -0.004 min
Response: 76010049
Conc: 28.35 ng/ml

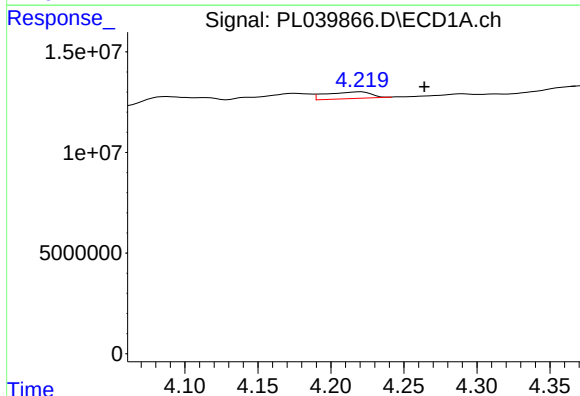


#6 beta-BHC

R.T.: 4.221 min
Delta R.T.: -0.043 min
Response: 7790866
Conc: 1.68 ng/ml

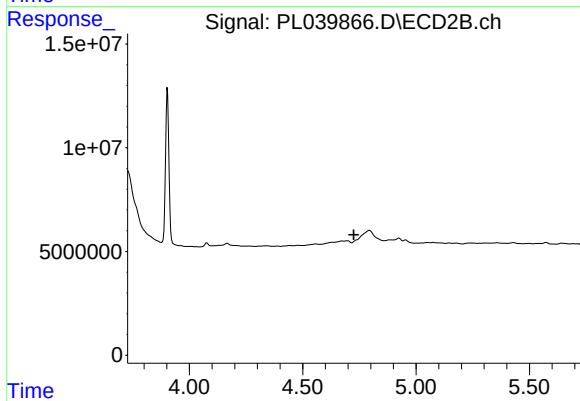

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

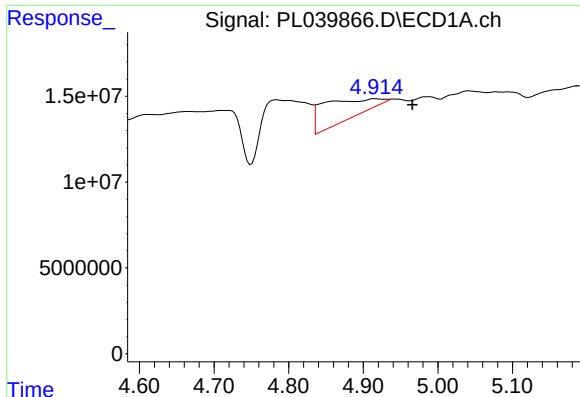

#8 Heptachlor epoxide


R.T.: 4.916 min
Delta R.T.: -0.050 min
Response: 56897801
Conc: 5.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

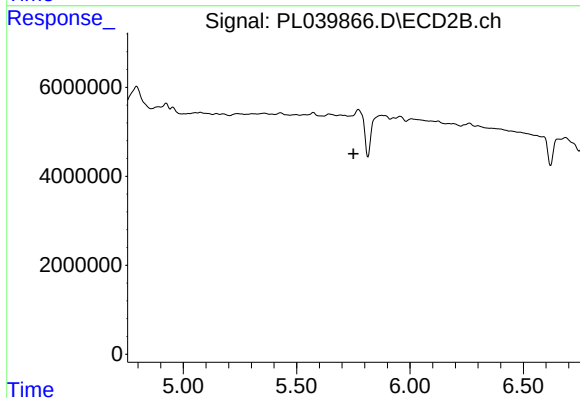


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

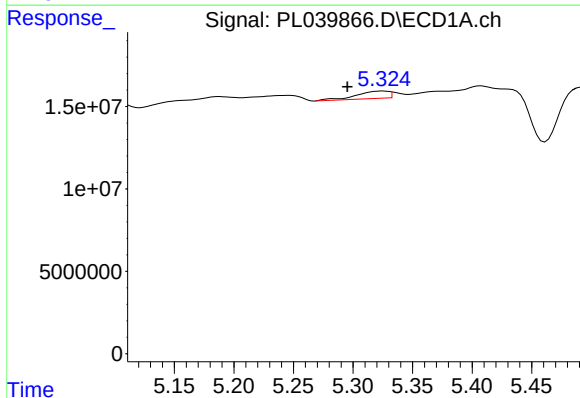


#9 Endosulfan I

R.T.: 5.325 min
Delta R.T.: 0.030 min
Response: 8812356
Conc: 1.01 ng/ml

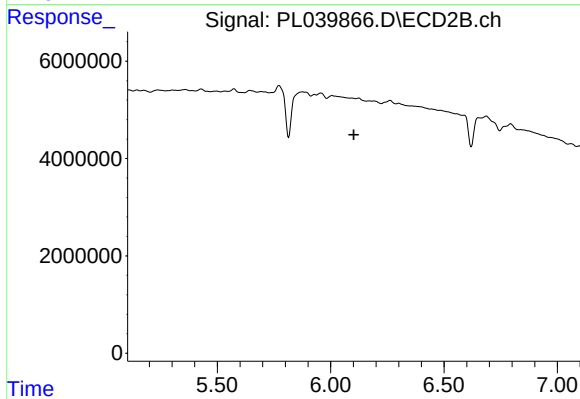

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

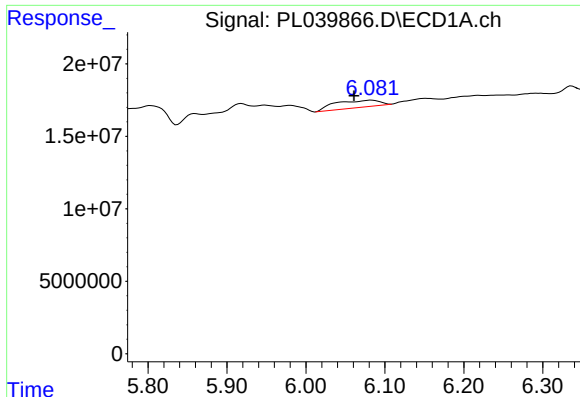

#15 Endosulfan II


R.T.: 6.083 min
Delta R.T.: 0.021 min
Response: 19321485
Conc: 2.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

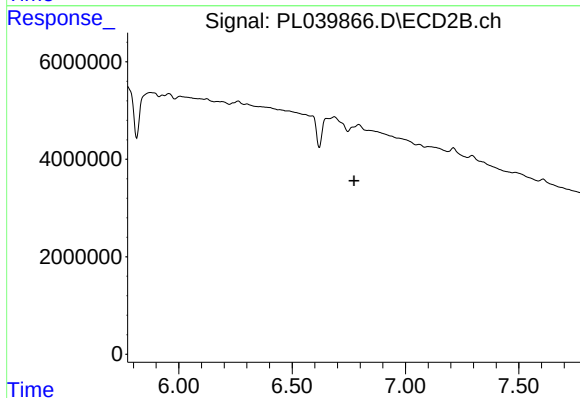


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

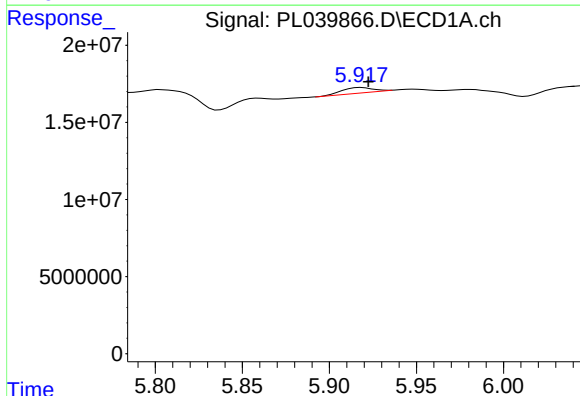


#16 4,4'-DDD

R.T.: 5.918 min
Delta R.T.: -0.004 min
Response: 4366073
Conc: 0.55 ng/ml

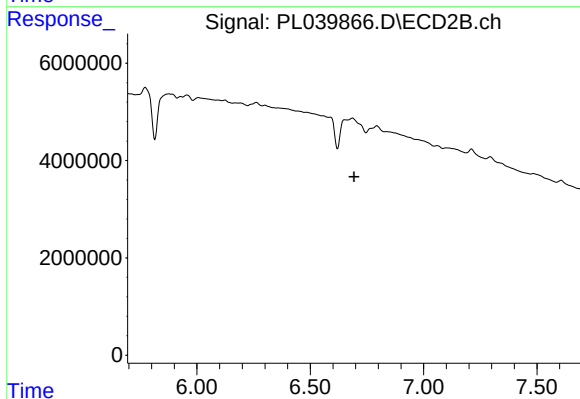

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

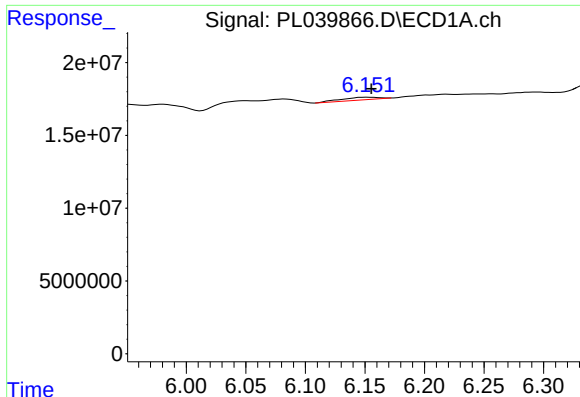

#17 4,4'-DDT


R.T.: 6.152 min
Delta R.T.: -0.003 min
Response: 3835055
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

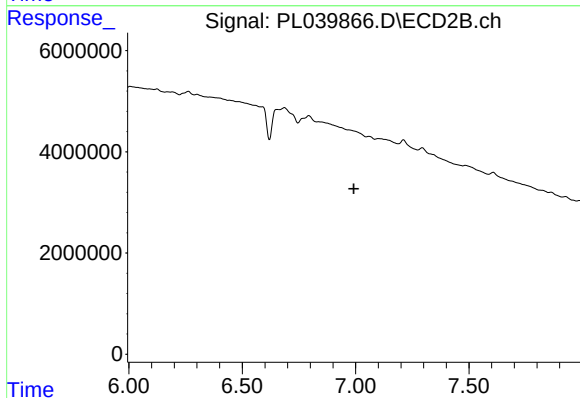


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

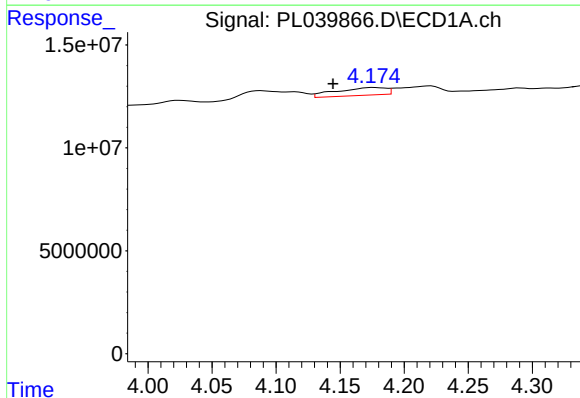


#23 Chlordane-1

R.T.: 4.176 min
Delta R.T.: 0.032 min
Response: 10137548
Conc: 32.02 ng/ml

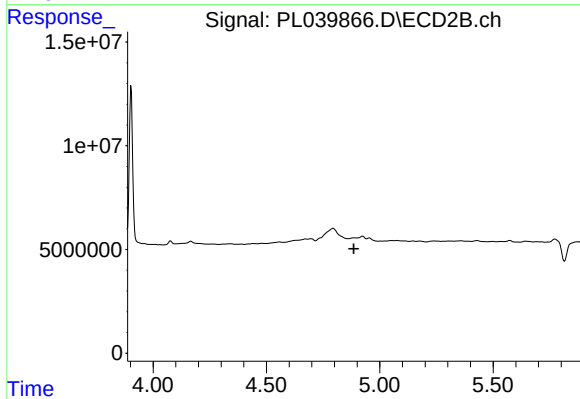

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

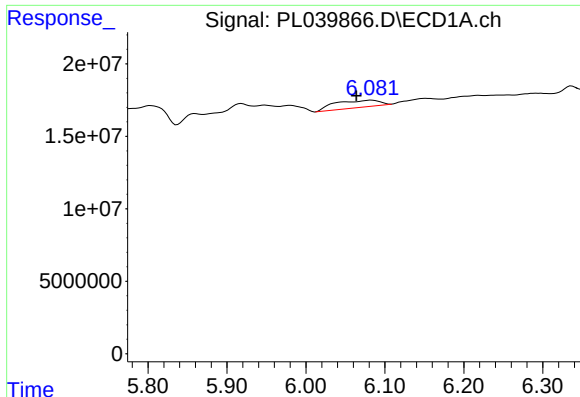

#27 Chlordane-5


R.T.: 6.083 min
Delta R.T.: 0.019 min
Response: 19321485
Conc: 59.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

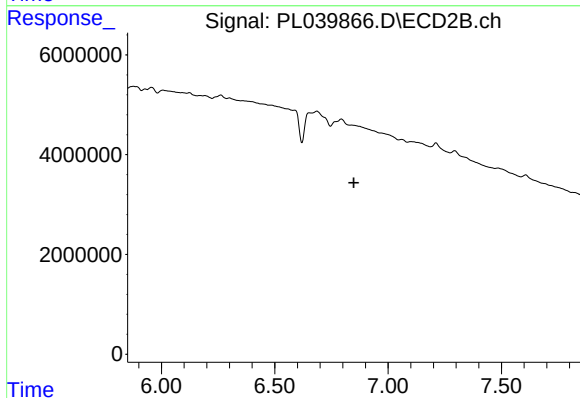


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

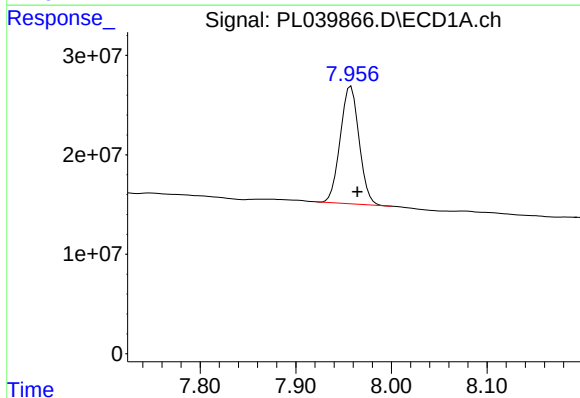

#28 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.007 min
Response: 161838077
Conc: 23.04 ng/ml

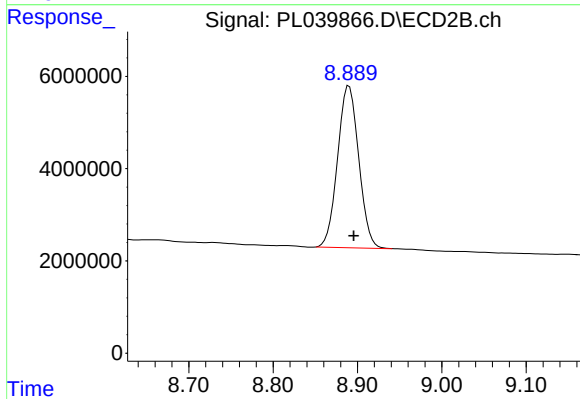

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: -0.005 min
Response: 61117510
Conc: 26.34 ng/ml