

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091219\
 Data File : PL052395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2019 15:24
 Operator : SG\AJ
 Sample : K4850-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AOC-7-(5)

Manual Integrations
 APPROVED

Ankita
 9/13/2019 3:44:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:11:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 12 03:37:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.923	115.2E6	26527610	12.787m	12.181
28)	SA Decachlor...	7.969	8.947	112.7E6	25080378	8.033	8.453

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091219\
Data File : PL052395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2019 15:24
Operator : SG\AJ
Sample : K4850-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AOC-7-(5)


Manual Integrations
APPROVED

Ankita
9/13/2019 3:44:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:11:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
Quant Title : GC Extractables
QLast Update : Thu Sep 12 03:37:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

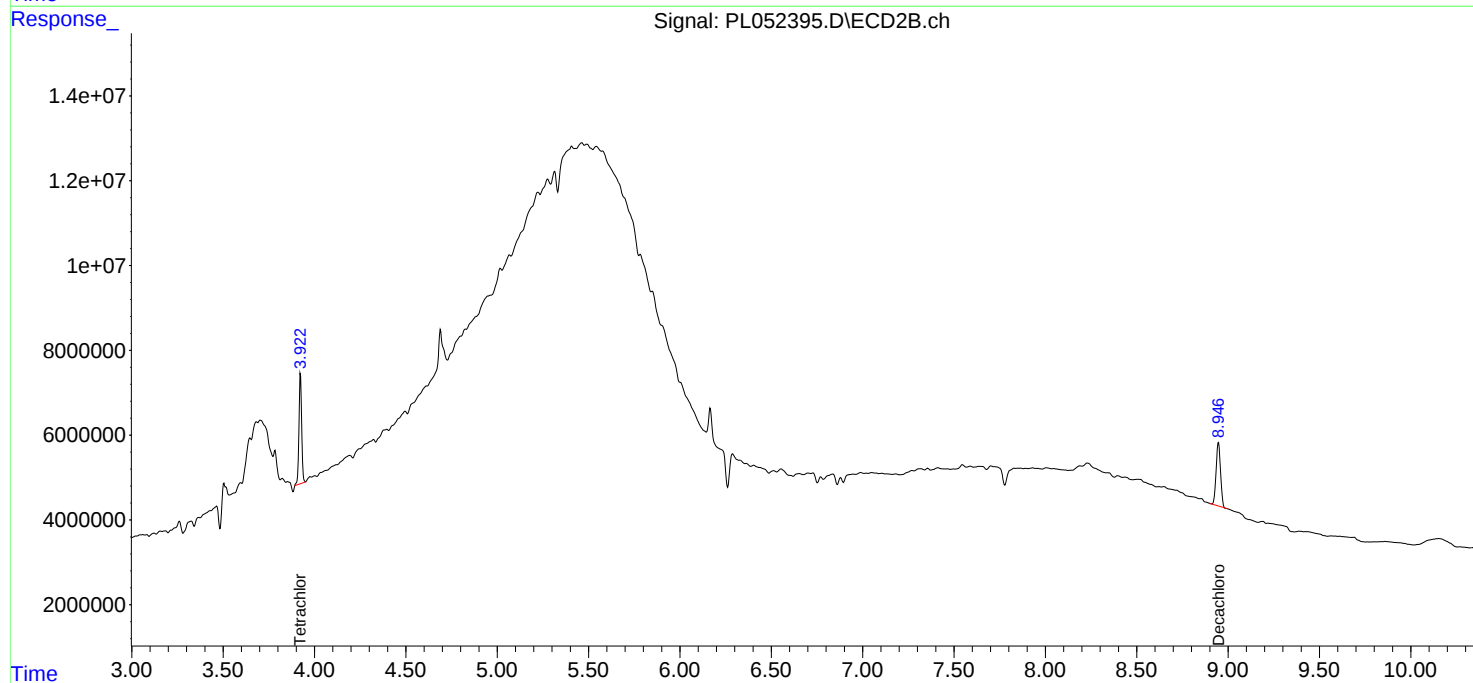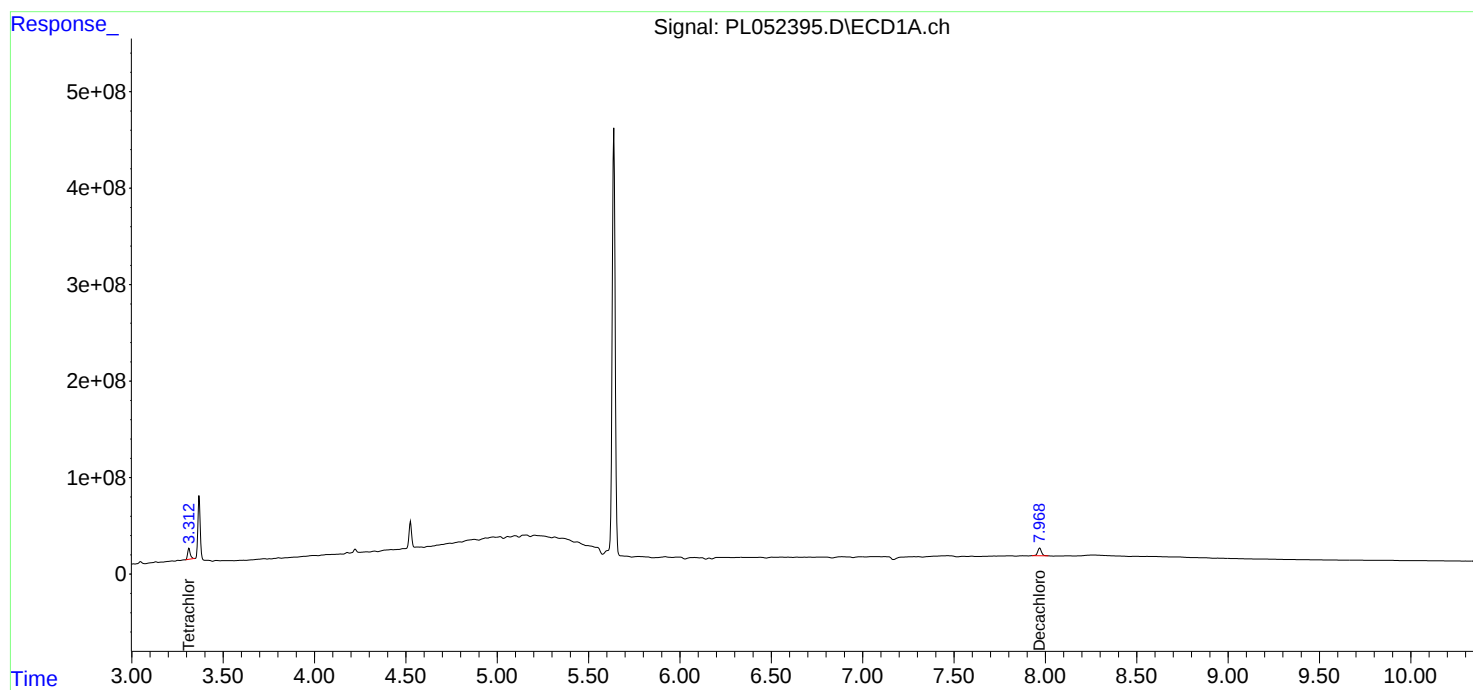

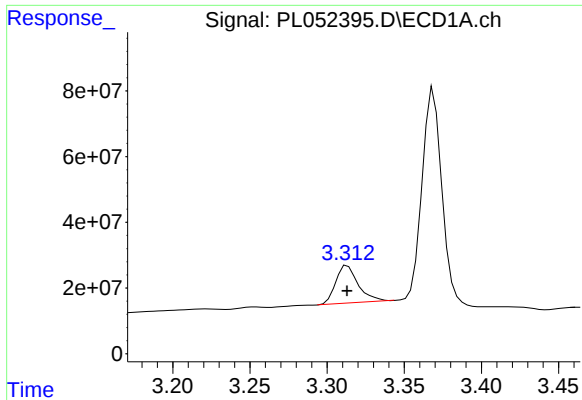


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.001 min
Response: 115209821
Conc: 12.79 ng/ml m

Instrument :
ECD_L
ClientSampleId :
AOC-7-(5)


Manual Integrations
APPROVED

Ankita
9/13/2019 3:44:54 PM

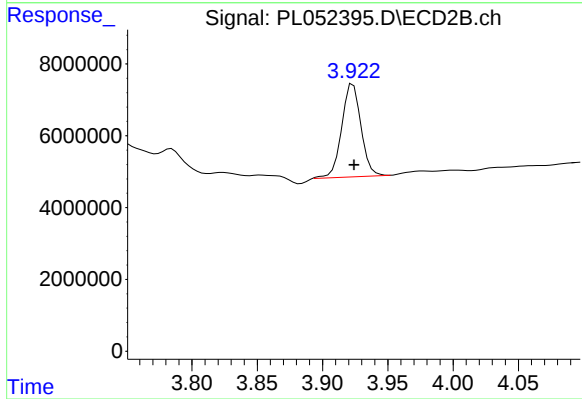


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: 0.000 min
Response: 26527610
Conc: 12.18 ng/ml

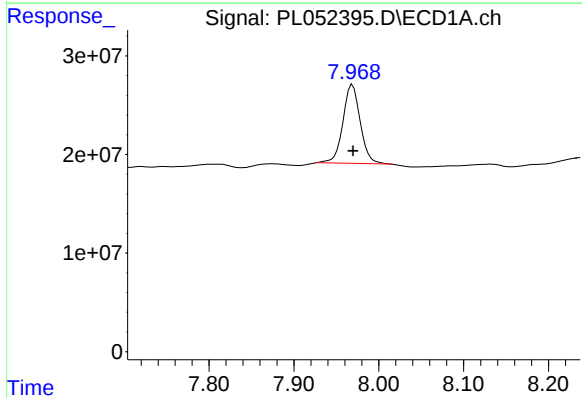

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 112707143
Conc: 8.03 ng/ml

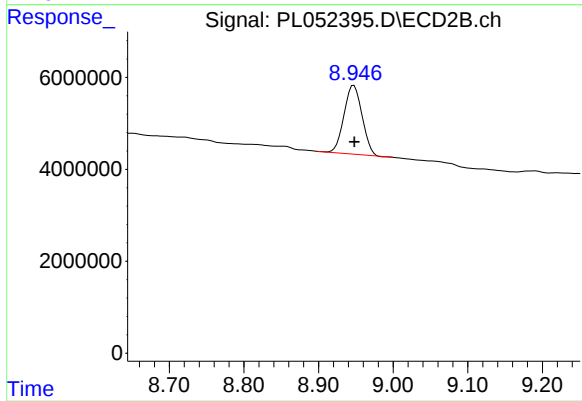

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: 0.000 min
Response: 25080378
Conc: 8.45 ng/ml