

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091219\
 Data File : PL052422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2019 21:44
 Operator : SG\AJ
 Sample : K4850-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AOC-7-(7)

Manual Integrations
 APPROVED

Ankita
 9/13/2019 3:45:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:16:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 12 03:37:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.922	179.5E6	49694142	19.927	22.819m
28)	SA Decachlor...	7.968	8.945	269.3E6	65753642	19.195	22.162
Target Compounds							
10)	B gamma-Chl...	5.184	6.011	29012595	22296481	1.771m	5.873 #
14)	MA Endrin	5.792	6.617	25918548	1728854	1.616m	0.552m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091219\
Data File : PL052422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2019 21:44
Operator : SG\AJ
Sample : K4850-07
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AOC-7-(7)


Manual Integrations
APPROVED

Ankita
9/13/2019 3:45:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:16:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
Quant Title : GC Extractables
QLast Update : Thu Sep 12 03:37:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

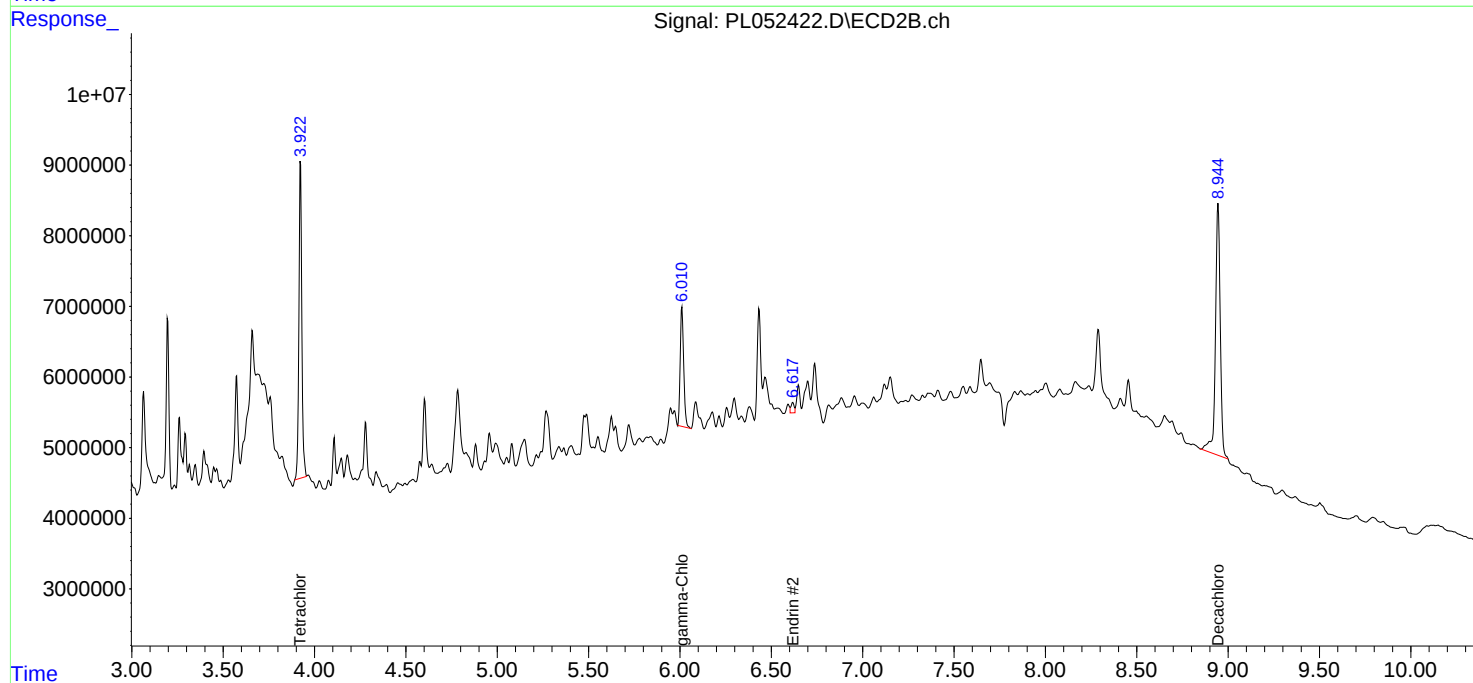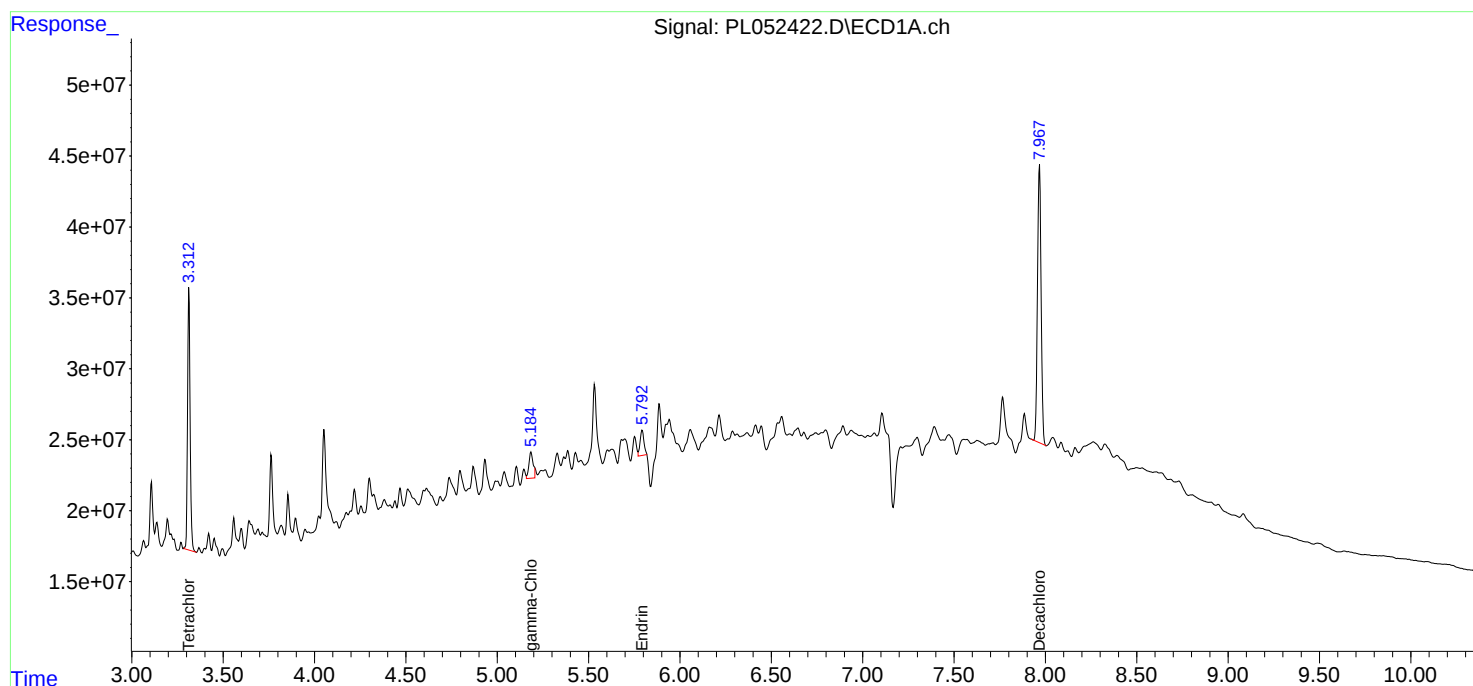

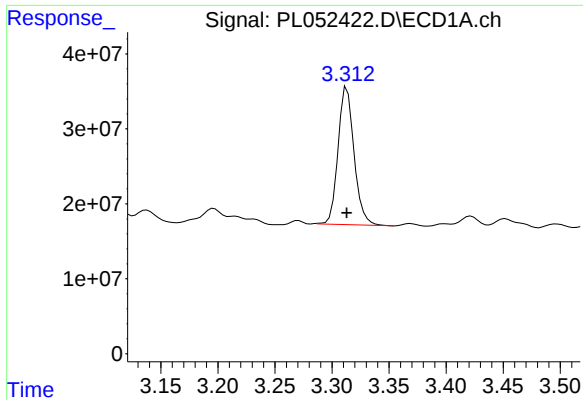


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 179541573
Conc: 19.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
AOC-7-(7)


Manual Integrations
APPROVED

Ankita
9/13/2019 3:45:34 PM

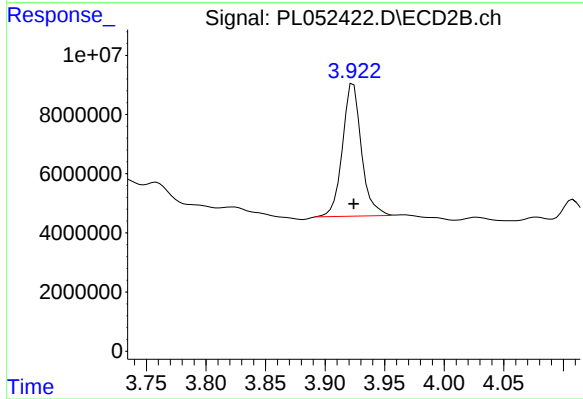


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.002 min
Response: 49694142
Conc: 22.82 ng/ml m

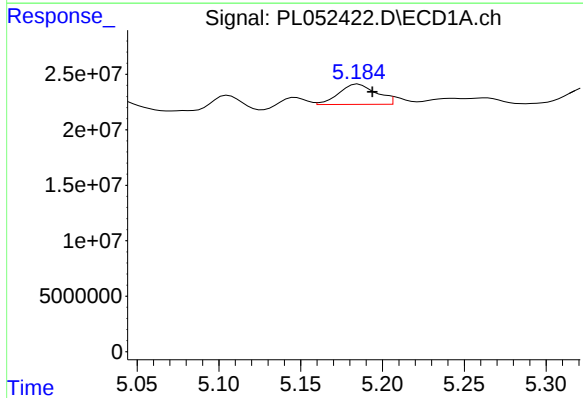


#10 gamma-Chlordane

R.T.: 5.184 min
Delta R.T.: -0.010 min
Response: 29012595
Conc: 1.77 ng/ml m

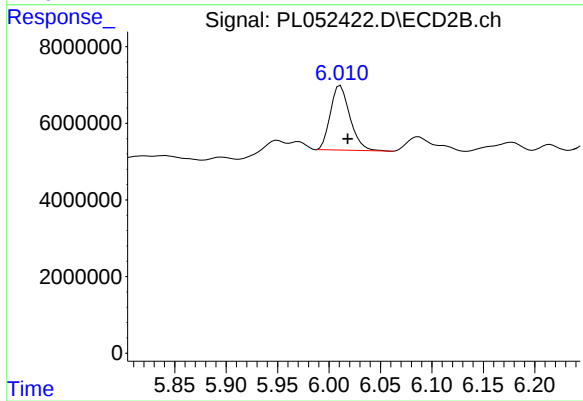

#10 gamma-Chlordane

R.T.: 6.011 min
Delta R.T.: -0.007 min
Response: 22296481
Conc: 5.87 ng/ml

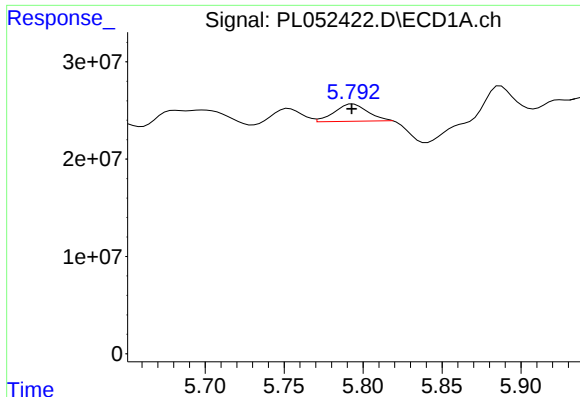


#14 Endrin

R.T.: 5.792 min
Delta R.T.: 0.000 min
Response: 25918548
Conc: 1.62 ng/ml m

Instrument :
ECD_L
ClientSampleId :
AOC-7-(7)


Manual Integrations
APPROVED

Ankita
9/13/2019 3:45:34 PM

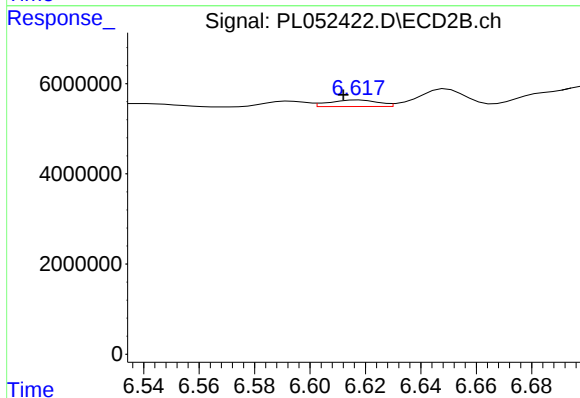


#14 Endrin

R.T.: 6.617 min
Delta R.T.: 0.004 min
Response: 1728854
Conc: 0.55 ng/ml m

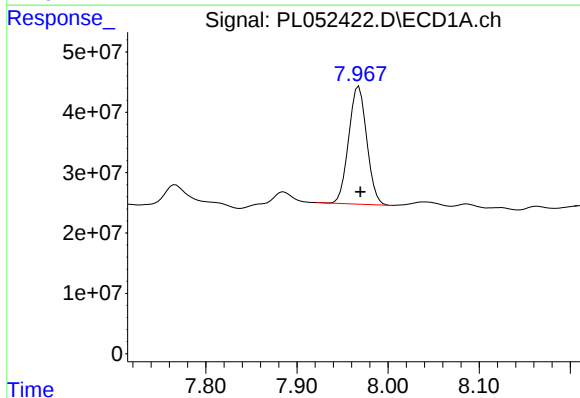

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.002 min
Response: 269311715
Conc: 19.19 ng/ml

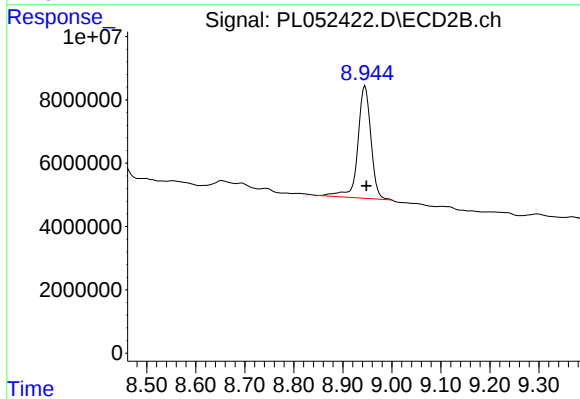

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.003 min
Response: 65753642
Conc: 22.16 ng/ml