

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091219\
 Data File : PL052427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2019 22:54
 Operator : SG\AJ
 Sample : K4850-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AOC-7-(6)

Manual Integrations
 APPROVED

Ankita
 9/13/2019 3:45:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:17:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 12 03:37:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.921	150.1E6	13021671	16.663m	5.979m#
28)	SA Decachlor...	7.968	8.944	56304443	9834761	4.013m	3.315m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091219\
Data File : PL052427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2019 22:54
Operator : SG\AJ
Sample : K4850-02
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AOC-7-(6)


Manual Integrations
APPROVED

Ankita
9/13/2019 3:45:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:17:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
Quant Title : GC Extractables
QLast Update : Thu Sep 12 03:37:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

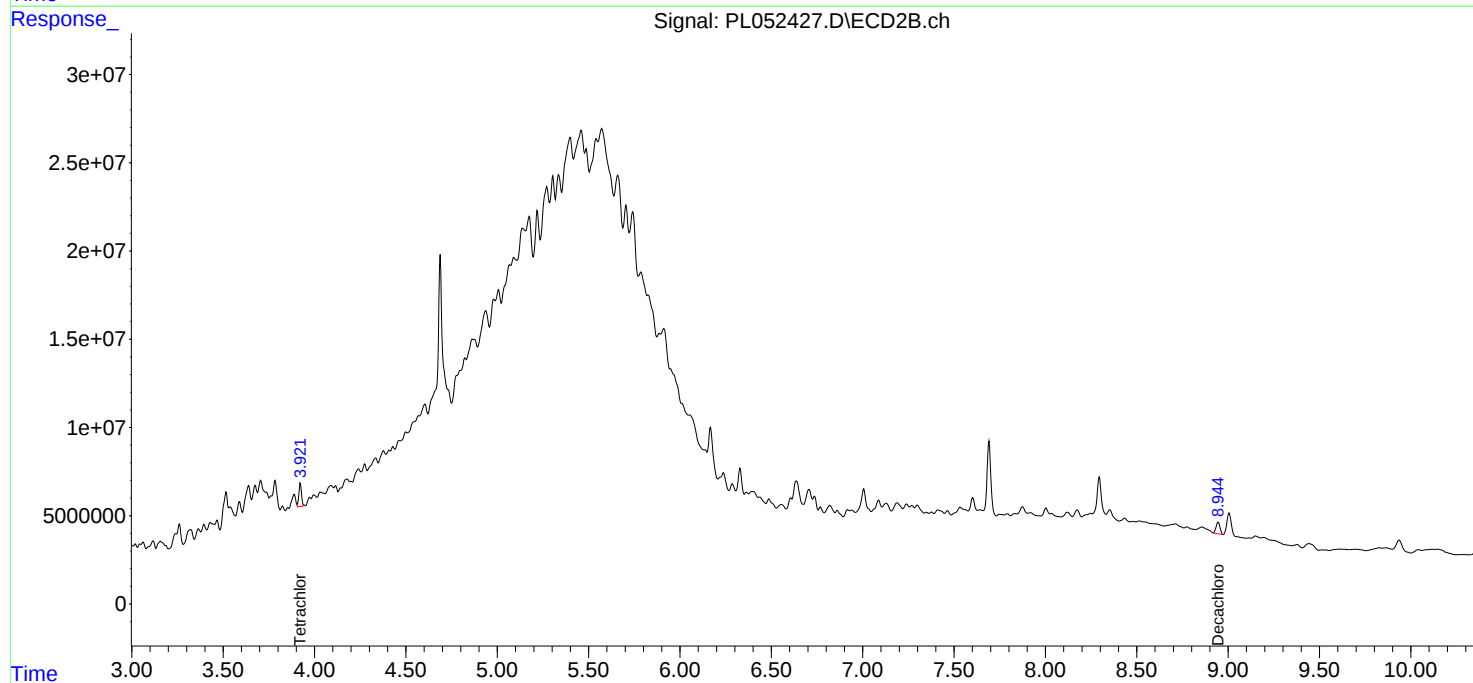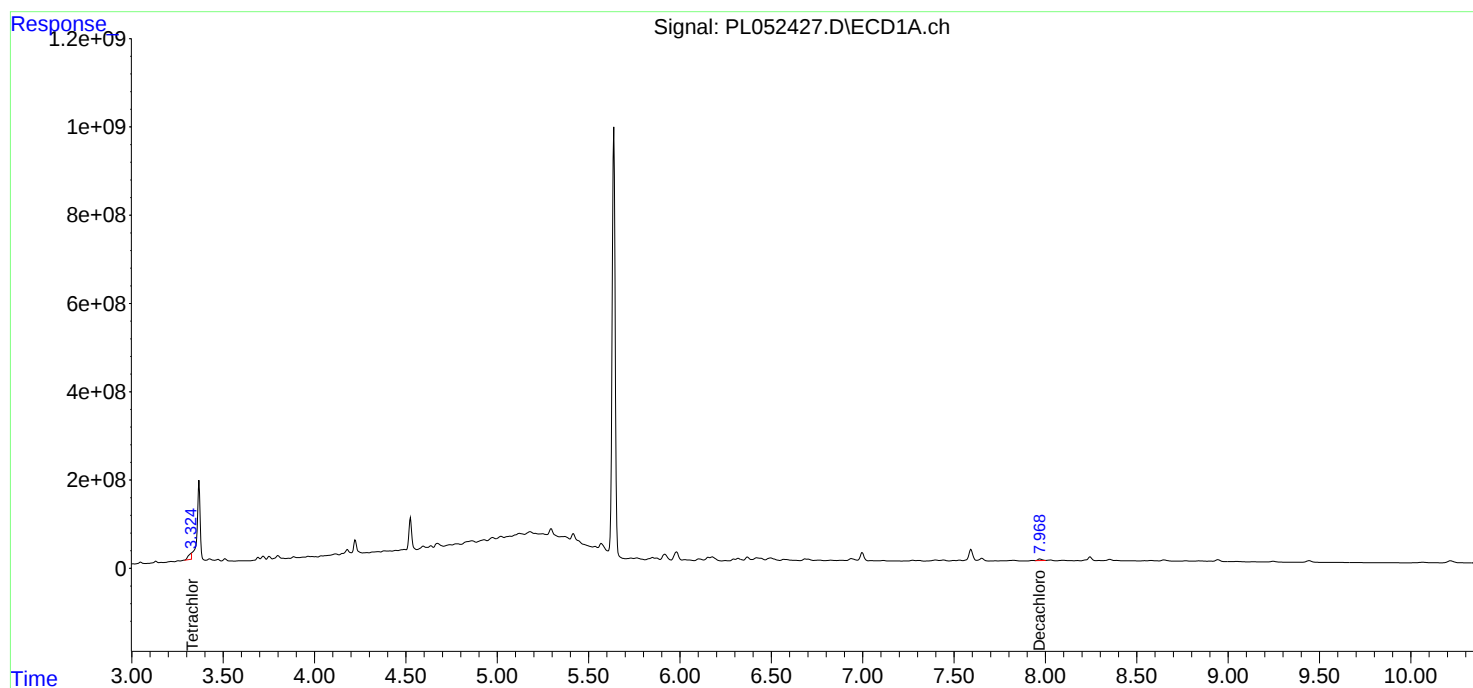

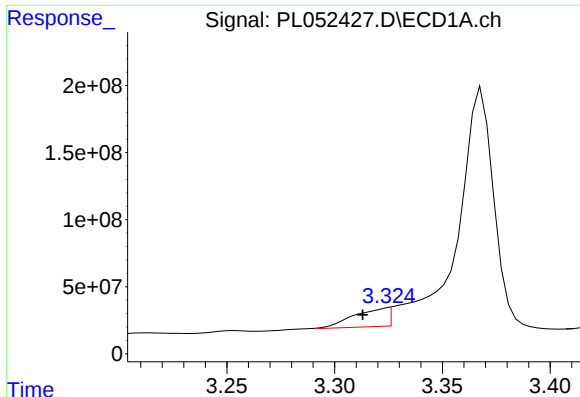


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.011 min
Response: 150133288
Conc: 16.66 ng/ml m

Instrument :
ECD_L
ClientSampleId :
AOC-7-(6)


Manual Integrations
APPROVED

Ankita
9/13/2019 3:45:40 PM

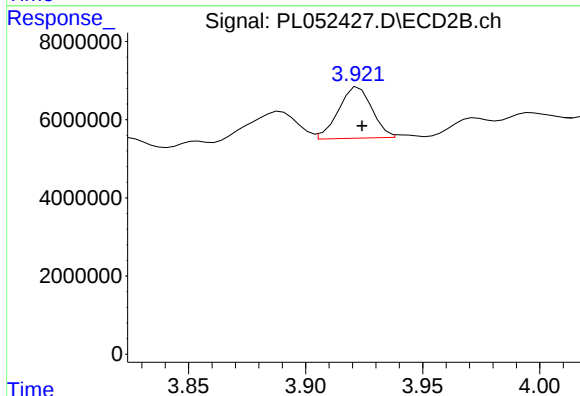


#1 Tetrachloro-m-xylene

R.T.: 3.921 min
Delta R.T.: -0.003 min
Response: 13021671
Conc: 5.98 ng/ml m

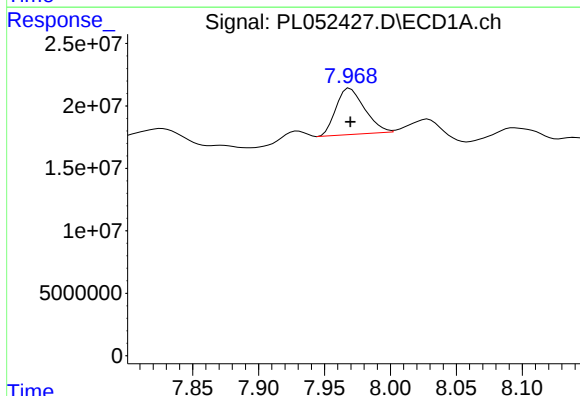

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.002 min
Response: 56304443
Conc: 4.01 ng/ml m

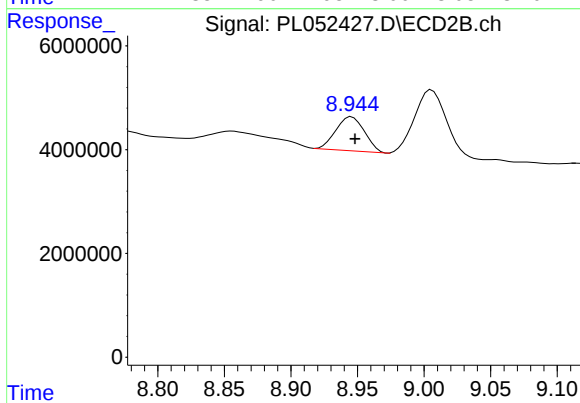

#28 Decachlorobiphenyl

R.T.: 8.944 min
Delta R.T.: -0.004 min
Response: 9834761
Conc: 3.31 ng/ml m