

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091222\
 Data File : PL077669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2022 18:56
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 13:03:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 12:55:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.625	38624864	86958016	23.305	23.377
28)	SA Decachlor...	8.906	7.724	31830301	63039503	25.004	24.596
Target Compounds							
23)	Chlordane-1	4.575	3.603	15031246	26837398	227.182	238.538
24)	Chlordane-2	5.109	4.173	16318938	29531846	234.722	241.985
25)	Chlordane-3	5.821	4.796	57935233	83482859	225.775	236.056
26)	Chlordane-4	5.899	4.858	70598355	88343578	229.220	236.916
27)	Chlordane-5	6.757	5.522	12140898	23002278	231.059	241.207



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091222\
Data File : PL077669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2022 18:56
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 13:03:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 12:55:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

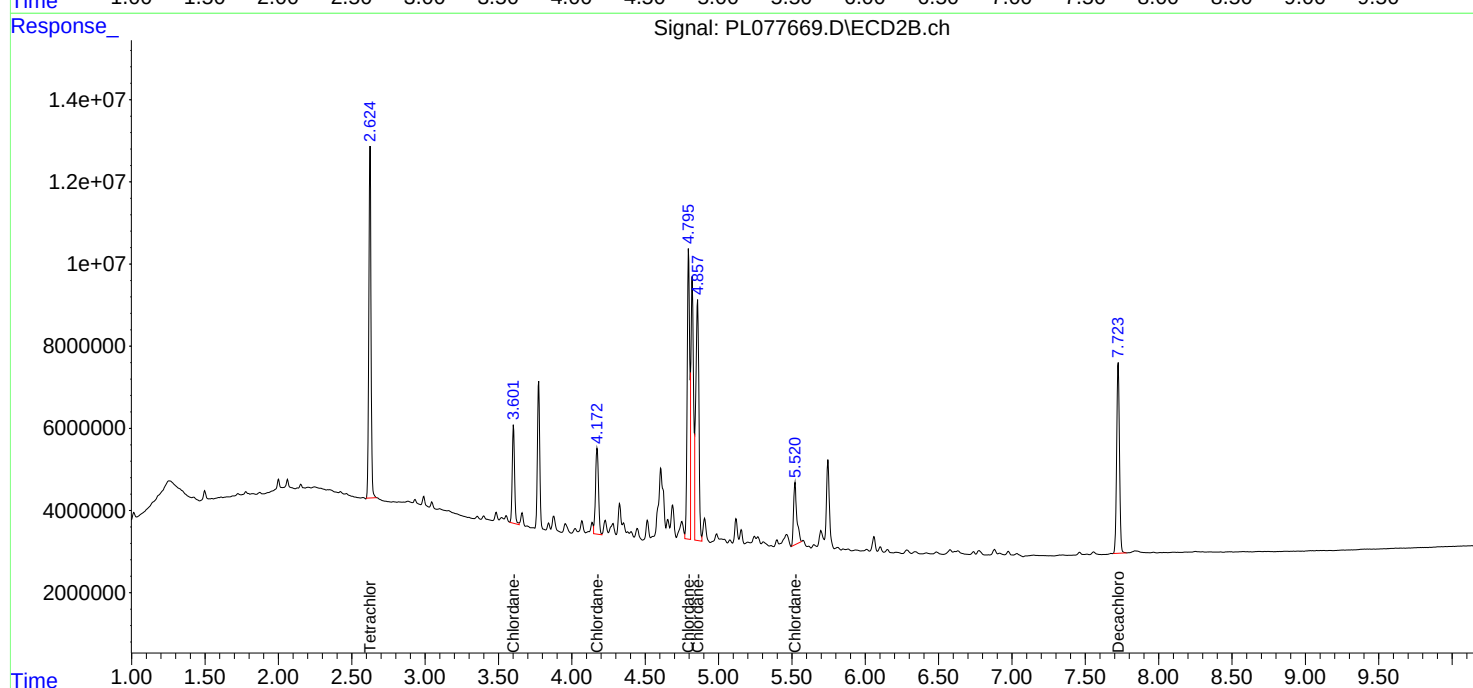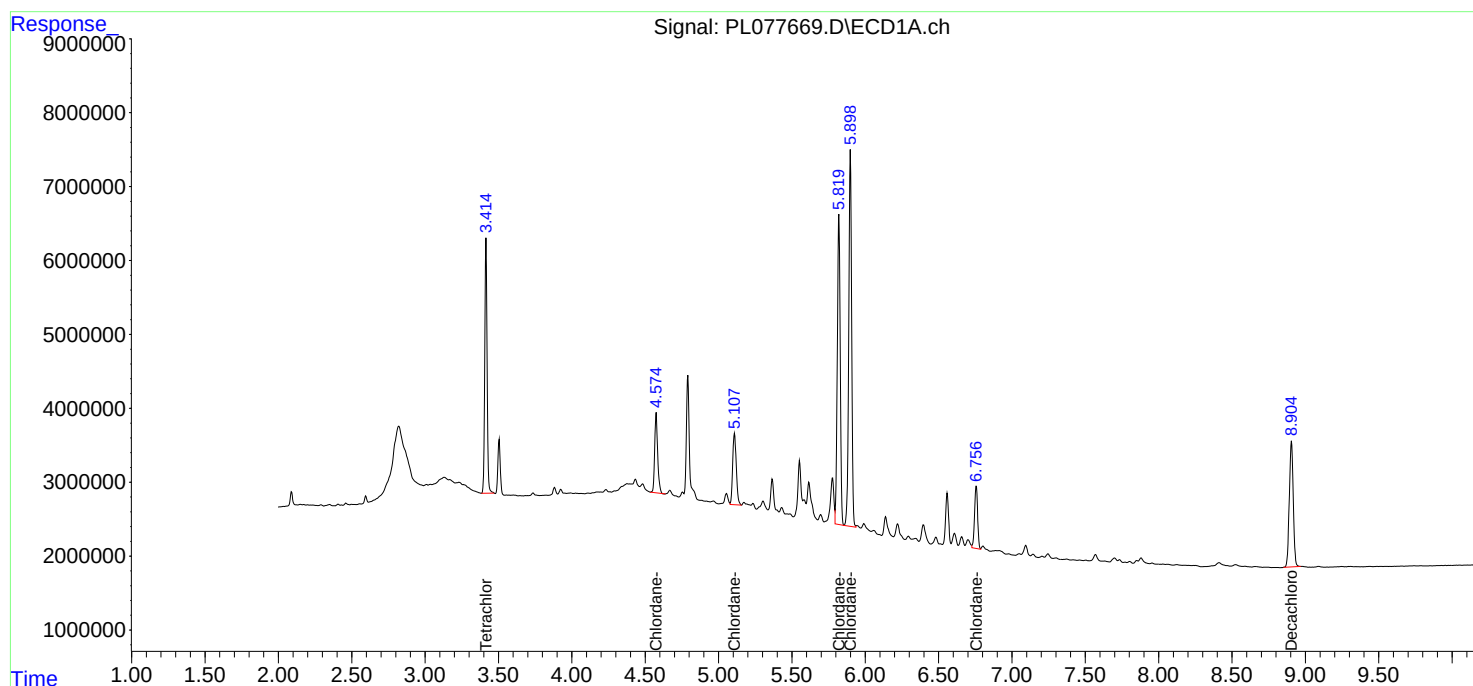


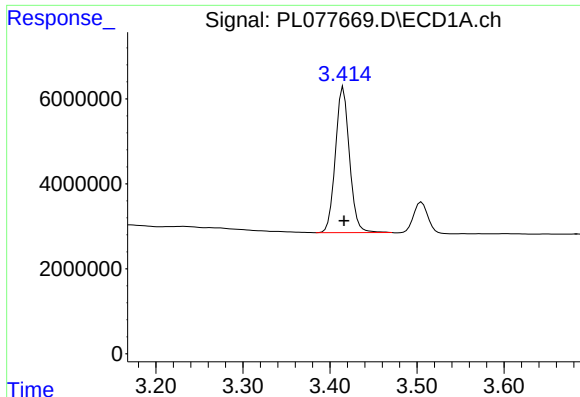

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 38624864
Conc: 23.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

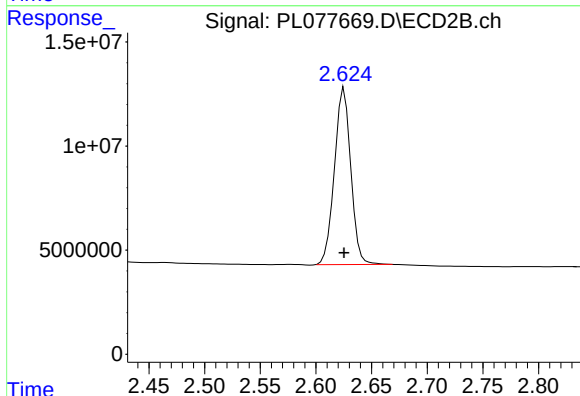


#1 Tetrachloro-m-xylene

R.T.: 2.625 min
Delta R.T.: 0.000 min
Response: 86958016
Conc: 23.38 ng/ml

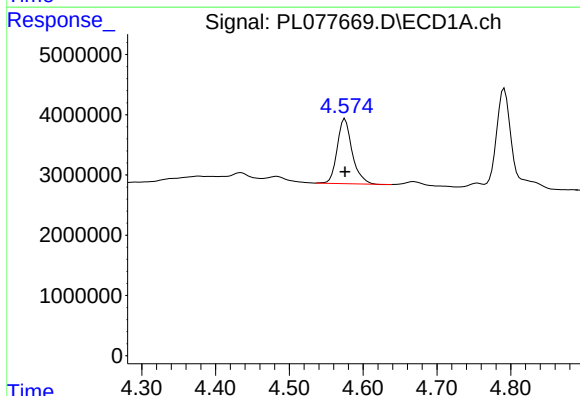


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.000 min
Response: 15031246
Conc: 227.18 ng/ml

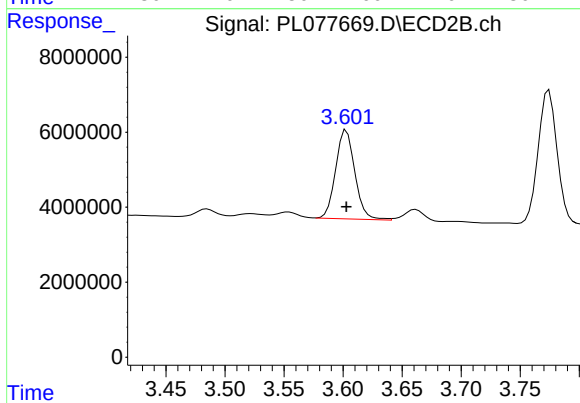

#23 Chlordane-1


R.T.: 3.603 min
Delta R.T.: 0.000 min
Response: 26837398
Conc: 238.54 ng/ml

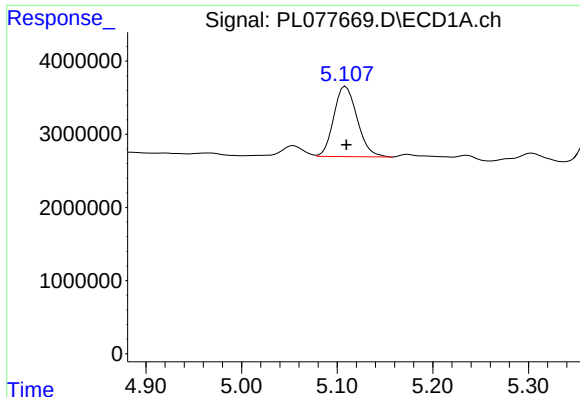

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 16318938
Conc: 234.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

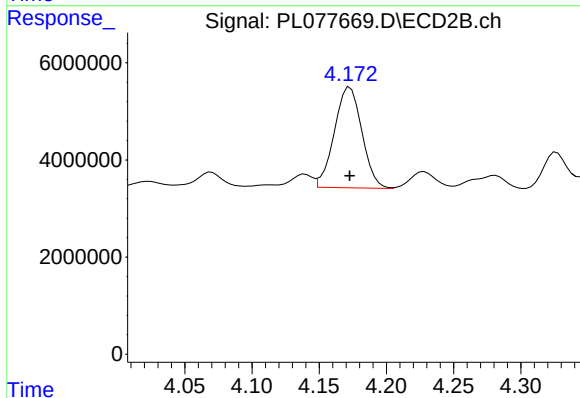


#24 Chlordane-2

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 29531846
Conc: 241.99 ng/ml

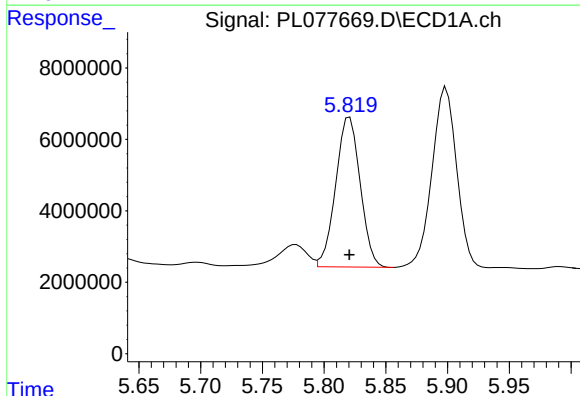


#25 Chlordane-3

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 57935233
Conc: 225.78 ng/ml

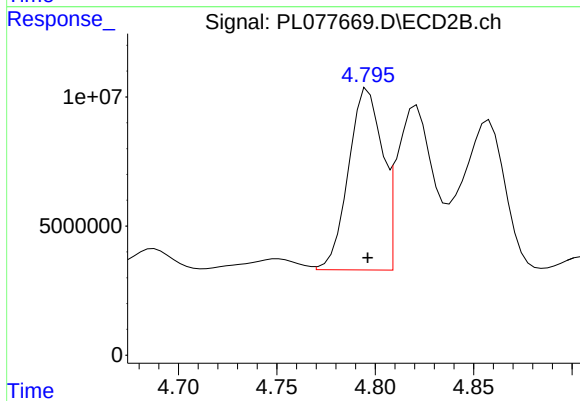

#25 Chlordane-3


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 83482859
Conc: 236.06 ng/ml

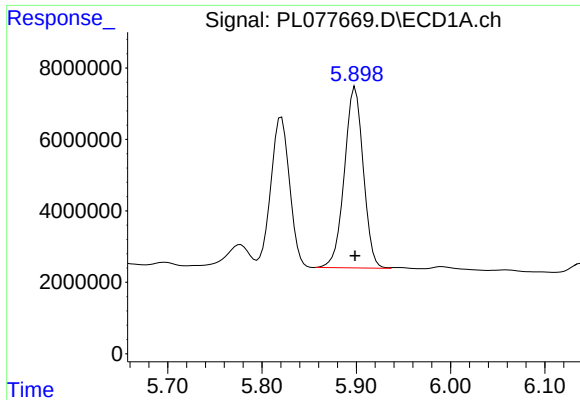

#26 Chlordane-4


R.T.: 5.899 min
Delta R.T.: 0.000 min
Response: 70598355
Conc: 229.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

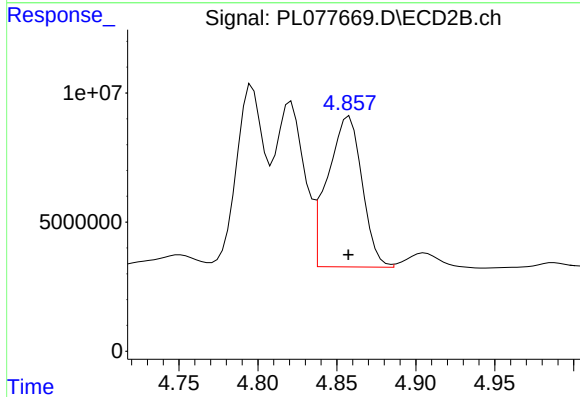


#26 Chlordane-4

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 88343578
Conc: 236.92 ng/ml

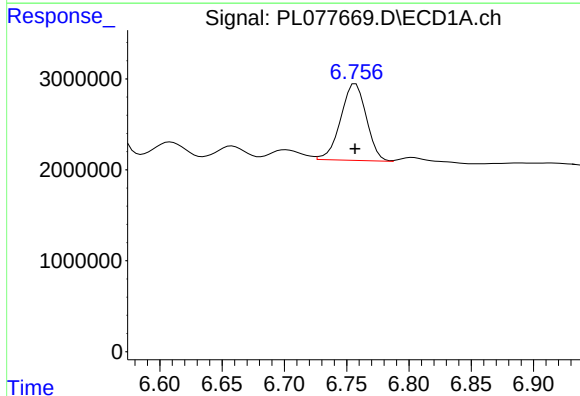


#27 Chlordane-5

R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 12140898
Conc: 231.06 ng/ml

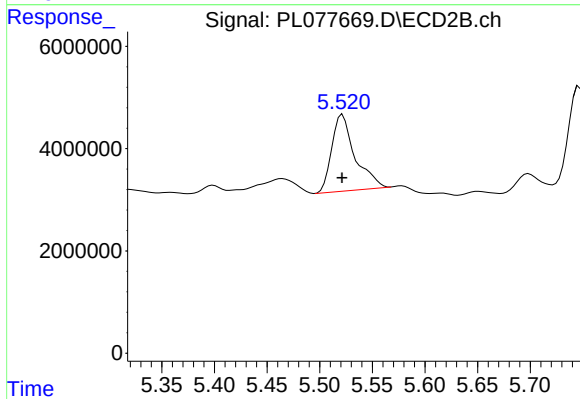

#27 Chlordane-5


R.T.: 5.522 min
Delta R.T.: 0.000 min
Response: 23002278
Conc: 241.21 ng/ml

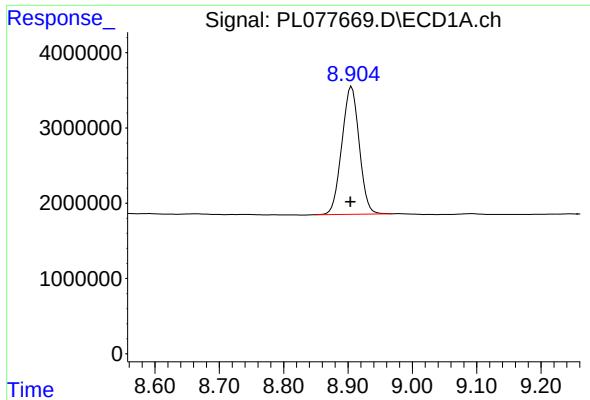

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: 0.002 min
Response: 31830301
Conc: 25.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

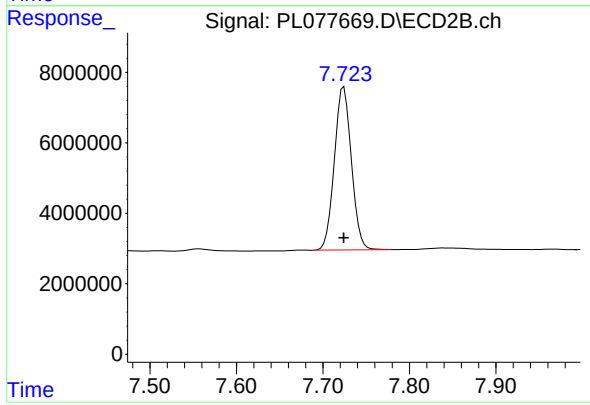

#28 Decachlorobiphenyl

R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 63039503
Conc: 24.60 ng/ml