

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091222\
 Data File : PL077677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2022 20:46
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL091222CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 13:14:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:12:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.625	83269222	189.4E6	52.123	52.851
28)	SA Decachlor...	8.903	7.723	64100573	131.2E6	49.728	51.064
Target Compounds							
23)	Chlordane-1	4.575	3.602	33231044	58760224	534.534	540.753
24)	Chlordane-2	5.109	4.172	34729936	62781494	520.889	524.098
25)	Chlordane-3	5.820	4.796	128.9E6	180.4E6	523.428	524.394
26)	Chlordane-4	5.898	4.857	154.5E6	191.7E6	519.285	528.350
27)	Chlordane-5	6.756	5.520	26448159	48935646	532.550	520.081



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091222\
Data File : PL077677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2022 20:46
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL091222CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 13:14:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:12:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

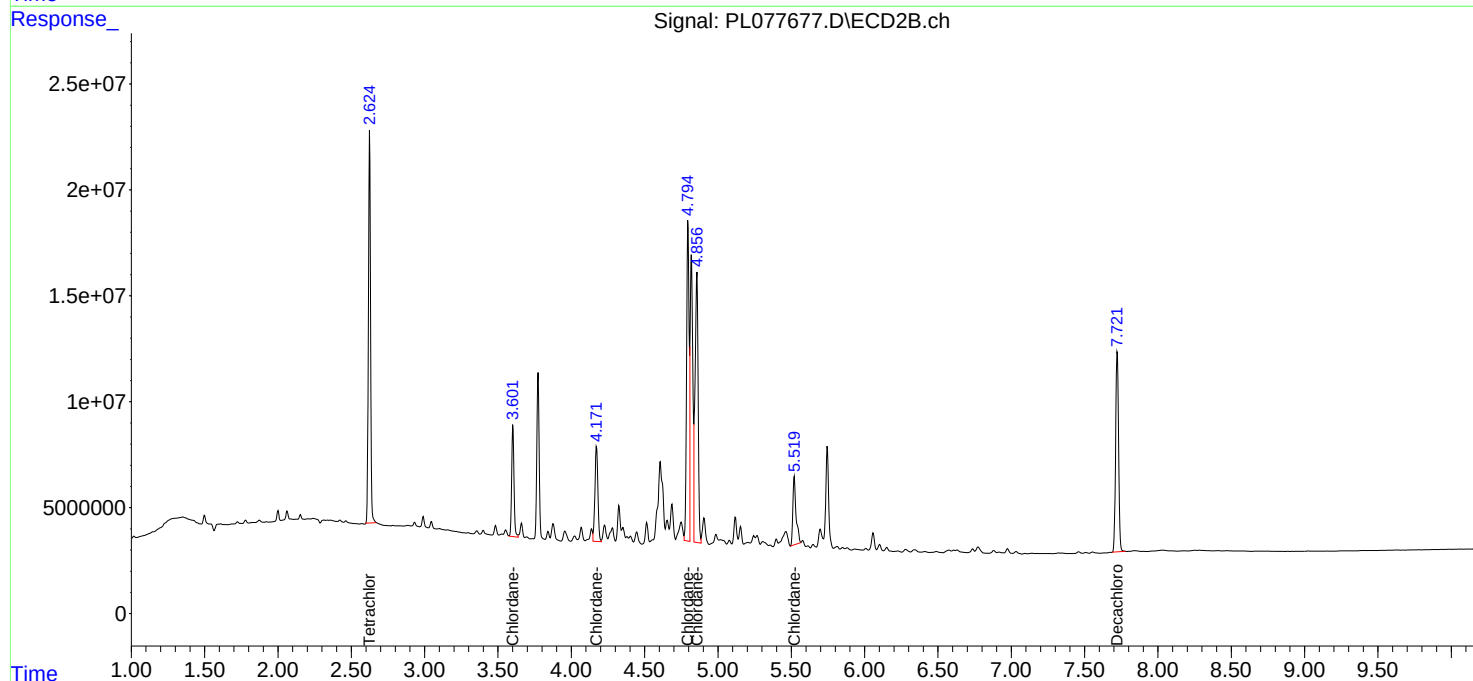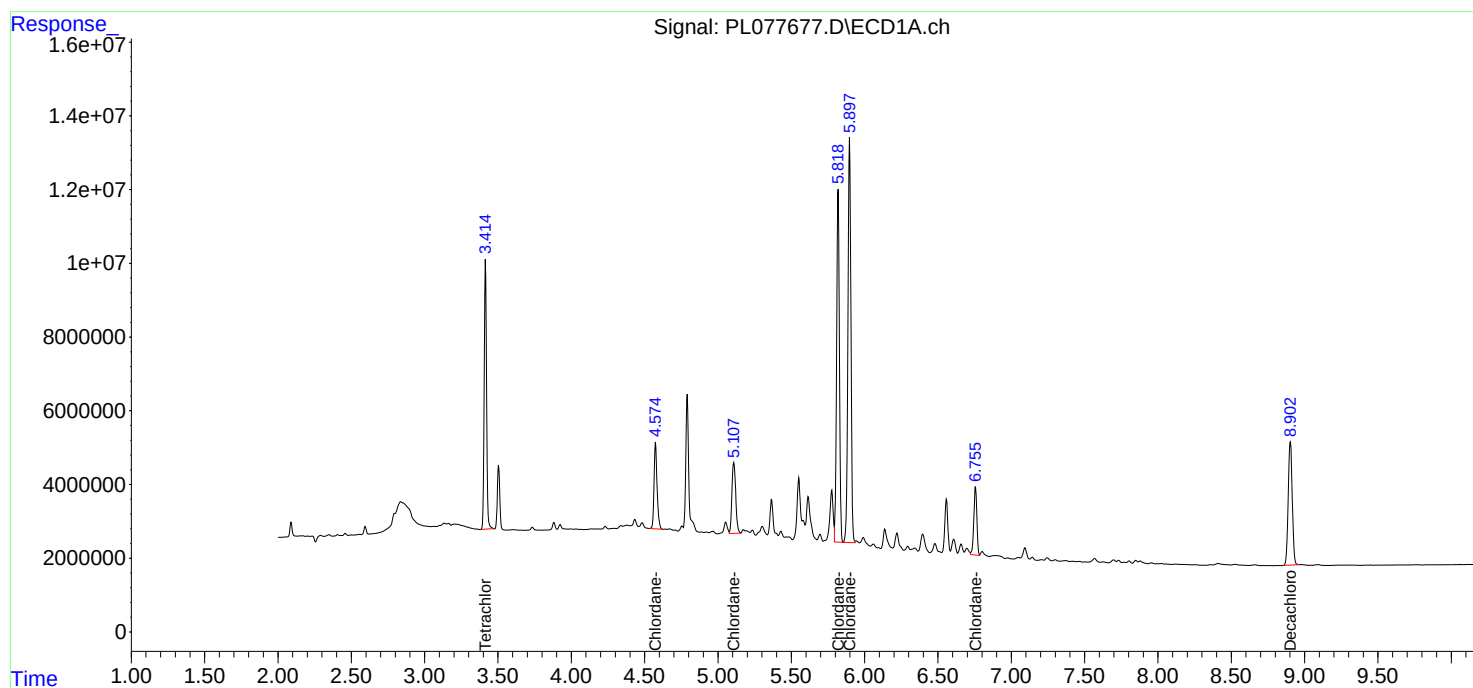


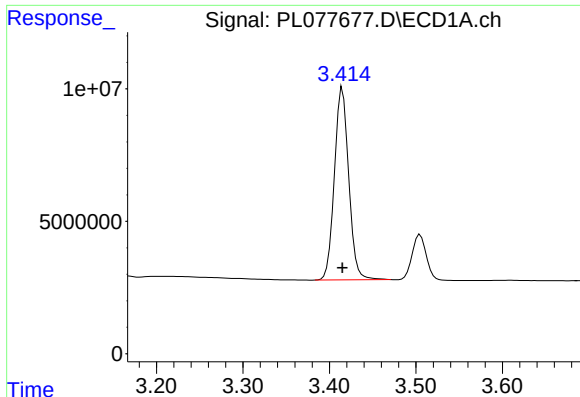

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 83269222
Conc: 52.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091222CHLOR

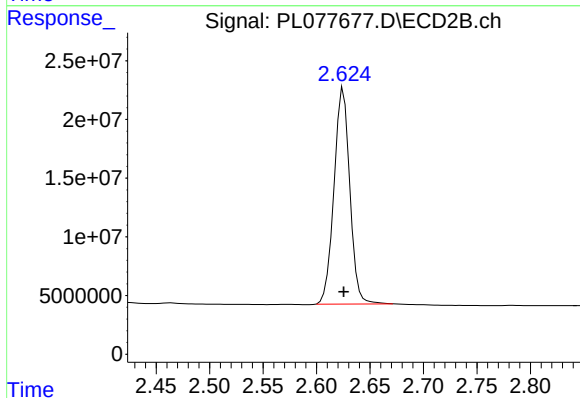


#1 Tetrachloro-m-xylene

R.T.: 2.625 min
Delta R.T.: 0.000 min
Response: 189366878
Conc: 52.85 ng/ml

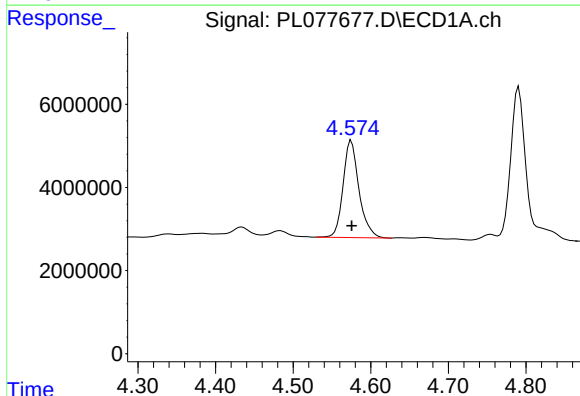


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.000 min
Response: 33231044
Conc: 534.53 ng/ml

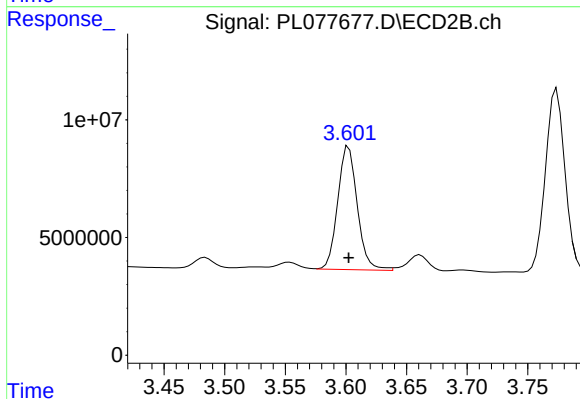

#23 Chlordane-1


R.T.: 3.602 min
Delta R.T.: 0.000 min
Response: 58760224
Conc: 540.75 ng/ml

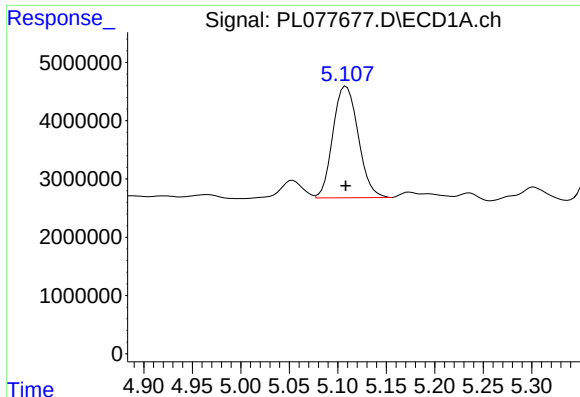

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 34729936
Conc: 520.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091222CHLOR

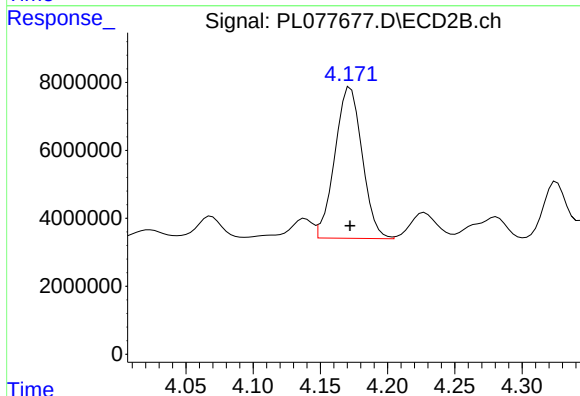


#24 Chlordane-2

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 62781494
Conc: 524.10 ng/ml

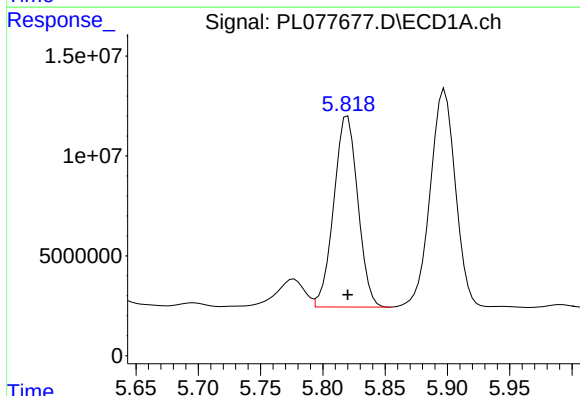


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 128900634
Conc: 523.43 ng/ml

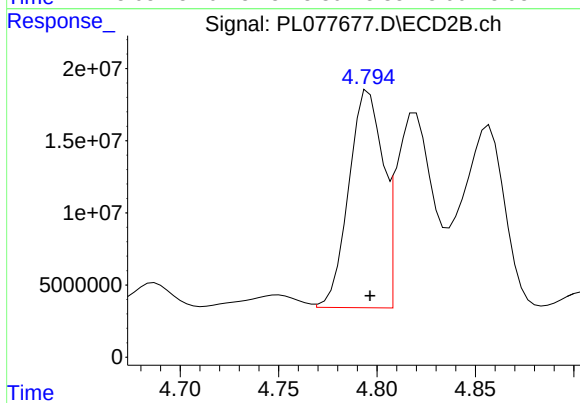

#25 Chlordane-3


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 180385099
Conc: 524.39 ng/ml

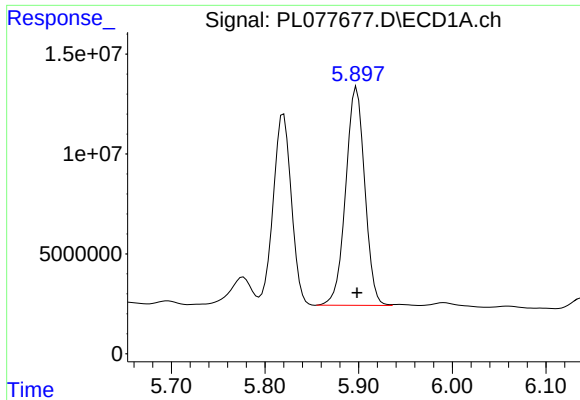

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 154523688
Conc: 519.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091222CHLOR

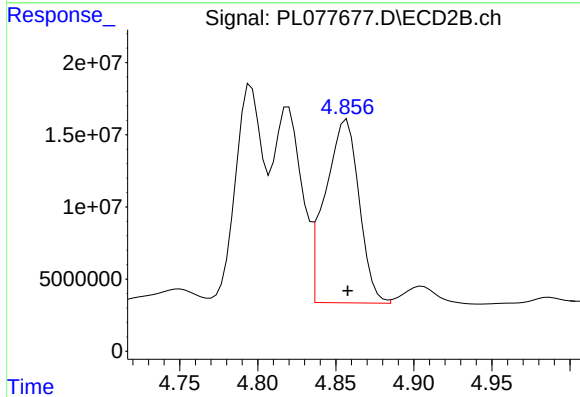


#26 Chlordane-4

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 191695012
Conc: 528.35 ng/ml

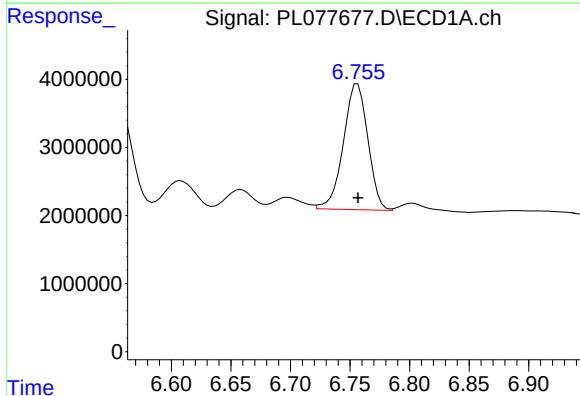


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 26448159
Conc: 532.55 ng/ml

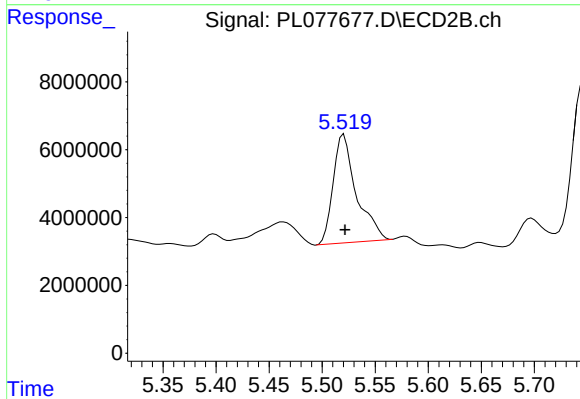

#27 Chlordane-5


R.T.: 5.520 min
Delta R.T.: -0.001 min
Response: 48935646
Conc: 520.08 ng/ml

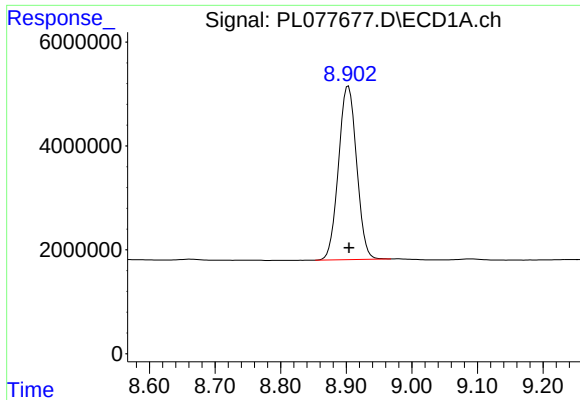

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: -0.001 min
Response: 64100573
Conc: 49.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091222CHLOR

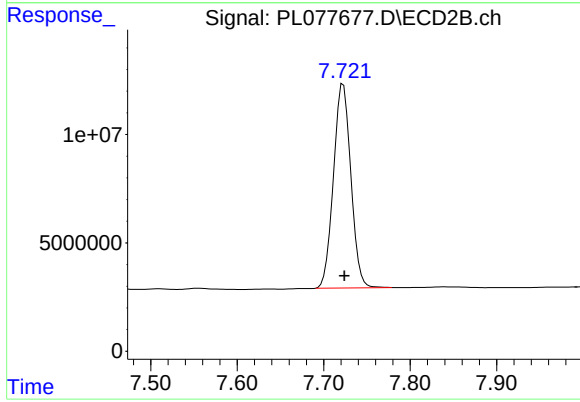

#28 Decachlorobiphenyl

R.T.: 7.723 min
Delta R.T.: -0.001 min
Response: 131194002
Conc: 51.06 ng/ml